

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
 Data File : BP000578.D
 Acq On : 09 Oct 2019 19:05
 Operator : JU
 Sample : K5201-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB8

Quant Time: Oct 10 01:21:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	229500	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	886953	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	521045	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	979904	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	874103	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	947253	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.36	96	27082	4.90	ng/uL	0.00
5) Phenol-d5	6.39	99	110010	6.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	238526	26.95	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	324970	21.79	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	189304	14.00	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	190348	28.23	ng/ul	0.00
22) 2-Nitrophenol-d4	7.64	143	204156	28.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.89	165	351944	25.61	ng/ul	0.00
29) 4-Chloroaniline-d4	8.10	131	21830	1.43	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1151707	31.58	ng/ul	0.00
47) Acenaphthylene-d8	9.65	160	1287755	28.70	ng/ul	0.00
52) 4-Nitrophenol-d4	9.91	143	32040	5.70	ng/ul	0.00
58) Fluorene-d10	10.32	176	956162	30.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	111735	23.94	ng/ul	0.00
71) Anthracene-d10	11.35	188	1482654	32.67	ng/ul	0.00
79) Pyrene-d10	12.73	212	1636938	33.12	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1588856	33.98	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.40	94	18847	1.056	ng/ul	92
45) Dimethylphthalate	9.51	163	112925	3.107	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000578.D
Acq On : 09 Oct 2019 19:05
Operator : JU
Sample : K5201-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Quant Time: Oct 10 01:21:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration

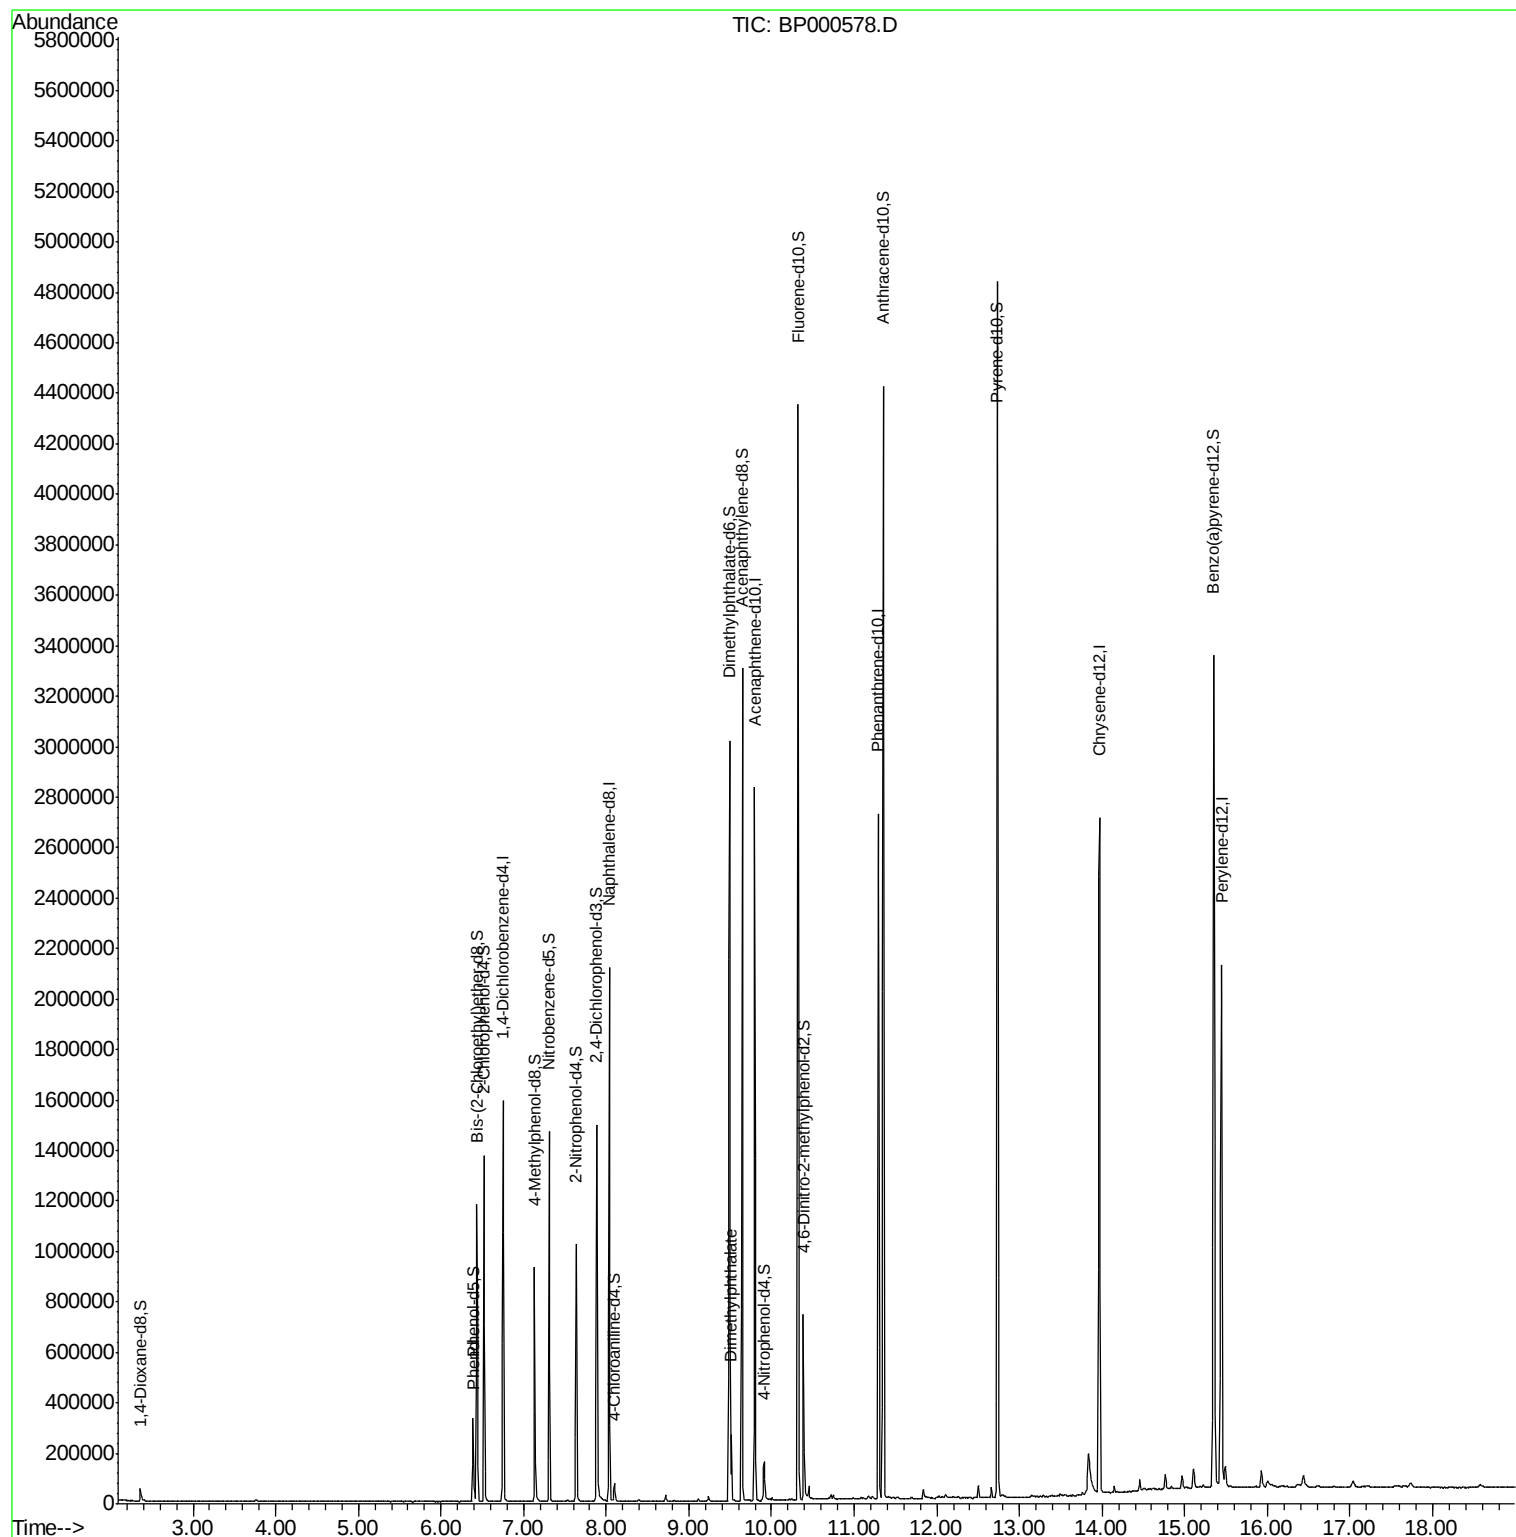

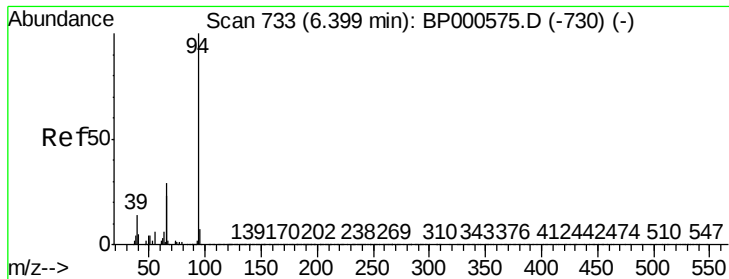

#6

Phenol

Concen: 1.056 ng/ul

RT: 6.40 min Scan# 733

Delta R.T. -0.00 min

Lab File: BP000578.D

Acq: 09 Oct 2019 19:05

Instrument :


BNA_P

ClientSampleId :

C0AB8

Tot Ion: 94 Resp: 18847


Ion	Ratio	Lower	Upper
94	100		
65	25.3	19.2	28.8
66	38.3	25.7	38.5

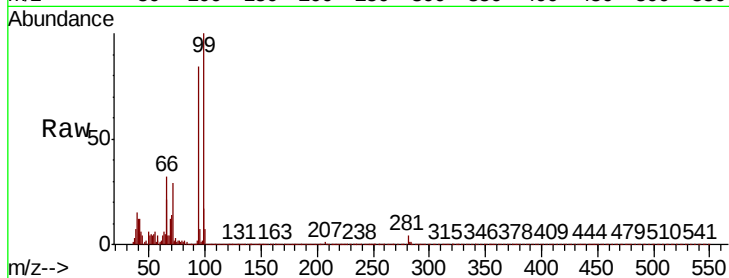


Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

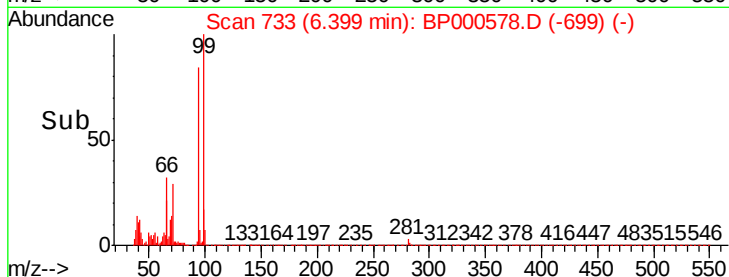

Time-->

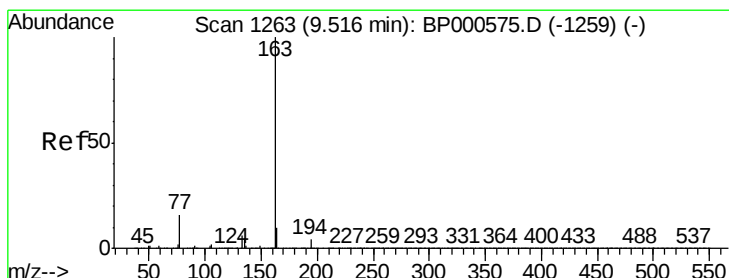

#45

Dimethylphthalate

Concen: 3.107 ng/ul

RT: 9.51 min Scan# 1262


Delta R.T. -0.01 min

Lab File: BP000578.D

Acq: 09 Oct 2019 19:05

Tgt Ion:163 Resp: 112925


Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.3	4.9
164	10.4	8.1	12.1

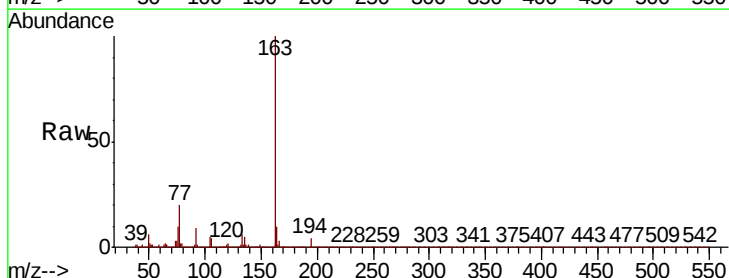

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

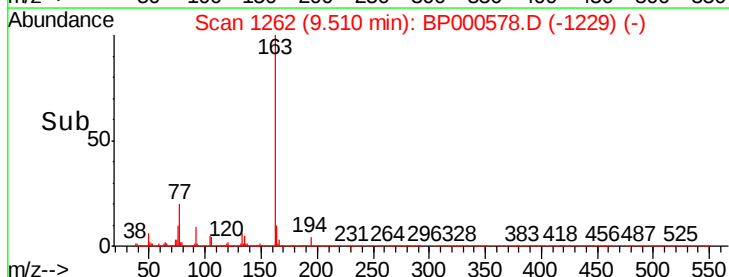

Time-->