

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
 Data File : BP000586.D
 Acq On : 09 Oct 2019 22:18
 Operator : JU
 Sample : K5100-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETJY2

Quant Time: Oct 10 01:22:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	237093	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	920809	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	528832	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	996441	20.00	ng/ul	0.00
78) Chrysene-d12	13.96	240	874434	20.00	ng/ul	0.00
86) Perylene-d12	15.44	264	964907	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.36	96	31705	5.55	ng/uL	0.00
5) Phenol-d5	6.39	99	120247	6.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	245690	26.87	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	337690	21.92	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	211430	15.13	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	193887	27.70	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	210899	28.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	353845	24.80	ng/ul	0.00
29) 4-Chloroaniline-d4	8.10	131	42782	2.70	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1088810	29.41	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	1292182	28.37	ng/ul	0.00
52) 4-Nitrophenol-d4	9.90	143	36973	6.48	ng/ul	0.00
58) Fluorene-d10	10.32	176	934362	29.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	120383	25.37	ng/ul	0.00
71) Anthracene-d10	11.35	188	1504796	32.60	ng/ul	0.00
79) Pyrene-d10	12.73	212	1614685	32.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.35	264	1591732	33.41	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	9.51	163	81484	2.209	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000586.D
Acq On : 09 Oct 2019 22:18
Operator : JU
Sample : K5100-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETJY2

Quant Time: Oct 10 01:22:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration

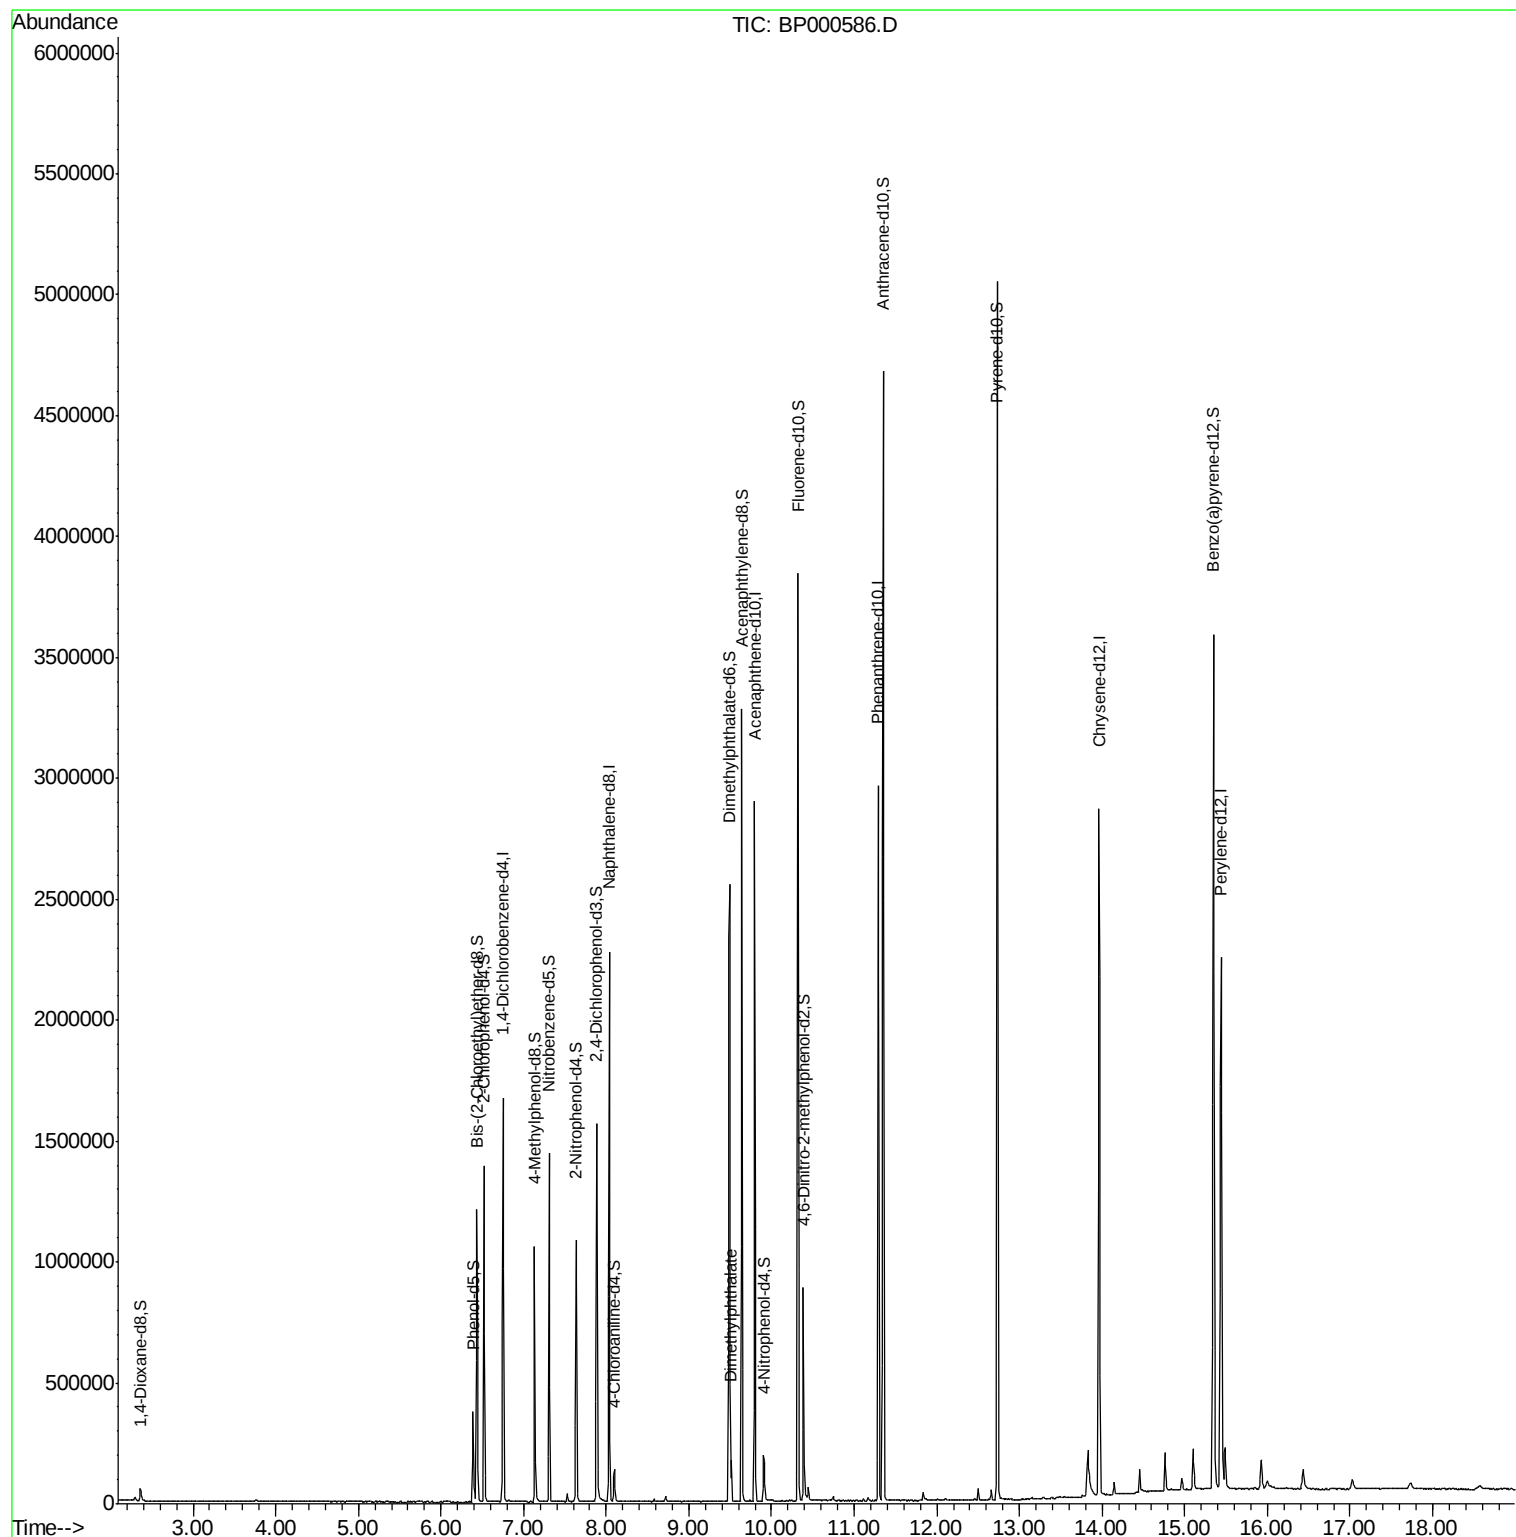


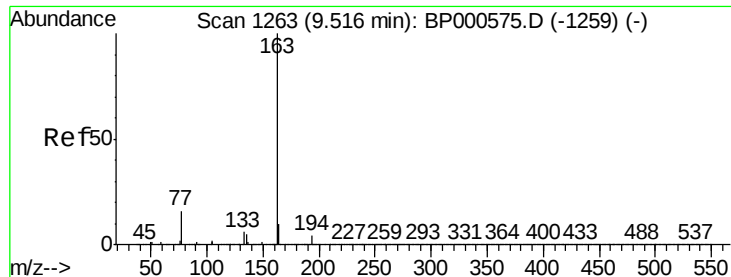

#45
 Dimethylphthalate
 Concen: 2.209 ng/ul
 RT: 9.51 min Scan# 1262
 Delta R.T. -0.01 min
 Lab File: BP000586.D
 Acq: 09 Oct 2019 22:18

Instrument :
 BNA_P
 ClientSampleId :
 ETJY2

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.3	4.9
164	10.2	8.1	12.1

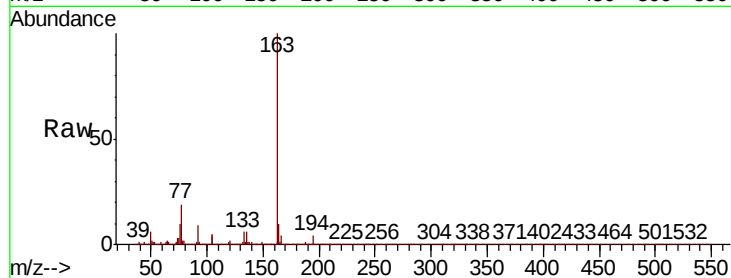

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

