

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
 Data File : BP000589.D
 Acq On : 09 Oct 2019 23:30
 Operator : JU
 Sample : K5100-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETJY5

Quant Time: Oct 10 01:23:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	206597	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	797307	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	465480	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	865972	20.00	ng/ul	0.00
78) Chrysene-d12	13.96	240	752910	20.00	ng/ul	0.00
86) Perylene-d12	15.44	264	816458	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.36	96	30082	6.04	ng/uL	0.00
5) Phenol-d5	6.39	99	132715	8.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	265573	33.33	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	369472	27.52	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	233831	19.21	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	211157	34.84	ng/ul	0.00
22) 2-Nitrophenol-d4	7.64	143	230878	35.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	386953	31.33	ng/ul	0.00
29) 4-Chloroaniline-d4	8.10	131	48498	3.53	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1166686	35.80	ng/ul	0.00
47) Acenaphthylene-d8	9.65	160	1395913	34.82	ng/ul	0.00
52) 4-Nitrophenol-d4	9.91	143	37316	7.43	ng/ul	0.00
58) Fluorene-d10	10.32	176	999700	35.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	119633	29.01	ng/ul	0.00
71) Anthracene-d10	11.35	188	1529752	38.14	ng/ul	0.00
79) Pyrene-d10	12.73	212	1611999	37.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.35	264	1564062	38.80	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	9.51	163	88489	2.725	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000589.D
Acq On : 09 Oct 2019 23:30
Operator : JU
Sample : K5100-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETJY5

Quant Time: Oct 10 01:23:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration

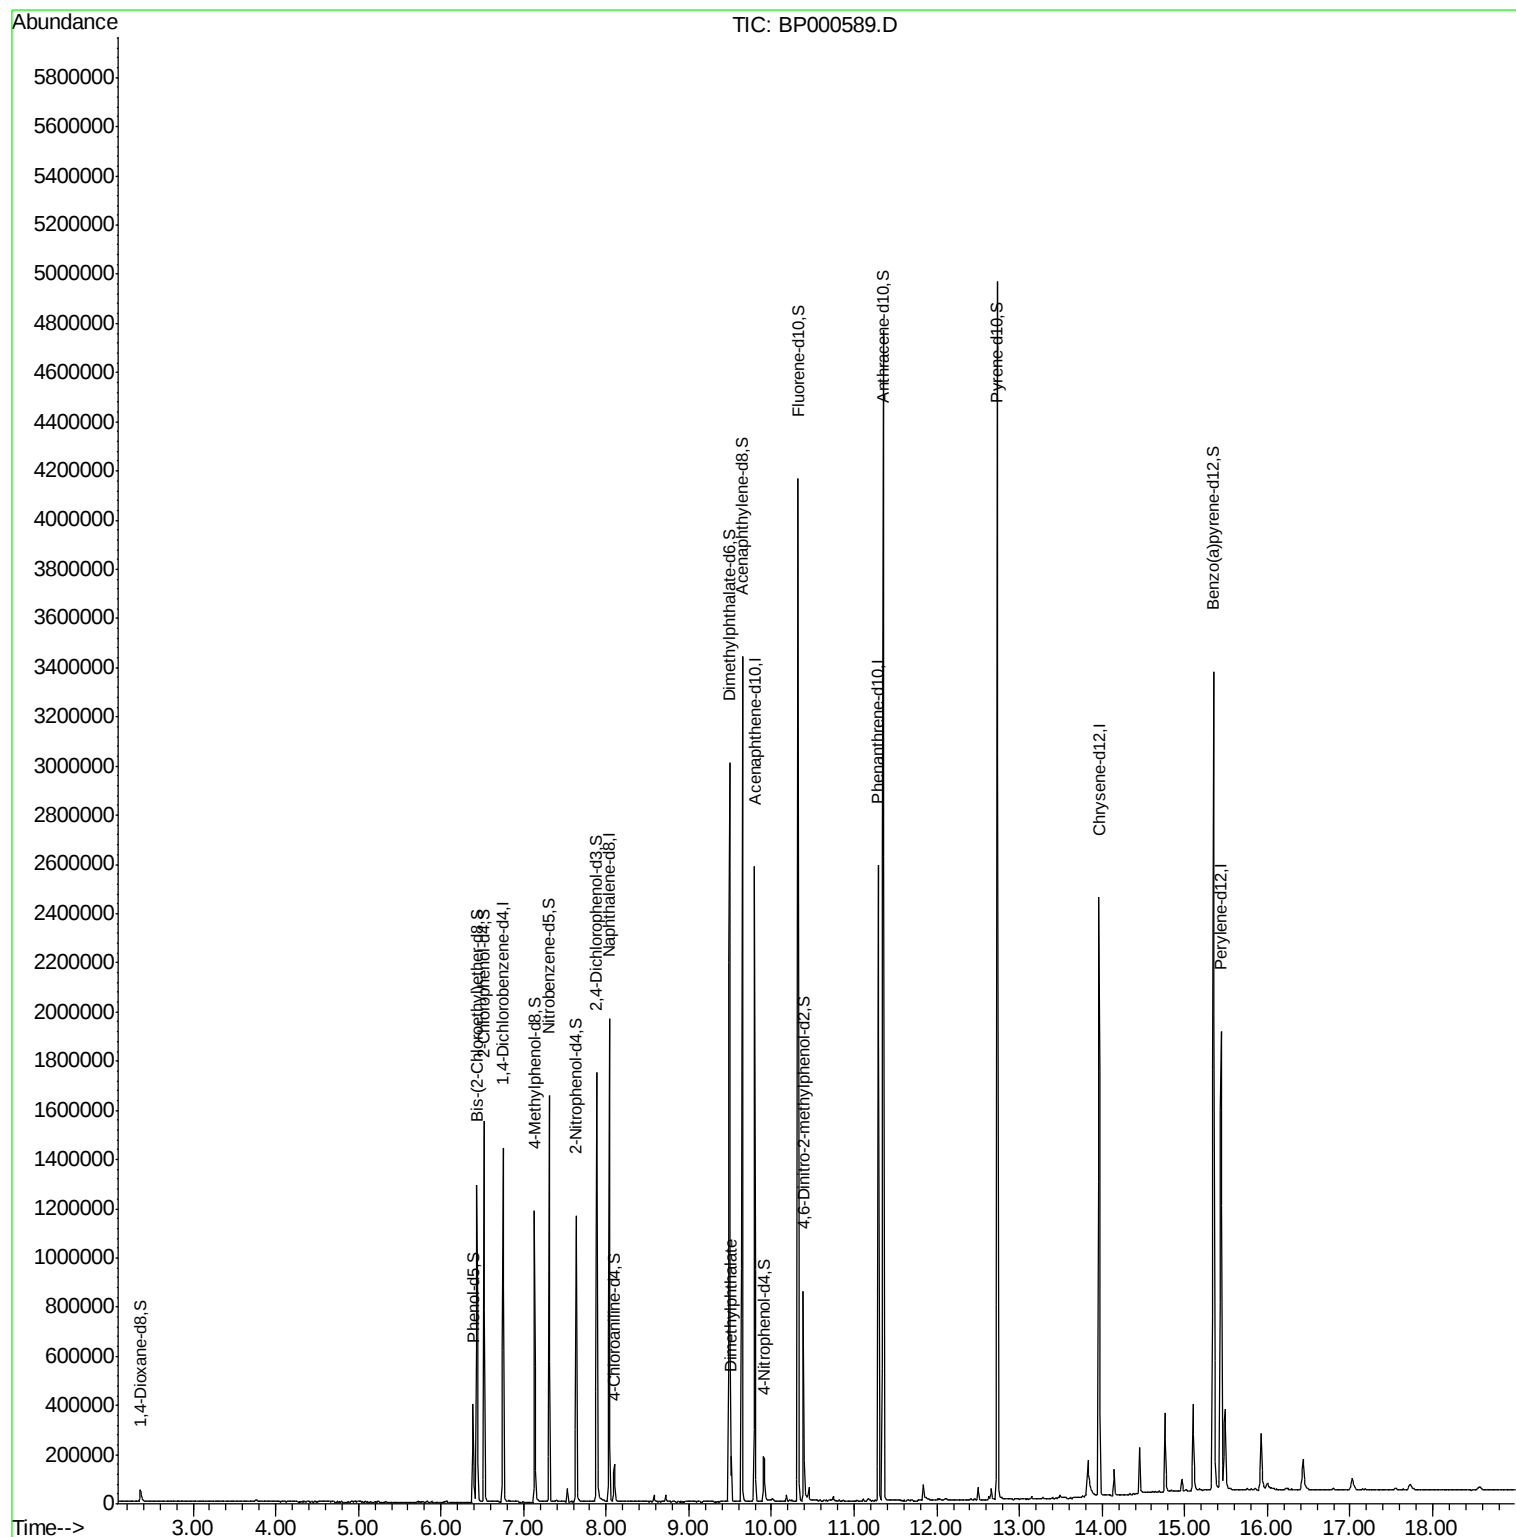

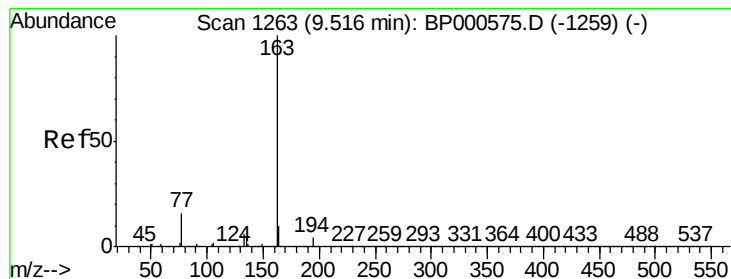

#45

Dimethylphthalate

Concen: 2.725 ng/ul

RT: 9.51 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BP000589.D

Acq: 09 Oct 2019 23:30

Instrument :

BNA_P

ClientSampleId :

ETJY5

Tot Ion:163 Resp: 88489

Ion Ratio Lower Upper

163 100

194 3.9 3.3 4.9

164 10.3 8.1 12.1

