

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
 Data File : BP000602.D
 Acq On : 10 Oct 2019 05:06
 Operator : JU
 Sample : K5097-09
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLME5

Quant Time: Oct 10 05:58:09 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	214492	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	823848	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	477477	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	904903	20.00	ng/ul	0.00
78) Chrysene-d12	13.96	240	804976	20.00	ng/ul	0.00
86) Perylene-d12	15.44	264	898237	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.36	96	18073	3.50	ng/uL	-0.01
5) Phenol-d5	6.39	99	329415	19.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	169503	20.49	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	279190	20.03	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	258797	20.47	ng/ul	0.00
19) Nitrobenzene-d5	7.31	128	127808	20.41	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	136733	20.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	248132	19.44	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	330563	23.29	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	708205	21.19	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	846805	20.59	ng/ul	0.00
52) 4-Nitrophenol-d4	9.90	143	78945	15.33	ng/ul	0.00
58) Fluorene-d10	10.32	176	602314	21.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	52056	12.08	ng/ul	0.00
71) Anthracene-d10	11.35	188	901537	21.51	ng/ul	0.00
79) Pyrene-d10	12.73	212	968277	21.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.35	264	956219	21.56	ng/ul	0.00
Target Compounds						
6) Phenol	6.40	94	55359	3.319	ng/ul	98
45) Dimethylphthalate	9.51	163	233087	6.999	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000602.D
Acq On : 10 Oct 2019 05:06
Operator : JU
Sample : K5097-09
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JLME5

Quant Time: Oct 10 05:58:09 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration

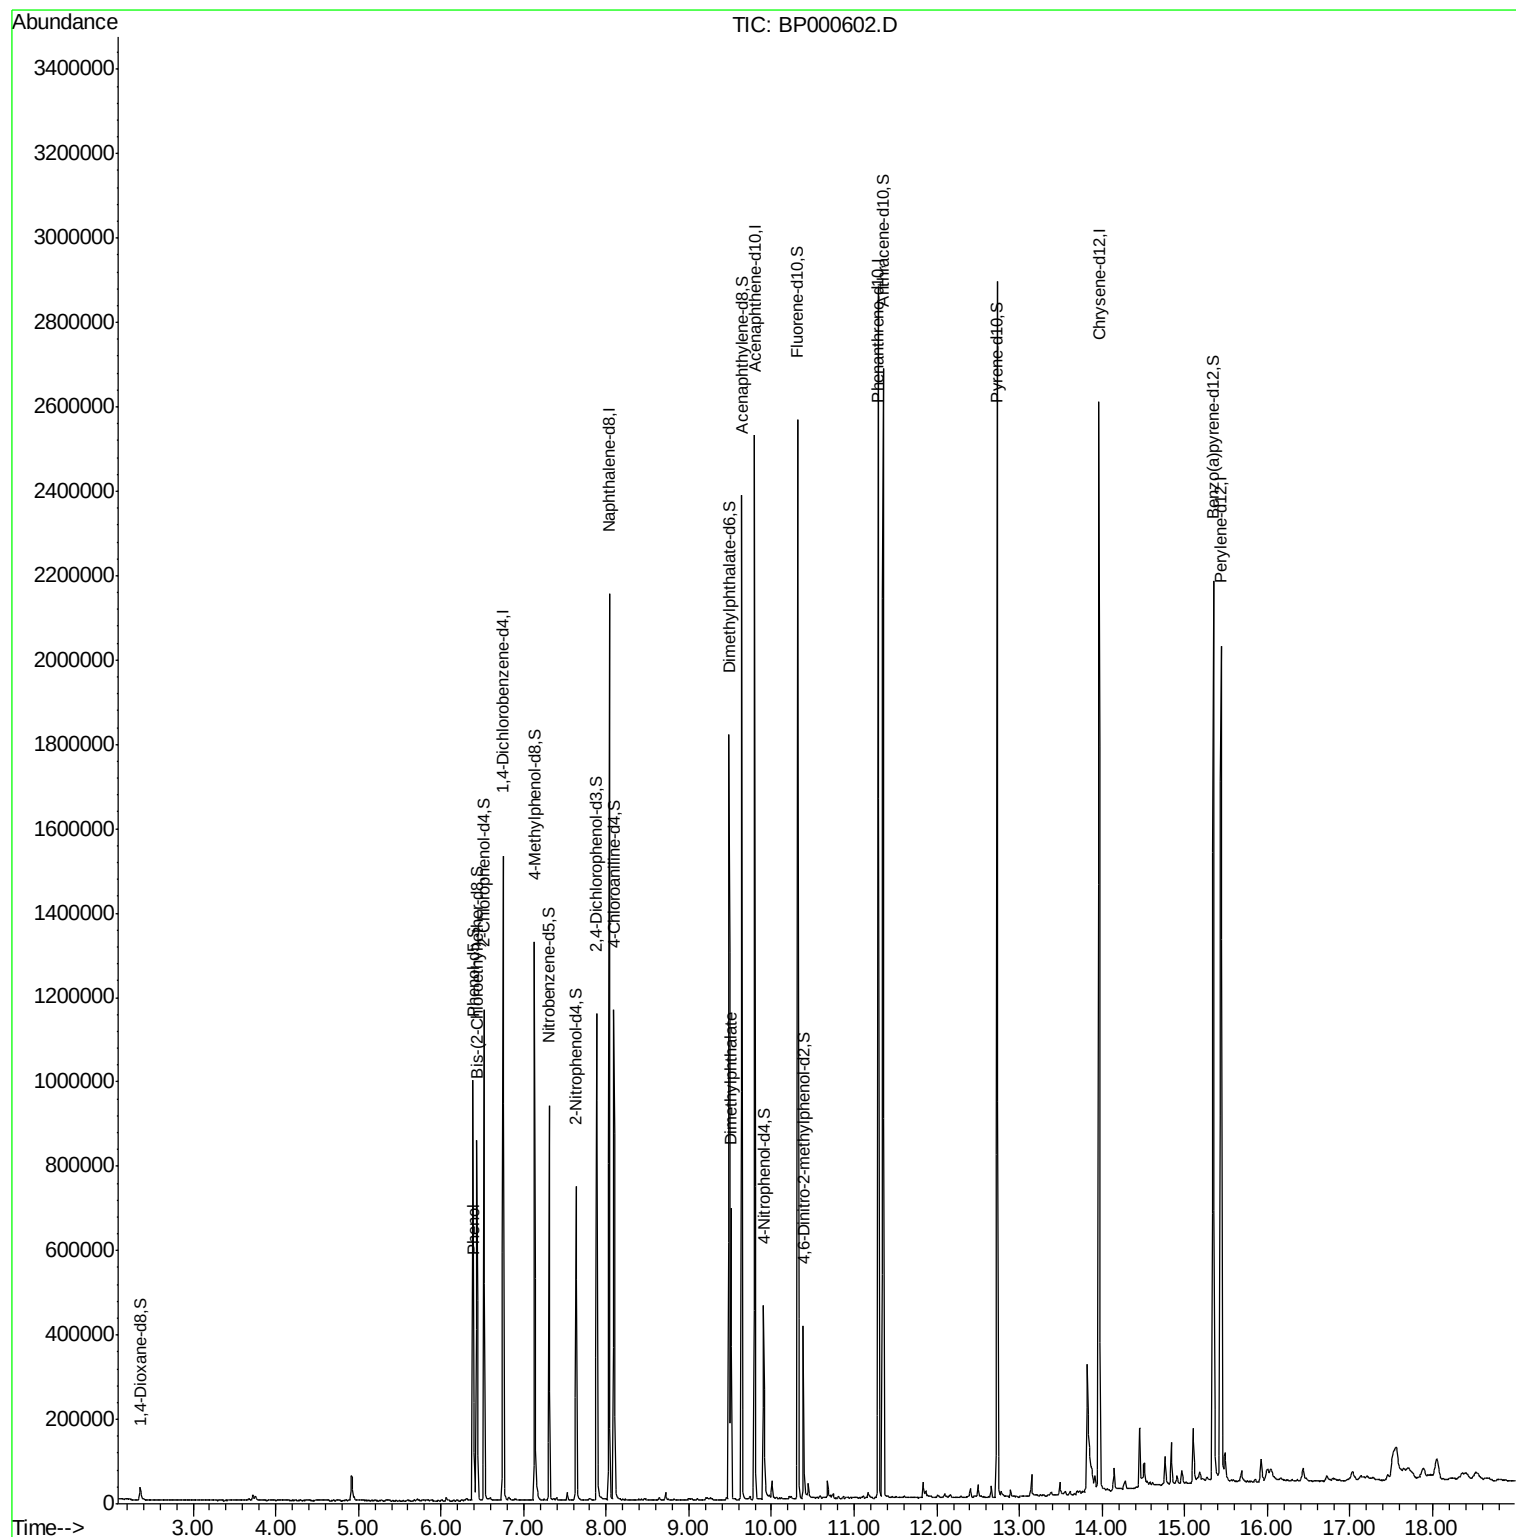

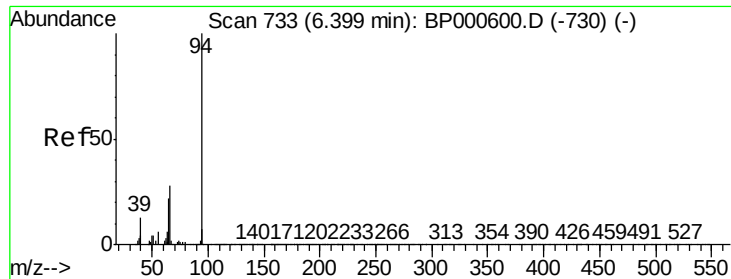

#6

Phenol

Concen: 3.319 ng/ul

RT: 6.40 min Scan# 733

Delta R.T. 0.00 min

Lab File: BP000602.D

Acq: 10 Oct 2019 05:06

Instrument :

BNA_P

ClientSampleId :

JLME5





Tot Ion: 94 Resp: 55359

Ion Ratio Lower Upper

94 100

65 23.8 19.2 28.8

66 33.7 25.7 38.5

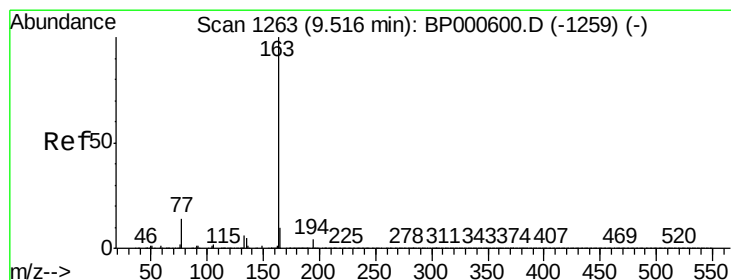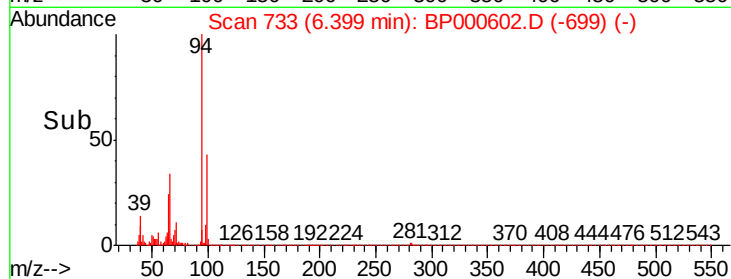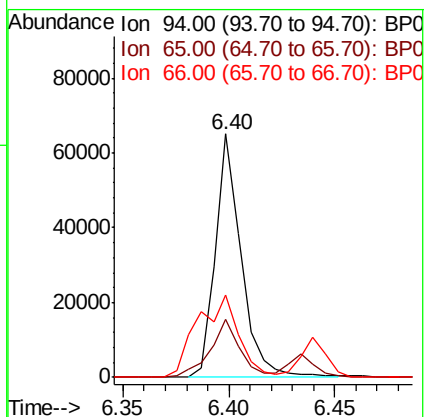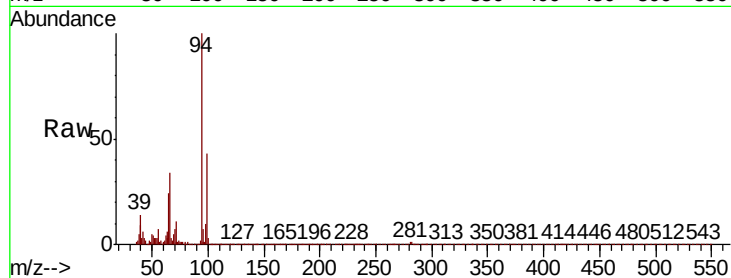

#45

Dimethylphthalate

Concen: 6.999 ng/ul

RT: 9.51 min Scan# 1262

Delta R.T. -0.01 min

Lab File: BP000602.D

Acq: 10 Oct 2019 05:06

Tgt Ion: 163 Resp: 233087

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.4 8.1 12.1

