

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
 Data File : BP000579.D
 Acq On : 09 Oct 2019 19:29
 Operator : JU
 Sample : K5201-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.364	44	47	60	rVB	48003	67587	1.58%	0.156%
2	3.764	281	285	289	rVB	7696	11470	0.27%	0.026%
3	6.387	728	731	736	rBV2	333212	336900	7.89%	0.777%
4	6.434	736	739	750	rVV	1180236	952637	22.32%	2.198%
5	6.522	750	754	765	rVV	1346820	1048541	24.57%	2.420%
6	6.752	790	793	797	rBV	1689899	1286628	30.15%	2.969%
7	6.816	802	804	811	rVB2	4515	5290	0.12%	0.012%
8	7.134	855	858	875	rBV	946971	768745	18.01%	1.774%
9	7.311	884	888	891	rBV	1422379	1113430	26.09%	2.569%
10	7.528	922	925	928	rBV	14021	11084	0.26%	0.026%
11	7.634	940	943	953	rBV	1086104	917417	21.50%	2.117%
12	7.881	982	985	1008	rBV	1526195	1488068	34.87%	3.434%
13	8.034	1008	1011	1015	rVV	2162564	1747125	40.94%	4.032%
14	8.099	1018	1022	1030	rVB	68504	66265	1.55%	0.153%
15	8.316	1054	1059	1062	rBV2	4218	4756	0.11%	0.011%
16	8.387	1068	1071	1076	rBV3	5643	6457	0.15%	0.015%
17	8.722	1125	1128	1135	rBV	27491	26839	0.63%	0.062%
18	9.116	1191	1195	1200	rVB2	12748	12599	0.30%	0.029%
19	9.205	1206	1210	1211	rBV4	3615	4561	0.11%	0.011%
20	9.240	1214	1216	1219	rVB2	7659	6602	0.15%	0.015%
21	9.493	1255	1259	1261	rBV	2886454	2275861	53.33%	5.252%
22	9.510	1261	1262	1266	rVB	380032	256437	6.01%	0.592%
23	9.646	1281	1285	1288	rBV	3303131	2824711	66.19%	6.519%
24	9.799	1307	1311	1314	rBV	2869117	2246473	52.64%	5.184%
25	9.910	1326	1330	1337	rBV	166334	186224	4.36%	0.430%
26	10.010	1344	1347	1351	rVB4	10312	10345	0.24%	0.024%
27	10.216	1379	1382	1384	rBV2	5789	5871	0.14%	0.014%
28	10.240	1384	1386	1389	rVB2	7315	5907	0.14%	0.014%
29	10.322	1396	1400	1403	rBV	4192624	3430758	80.40%	7.917%
30	10.387	1408	1411	1419	rBV	783436	739462	17.33%	1.706%
31	10.446	1419	1421	1429	rVB	48613	53199	1.25%	0.123%
32	10.634	1450	1453	1457	rBV5	5499	6929	0.16%	0.016%
33	10.722	1465	1468	1470	rVV	14359	12211	0.29%	0.028%
34	10.746	1470	1472	1476	rVB	18399	17320	0.41%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
 Data File : BP000579.D
 Acq On : 09 Oct 2019 19:29
 Operator : JU
 Sample : K5201-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	10.987	1510	1513	1516	rBV5	5392	5920	0.14%	0.014%
36	11.110	1532	1534	1537	rVB	8560	8141	0.19%	0.019%
37	11.175	1541	1545	1550	rVV	14876	18264	0.43%	0.042%
38	11.222	1550	1553	1555	rVB	9282	8137	0.19%	0.019%
39	11.293	1562	1565	1569	rBV	2698422	2409087	56.45%	5.559%
40	11.351	1571	1575	1579	rBV	4289436	3601800	84.40%	8.312%
41	11.516	1600	1603	1610	rVB3	6104	9298	0.22%	0.021%
42	11.840	1654	1658	1662	rBV	67637	71833	1.68%	0.166%
43	12.016	1685	1688	1690	rBV3	9873	11236	0.26%	0.026%
44	12.104	1700	1703	1712	rVB3	12882	20750	0.49%	0.048%
45	12.193	1716	1718	1723	rVB	6518	6603	0.15%	0.015%
46	12.410	1752	1755	1759	rVB	9485	9371	0.22%	0.022%
47	12.451	1759	1762	1765	rBV5	5147	5687	0.13%	0.013%
48	12.498	1767	1770	1779	rVB	46060	45848	1.07%	0.106%
49	12.634	1790	1793	1794	rBV2	14399	12951	0.30%	0.030%
50	12.657	1794	1797	1803	rVV	43377	43280	1.01%	0.100%
51	12.734	1806	1810	1814	rVV	4721020	4267316	100.00%	9.848%
52	12.787	1816	1819	1821	rVV	23277	29097	0.68%	0.067%
53	12.804	1821	1822	1830	rVB3	23970	21651	0.51%	0.050%
54	13.145	1877	1880	1888	rBV	37961	41922	0.98%	0.097%
55	13.287	1901	1904	1908	rVB2	5229	6259	0.15%	0.014%
56	13.375	1917	1919	1920	rBV2	6244	4518	0.11%	0.010%
57	13.469	1933	1935	1936	rBV	5908	4564	0.11%	0.011%
58	13.493	1936	1939	1941	rVV	53114	39948	0.94%	0.092%
59	13.769	1983	1986	1988	rVB	14776	15113	0.35%	0.035%
60	13.804	1989	1992	1993	rBV	24161	22408	0.53%	0.052%
61	13.834	1993	1997	2015	rVB2	247909	478483	11.21%	1.104%
62	13.969	2015	2020	2023	rBV	2692974	2473835	57.97%	5.709%
63	14.145	2047	2050	2054	rBV	106043	96325	2.26%	0.222%
64	14.457	2099	2103	2107	rBV	142313	127971	3.00%	0.295%
65	14.769	2152	2156	2162	rBV	149985	155494	3.64%	0.359%
66	14.969	2186	2190	2194	rBV	48943	55302	1.30%	0.128%
67	15.104	2209	2213	2222	rBV	155500	192168	4.50%	0.443%
68	15.351	2249	2255	2265	rBV	3442271	4072874	95.44%	9.399%
69	15.439	2265	2270	2275	rVV	1993455	2503814	58.67%	5.778%
70	15.487	2275	2278	2286	rVB	143644	191522	4.49%	0.442%
71	15.928	2349	2353	2361	rBV	103975	154149	3.61%	0.356%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000579.D
Acq On : 09 Oct 2019 19:29
Operator : JU
Sample : K5201-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

72	16.004	2363	2366	2371	rBV4	20168	31217	0.73%	0.072%
73	16.434	2435	2439	2446	rVB	61668	104104	2.44%	0.240%


Sum of corrected areas: 43332969

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000579.D
Acq On : 09 Oct 2019 19:29
Operator : JU
Sample : K5201-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

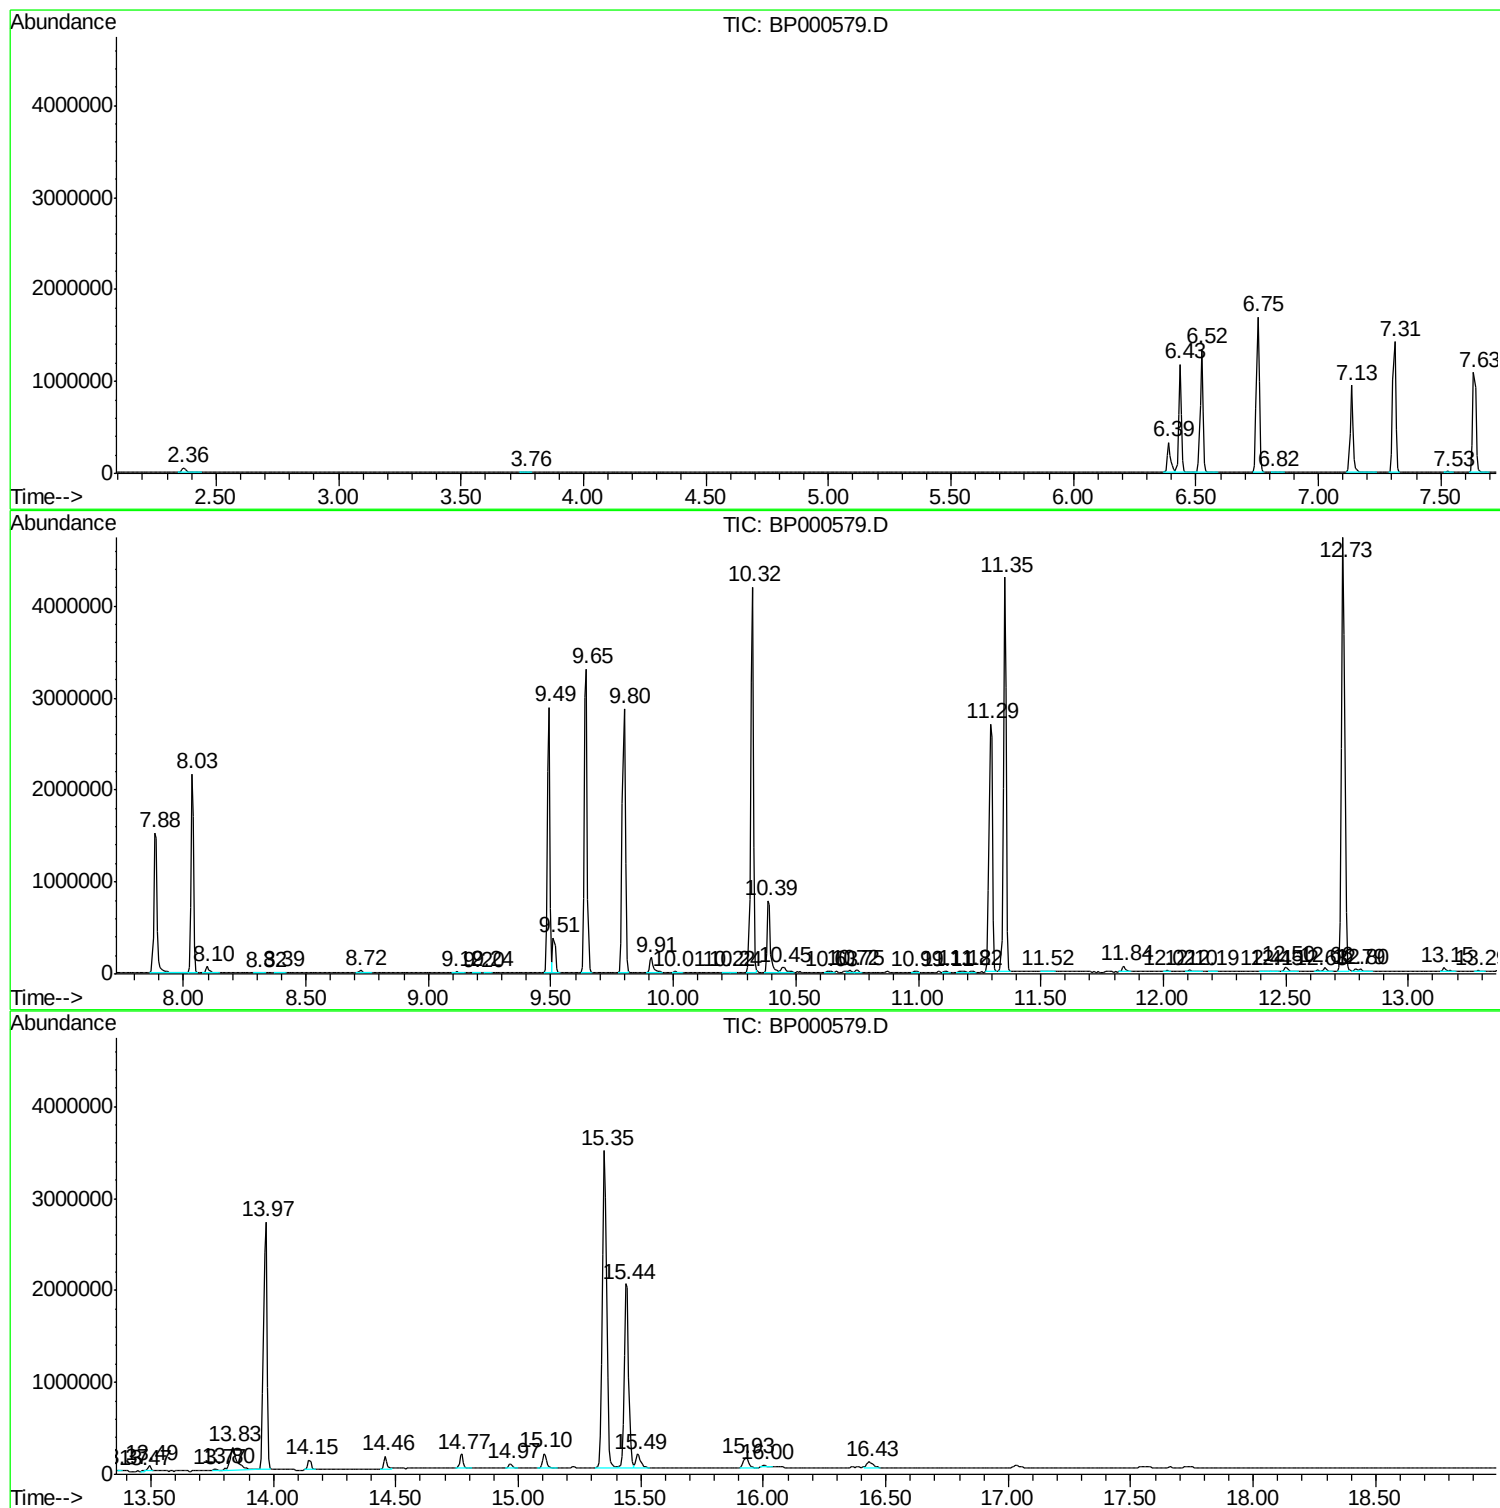

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000579.D
Acq On : 09 Oct 2019 19:29
Operator : JU
Sample : K5201-05
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic13.83 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
13.83	3.87 ng/ul	478483	Chrysene-d12		13.97	
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	9-Eicosene, (E)-		280	C20H40	074685-29-3	55
2	1-Hexadecanesulfonyl chloride		324	C16H33ClO2S	038775-38-1	43
3	Ethanol, 2-(tetradecyloxy)-		258	C16H34O2	002136-70-1	42
4	Diethylene glycol dibenzoate		314	C18H18O5	000120-55-8	38
5	1-Nonadecene		266	C19H38	018435-45-5	38

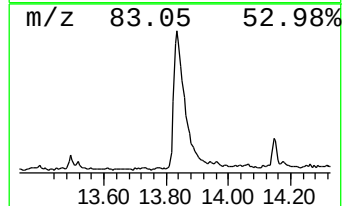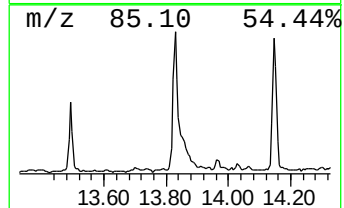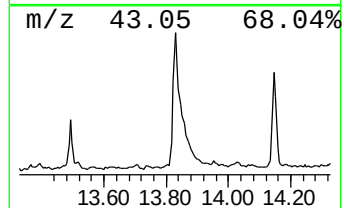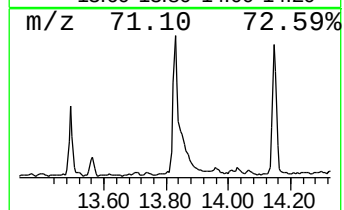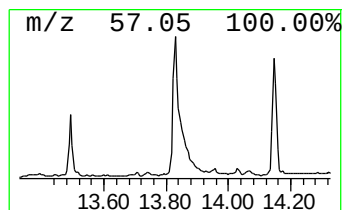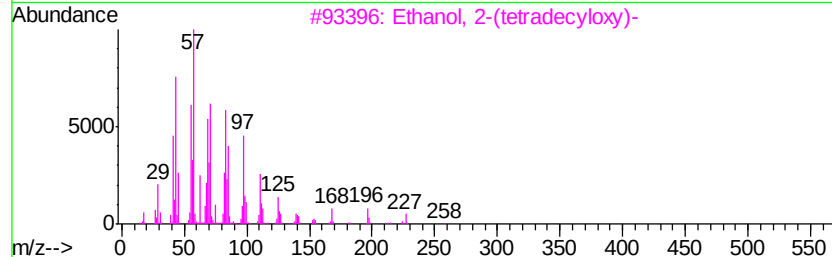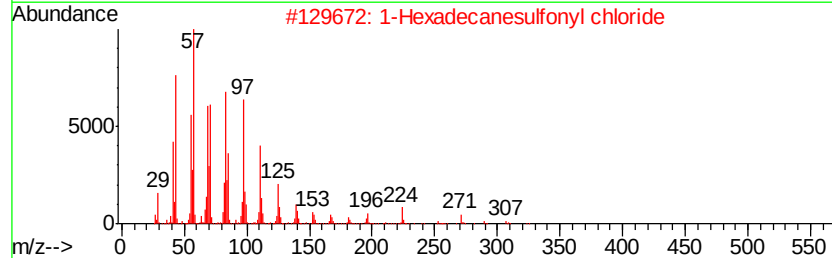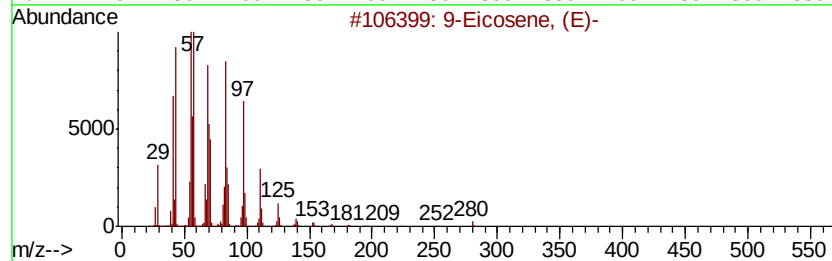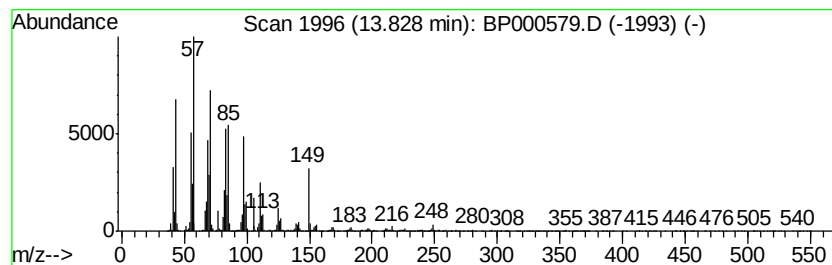

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
Data File : BP000579.D
Acq On : 09 Oct 2019 19:29
Operator : JU
Sample : K5201-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB9

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Cyc...	13.83	3.9	ng/ul	478483	5	13.97	2473840	20.0