

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
 Data File : BP000580.D
 Acq On : 09 Oct 2019 19:54
 Operator : JU
 Sample : K5201-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.358	43	46	56	rBV	44335	64135	1.49%	0.151%
2	3.728	275	279	281	rBV	3626	4978	0.12%	0.012%
3	3.758	281	284	289	rVB	8256	12010	0.28%	0.028%
4	4.299	373	376	382	rBV	5409	7171	0.17%	0.017%
5	4.616	426	430	439	rVB	3001	6215	0.14%	0.015%
6	6.387	728	731	736	rBV2	329695	327672	7.63%	0.770%
7	6.434	736	739	751	rVB	1149425	913689	21.26%	2.147%
8	6.522	751	754	758	rBV	1314558	1014187	23.60%	2.384%
9	6.752	790	793	797	rBV	1566748	1246485	29.01%	2.929%
10	6.822	802	805	810	rVB	5542	6621	0.15%	0.016%
11	7.134	855	858	874	rBV	927864	746722	17.38%	1.755%
12	7.310	884	888	891	rBV	1440925	1077779	25.08%	2.533%
13	7.528	922	925	929	rVB	15922	13308	0.31%	0.031%
14	7.634	940	943	954	rBV	1008462	887867	20.66%	2.087%
15	7.881	982	985	1008	rBV	1443728	1447690	33.69%	3.402%
16	8.034	1008	1011	1015	rVV	2051573	1701480	39.59%	3.999%
17	8.098	1019	1022	1032	rVB	67255	64344	1.50%	0.151%
18	8.316	1055	1059	1063	rBV	5373	5544	0.13%	0.013%
19	8.387	1068	1071	1077	rBV	10385	11879	0.28%	0.028%
20	8.722	1124	1128	1135	rBV	25925	26185	0.61%	0.062%
21	9.116	1190	1195	1199	rVB2	5421	6480	0.15%	0.015%
22	9.204	1204	1210	1211	rBV4	3465	5212	0.12%	0.012%
23	9.269	1219	1221	1228	rVB5	4076	6833	0.16%	0.016%
24	9.493	1255	1259	1261	rBV	2888697	2225147	51.78%	5.229%
25	9.510	1261	1262	1267	rVB	240453	163981	3.82%	0.385%
26	9.645	1281	1285	1288	rBV	3113614	2710771	63.08%	6.371%
27	9.798	1307	1311	1314	rBV	2838147	2209840	51.42%	5.194%
28	9.910	1326	1330	1339	rBV	170995	192910	4.49%	0.453%
29	10.010	1344	1347	1352	rVB4	9123	9582	0.22%	0.023%
30	10.240	1384	1386	1389	rVB2	5833	5117	0.12%	0.012%
31	10.322	1396	1400	1403	rBV	4010748	3328711	77.46%	7.823%
32	10.387	1408	1411	1419	rBV	811796	754490	17.56%	1.773%
33	10.445	1419	1421	1430	rVB	48629	52360	1.22%	0.123%
34	10.634	1450	1453	1456	rBV4	4652	5453	0.13%	0.013%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
 Data File : BP000580.D
 Acq On : 09 Oct 2019 19:54
 Operator : JU
 Sample : K5201-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AC0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

35	10.722	1465	1468	1470	rBV	12121	10351	0.24%	0.024%
36	10.745	1470	1472	1476	rVB2	19153	17086	0.40%	0.040%
37	10.987	1510	1513	1516	rBV5	5665	5859	0.14%	0.014%
38	11.110	1532	1534	1538	rVB	9763	7594	0.18%	0.018%
39	11.169	1541	1544	1550	rVV	12861	16664	0.39%	0.039%
40	11.222	1550	1553	1556	rVB	12496	10417	0.24%	0.024%
41	11.292	1562	1565	1569	rBV	2704911	2414513	56.19%	5.675%
42	11.351	1571	1575	1579	rBV	4284417	3518778	81.88%	8.270%
43	11.439	1587	1590	1594	rVB	6438	5443	0.13%	0.013%
44	11.522	1600	1604	1606	rBV2	7594	10593	0.25%	0.025%
45	11.834	1654	1657	1665	rBV4	40423	53672	1.25%	0.126%
46	12.016	1684	1688	1692	rBV5	14399	24325	0.57%	0.057%
47	12.104	1700	1703	1714	rVB4	13415	23105	0.54%	0.054%
48	12.198	1716	1719	1723	rVB	5897	5955	0.14%	0.014%
49	12.410	1752	1755	1759	rVB	13310	11802	0.27%	0.028%
50	12.451	1759	1762	1765	rBV5	6154	6767	0.16%	0.016%
51	12.498	1767	1770	1775	rVB	45520	44843	1.04%	0.105%
52	12.634	1790	1793	1794	rBV2	7064	6831	0.16%	0.016%
53	12.657	1794	1797	1803	rVV	44212	40548	0.94%	0.095%
54	12.734	1806	1810	1814	rVV	4809955	4297278	100.00%	10.099%
55	12.786	1816	1819	1821	rVV2	32805	37420	0.87%	0.088%
56	12.804	1821	1822	1831	rVB2	30607	26115	0.61%	0.061%
57	13.145	1877	1880	1889	rBV	48510	47584	1.11%	0.112%
58	13.286	1901	1904	1908	rBV5	5528	7118	0.17%	0.017%
59	13.492	1936	1939	1942	rBV	77124	63365	1.47%	0.149%
60	13.763	1983	1985	1989	rVB	7150	7608	0.18%	0.018%
61	13.804	1989	1992	1993	rBV	14085	13939	0.32%	0.033%
62	13.828	1993	1996	2012	rVB2	199915	363407	8.46%	0.854%
63	13.969	2015	2020	2023	rBV	2536524	2454931	57.13%	5.770%
64	14.145	2047	2050	2058	rBV	136617	127135	2.96%	0.299%
65	14.457	2099	2103	2107	rBV	157676	146614	3.41%	0.345%
66	14.763	2152	2155	2161	rBV	149922	155054	3.61%	0.364%
67	14.969	2186	2190	2195	rBV	47040	55905	1.30%	0.131%
68	15.104	2209	2213	2221	rBV	139391	173664	4.04%	0.408%
69	15.351	2249	2255	2264	rBV	3467264	4132545	96.17%	9.712%
70	15.439	2265	2270	2275	rVV	2104482	2535390	59.00%	5.959%
71	15.486	2275	2278	2287	rVB	122817	165530	3.85%	0.389%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000580.D
Acq On : 09 Oct 2019 19:54
Operator : JU
Sample : K5201-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

72	15.927	2348	2353	2361	rBV	82082	129842	3.02%	0.305%
73	16.433	2435	2439	2452	rVB3	52987	111491	2.59%	0.262%


Sum of corrected areas: 42549929

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000580.D
Acq On : 09 Oct 2019 19:54
Operator : JU
Sample : K5201-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

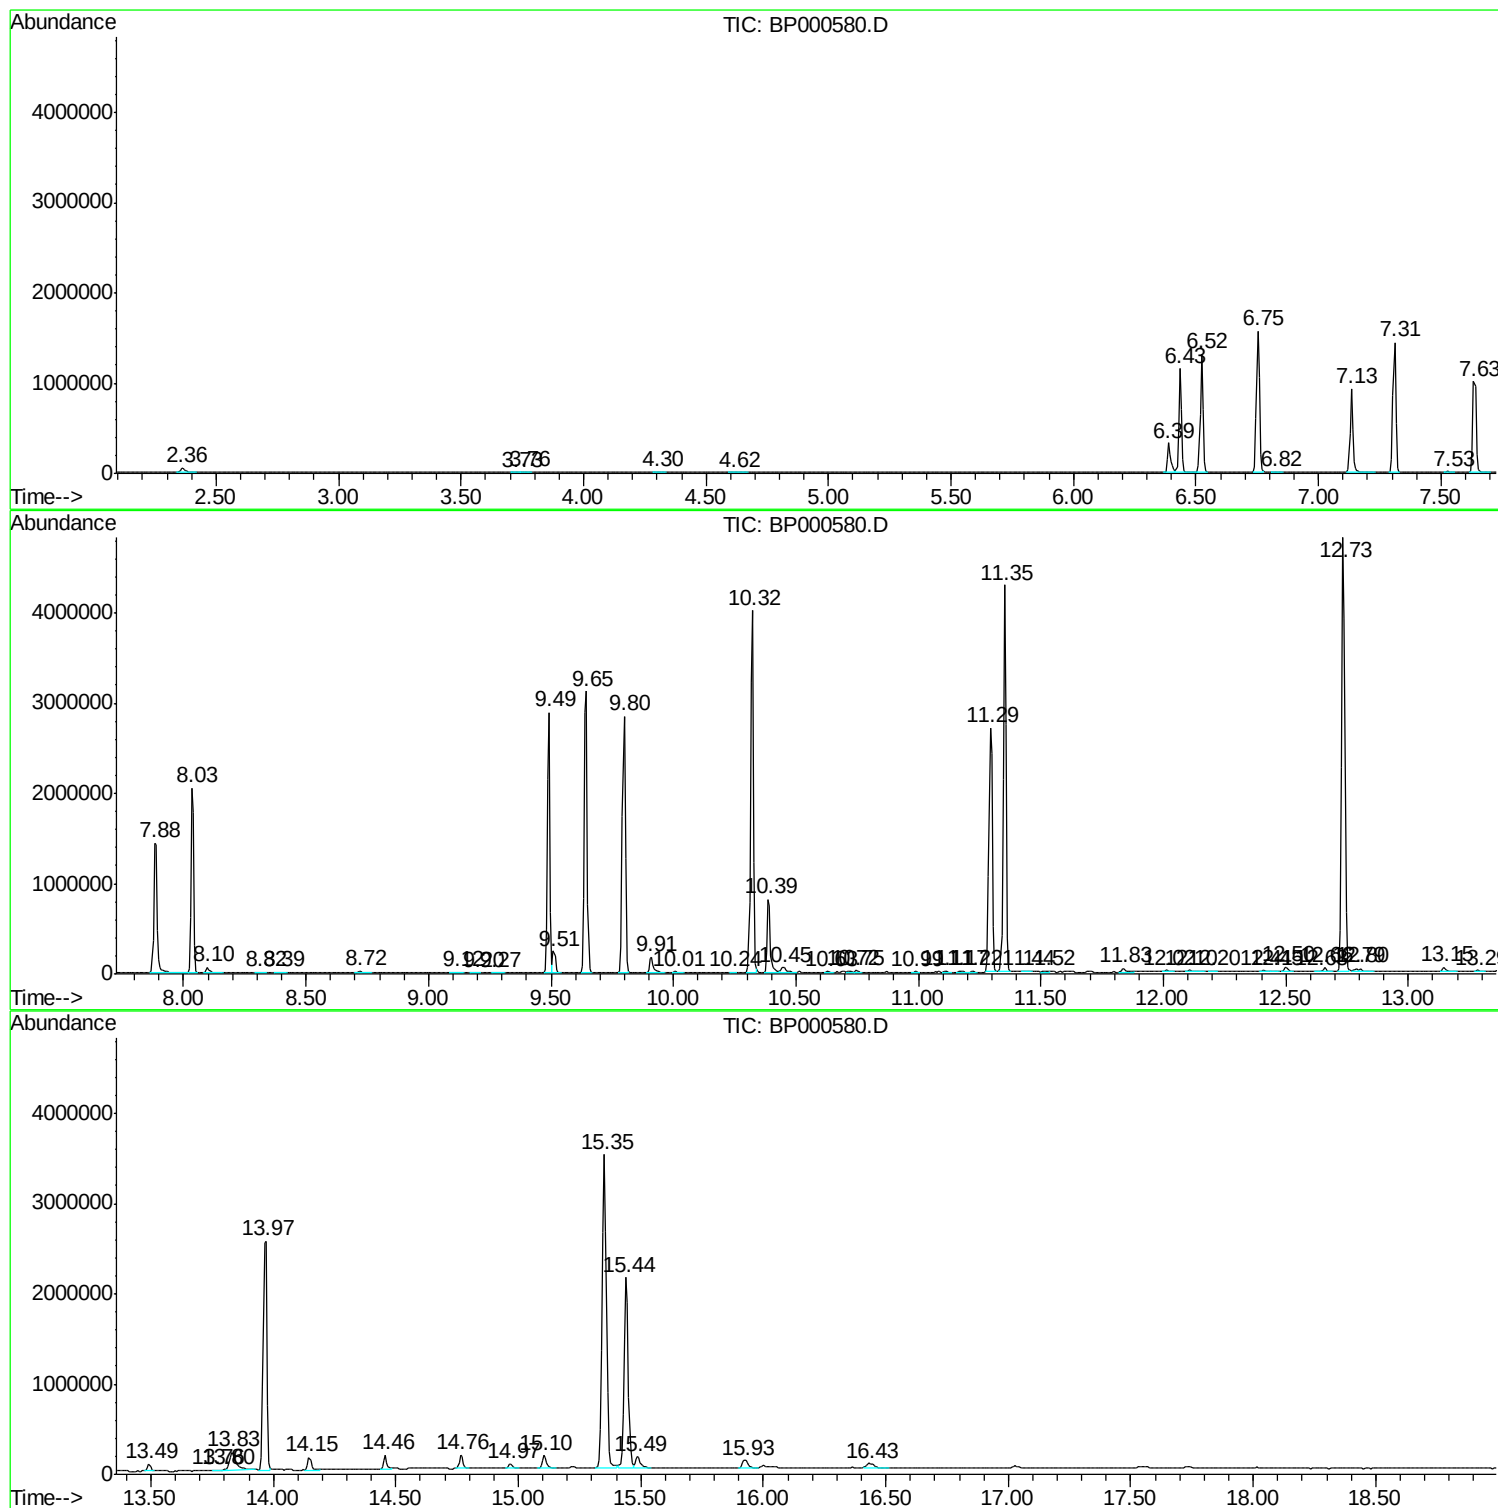

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000580.D
Acq On : 09 Oct 2019 19:54
Operator : JU
Sample : K5201-06
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
C0AC0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.		
13.83	2.96 ng/ul	363407	Chrysene-d12	13.97		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexadecane		226	C16H34	000544-76-3	87
2	Ethanol, 2-(hexadecyloxy)-		286	C18H38O2	002136-71-2	87
3	2- Chloropropionic acid, hexadec...		332	C19H37ClO2	086711-81-1	60
4	Silane, trichlorooctadecyl-		386	C18H37Cl3Si	000112-04-9	60
5	Tetradecane, 2-methyl-		212	C15H32	001560-95-8	53

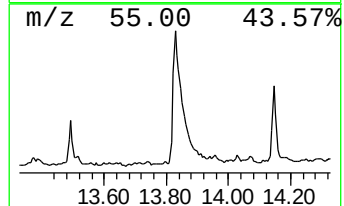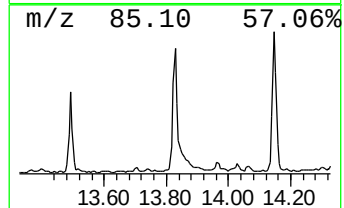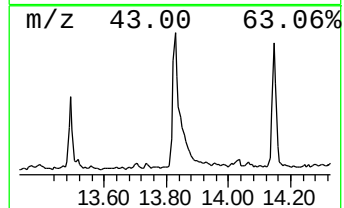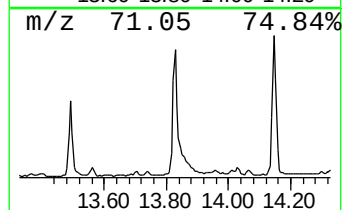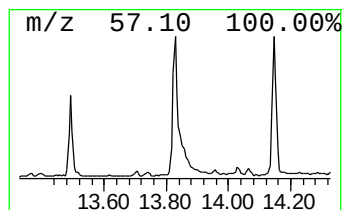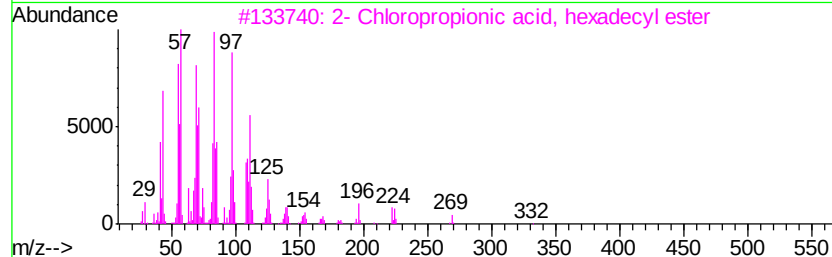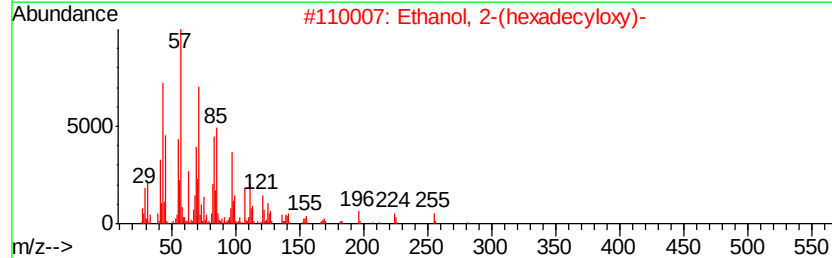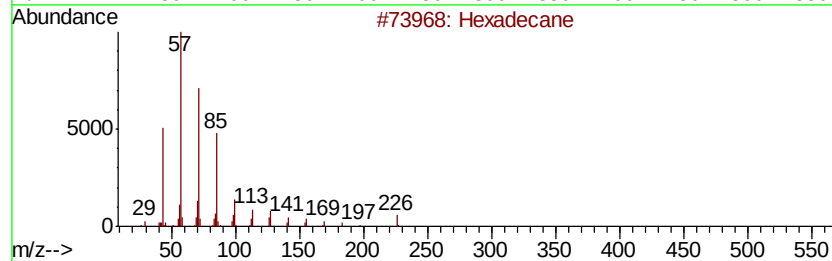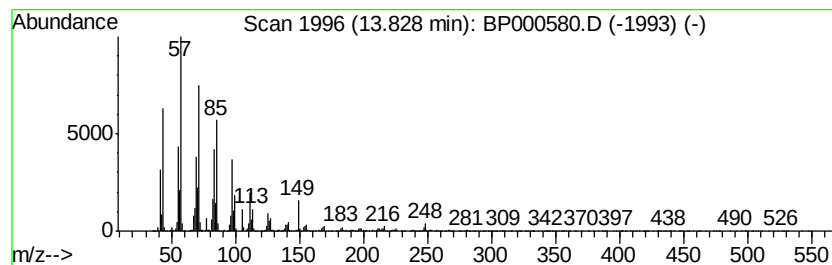

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
Data File : BP000580.D
Acq On : 09 Oct 2019 19:54
Operator : JU
Sample : K5201-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AC0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	13.83	3.0	ng/ul	363407	5	13.97	2454930	20.0