

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
 Data File : BP000586.D
 Acq On : 09 Oct 2019 22:18
 Operator : JU
 Sample : K5100-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 ETJY2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.299	31	36	41	rVB	12971	18173	0.42%	0.042%
2	2.364	44	47	59	rVB	52138	73899	1.70%	0.169%
3	3.764	281	285	290	rVB	9258	13794	0.32%	0.032%
4	6.387	728	731	736	rBV	371463	355860	8.18%	0.814%
5	6.434	736	739	749	rVB	1206911	966143	22.21%	2.211%
6	6.522	750	754	758	rBV	1389547	1076806	24.76%	2.464%
7	6.752	790	793	802	rBV	1669633	1300518	29.90%	2.976%
8	6.822	802	805	810	rVB	5646	6538	0.15%	0.015%
9	7.134	855	858	872	rBV	1058778	848529	19.51%	1.942%
10	7.310	884	888	891	rBV	1440996	1114353	25.62%	2.550%
11	7.528	921	925	930	rBV	32283	26796	0.62%	0.061%
12	7.634	940	943	959	rBV	1082848	927250	21.32%	2.122%
13	7.881	982	985	1008	rBV	1561825	1492889	34.32%	3.417%
14	8.034	1008	1011	1015	rVV	2274208	1776253	40.84%	4.065%
15	8.099	1018	1022	1031	rVB	133655	129608	2.98%	0.297%
16	8.581	1099	1104	1108	rBV	11594	11055	0.25%	0.025%
17	8.722	1124	1128	1139	rVB	25310	27670	0.64%	0.063%
18	9.493	1255	1259	1261	rBV	2550324	2167730	49.84%	4.961%
19	9.510	1261	1262	1267	rVB	238605	156901	3.61%	0.359%
20	9.640	1281	1284	1288	rBV	3274669	2791297	64.18%	6.388%
21	9.799	1307	1311	1314	rBV	2892520	2256096	51.87%	5.163%
22	9.904	1326	1329	1339	rBV	189383	206937	4.76%	0.474%
23	10.004	1344	1346	1353	rVB6	7022	9593	0.22%	0.022%
24	10.216	1378	1382	1384	rBV2	6600	7130	0.16%	0.016%
25	10.322	1396	1400	1403	rBV	3833598	3355040	77.14%	7.678%
26	10.387	1408	1411	1419	rBV	881008	762239	17.53%	1.744%
27	10.446	1419	1421	1430	rVB	52985	54402	1.25%	0.125%
28	10.628	1449	1452	1457	rBV7	3052	5165	0.12%	0.012%
29	10.716	1461	1467	1469	rVV5	3530	6188	0.14%	0.014%
30	10.746	1469	1472	1477	rVB2	16573	15562	0.36%	0.036%
31	11.110	1531	1534	1538	rVB2	8639	7944	0.18%	0.018%
32	11.169	1540	1544	1551	rBV	11746	14720	0.34%	0.034%
33	11.293	1561	1565	1569	rBV	2954583	2470826	56.81%	5.655%
34	11.351	1571	1575	1578	rBV	4666316	3782082	86.96%	8.656%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000586.D
Acq On : 09 Oct 2019 22:18
Operator : JU
Sample : K5100-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETJY2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Title : SVOA CALIBRATION

35	11.834	1654	1657	1661	rBV2	35227	36520	0.84%	0.084%
36	11.863	1661	1662	1672	rVB	8454	11539	0.27%	0.026%
37	12.010	1683	1687	1692	rBV7	4223	9149	0.21%	0.021%
38	12.498	1767	1770	1777	rVB	47462	41883	0.96%	0.096%
39	12.657	1794	1797	1804	rVB	44309	38418	0.88%	0.088%
40	12.734	1806	1810	1814	rBV	5035387	4349304	100.00%	9.954%
41	12.898	1835	1838	1840	rBV	5326	4958	0.11%	0.011%
42	13.145	1875	1880	1889	rBV8	9540	21268	0.49%	0.049%
43	13.287	1901	1904	1909	rVB2	7186	7098	0.16%	0.016%
44	13.492	1936	1939	1942	rBV3	8986	7921	0.18%	0.018%
45	13.545	1945	1948	1955	rBV3	4819	8763	0.20%	0.020%
46	13.763	1982	1985	1988	rBV	7542	9435	0.22%	0.022%
47	13.828	1989	1996	2011	rBV3	191864	439168	10.10%	1.005%
48	13.963	2015	2019	2023	rBV	2833327	2502914	57.55%	5.728%
49	14.145	2047	2050	2058	rBV	53547	53870	1.24%	0.123%
50	14.457	2099	2103	2117	rBV	96044	123875	2.85%	0.284%
51	14.763	2152	2155	2162	rBV	154722	146783	3.37%	0.336%
52	14.963	2186	2189	2194	rBV	45036	50737	1.17%	0.116%
53	15.104	2209	2213	2218	rBV	166735	198330	4.56%	0.454%
54	15.351	2249	2255	2264	rBV	3532261	4151946	95.46%	9.502%
55	15.439	2264	2270	2275	rVV	2194369	2564076	58.95%	5.868%
56	15.486	2275	2278	2289	rVB	170069	225040	5.17%	0.515%
57	15.922	2348	2352	2359	rBV	114860	185564	4.27%	0.425%
58	15.998	2362	2365	2372	rVV6	22009	36437	0.84%	0.083%
59	16.433	2434	2439	2452	rVB2	79572	152695	3.51%	0.349%
60	17.028	2536	2540	2552	rVB2	38127	80457	1.85%	0.184%


Sum of corrected areas: 43694134

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000586.D
Acq On : 09 Oct 2019 22:18
Operator : JU
Sample : K5100-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETJY2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

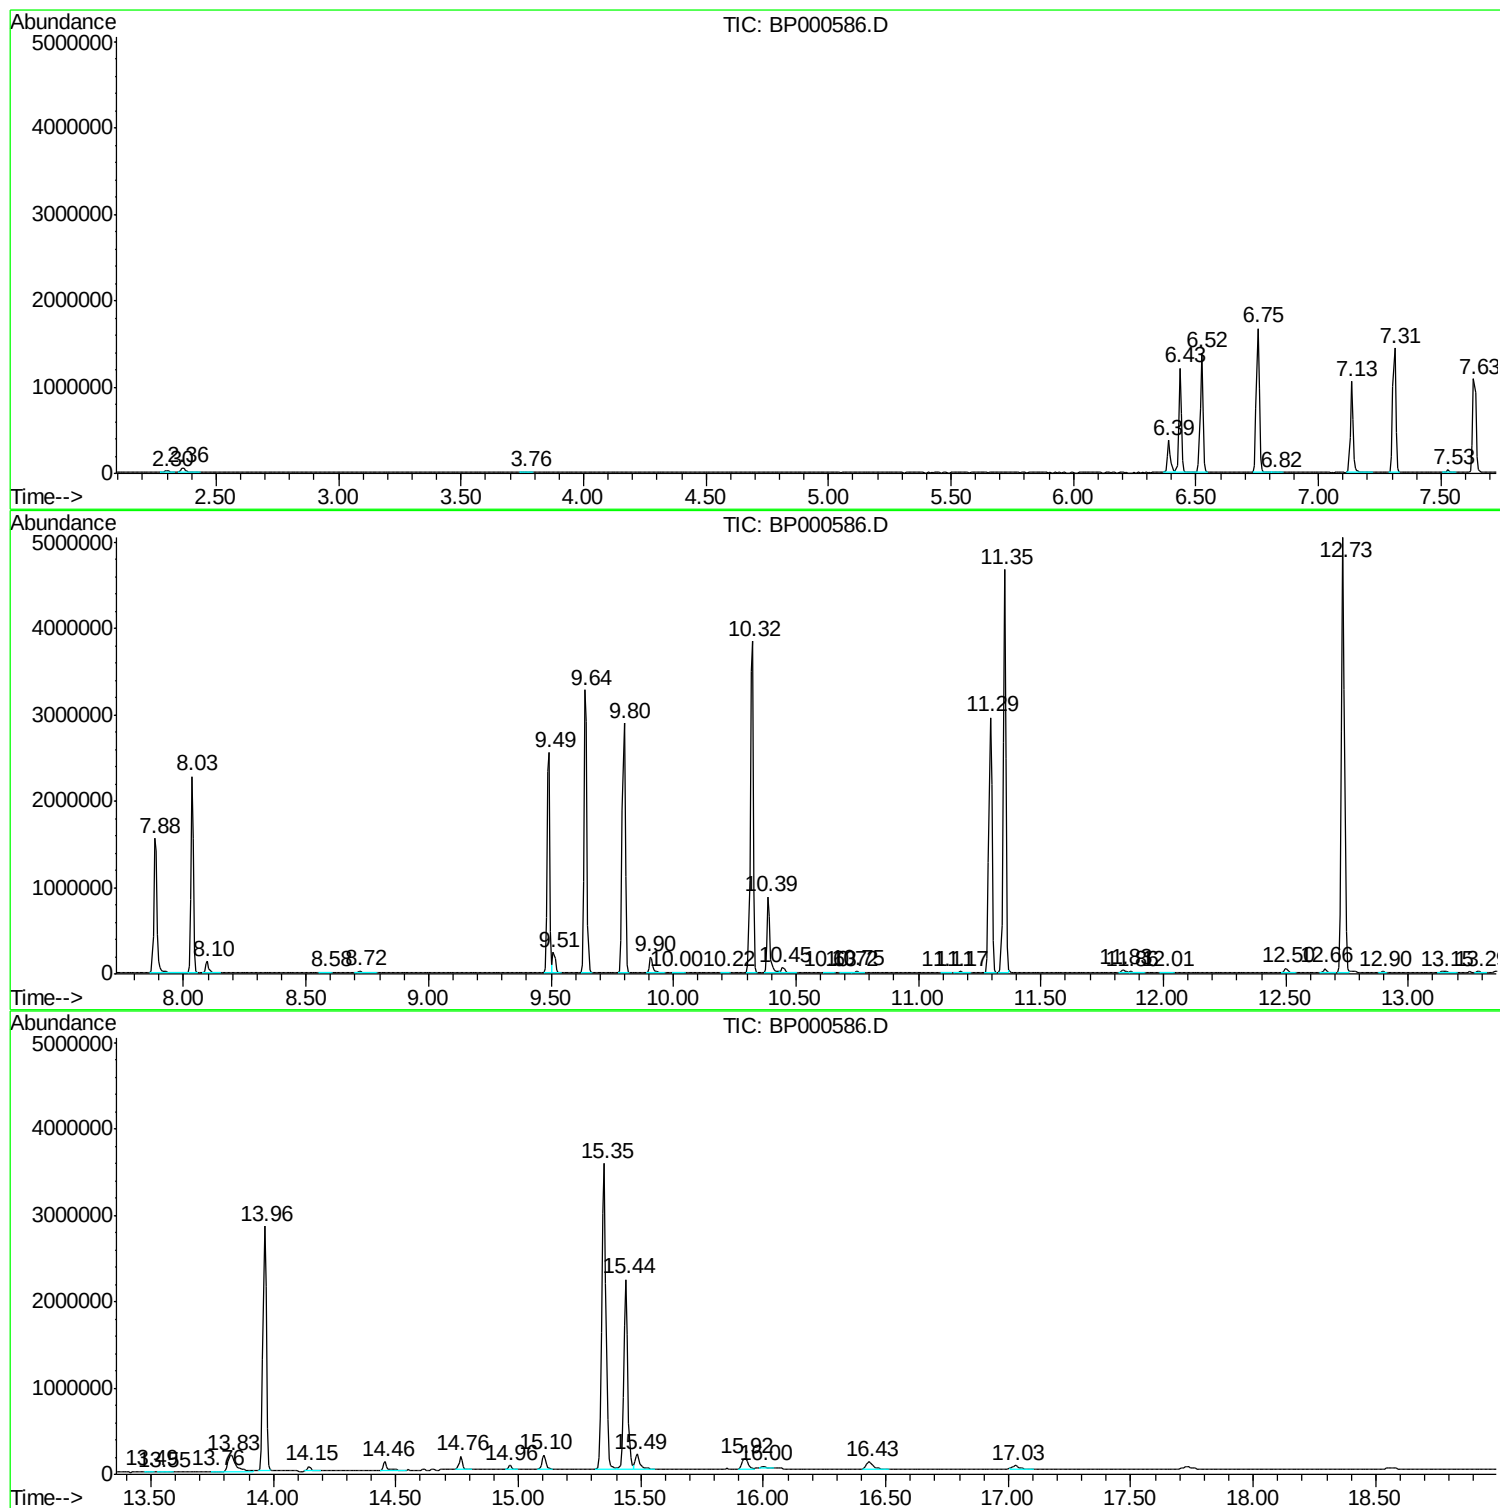

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP100919\
Data File : BP000586.D
Acq On : 09 Oct 2019 22:18
Operator : JU
Sample : K5100-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETJY2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2- Chloropropionic acid, oc... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.83	3.51 ng/ul	439168	Chrysene-d12	13.96

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-	Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	97
2	1-Heneicosyl	formate	340	C22H44O2	077899-03-7	95
3	Cyclohexadecane		224	C16H32	000295-65-8	94
4	Cyclopentadecane		210	C15H30	000295-48-7	93
5	Trifluoroacetic acid, n-octadecy...		366	C20H37F3O2	079392-43-1	91

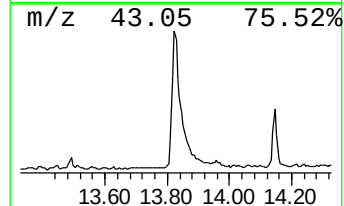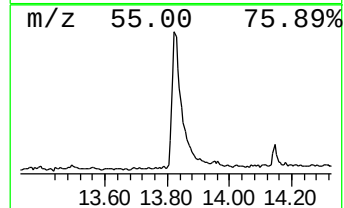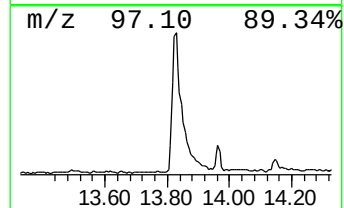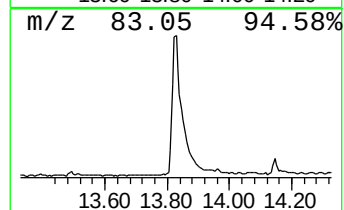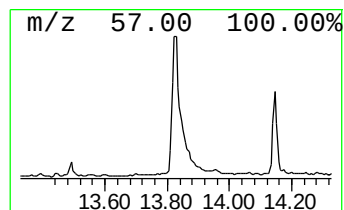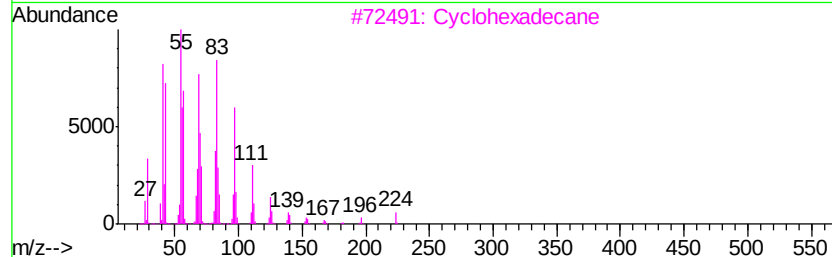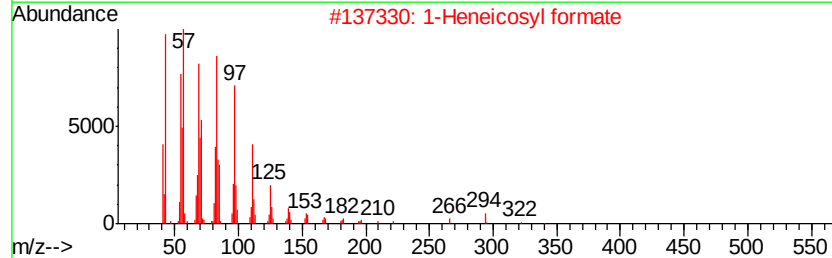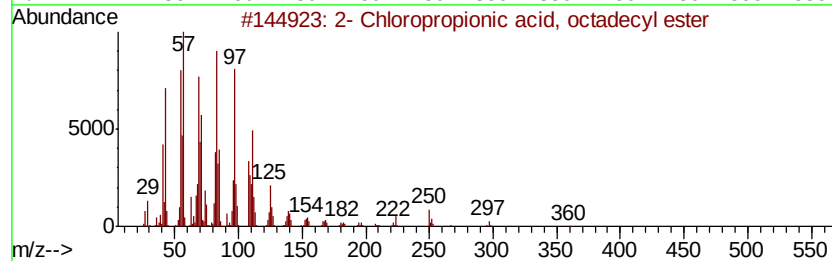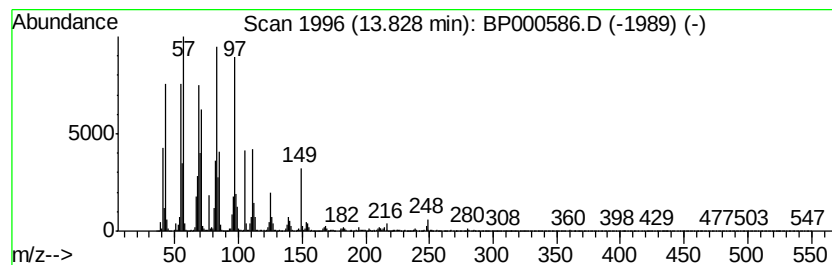

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP100919\
Data File : BP000586.D
Acq On : 09 Oct 2019 22:18
Operator : JU
Sample : K5100-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
ETJY2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2- Chloropropioni...	13.83	3.5	ng/ul	439168	5	13.96	2502910	20.0