

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101019\
 Data File : BP000619.D
 Acq On : 10 Oct 2019 16:28
 Operator : JU
 Sample : K5292-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190855-AMENDED-COMP-B

Quant Time: Oct 11 04:48:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 01 18:03:42 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	263473	20.00	ng	-0.02
21) Naphthalene-d8	8.03	136	971285	20.00	ng	-0.02
39) Acenaphthene-d10	9.80	164	554114	20.00	ng	-0.02
64) Phenanthrene-d10	11.29	188	1001152	20.00	ng	-0.02
76) Chrysene-d12	13.97	240	826989	20.00	ng	-0.01
87) Perylene-d12	15.44	264	912254	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	25023	1.53	ng	-0.01
7) Phenol-d6	6.39	99	205982	10.43	ng	-0.02
23) Nitrobenzene-d5	7.31	82	795455	50.02	ng	-0.02
42) 2,4,6-Tribromophenol	10.59	330	5382	0.91	ng	-0.02
45) 2-Fluorobiphenyl	9.12	172	1493708	43.62	ng	-0.02
79) Terphenyl-d14	12.90	244	1752485	42.91	ng	-0.02
Target Compounds						
10) Phenol	6.40	94	45138	2.232	ng	93
50) Dimethylphthalate	9.51	163	349718	9.083	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101019\
Data File : BP000619.D
Acq On : 10 Oct 2019 16:28
Operator : JU
Sample : K5292-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190855-AMENDED-COMP-B

Quant Time: Oct 11 04:48:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 01 18:03:42 2019
Response via : Initial Calibration

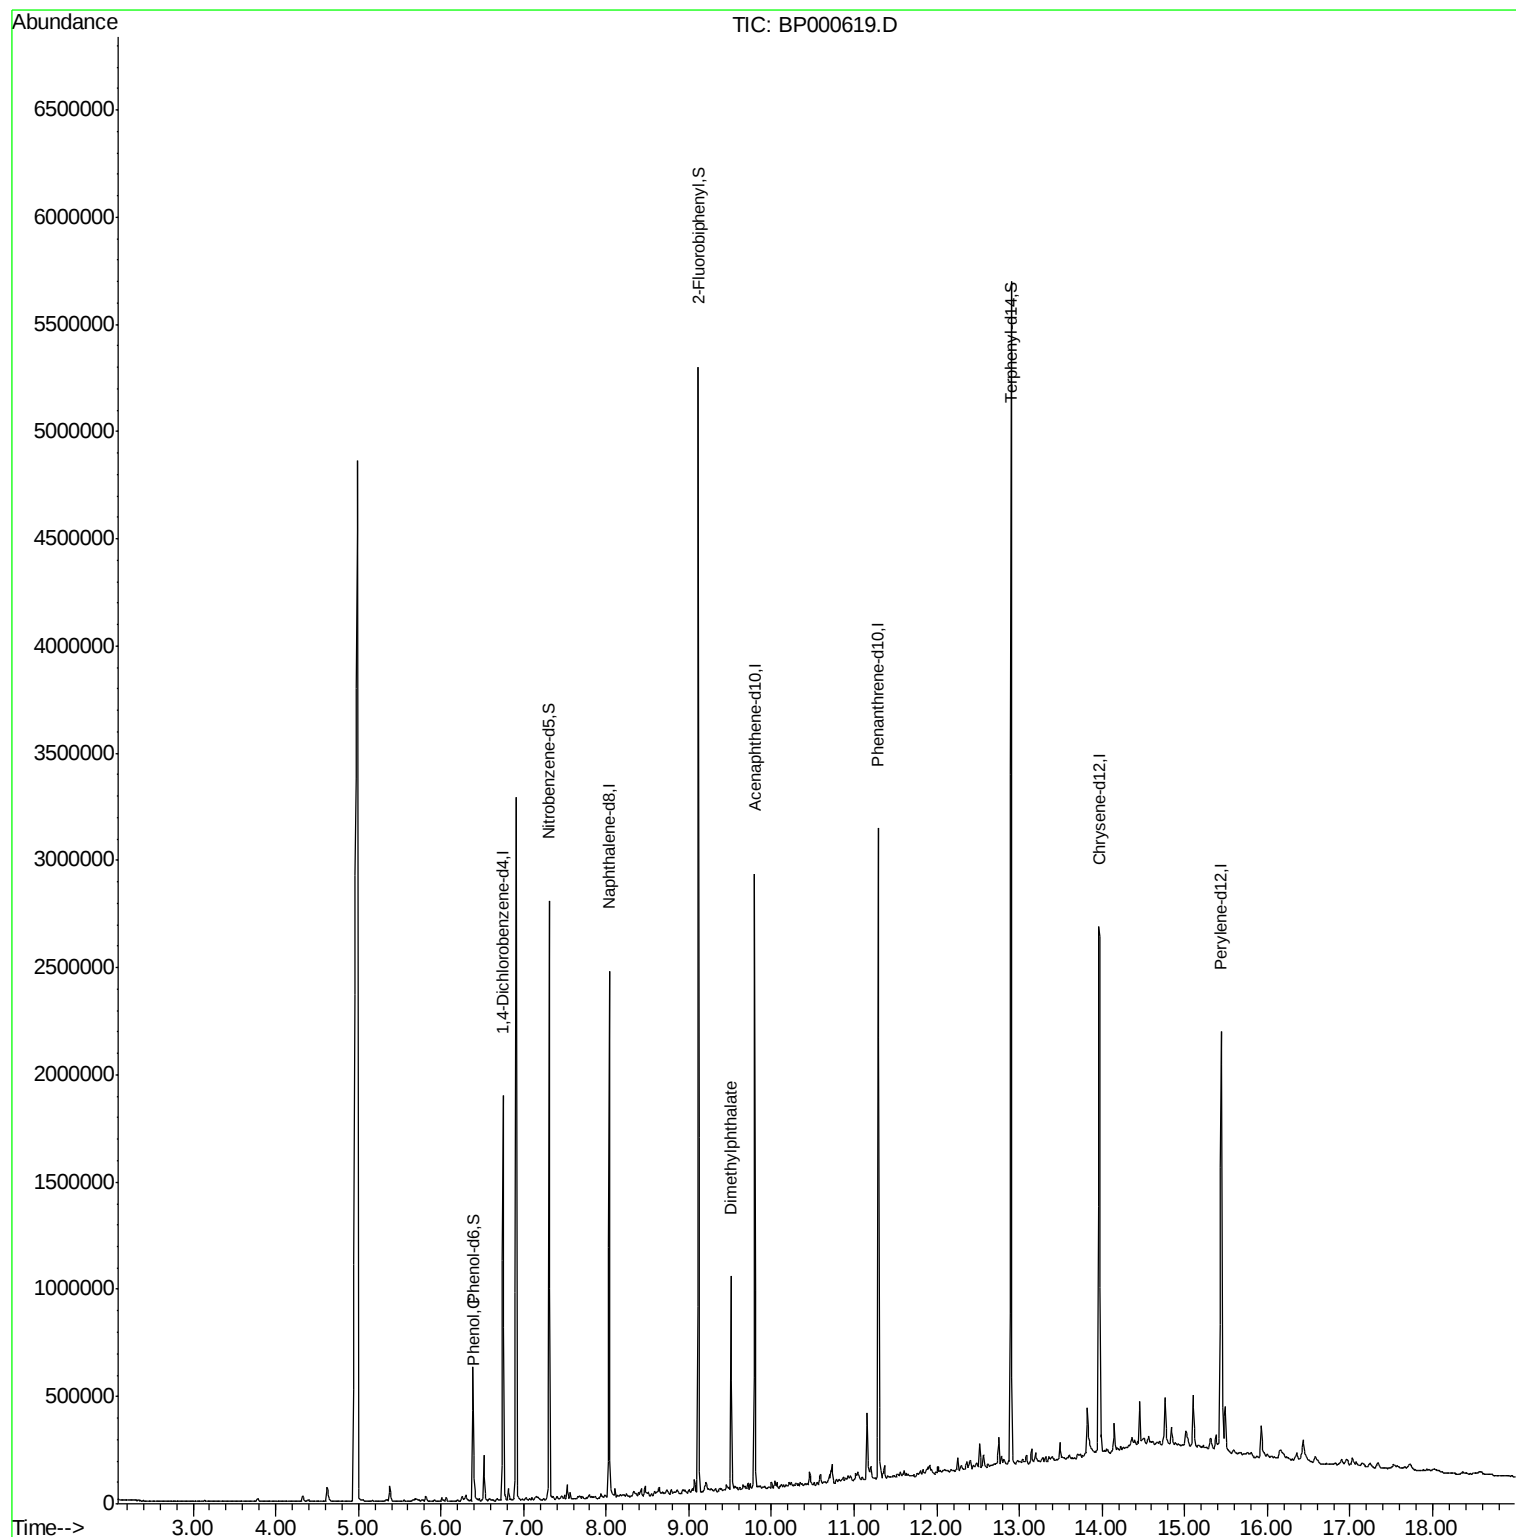

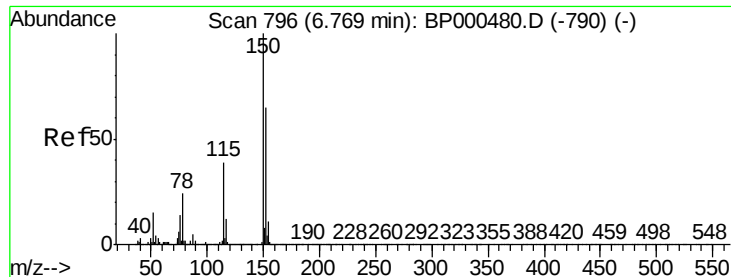


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. -0.02 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28

Instrument :
BNA_P
ClientSampleId :
20190855-AMENDED-COMP-B

Tot Ion:152 Resp: 263473
Ion Ratio Lower Upper
152 100
150 157.6 124.1 186.1
115 58.3 48.7 73.1

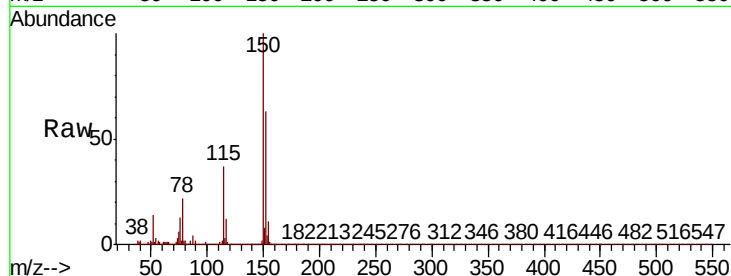


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

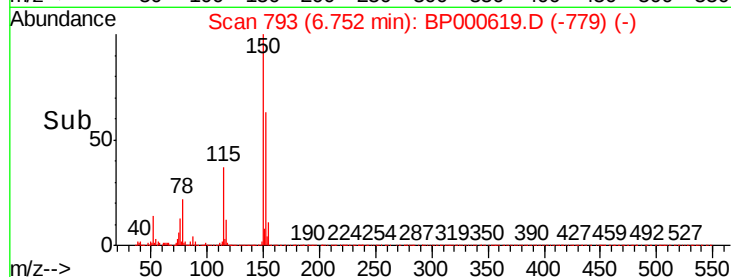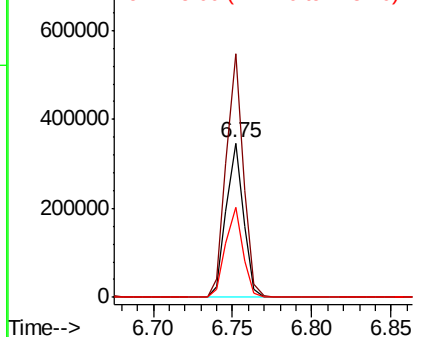



#5


2-Fluorophenol
Concen: 1.527 ng
RT: 5.38 min Scan# 560
Delta R.T. -0.01 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28

Tgt Ion:112 Resp: 25023
Ion Ratio Lower Upper
112 100
64 48.8 34.2 51.4
63 24.9 17.9 26.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

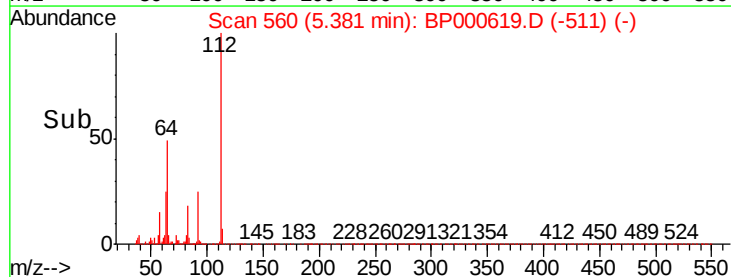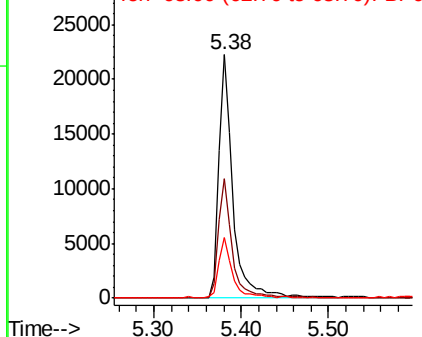

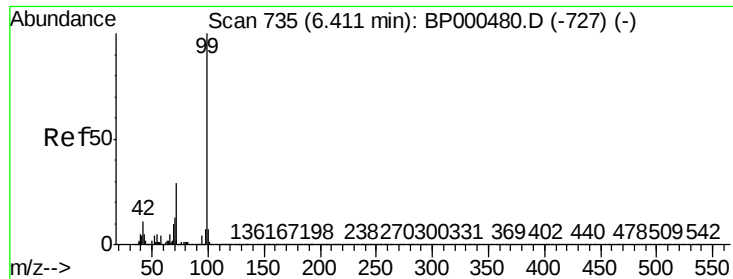

#7

Phenol-d6

Concen: 10.429 ng

RT: 6.39 min Scan# 731

Delta R.T. -0.02 min

Lab File: BP000619.D

Acq: 10 Oct 2019 16:28

Instrument :

BNA_P

ClientSampleId :

20190855-AMENDED-COMP-B


Tot Ion: 99 Resp: 205982

Ion Ratio Lower Upper

99 100

42 11.6 8.6 12.8




71 28.8 23.0 34.4

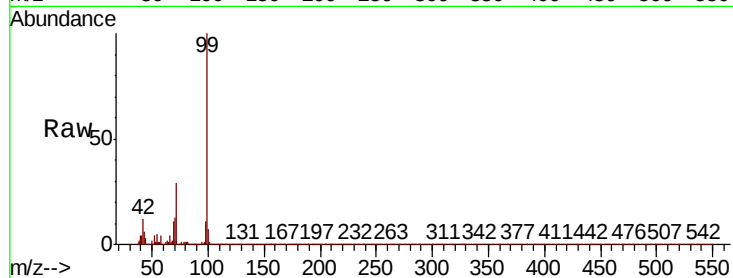

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

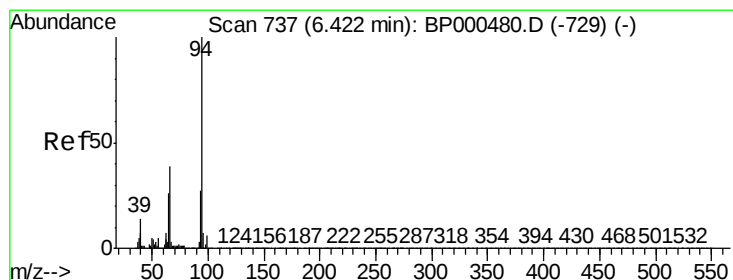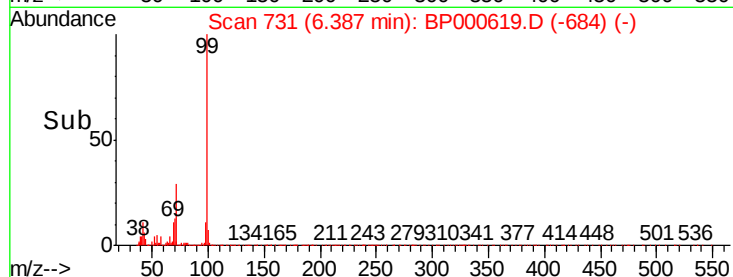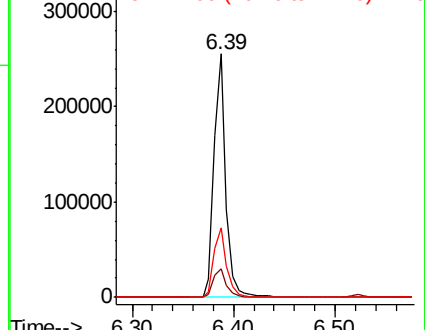

#10

Phenol

Concen: 2.232 ng

RT: 6.40 min Scan# 733

Delta R.T. -0.02 min

Lab File: BP000619.D

Acq: 10 Oct 2019 16:28


Tgt Ion: 94 Resp: 45138

Ion Ratio Lower Upper

94 100

65 24.3 5.9 45.9



66 32.6 18.8 58.8

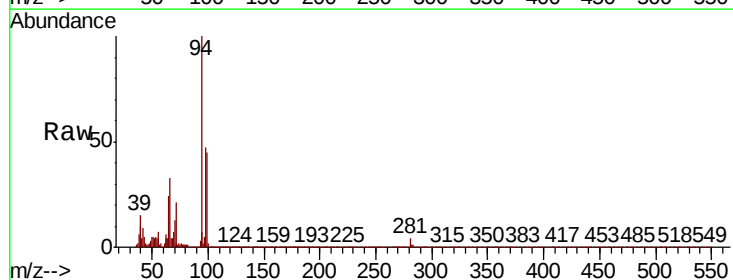


Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0



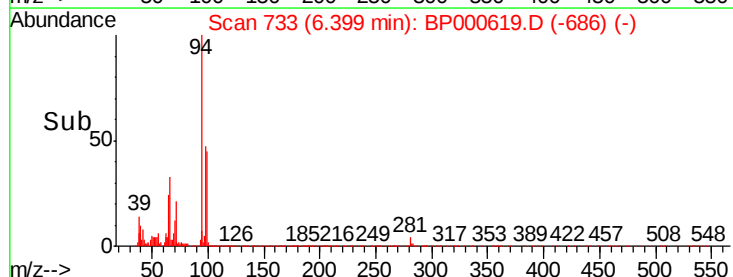
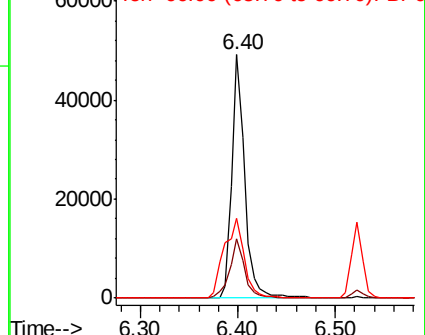


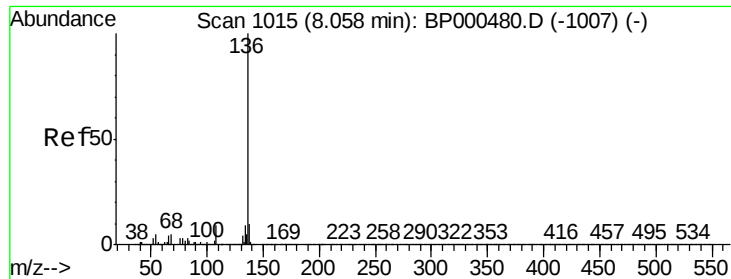

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.03 min Scan# 1011
Delta R.T. -0.02 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28




Instrument :
BNA_P
ClientSampleId :
20190855-AMENDED-COMP-B


Tot Ion:136	Resp: 971285
Ion Ratio	Lower Upper
136 100	
137 11.2	8.2 12.4
54 6.0	4.1 6.1
68 5.9	4.1 6.1

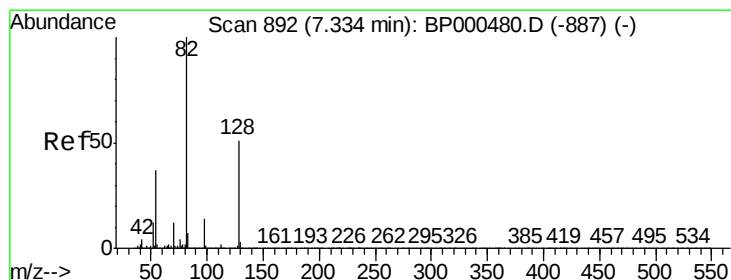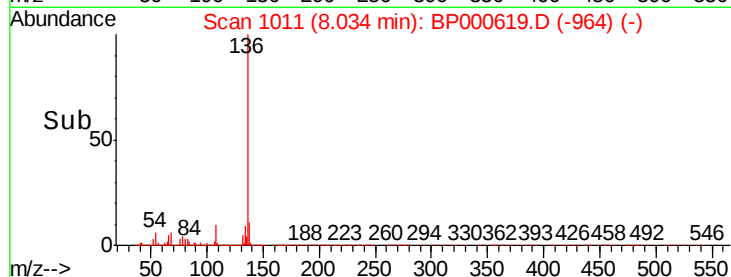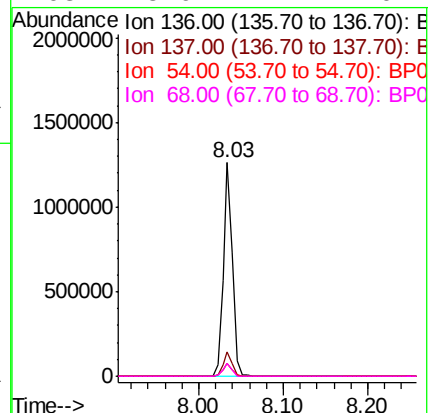

#23
Nitrobenzene-d5
Concen: 50.019 ng
RT: 7.31 min Scan# 888
Delta R.T. -0.02 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28

Tgt	Ion: 82	Resp:	795455
Ion	Ratio	Lower	Upper
82	100		
128	49.9	40.9	61.3
54	37.8	29.4	44.2


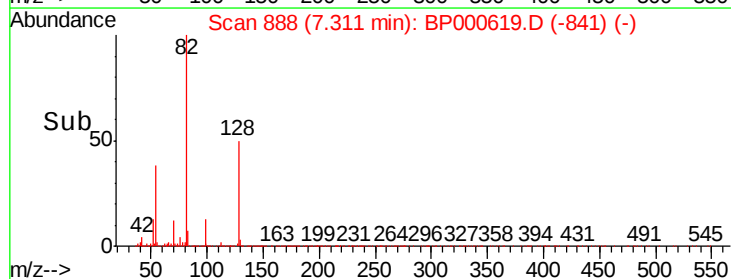
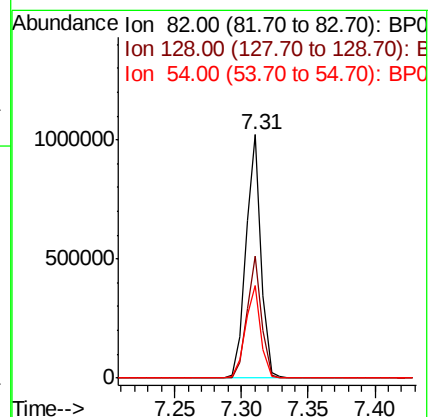
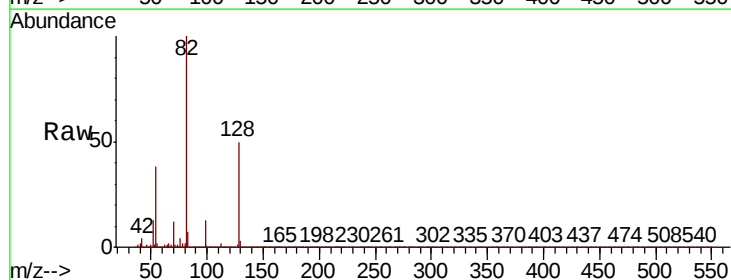


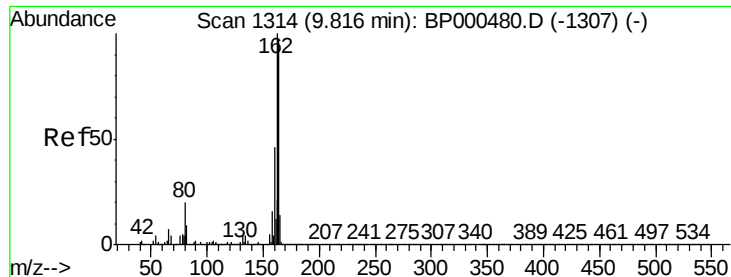

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.80 min Scan# 1311
Delta R.T. -0.02 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28




Instrument :
BNA_P
ClientSampleId :
20190855-AMENDED-COMP-B


Tot Ion:164 Resp: 554114
Ion Ratio Lower Upper
164 100
162 100.9 82.2 123.2
160 45.0 37.6 56.4

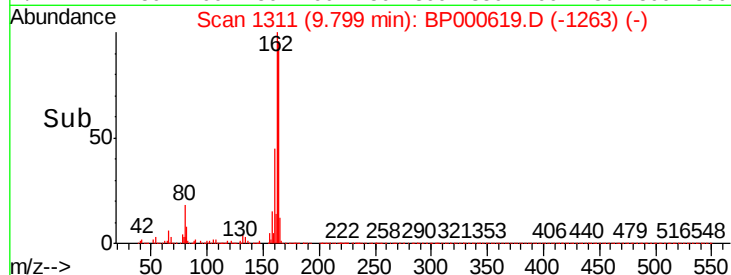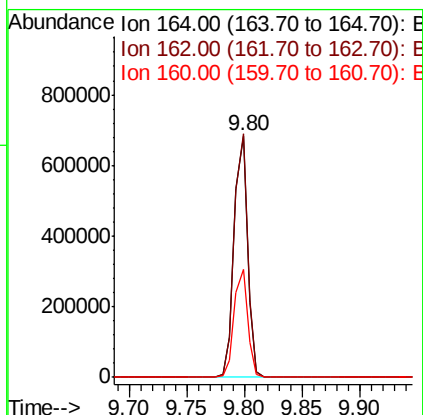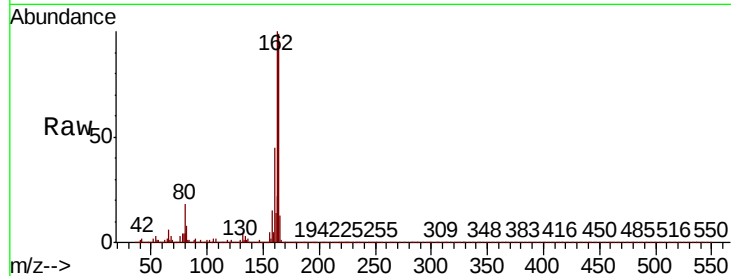

#42
2,4,6-Tribromophenol
Concen: 0.911 ng
RT: 10.59 min Scan# 1446
Delta R.T. -0.02 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28

Tgt Ion:330 Resp: 5382
Ion Ratio Lower Upper
330 100
332 94.0 77.1 115.7
141 31.3 26.0 39.0

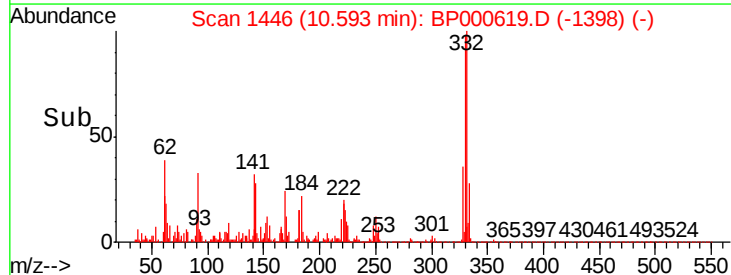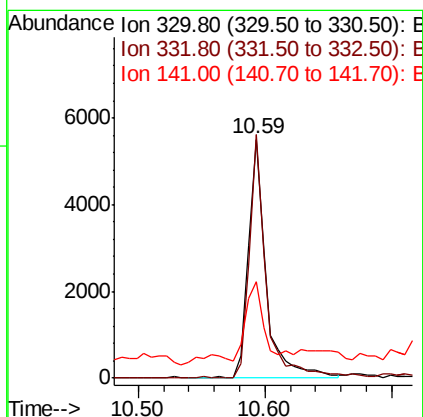


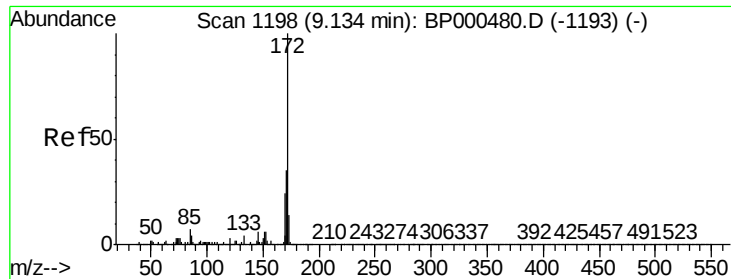




#45
2-Fluorobiphenyl
Concen: 43.616 ng
RT: 9.12 min Scan# 1195
Delta R.T. -0.02 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28

Instrument :
BNA_P
ClientSampleId :
20190855-AMENDED-COMP-B

Tot Ion:172 Resp: 1493708
Ion Ratio Lower Upper
172 100
171 35.5 28.4 42.6
170 23.8 19.1 28.7




Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

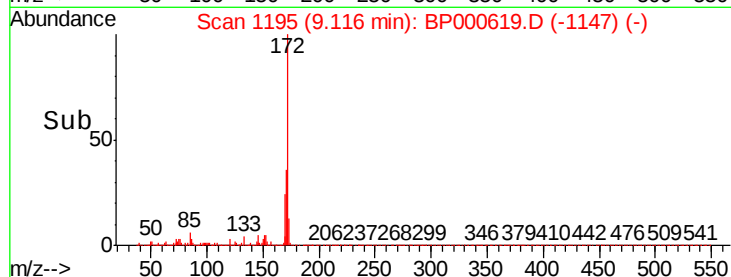
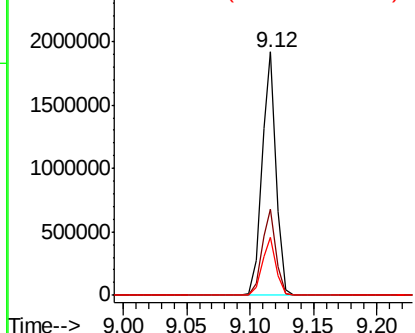



#50
Dimethylphthalate
Concen: 9.083 ng
RT: 9.51 min Scan# 1262
Delta R.T. -0.03 min
Lab File: BP000619.D
Acq: 10 Oct 2019 16:28

Tgt Ion:163 Resp: 349718
Ion Ratio Lower Upper
163 100
194 4.2 3.4 5.2
164 10.1 8.0 12.0



Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

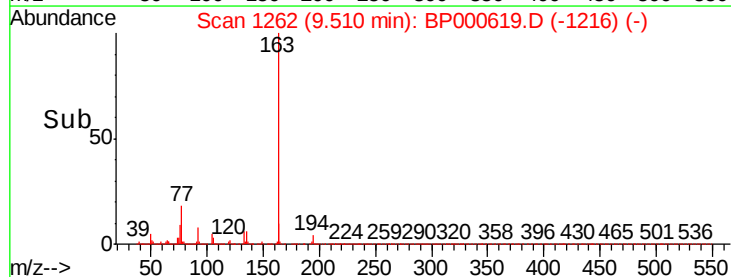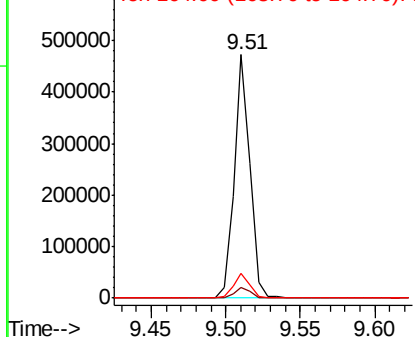

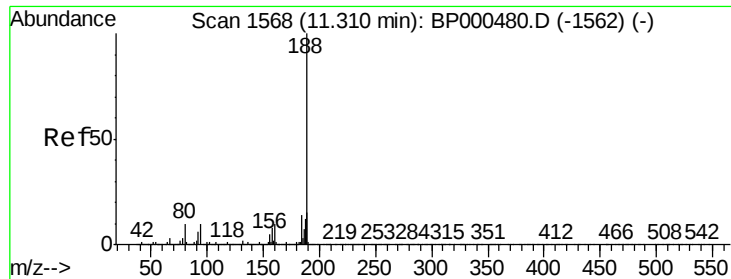

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.29 min Scan# 1565

Delta R.T. -0.02 min

Lab File: BP000619.D

Acq: 10 Oct 2019 16:28

Instrument :

BNA_P

ClientSampleId :

20190855-AMENDED-COMP-B


Tot Ion:188 Resp: 1001152

Ion Ratio Lower Upper

188 100

94 10.2 8.2 12.2




80 10.3 8.3 12.5

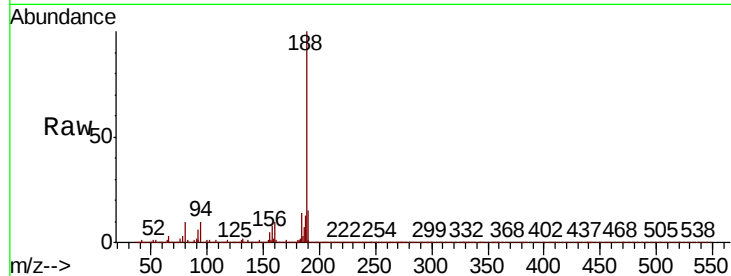

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

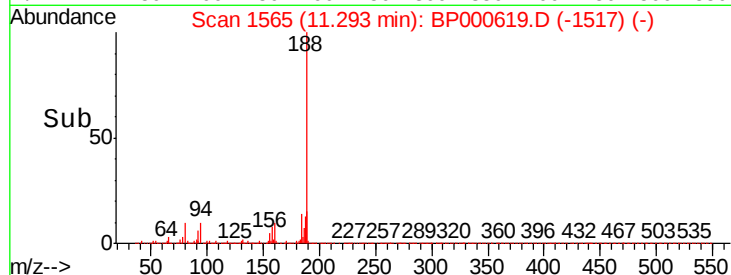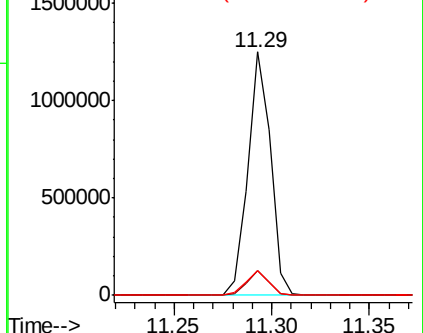

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.97 min Scan# 2020

Delta R.T. -0.01 min

Lab File: BP000619.D

Acq: 10 Oct 2019 16:28


Tgt Ion:240 Resp: 826989

Ion Ratio Lower Upper

240 100

120 10.7 10.1 15.1



236 26.8 22.7 34.1




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

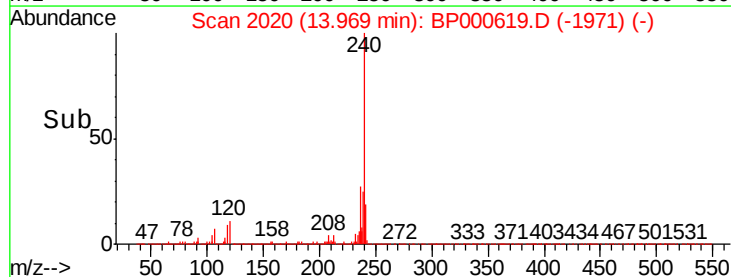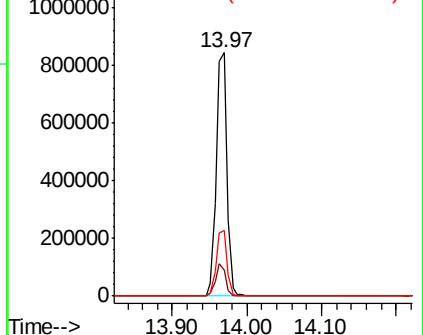

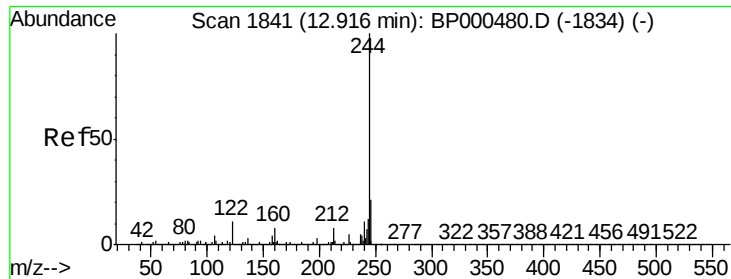

#79

Terphenyl-d14

Concen: 42.906 ng

RT: 12.90 min Scan# 1838

Delta R.T. -0.02 min

Lab File: BP000619.D

Acq: 10 Oct 2019 16:28

Instrument :

BNA_P

ClientSampleId :

20190855-AMENDED-COMP-B


Tot Ion:244 Resp: 1752485

Ion Ratio Lower Upper

244 100

212 7.2 6.0 9.0

122 12.0 8.9 13.3






Abundance

Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

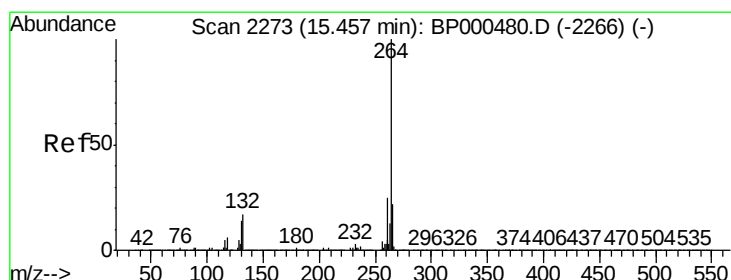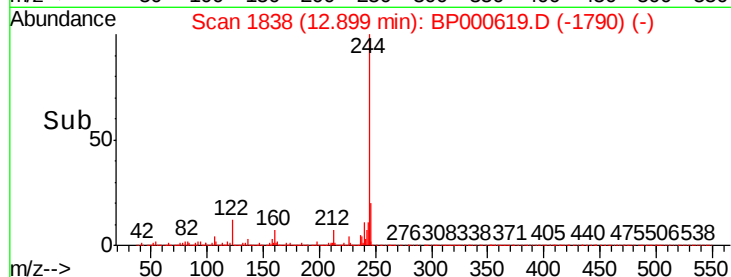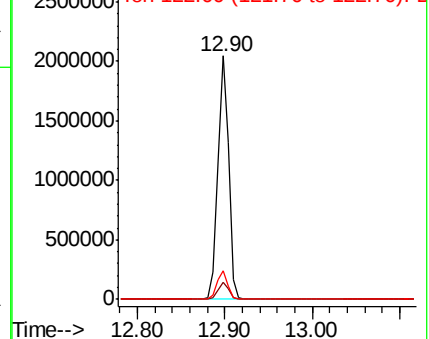

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2270

Delta R.T. -0.02 min

Lab File: BP000619.D

Acq: 10 Oct 2019 16:28


Tgt Ion:264 Resp: 912254

Ion Ratio Lower Upper

264 100

260 24.8 20.3 30.5

265 22.1 18.0 27.0



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

