

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101019\
 Data File : BP000624.D
 Acq On : 10 Oct 2019 18:28
 Operator : JU
 Sample : K5297-10
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TP-4

Quant Time: Oct 11 05:01:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 01 18:03:42 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	260161	20.00	ng	-0.02
21) Naphthalene-d8	8.03	136	955046	20.00	ng	-0.02
39) Acenaphthene-d10	9.79	164	536492	20.00	ng	-0.02
64) Phenanthrene-d10	11.29	188	966061	20.00	ng	-0.02
76) Chrysene-d12	13.96	240	825880	20.00	ng	-0.02
87) Perylene-d12	15.44	264	887530	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	1504081	92.93	ng	-0.02
7) Phenol-d6	6.39	99	1928980	98.91	ng	-0.02
23) Nitrobenzene-d5	7.31	82	1046040	66.89	ng	-0.02
42) 2,4,6-Tribromophenol	10.59	330	516783	90.39	ng	-0.02
45) 2-Fluorobiphenyl	9.12	172	2097370	63.25	ng	-0.02
79) Terphenyl-d14	12.90	244	2315733	56.77	ng	-0.02
Target Compounds						
10) Phenol	6.40	94	75931	3.802	ng	91
50) Dimethylphthalate	9.51	163	335874	9.010	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101019\
Data File : BP000624.D
Acq On : 10 Oct 2019 18:28
Operator : JU
Sample : K5297-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TP-4

Quant Time: Oct 11 05:01:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 01 18:03:42 2019
Response via : Initial Calibration

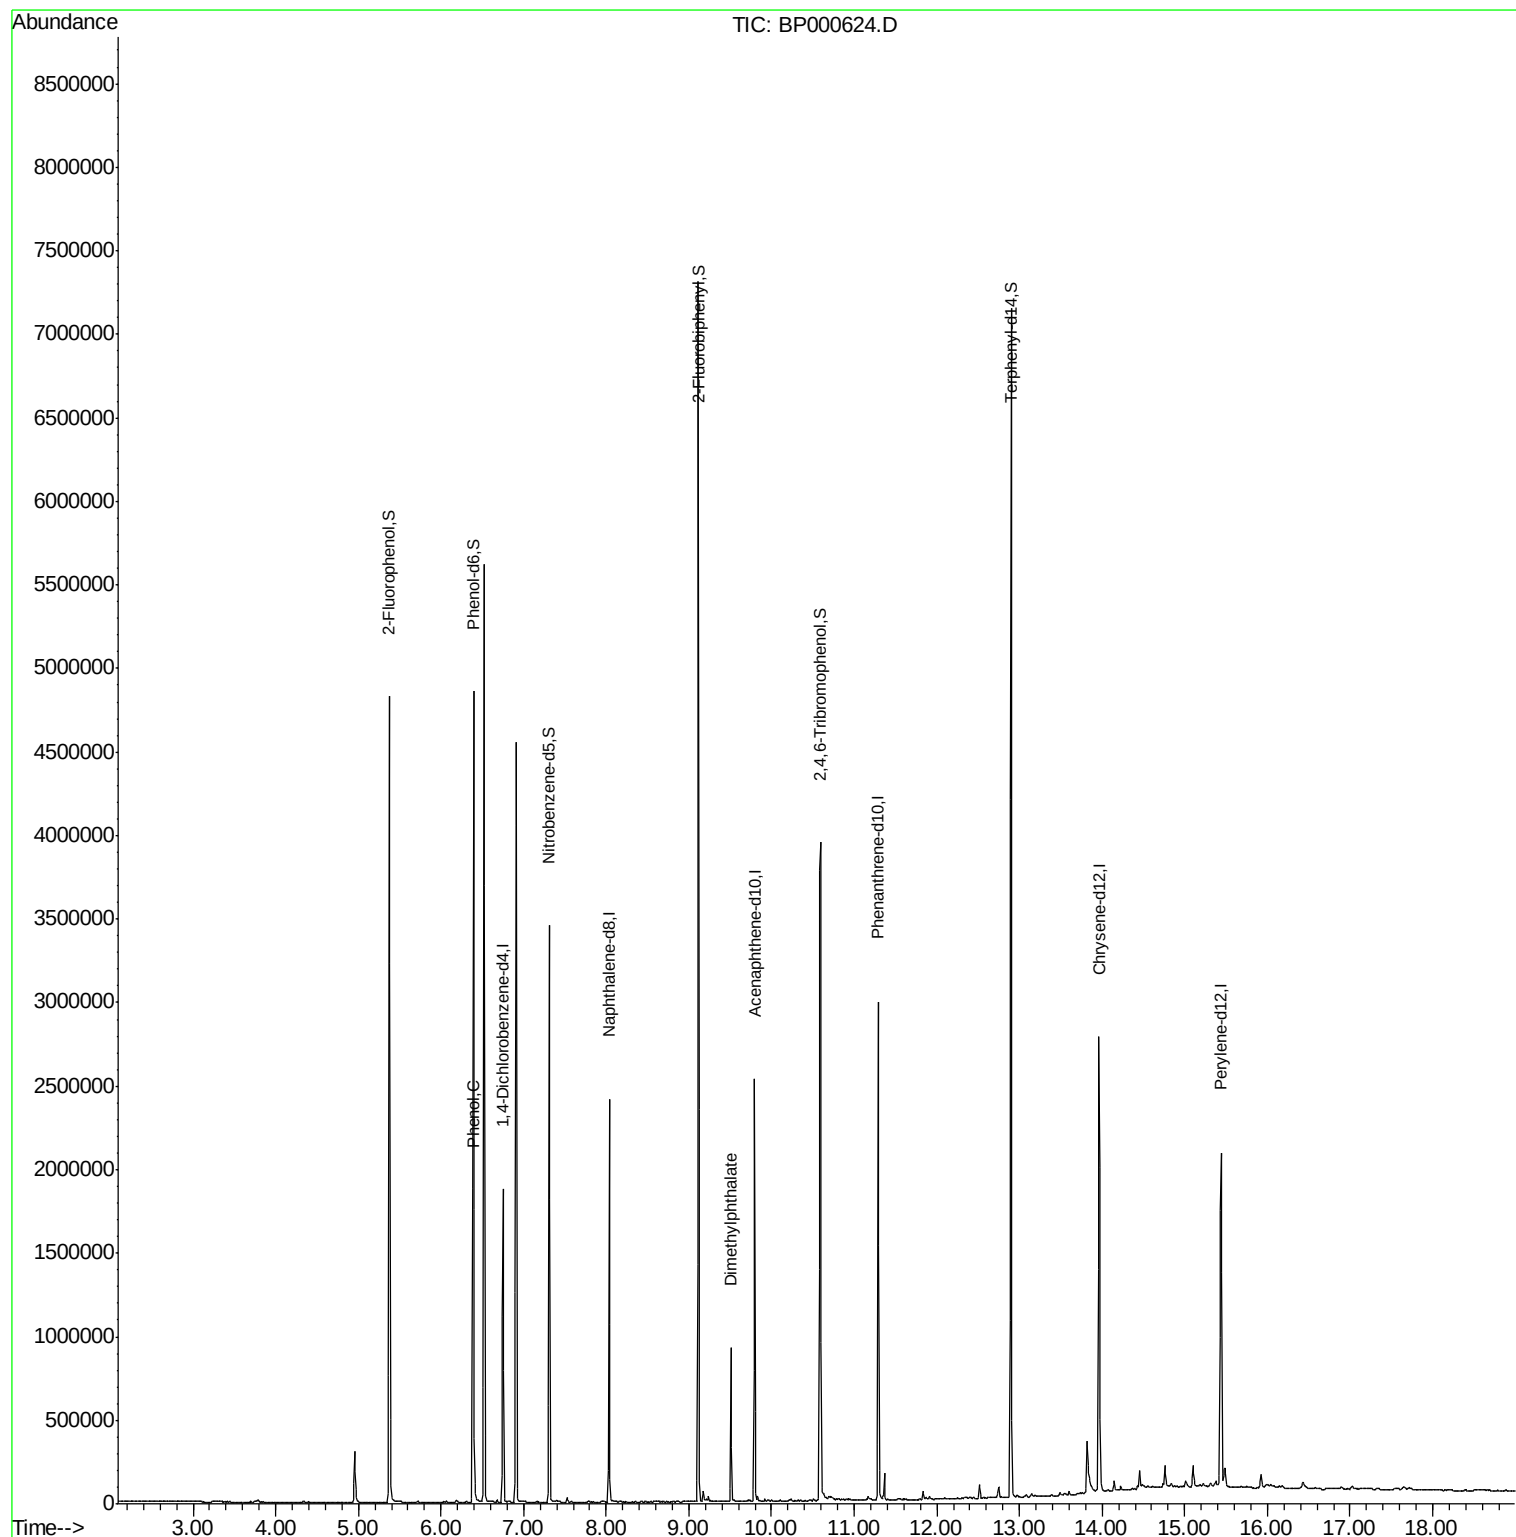




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.75 min Scan# 793
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28

Instrument :
BNA_P
ClientSampleId :
TP-4

Tot Ion	Ratio	Lower	Upper
152	100		
150	157.1	124.1	186.1
115	58.5	48.7	73.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

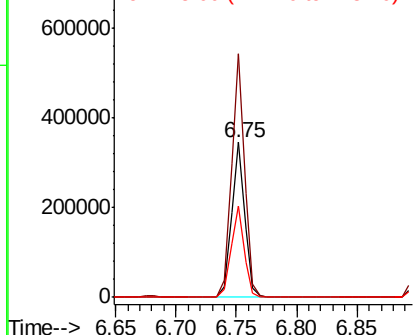



#5


2-Fluorophenol
Concen: 92.932 ng
RT: 5.38 min Scan# 559
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28

Tgt Ion	Ratio	Lower	Upper
112	100		
64	45.1	34.2	51.4
63	23.0	17.9	26.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

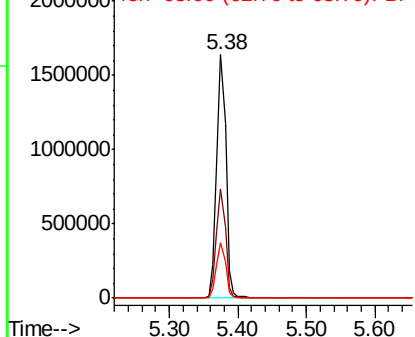

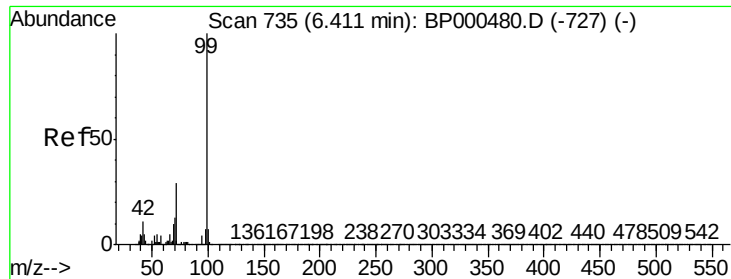

#7

Phenol-d6

Concen: 98.905 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.02 min

Lab File: BP000624.D

Acq: 10 Oct 2019 18:28

Instrument :

BNA_P

ClientSampled :

TP-4





Tot Ion: 99 Resp: 1928980

Ion Ratio Lower Upper

99 100

42 10.6 8.6 12.8

71 28.4 23.0 34.4

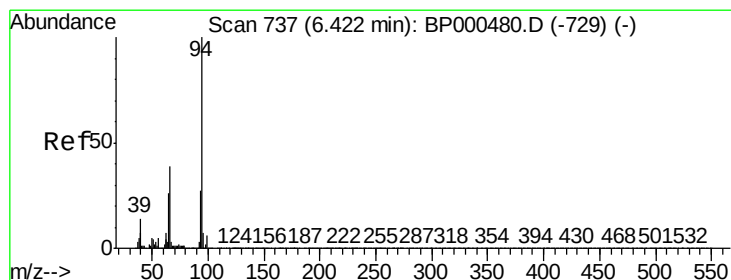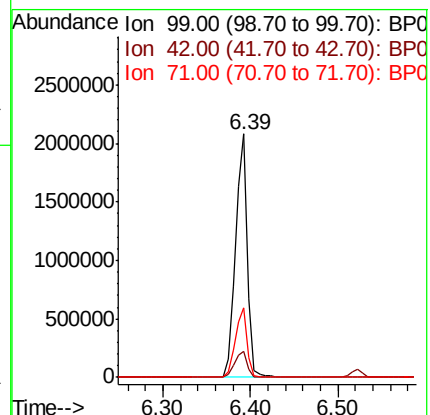

#10

Phenol

Concen: 3.802 ng

RT: 6.40 min Scan# 734

Delta R.T. -0.02 min

Lab File: BP000624.D

Acq: 10 Oct 2019 18:28




Tgt Ion: 94 Resp: 75931


Ion Ratio Lower Upper

94 100

65 23.4 5.9 45.9

66 31.8 18.8 58.8

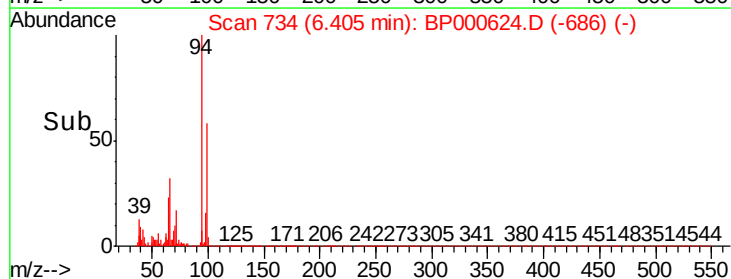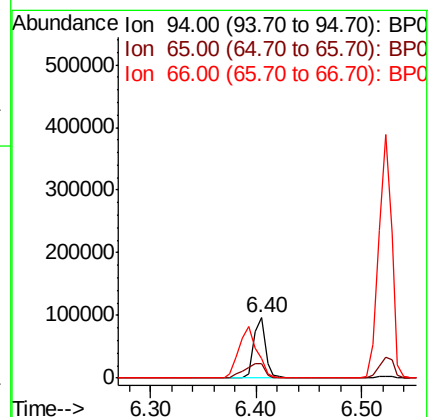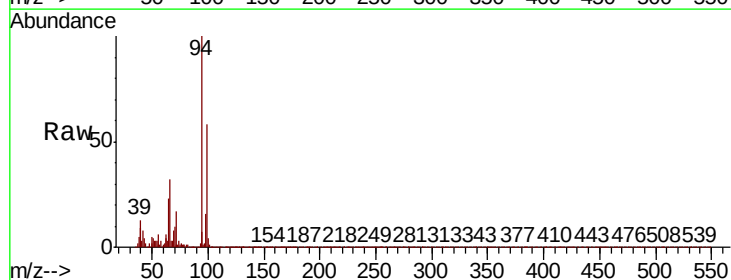



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.03 min Scan# 1011

Delta R.T. -0.02 min

Lab File: BP000624.D

Acq: 10 Oct 2019 18:28

Instrument :

BNA_P

ClientSampleId :

TP-4

Tot Ion:136 Resp: 955046


Ion Ratio Lower Upper

136 100

137 11.1 8.2 12.4

54 5.8 4.1 6.1

68 5.7 4.1 6.1



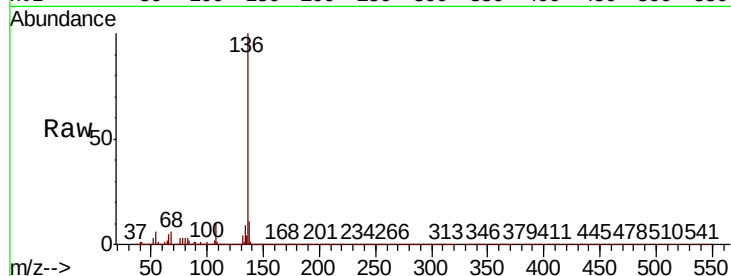


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0

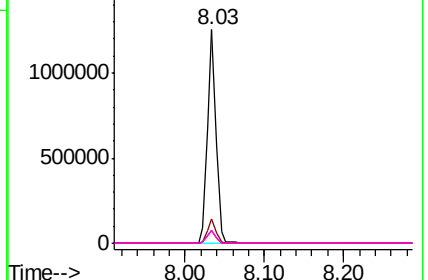

#23

Nitrobenzene-d5

Concen: 66.894 ng

RT: 7.31 min Scan# 888

Delta R.T. -0.02 min

Lab File: BP000624.D

Acq: 10 Oct 2019 18:28


Tgt Ion: 82 Resp: 1046040

Ion Ratio Lower Upper

82 100

128 50.1 40.9 61.3



54 38.0 29.4 44.2




Abundance Ion 82.00 (81.70 to 82.70): BP0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BP0



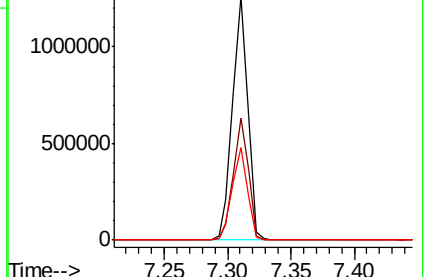



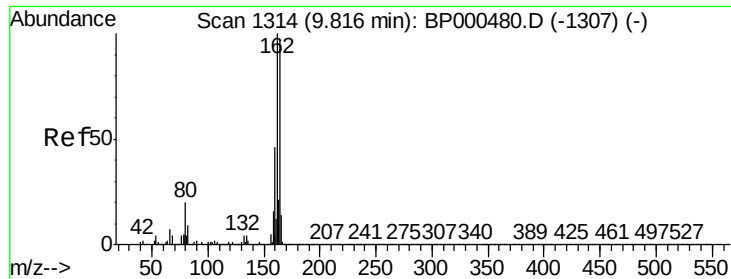

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.79 min Scan# 1310
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28




Instrument :
BNA_P
ClientSampleId :
TP-4


Tot Ion:164 Resp: 536492
Ion Ratio Lower Upper
164 100
162 99.8 82.2 123.2
160 45.0 37.6 56.4

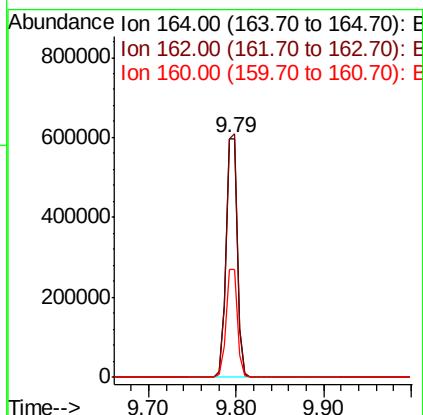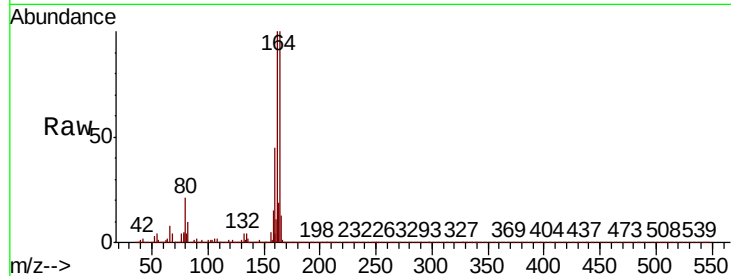

#42
2,4,6-Tribromophenol
Concen: 90.395 ng
RT: 10.59 min Scan# 1446
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28

Tgt Ion:330 Resp: 516783
Ion Ratio Lower Upper
330 100
332 95.7 77.1 115.7
141 32.9 26.0 39.0



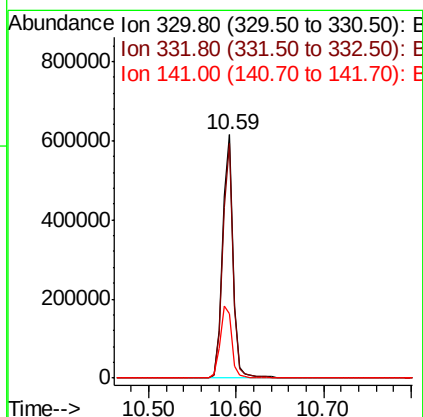



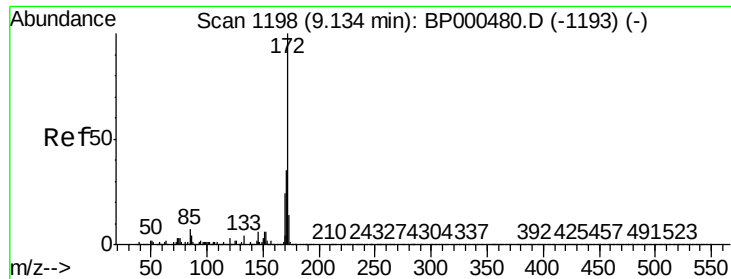

#45
2-Fluorobiphenyl
Concen: 63.254 ng
RT: 9.12 min Scan# 1195
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28




Instrument :
BNA_P
ClientSampleId :
TP-4


Tot Ion:172 Resp: 2097370
Ion Ratio Lower Upper
172 100
171 36.2 28.4 42.6
170 24.3 19.1 28.7

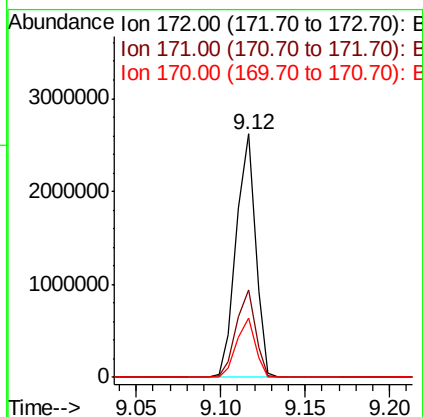

#50
Dimethylphthalate
Concen: 9.010 ng
RT: 9.51 min Scan# 1262
Delta R.T. -0.03 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28

Tgt Ion:163 Resp: 335874
Ion Ratio Lower Upper
163 100
194 4.1 3.4 5.2
164 10.0 8.0 12.0



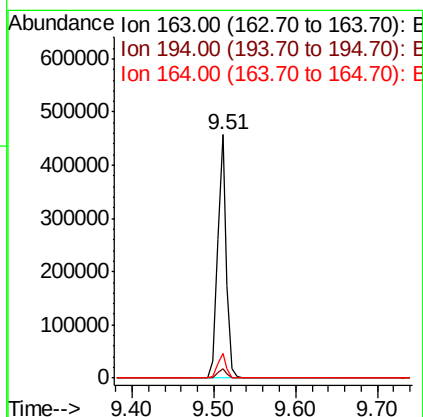





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.29 min Scan# 1565
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28




Instrument :
BNA_P
ClientSampleId :
TP-4


Tot Ion:188 Resp: 966061
Ion Ratio Lower Upper
188 100
94 9.6 8.2 12.2
80 9.6 8.3 12.5

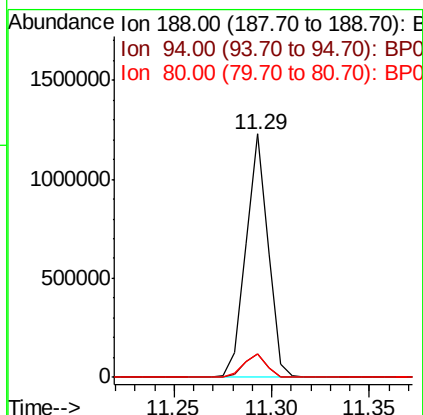

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.96 min Scan# 2019
Delta R.T. -0.02 min
Lab File: BP000624.D
Acq: 10 Oct 2019 18:28

Tgt Ion:240 Resp: 825880
Ion Ratio Lower Upper
240 100
120 12.7 10.1 15.1
236 26.9 22.7 34.1

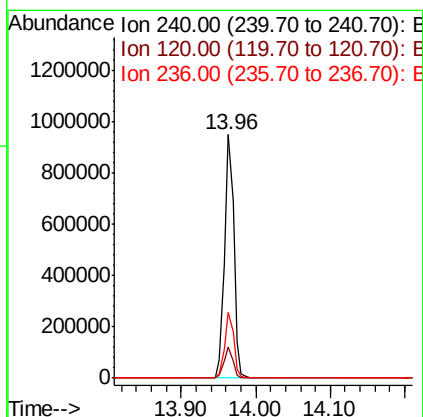

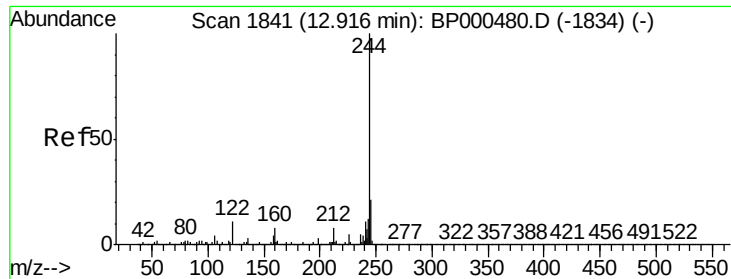

#79

Terphenyl-d14

Concen: 56.772 ng

RT: 12.90 min Scan# 1838

Delta R.T. -0.02 min

Lab File: BP000624.D

Acq: 10 Oct 2019 18:28

Instrument :

BNA_P

ClientSampleId :

TP-4


Tot Ion:244 Resp: 2315733

Ion Ratio Lower Upper

244 100

212 7.5 6.0 9.0




122 12.0 8.9 13.3

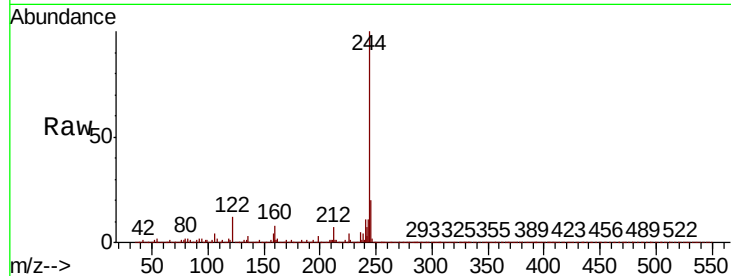

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

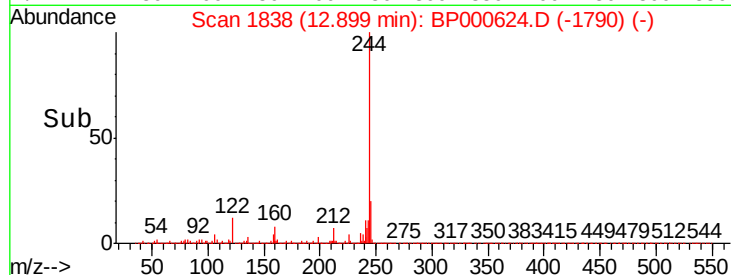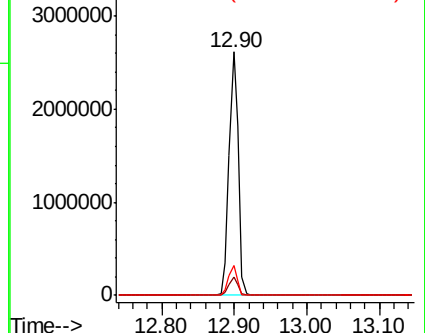

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.44 min Scan# 2270

Delta R.T. -0.02 min

Lab File: BP000624.D

Acq: 10 Oct 2019 18:28


Tgt Ion:264 Resp: 887530

Ion Ratio Lower Upper

264 100

260 24.0 20.3 30.5

265 21.4 18.0 27.0



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

