
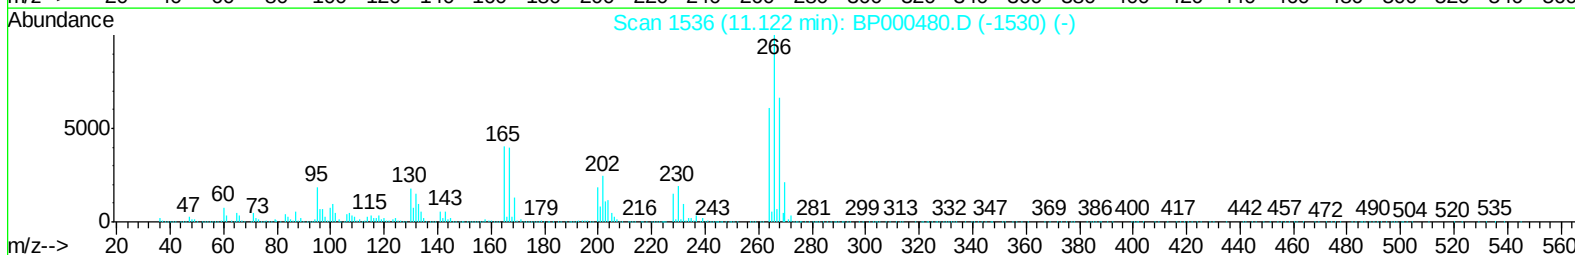
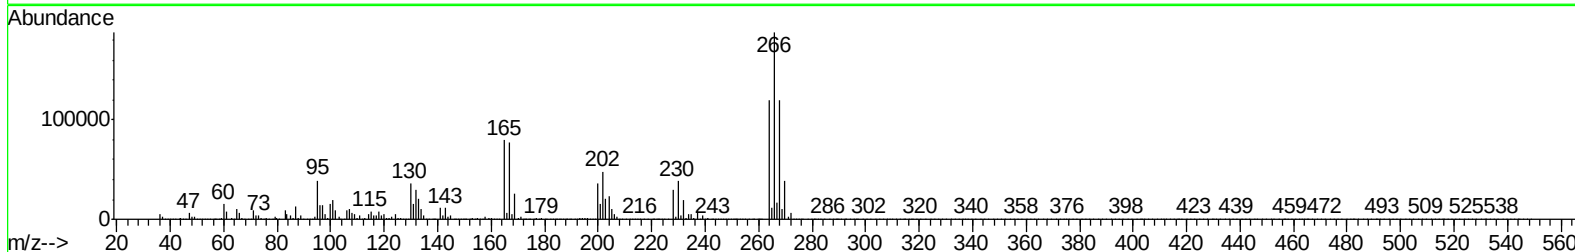


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101019\
 Data File : BP000605.D
 Acq On : 10 Oct 2019 10:27
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 05:43:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 01 18:03:42 2019
 Response via : Initial Calibration

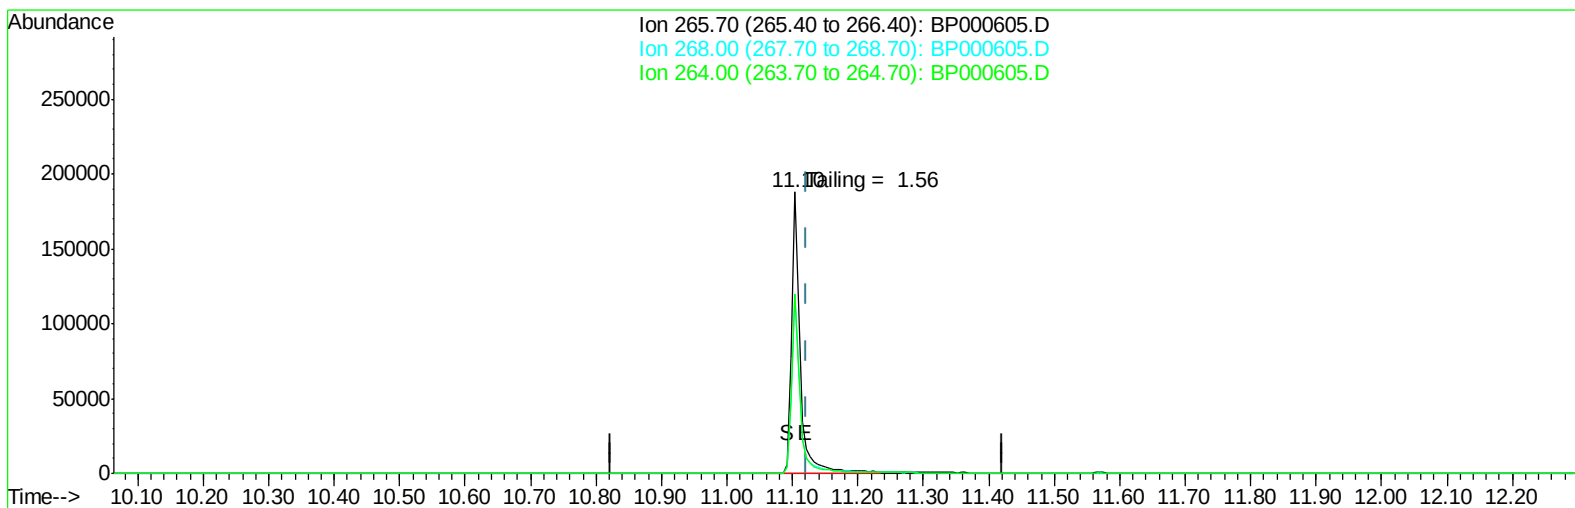

TIC: BP000605.D

(70) Pentachlorophenol (C)




11.104min (-0.018) 273381.57ng

response 176977

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	63.45
264.00	61.20	63.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101019\
Data File : BP000605.D
Acq On : 10 Oct 2019 10:27
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 05:43:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 01 18:03:42 2019
Response via : Initial Calibration

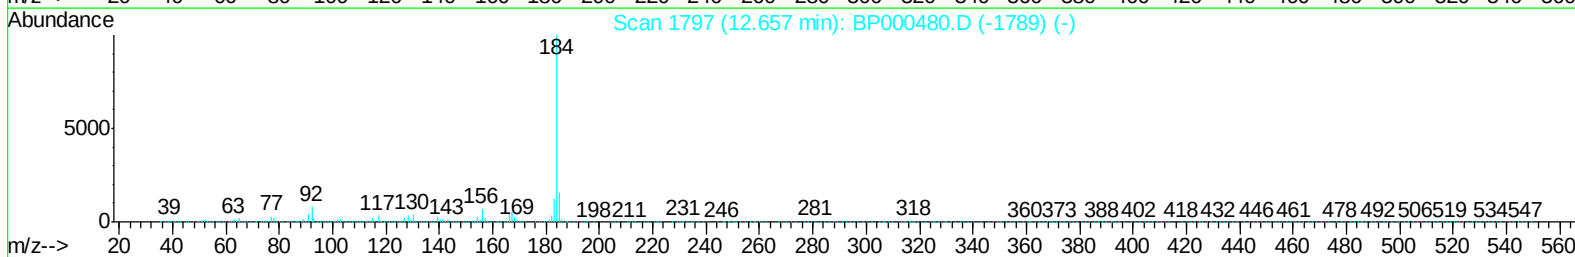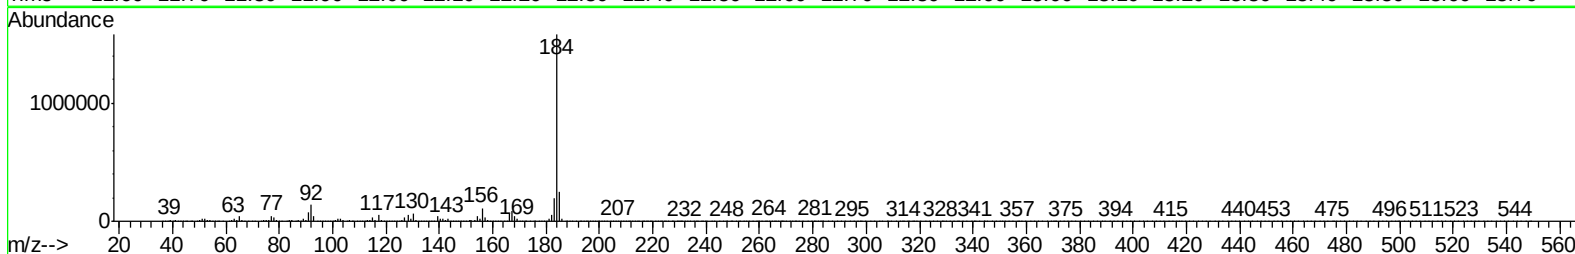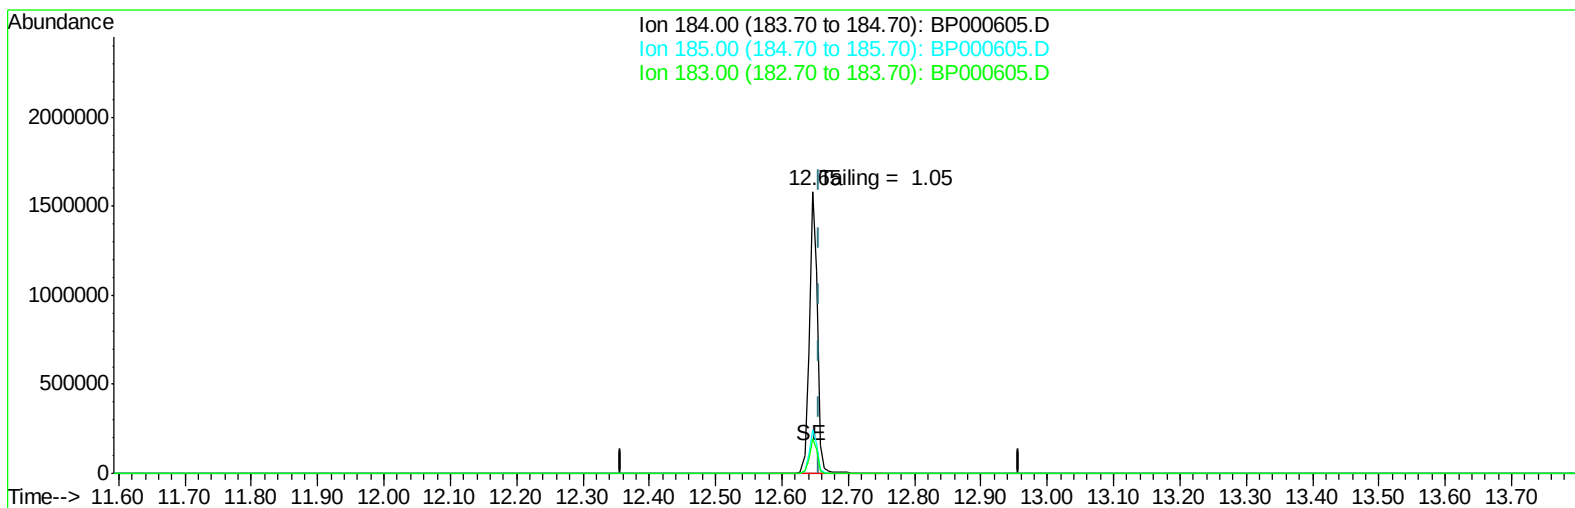

TIC: BP000605.D

(77) Benzidine

12.646min (-0.012) 2079503.07ng

response 1324781

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	15.51
183.00	12.10	12.11
0.00	0.00	0.00