


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_P\DATA\BP101019\  
 Data File : BP000605.D  
 Acq On : 10 Oct 2019 10:27  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_P\METHODS\8270-BP100119.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Oct 01 18:03:42 2019

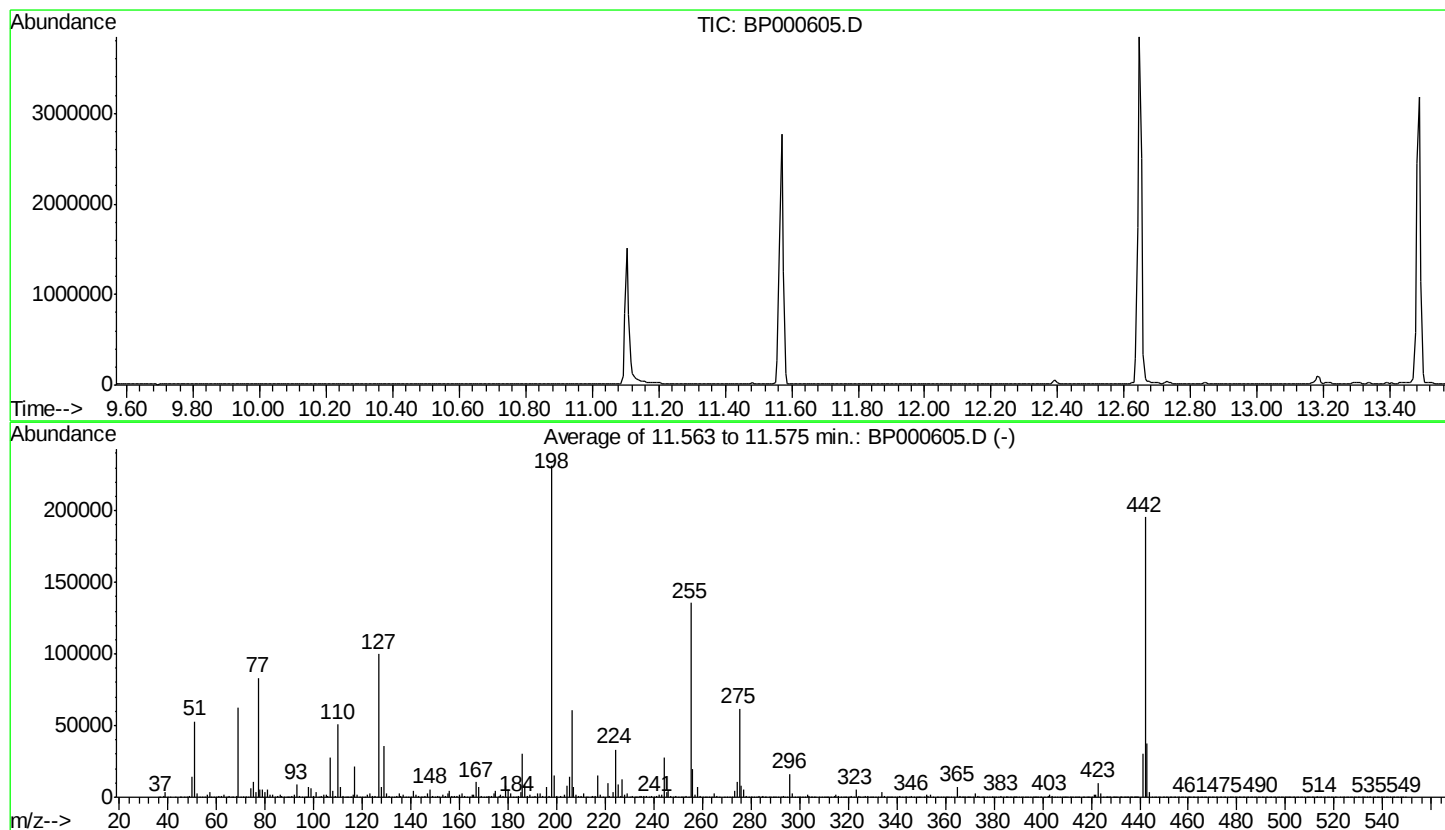

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 23.0      | 53143   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 1146    | PASS             |
| 69          | 198          | 0.00         | 100          | 27.2      | 62869   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 292     | PASS             |
| 127         | 198          | 10           | 80           | 43.2      | 99906   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 671     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 231408  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 15502   | PASS             |
| 275         | 198          | 10           | 60           | 26.7      | 61765   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 7275    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.1      | 30205   | PASS             |
| 442         | 198          | 50           | 100          | 84.5      | 195525  | PASS             |
| 443         | 442          | 15           | 24           | 19.0      | 37210   | PASS             |