

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101022\
 Data File : BP012028.D
 Acq On : 10 Oct 2022 17:49
 Operator : CG/JU
 Sample : SSTD04065
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040627

Quant Time: Oct 11 00:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 00:41:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.863	152	163314	20.000	ng/ul	0.00
20) Naphthalene-d8	10.669	136	684093	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.510	164	394143	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.269	188	800222	20.000	ng/ul	0.00
79) Chrysene-d12	21.357	240	834220	20.000	ng/ul	0.00
88) Perylene-d12	23.780	264	872155	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	26860	7.254	ng/uL	0.00
4) Pyridine-d5	3.705	84	238926	22.028	ng/ul	0.00
7) Phenol-d5	7.028	99	580936	41.204	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	343058	43.898	ng/ul	0.00
11) 2-Chlorophenol-d4	7.393	132	459589	41.294	ng/ul	0.00
15) 4-Methylphenol-d8	8.575	113	433988	37.237	ng/ul	0.00
21) Nitrobenzene-d5	9.034	128	216416	41.533	ng/ul	0.00
24) 2-Nitrophenol-d4	9.752	143	225198	40.396	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.293	165	410234	39.784	ng/ul	0.00
31) 4-Chloroaniline-d4	10.810	131	596445	37.941	ng/ul	0.00
46) Dimethylphthalate-d6	13.922	166	1108829	39.341	ng/ul	0.00
49) Acenaphthylene-d8	14.204	160	1377971	42.886	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143	234570	40.190	ng/ul	0.00
60) Fluorene-d10	15.504	176	978605	39.980	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.634	200	182285	37.635	ng/ul	0.00
73) Anthracene-d10	17.369	188	1531478	42.014	ng/ul	0.00
81) Pyrene-d10	19.604	212	1740806	41.204	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.621	264	1840913	42.166	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.311	88	28017	7.005	ng/uL	94
5) Pyridine	3.723	79	238180	22.625	ng/ul	99
6) Benzaldehyde	7.005	77	312319	50.569	ng/ul	99
8) Phenol	7.058	94	611471	41.815	ng/ul	99
10) Bis(2-Chloroethyl)ether	7.287	93	478483	41.121	ng/ul	99
12) 2-Chlorophenol	7.422	128	492313	41.376	ng/ul	98
13) 2-Methylphenol	8.310	108	446698	38.772	ng/ul	100
14) 2,2'-oxybis(1-Chloropr...	8.399	45	561218	48.925	ng/ul	99
16) Acetophenone	8.693	105	697393	39.247	ng/ul	99
17) N-Nitroso-di-n-propyla...	8.681	70	319729	38.229	ng/ul	98
18) 4-Methylphenol	8.640	108	483479	38.087	ng/ul	100
19) Hexachloroethane	8.940	117	199901	45.045	ng/ul	99
22) Nitrobenzene	9.075	77	524790	46.829	ng/ul	97
23) Isophorone	9.605	82	939222	41.315	ng/ul	99
25) 2-Nitrophenol	9.787	139	260105	40.851	ng/ul	98
26) 2,4-Dimethylphenol	9.846	107	492779	41.199	ng/ul	100
27) Bis(2-Chloroethoxy)met...	10.087	93	593279	40.450	ng/ul	100
29) 2,4-Dichlorophenol	10.316	162	425166	39.793	ng/ul	99
30) Naphthalene	10.722	128	1514979	41.231	ng/ul	99
32) 4-Chloroaniline	10.840	127	626300	38.943	ng/ul	99
33) Hexachlorobutadiene	10.999	225	250299	39.578	ng/ul	99
34) Caprolactam	11.634	113	64871	17.155	ng/ul	97
35) 4-Chloro-3-methylphenol	11.963	107	442832	39.090	ng/ul	98
36) 2-Methylnaphthalene	12.334	142	981911	38.266	ng/ul	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101022\
 Data File : BP012028.D
 Acq On : 10 Oct 2022 17:49
 Operator : CG/JU
 Sample : SST04065
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST040627

Quant Time: Oct 11 00:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 00:41:15 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.551	142	989861	38.445	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.698	216	470745	41.184	ng/ul	100
40) Hexachlorocyclopentadiene	12.675	237	219366	33.594	ng/ul	98
41) 2,4,6-Trichlorophenol	12.940	196	312513	40.844	ng/ul	98
42) 2,4,5-Trichlorophenol	13.016	196	335665	40.274	ng/ul	99
43) 1,1'-Biphenyl	13.346	154	1228291	42.133	ng/ul	99
44) 2-Chloronaphthalene	13.387	162	983224	42.659	ng/ul	98
45) 2-Nitroaniline	13.598	65	256366	45.566	ng/ul	97
47) Dimethylphthalate	13.969	163	1168167	39.547	ng/ul	99
48) 2,6-Dinitrotoluene	14.093	165	222098	38.581	ng/ul	98
50) Acenaphthylene	14.234	152	1528870	42.842	ng/ul	99
51) 3-Nitroaniline	14.422	138	253951	38.060	ng/ul	94
52) Acenaphthene	14.575	153	1063286	42.232	ng/ul	99
53) 2,4-Dinitrophenol	14.634	184	130642	33.473	ng/ul	97
55) 4-Nitrophenol	14.734	109	174564	44.305	ng/ul	96
56) Dibenzofuran	14.910	168	1417408	41.103	ng/ul	98
57) 2,4-Dinitrotoluene	14.881	165	345325	41.039	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.140	232	276419	38.177	ng/ul	99
59) Diethylphthalate	15.340	149	1169166	39.509	ng/ul	99
61) Fluorene	15.563	166	1154854	40.888	ng/ul	98
62) 4-Chlorophenyl-phenyle...	15.557	204	537815	38.464	ng/ul	100
63) 4-Nitroaniline	15.592	138	248112	38.968	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.645	198	200971	39.167	ng/ul#	99
67) N-Nitrosodiphenylamine	15.775	169	980510	41.537	ng/ul	98
68) 4-Bromophenyl-phenylether	16.457	248	318323	39.108	ng/ul	99
69) Hexachlorobenzene	16.569	284	360347	38.903	ng/ul	99
70) Atrazine	16.734	200	317458	37.271	ng/ul	98
71) Pentachlorophenol	16.916	266	220817	36.246	ng/ul	98
72) Phenanthrene	17.310	178	1854691	42.174	ng/ul	100
74) Anthracene	17.404	178	1885660	42.616	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.304	216	472644	42.792	ng/ul	100
76) Pentachlorobenzene	14.828	250	472498	40.034	ng/ul	99
77) Carbazole	17.681	167	1762785	44.093	ng/ul	99
78) Di-n-butylphthalate	18.222	149	1970928	40.257	ng/ul	98
80) Fluoranthene	19.281	202	2152102	41.624	ng/ul	99
82) Pyrene	19.633	202	2280589	42.364	ng/ul	99
83) Butylbenzylphthalate	20.504	149	917152	39.420	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.280	252	784281	40.838	ng/ul	99
85) Benzo(a)anthracene	21.345	228	2278375	41.764	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.263	149	1332710	38.027	ng/ul	99
87) Chrysene	21.398	228	2148409	41.964	ng/ul	100
89) Di-n-octyl phthalate	22.192	149	2324516	41.775	ng/ul	100
90) Benzo(b)fluoranthene	23.039	252	2362798	42.445	ng/ul	99
91) Benzo(k)fluoranthene	23.092	252	2326799	43.406	ng/ul	100
93) Benzo(a)pyrene	23.674	252	2128708	42.850	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.310	276	2650261	41.913	ng/ul	99
95) Dibenzo(a,h)anthracene	26.321	278	2373799	42.260	ng/ul	99
96) Benzo(g,h,i)perylene	27.080	276	2358058	42.064	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101022\
 Data File : BP012028.D
 Acq On : 10 Oct 2022 17:49
 Operator : CG/JU
 Sample : SSTD04065
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD040627

Quant Time: Oct 11 00:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 00:41:15 2022
 Response via : Initial Calibration




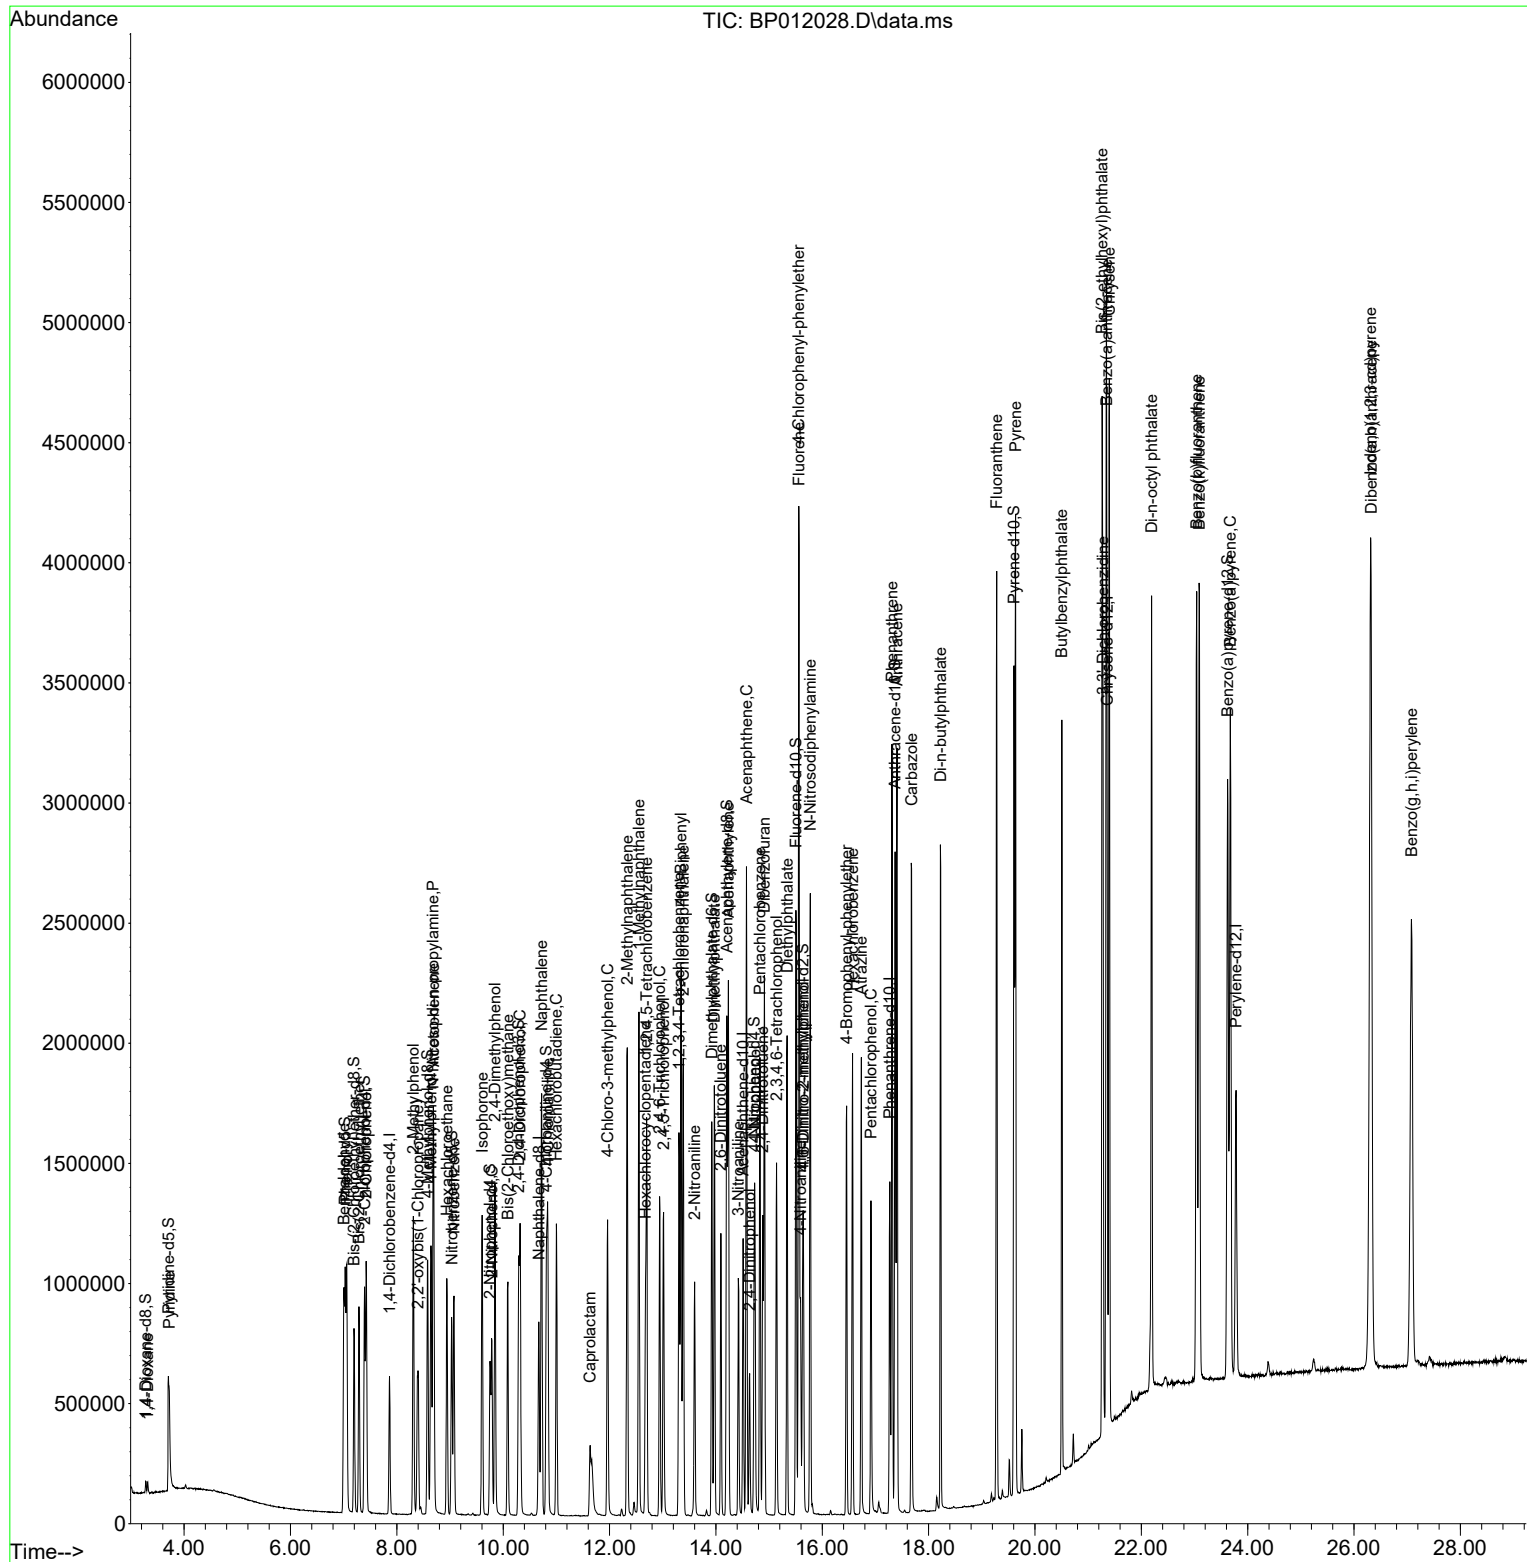


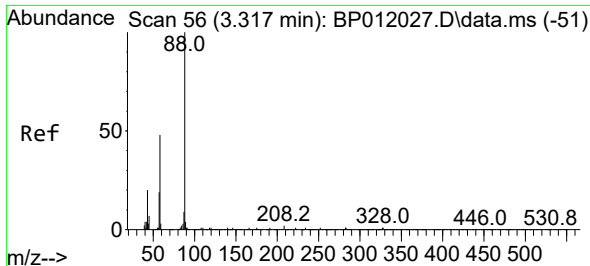

#2
1,4-Dioxane
Concen: 7.005 ng/uL
RT: 3.311 min Scan# 51
Delta R.T. -0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion: 88 Resp: 28017
Ion Ratio Lower Upper
88 100
43 18.0 17.2 25.8
58 49.9 37.4 56.0

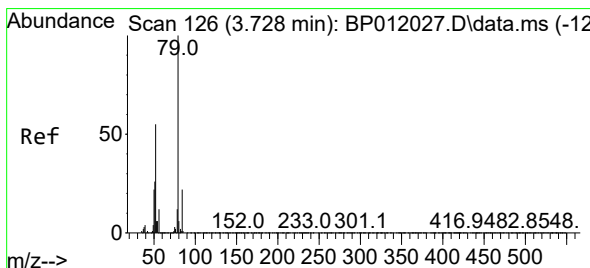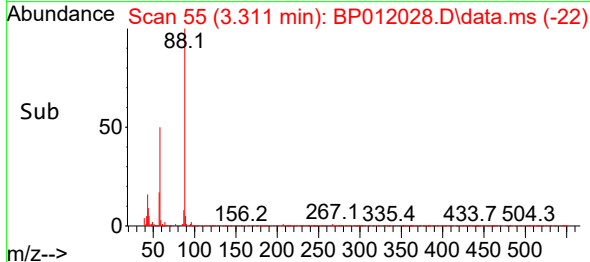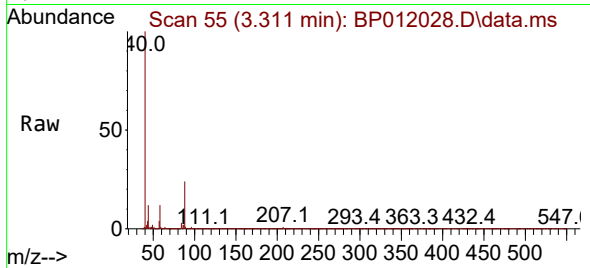

#5
Pyridine
Concen: 22.625 ng/uL
RT: 3.723 min Scan# 125
Delta R.T. -0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion: 79 Resp: 238180
Ion Ratio Lower Upper
79 100
52 54.7 44.2 66.4
51 28.0 22.9 34.3


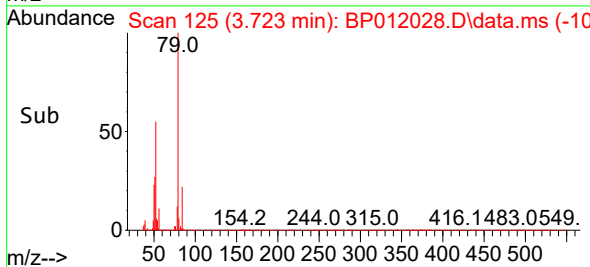

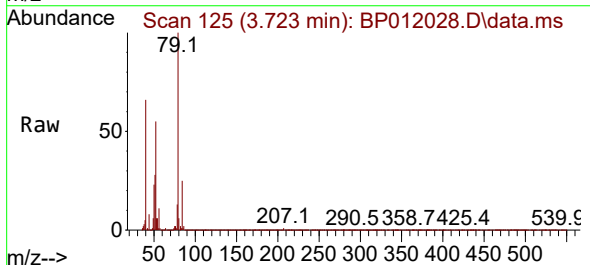




#6
Benzaldehyde
Concen: 50.569 ng/ul
RT: 7.005 min Scan# 683
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion: 77 Resp: 312319
Ion Ratio Lower Upper
77 100
105 101.4 79.8 119.8
106 97.5 77.6 116.4

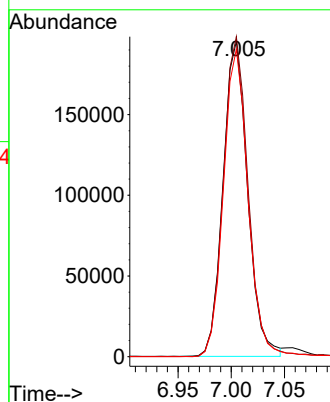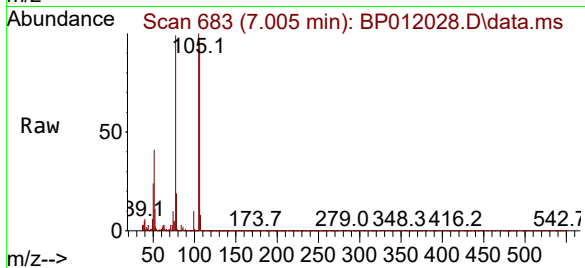

#8
Phenol
Concen: 41.815 ng/ul
RT: 7.058 min Scan# 692
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion: 94 Resp: 611471
Ion Ratio Lower Upper
94 100
65 26.4 20.8 31.2
66 33.3 27.4 41.0




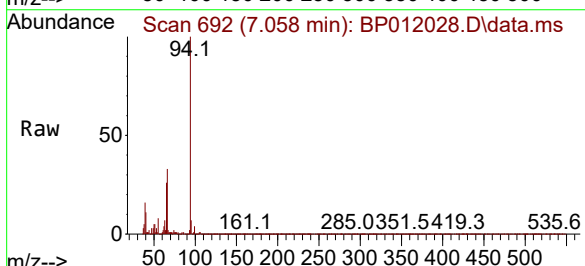




#10
Bis(2-Chloroethyl)ether
Concen: 41.121 ng/ul
RT: 7.287 min Scan# 731
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion: 93 Resp: 478483
Ion Ratio Lower Upper
93 100
63 76.6 61.5 92.3
95 32.7 26.6 40.0



#12
2-Chlorophenol
Concen: 41.376 ng/ul
RT: 7.422 min Scan# 754
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:128 Resp: 492313
Ion Ratio Lower Upper
128 100
64 44.7 34.9 52.3
130 31.8 26.1 39.1



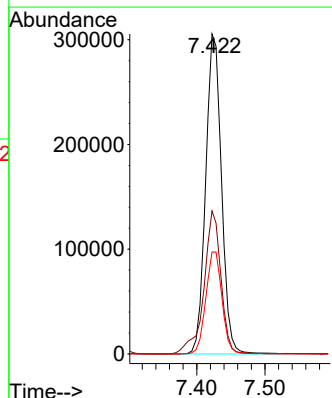





#13
2-Methylphenol
Concen: 38.772 ng/ul
RT: 8.310 min Scan# 905
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:108 Resp: 446698
Ion Ratio Lower Upper
108 100
107 90.5 72.4 108.6

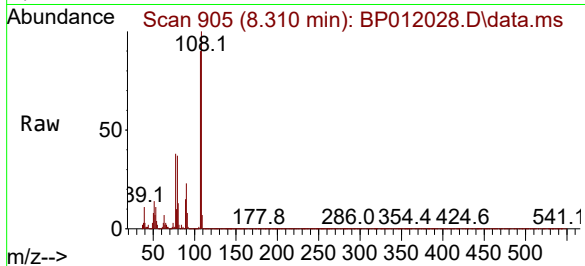

#14
2,2'-oxybis(1-Chloropropane)
Concen: 48.925 ng/ul
RT: 8.399 min Scan# 920
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion: 45 Resp: 561218
Ion Ratio Lower Upper
45 100
77 16.4 13.4 20.0
79 13.0 9.9 14.9




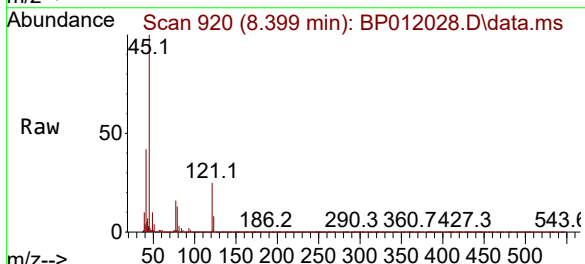




#16
Acetophenone
Concen: 39.247 ng/ul
RT: 8.693 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:105 Resp: 697393
Ion Ratio Lower Upper
105 100
77 74.4 59.2 88.8
51 23.1 19.8 29.6



#17
N-Nitroso-di-n-propylamine
Concen: 38.229 ng/ul
RT: 8.681 min Scan# 968
Delta R.T. 0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion: 70 Resp: 319729
Ion Ratio Lower Upper
70 100
42 48.9 39.9 59.9
101 10.0 7.0 10.6
130 22.3 16.8 25.2



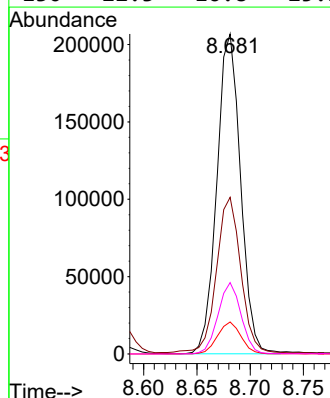





#18
4-Methylphenol
Concen: 38.087 ng/ul
RT: 8.640 min Scan# 961
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:108 Resp: 483479
Ion Ratio Lower Upper
108 100
107 113.0 90.1 135.1



#19
Hexachloroethane
Concen: 45.045 ng/ul
RT: 8.940 min Scan# 1012
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:117 Resp: 199901
Ion Ratio Lower Upper
117 100
201 92.1 74.2 111.4
199 58.3 46.3 69.5



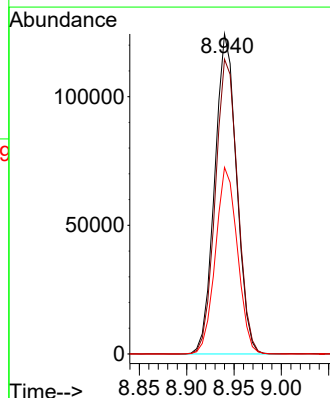





#22
Nitrobenzene
Concen: 46.829 ng/ul
RT: 9.075 min Scan# 1035
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion: 77 Resp: 524790
Ion Ratio Lower Upper
77 100
123 48.0 36.6 54.8
65 12.5 9.6 14.4

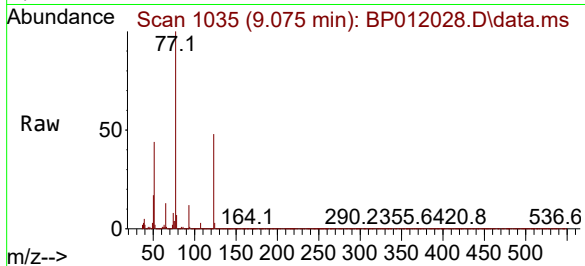

#23
Isophorone
Concen: 41.315 ng/ul
RT: 9.605 min Scan# 1125
Delta R.T. 0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion: 82 Resp: 939222
Ion Ratio Lower Upper
82 100
95 6.6 5.2 7.8
138 18.3 14.4 21.6




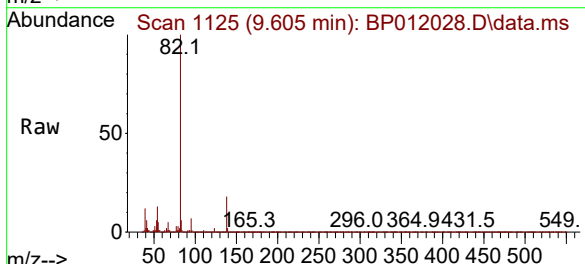




#25
2-Nitrophenol
Concen: 40.851 ng/ul
RT: 9.787 min Scan# 1156
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:139 Resp: 260105
Ion Ratio Lower Upper
139 100
65 45.6 37.7 56.5
109 26.3 21.2 31.8



#26
2,4-Dimethylphenol
Concen: 41.199 ng/ul
RT: 9.846 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:107 Resp: 492779
Ion Ratio Lower Upper
107 100
121 51.9 41.1 61.7
122 89.1 71.1 106.7









#27
 Bis(2-Chloroethoxy)methane
 Concen: 40.450 ng/ul
 RT: 10.087 min Scan# 1207
 Delta R.T. 0.000 min
 Lab File: BP012028.D
 Acq: 10 Oct 2022 17:49




Instrument :
 BNA_P
 ClientSampleId :
 SSTD040627


Tgt Ion: 93 Resp: 593279
 Ion Ratio Lower Upper
 93 100
 95 32.6 26.2 39.2
 123 11.2 9.2 13.8



#29
 2,4-Dichlorophenol
 Concen: 39.793 ng/ul
 RT: 10.316 min Scan# 1246
 Delta R.T. 0.000 min
 Lab File: BP012028.D
 Acq: 10 Oct 2022 17:49

Tgt Ion: 162 Resp: 425166
 Ion Ratio Lower Upper
 162 100
 164 65.3 52.5 78.7
 98 35.5 27.9 41.9









#30
Naphthalene
Concen: 41.231 ng/ul
RT: 10.722 min Scan# 1315
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:128 Resp: 1514979
Ion Ratio Lower Upper
128 100
129 11.1 8.8 13.2
127 13.2 10.1 15.1

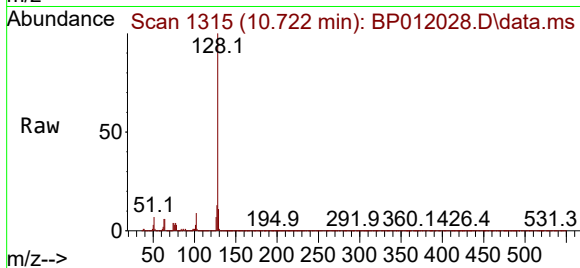

#32
4-Chloroaniline
Concen: 38.943 ng/ul
RT: 10.840 min Scan# 1335
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:127 Resp: 626300
Ion Ratio Lower Upper
127 100
129 32.0 25.8 38.8

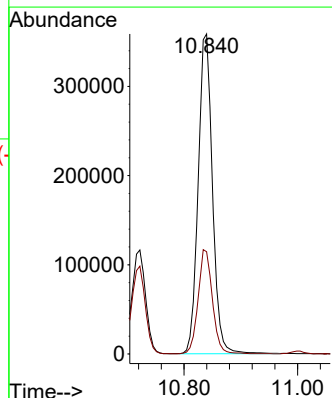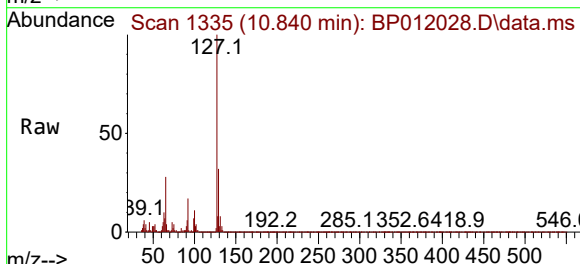



#33

Hexachlorobutadiene

Concen: 39.578 ng/ul

RT: 10.999 min Scan# 1

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:225 Resp: 250299

Ion Ratio Lower Upper

225 100

223 61.0 49.8 74.8

227 62.9 51.0 76.4

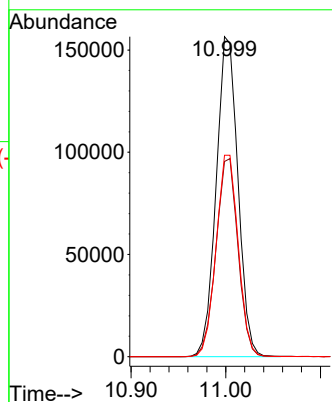

#34

Caprolactam

Concen: 17.155 ng/ul

RT: 11.634 min Scan# 1470

Delta R.T. -0.006 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:113 Resp: 64871


Ion Ratio Lower Upper

113 100

55 159.3 132.9 199.3

56 122.2 97.7 146.5







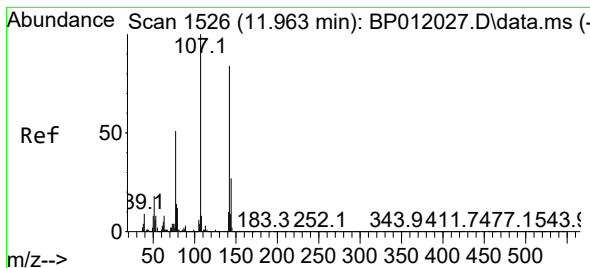

#35
4-Chloro-3-methylphenol
Concen: 39.090 ng/ul
RT: 11.963 min Scan# 1526
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:107 Resp: 442832
Ion Ratio Lower Upper
107 100
144 26.8 21.8 32.6
142 82.2 67.1 100.7

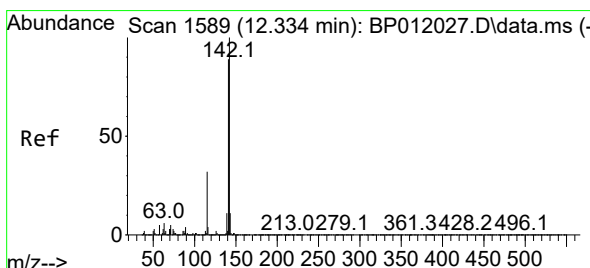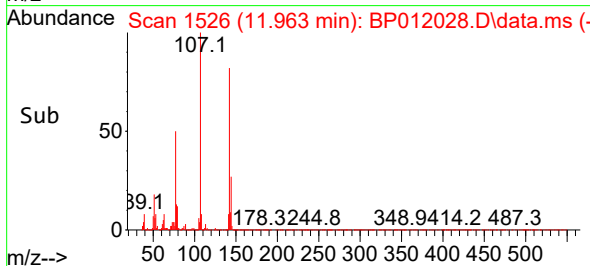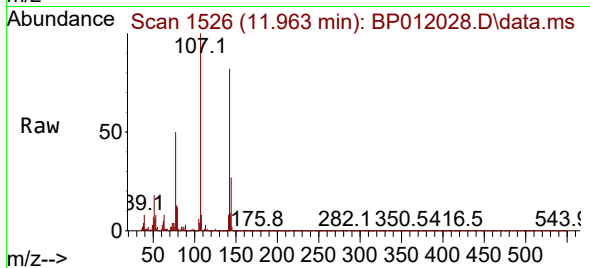

#36
2-Methylnaphthalene
Concen: 38.266 ng/ul
RT: 12.334 min Scan# 1589
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:142 Resp: 981911
Ion Ratio Lower Upper
142 100
141 89.5 71.4 107.0


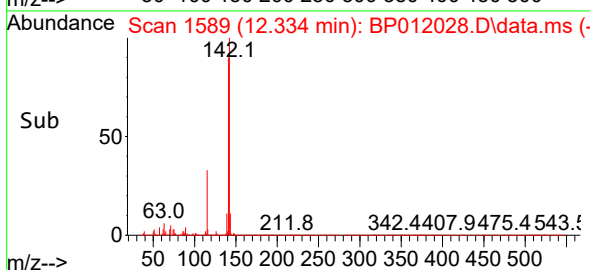

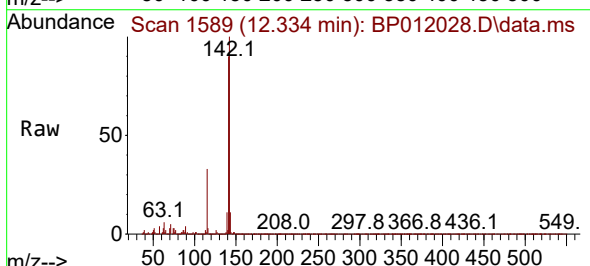




#37
1-Methylnaphthalene
Concen: 38.445 ng/ul
RT: 12.551 min Scan# 1626
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:142 Resp: 989861
Ion Ratio Lower Upper
142 100
141 91.6 74.3 111.5
116 3.6 2.8 4.2



#39
1,2,4,5-Tetrachlorobenzene
Concen: 41.184 ng/ul
RT: 12.698 min Scan# 1651
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:216 Resp: 470745
Ion Ratio Lower Upper
216 100
214 79.7 63.8 95.6
179 20.8 17.3 25.9
108 18.8 15.2 22.8









#40
Hexachlorocyclopentadiene
Concen: 33.594 ng/ul
RT: 12.675 min Scan# 1647
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:237 Resp: 219366
Ion Ratio Lower Upper
237 100
235 64.0 52.4 78.6
272 12.5 10.6 16.0



#41
2,4,6-Trichlorophenol
Concen: 40.844 ng/ul
RT: 12.940 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:196 Resp: 312513
Ion Ratio Lower Upper
196 100
198 96.0 75.2 112.8
200 30.0 23.4 35.2





#42

2,4,5-Trichlorophenol

Concen: 40.274 ng/ul

RT: 13.016 min Scan# 1705

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:196 Resp: 335665

Ion Ratio Lower Upper

196 100

198 95.9 76.5 114.7

200 29.8 25.3 37.9



#43

1,1'-Biphenyl

Concen: 42.133 ng/ul

RT: 13.346 min Scan# 1761

Delta R.T. 0.006 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:154 Resp: 1228291


Ion Ratio Lower Upper

154 100

153 40.2 31.8 47.8

76 13.0 10.9 16.3









#44
2-Chloronaphthalene
Concen: 42.659 ng/ul
RT: 13.387 min Scan# 1768
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:162 Resp: 983224
Ion Ratio Lower Upper
162 100
164 33.1 26.1 39.1
127 38.9 30.2 45.2

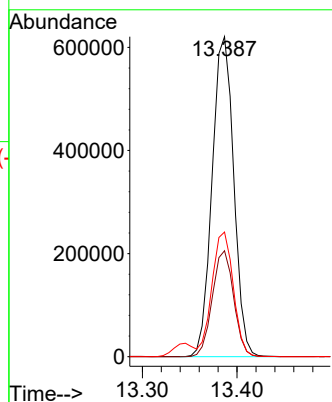

#45
2-Nitroaniline
Concen: 45.566 ng/ul
RT: 13.598 min Scan# 1804
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion: 65 Resp: 256366
Ion Ratio Lower Upper
65 100
92 72.6 57.3 85.9
138 114.8 88.8 133.2









#47
Dimethylphthalate
Concen: 39.547 ng/ul
RT: 13.969 min Scan# 1867
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:163 Resp: 1168167
Ion Ratio Lower Upper
163 100
194 3.8 3.1 4.7
164 10.4 8.0 12.0

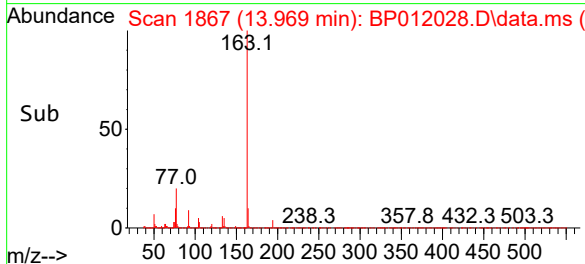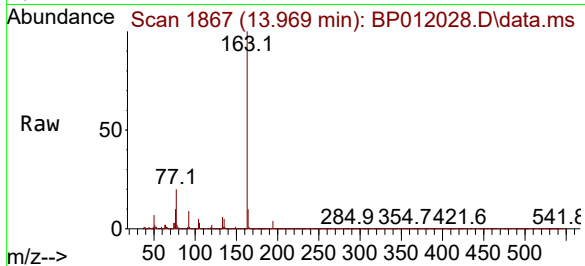

#48
2,6-Dinitrotoluene
Concen: 38.581 ng/ul
RT: 14.093 min Scan# 1888
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:165 Resp: 222098
Ion Ratio Lower Upper
165 100
89 58.1 48.2 72.2
121 23.7 19.3 28.9

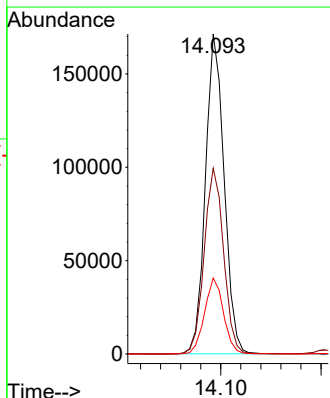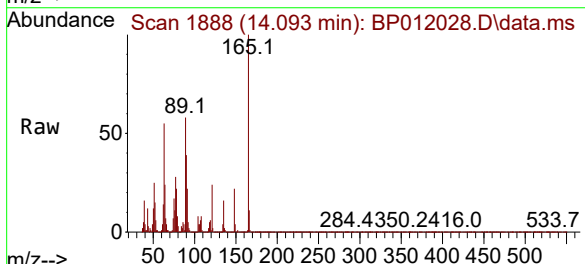



#50

Acenaphthylene

Concen: 42.842 ng/ul

RT: 14.234 min Scan# 1912

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:152 Resp: 1528870

Ion Ratio Lower Upper

152 100

151 20.1 15.8 23.6

153 13.2 10.5 15.7

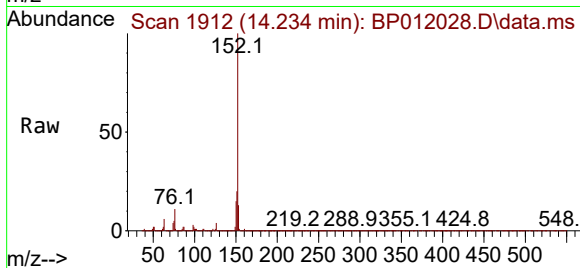

#51

3-Nitroaniline

Concen: 38.060 ng/ul

RT: 14.422 min Scan# 1944

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:138 Resp: 253951


Ion Ratio Lower Upper

138 100

108 10.7 10.2 15.4

92 113.3 96.6 144.8

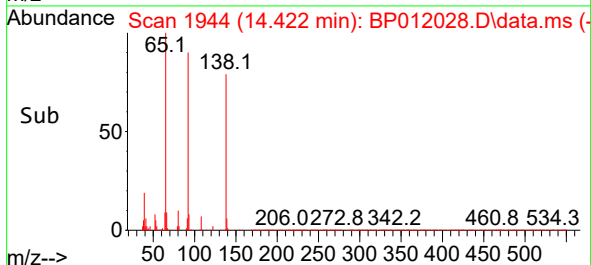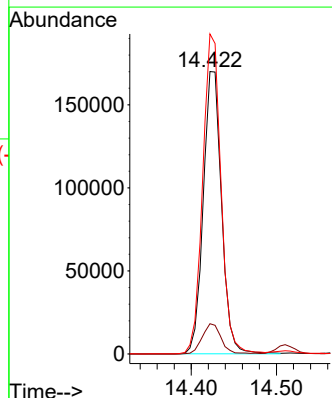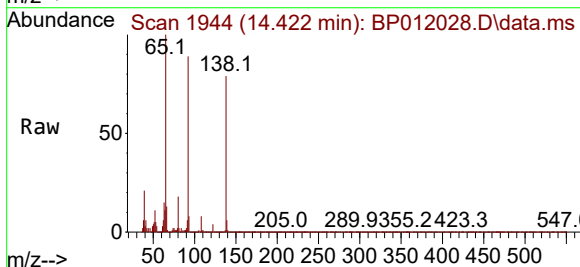



#52

Acenaphthene

Concen: 42.232 ng/ul

RT: 14.575 min Scan# 1970

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:153 Resp: 1063286

Ion Ratio Lower Upper

153 100

152 48.4 39.2 58.8

154 87.4 70.4 105.6



#53

2,4-Dinitrophenol

Concen: 33.473 ng/ul

RT: 14.634 min Scan# 1980

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:184 Resp: 130642


Ion Ratio Lower Upper

184 100

63 61.3 52.0 78.0

154 58.8 46.6 70.0









#55
4-Nitrophenol
Concen: 44.305 ng/ul
RT: 14.734 min Scan# 1997
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:109 Resp: 174564
Ion Ratio Lower Upper
109 100
139 146.2 124.5 186.7
65 135.2 107.8 161.6



#56
Dibenzofuran
Concen: 41.103 ng/ul
RT: 14.910 min Scan# 2027
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:168 Resp: 1417408
Ion Ratio Lower Upper
168 100
139 38.4 30.0 45.0









#57
2,4-Dinitrotoluene
Concen: 41.039 ng/ul
RT: 14.881 min Scan# 2022
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:165 Resp: 345325
Ion Ratio Lower Upper
165 100
63 42.9 32.9 49.3
182 2.5 2.1 3.1

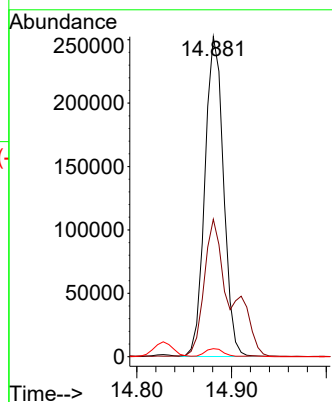

#58
2,3,4,6-Tetrachlorophenol
Concen: 38.177 ng/ul
RT: 15.140 min Scan# 2066
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:232 Resp: 276419
Ion Ratio Lower Upper
232 100
131 50.0 39.3 58.9
130 2.7 1.8 2.8
166 33.0 25.7 38.5


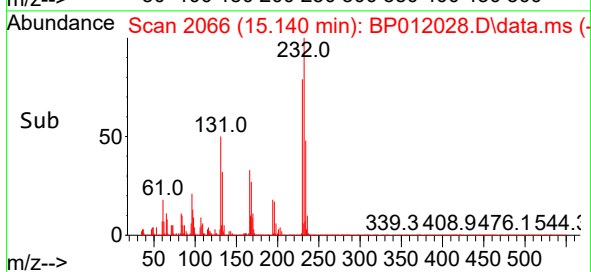






#59
Diethylphthalate
Concen: 39.509 ng/ul
RT: 15.340 min Scan# 2100
Delta R.T. 0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:149 Resp: 1169166
Ion Ratio Lower Upper
149 100
177 21.8 16.8 25.2
150 12.1 10.0 15.0

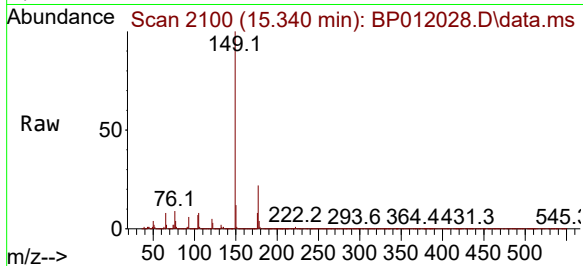

#61
Fluorene
Concen: 40.888 ng/ul
RT: 15.563 min Scan# 2138
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:166 Resp: 1154854
Ion Ratio Lower Upper
166 100
165 97.4 79.3 118.9
167 13.6 10.7 16.1




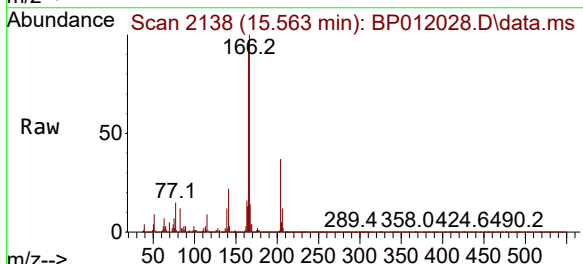




#62
4-Chlorophenyl-phenylether
Concen: 38.464 ng/ul
RT: 15.557 min Scan# 2137
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:204 Resp: 537815
Ion Ratio Lower Upper
204 100
206 32.8 25.9 38.9
141 59.8 47.9 71.9

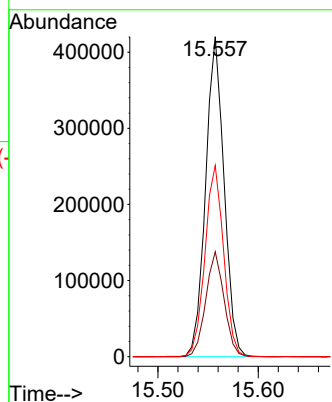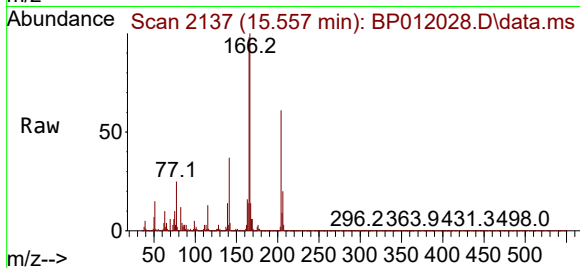

#63
4-Nitroaniline
Concen: 38.968 ng/ul
RT: 15.592 min Scan# 2143
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:138 Resp: 248112
Ion Ratio Lower Upper
138 100
92 51.0 40.8 61.2
108 72.2 59.5 89.3




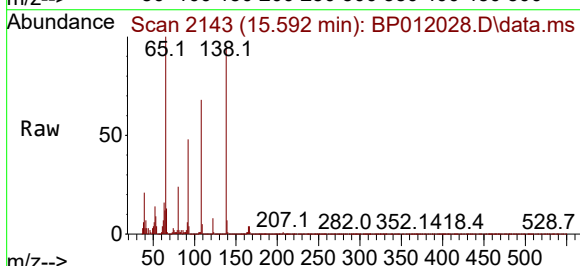




#66
4,6-Dinitro-2-methylphenol
Concen: 39.167 ng/ul
RT: 15.645 min Scan# 2152
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:198 Resp: 200971
Ion Ratio Lower Upper
198 100
182 5.2 5.6 8.4#
77 25.6 20.3 30.5

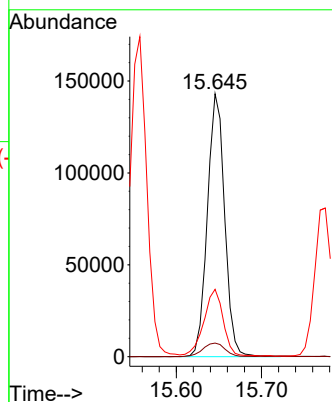

#67
N-Nitrosodiphenylamine
Concen: 41.537 ng/ul
RT: 15.775 min Scan# 2174
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:169 Resp: 980510
Ion Ratio Lower Upper
169 100
168 67.2 52.2 78.2
167 37.5 30.1 45.1









#68
4-Bromophenyl-phenylether
Concen: 39.108 ng/ul
RT: 16.457 min Scan# 2290
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:248 Resp: 318323
Ion Ratio Lower Upper
248 100
250 93.7 75.1 112.7
141 72.7 58.8 88.2



#69
Hexachlorobenzene
Concen: 38.903 ng/ul
RT: 16.569 min Scan# 2309
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:284 Resp: 360347
Ion Ratio Lower Upper
284 100
142 40.1 32.1 48.1
249 31.9 26.0 39.0





#70

Atrazine

Concen: 37.271 ng/ul

RT: 16.734 min Scan# 21

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:200 Resp: 317458

Ion Ratio Lower Upper

200 100

173 26.6 20.9 31.3

215 47.4 37.0 55.4

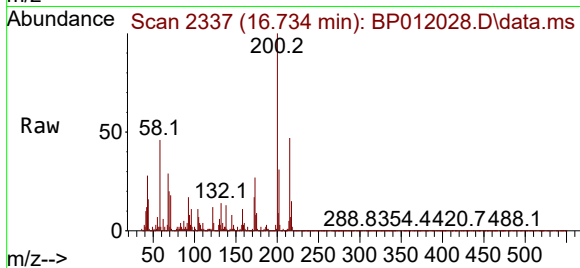

#71

Pentachlorophenol

Concen: 36.246 ng/ul

RT: 16.916 min Scan# 2368

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:266 Resp: 220817


Ion Ratio Lower Upper

266 100

264 63.7 49.7 74.5

268 63.4 49.7 74.5


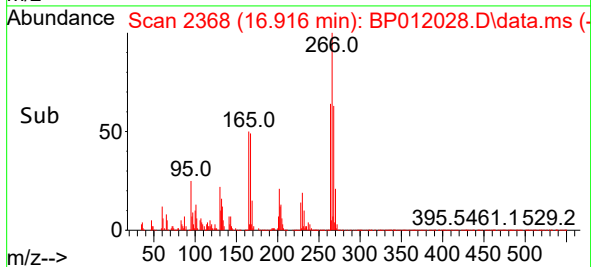

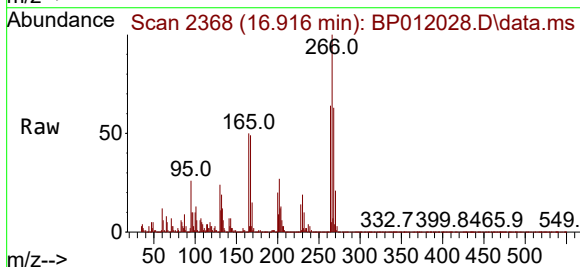


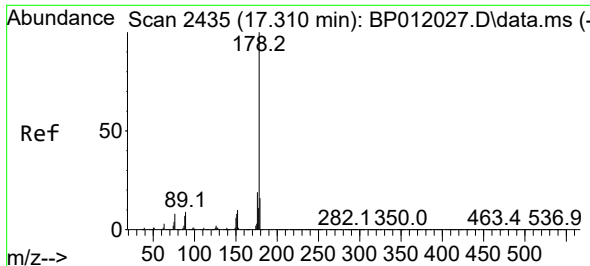

#72
Phenanthrene
Concen: 42.174 ng/ul
RT: 17.310 min Scan# 2435
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:178 Resp: 1854691
Ion Ratio Lower Upper
178 100
179 15.5 12.5 18.7
176 19.6 15.5 23.3

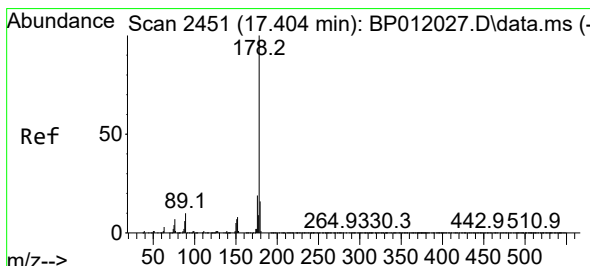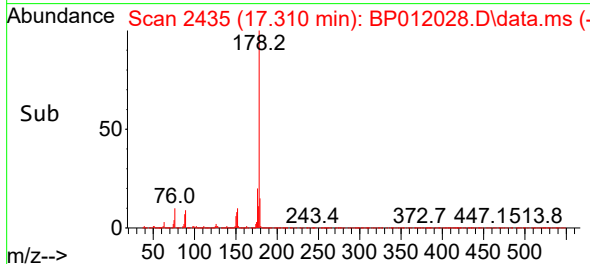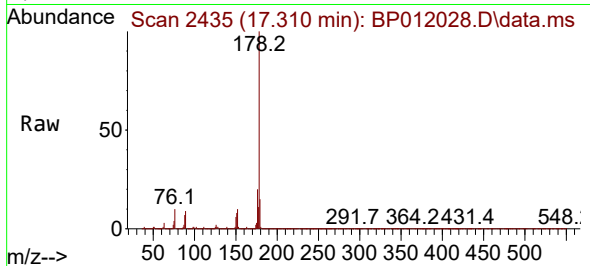

#74
Anthracene
Concen: 42.616 ng/ul
RT: 17.404 min Scan# 2451
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:178 Resp: 1885660
Ion Ratio Lower Upper
178 100
179 15.4 12.5 18.7
176 18.9 15.2 22.8


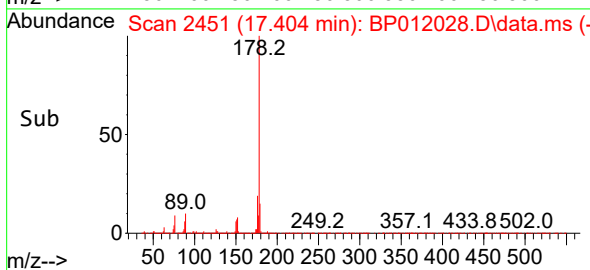

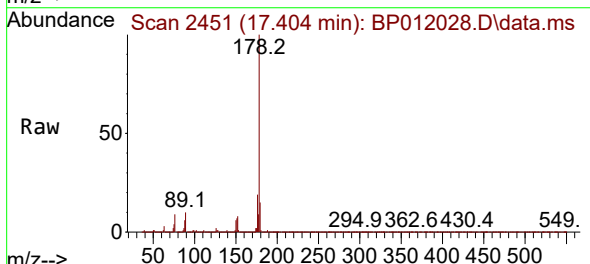




#75
1,2,3,4-Tetrachlorobenzene
Concen: 42.792 ng/uL
RT: 13.304 min Scan# 1754
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:216 Resp: 472644
Ion Ratio Lower Upper
216 100
214 80.1 64.0 96.0
218 47.7 38.2 57.2

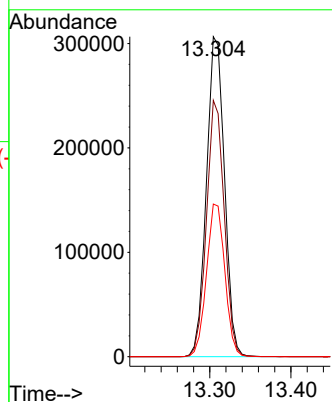

#76
Pentachlorobenzene
Concen: 40.034 ng/uL
RT: 14.828 min Scan# 2013
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:250 Resp: 472498
Ion Ratio Lower Upper
250 100
248 64.2 50.9 76.3
252 64.1 51.5 77.3







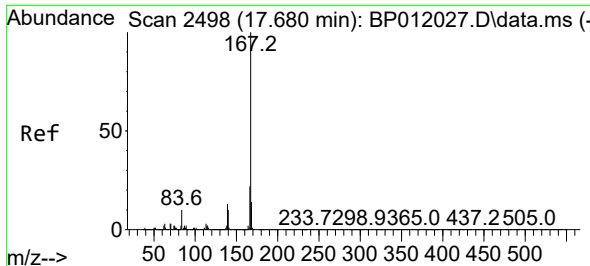

#77
 Carbazole
 Concen: 44.093 ng/ul
 RT: 17.681 min Scan# 2498
 Delta R.T. 0.000 min
 Lab File: BP012028.D
 Acq: 10 Oct 2022 17:49




Instrument :
 BNA_P
 ClientSampleId :
 SSTD040627


Tgt Ion:167 Resp: 1762785
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.2 25.8
 139 12.7 10.7 16.1

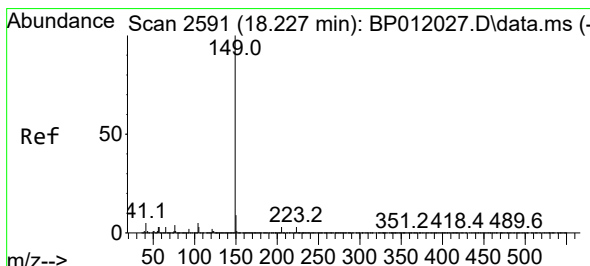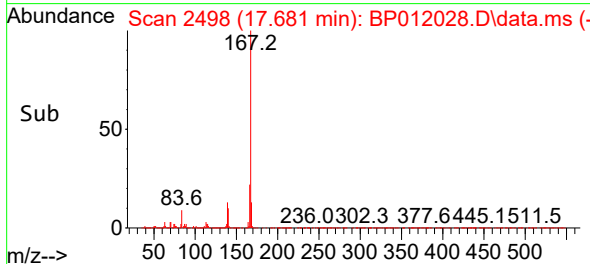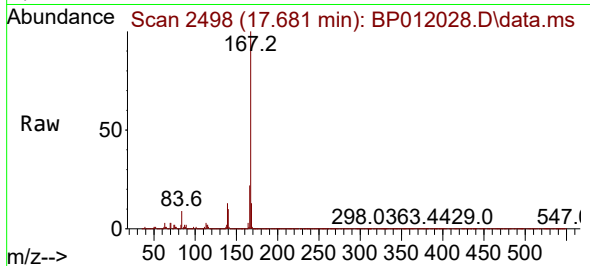

#78
 Di-n-butylphthalate
 Concen: 40.257 ng/ul
 RT: 18.222 min Scan# 2590
 Delta R.T. -0.006 min
 Lab File: BP012028.D
 Acq: 10 Oct 2022 17:49

Tgt Ion:149 Resp: 1970928
 Ion Ratio Lower Upper
 149 100
 150 9.5 7.0 10.6
 104 5.1 3.7 5.5


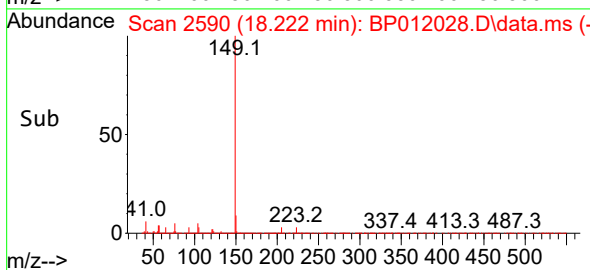

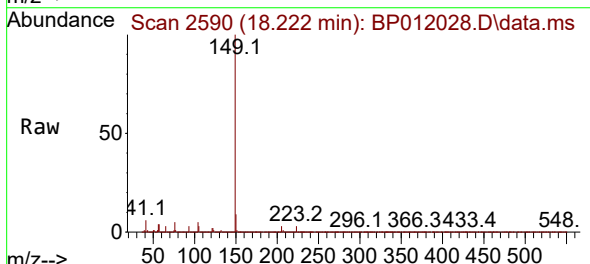




#80
Fluoranthene
Concen: 41.624 ng/ul
RT: 19.281 min Scan# 21
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:202 Resp: 2152102
Ion Ratio Lower Upper
202 100
101 12.3 10.2 15.2
100 9.1 7.7 11.5



#82
Pyrene
Concen: 42.364 ng/ul
RT: 19.633 min Scan# 2830
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:202 Resp: 2280589
Ion Ratio Lower Upper
202 100
101 14.7 11.6 17.4
100 12.1 9.8 14.8





#83

Butylbenzylphthalate

Concen: 39.420 ng/ul

RT: 20.504 min Scan# 2978

Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:149 Resp: 917152

Ion Ratio Lower Upper

149 100

91 70.0 56.6 84.8

206 19.2 15.0 22.6

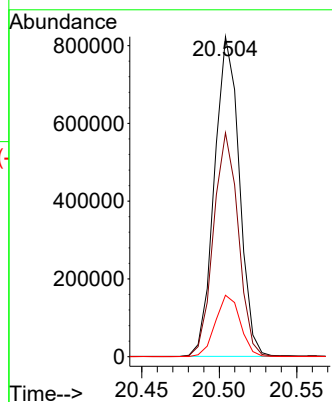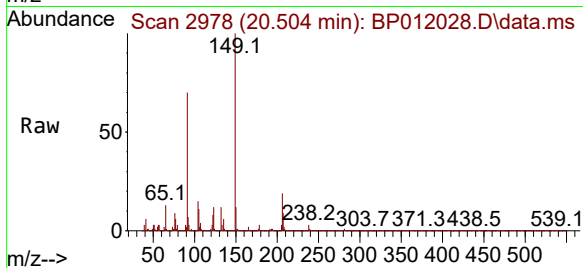

#84

3,3'-Dichlorobenzidine

Concen: 40.838 ng/ul

RT: 21.280 min Scan# 3110

Delta R.T. 0.006 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:252 Resp: 784281


Ion Ratio Lower Upper

252 100

254 63.6 50.5 75.7

126 11.8 11.0 16.4




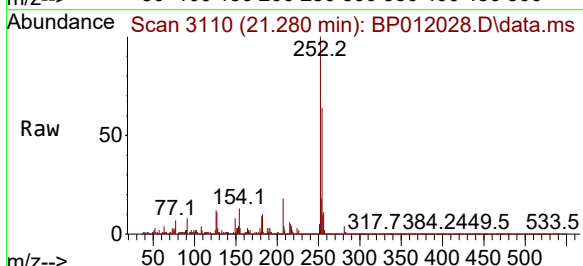




#85
Benzo(a)anthracene
Concen: 41.764 ng/ul
RT: 21.345 min Scan# 3121
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:228 Resp: 2278375
Ion Ratio Lower Upper
228 100
229 20.0 15.5 23.3
226 28.1 21.8 32.6



#86
Bis(2-ethylhexyl)phthalate
Concen: 38.027 ng/ul
RT: 21.263 min Scan# 3107
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:149 Resp: 1332710
Ion Ratio Lower Upper
149 100
167 26.8 21.0 31.6
279 3.7 2.9 4.3





#87

Chrysene

Concen: 41.964 ng/ul

RT: 21.398 min Scan# 31

Delta R.T. 0.006 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:228 Resp: 2148409

Ion Ratio Lower Upper

228 100

226 30.4 24.1 36.1

229 19.7 15.8 23.6



#89

Di-n-octyl phthalate

Concen: 41.775 ng/ul




RT: 22.192 min Scan# 3265


Delta R.T. 0.000 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Tgt Ion:149 Resp: 2324516









#90
Benzo(b)fluoranthene
Concen: 42.445 ng/ul
RT: 23.039 min Scan# 3409
Delta R.T. 0.000 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49




Instrument :
BNA_P
ClientSampleId :
SSTD040627


Tgt Ion:252 Resp: 2362798
Ion Ratio Lower Upper
252 100
253 22.5 17.8 26.8
125 12.2 9.9 14.9

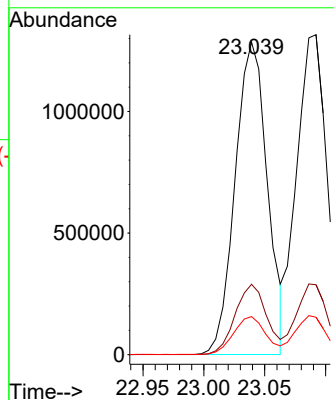

#91
Benzo(k)fluoranthene
Concen: 43.406 ng/ul
RT: 23.092 min Scan# 3418
Delta R.T. 0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:252 Resp: 2326799
Ion Ratio Lower Upper
252 100
253 21.8 17.4 26.0
125 11.7 9.4 14.2

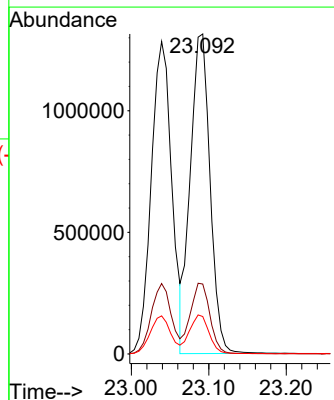



#93

Benzo(a)pyrene

Concen: 42.850 ng/ul

RT: 23.674 min Scan# 3

Delta R.T. 0.006 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49

Instrument :

BNA_P

ClientSampleId :

SSTD040627





Tgt Ion:252 Resp: 2128708

Ion Ratio Lower Upper

252 100

253 22.3 17.3 25.9

125 12.9 10.8 16.2

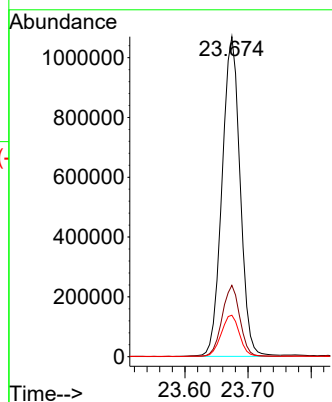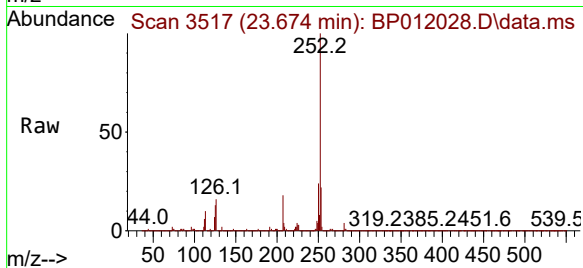

#94

Indeno(1,2,3-cd)pyrene

Concen: 41.913 ng/ul

RT: 26.310 min Scan# 3965

Delta R.T. 0.006 min

Lab File: BP012028.D

Acq: 10 Oct 2022 17:49




Tgt Ion:276 Resp: 2650261


Ion Ratio Lower Upper

276 100

138 30.5 24.1 36.1

277 25.8 20.0 30.0




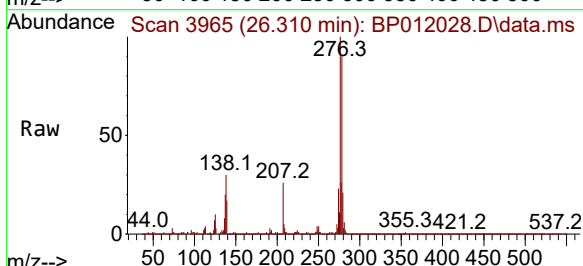




#95
Dibenzo(a,h)anthracene
Concen: 42.260 ng/ul
RT: 26.321 min Scan# 3966
Delta R.T. 0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Instrument :
BNA_P
ClientSampleId :
SSTD040627

Tgt Ion:278 Resp: 2373799
Ion Ratio Lower Upper
278 100
139 19.3 15.4 23.0
279 23.8 19.6 29.4



#96
Benzo(g,h,i)perylene
Concen: 42.064 ng/ul
RT: 27.080 min Scan# 4096
Delta R.T. 0.006 min
Lab File: BP012028.D
Acq: 10 Oct 2022 17:49

Tgt Ion:276 Resp: 2358058
Ion Ratio Lower Upper
276 100
138 26.0 20.9 31.3
277 24.0 19.0 28.4

