

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101022\
 Data File : BP012031.D
 Acq On : 10 Oct 2022 20:08
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV630

Quant Time: Oct 11 01:49:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 01:38:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.858	152	196224	20.000	ng/u1	0.00
20) Naphthalene-d8	10.669	136	834155	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.510	164	454844	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.269	188	857915	20.000	ng/u1	0.00
79) Chrysene-d12	21.357	240	882358	20.000	ng/u1	0.00
88) Perylene-d12	23.774	264	949927	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	13044	6.278	ng/uL	0.00
4) Pyridine-d5	3.705	84	115350	17.094	ng/u1	0.00
7) Phenol-d5	7.028	99	326289	19.561	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.193	67	197968	20.077	ng/u1	0.00
11) 2-Chlorophenol-d4	7.393	132	255374	19.947	ng/u1	0.00
15) 4-Methylphenol-d8	8.575	113	244895	19.529	ng/u1	0.00
21) Nitrobenzene-d5	9.028	128	119414	19.757	ng/u1	0.00
24) 2-Nitrophenol-d4	9.752	143	119209	19.448	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.287	165	230006	19.947	ng/u1	0.00
31) 4-Chloroaniline-d4	10.810	131	331053	18.521	ng/u1	0.00
46) Dimethylphthalate-d6	13.922	166	572034	18.958	ng/u1	0.00
49) Acenaphthylene-d8	14.198	160	741817	20.047	ng/u1	0.00
54) 4-Nitrophenol-d4	14.716	143	107664	16.617	ng/u1	0.00
60) Fluorene-d10	15.504	176	516517	19.024	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.628	200	80319	17.280	ng/u1	0.00
73) Anthracene-d10	17.363	188	761022	19.581	ng/u1	0.00
81) Pyrene-d10	19.598	212	842788	19.435	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.616	264	907024	19.348	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.317	88	12995	6.003	ng/uL	97
5) Pyridine	3.723	79	108067	15.960	ng/u1	99
6) Benzaldehyde	7.005	77	187427	24.237	ng/u1	98
8) Phenol	7.052	94	343691	19.567	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.287	93	276135	20.111	ng/u1	99
12) 2-Chlorophenol	7.422	128	279776	20.139	ng/u1	99
13) 2-Methylphenol	8.311	108	253022	19.733	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.393	45	328466	20.428	ng/u1	98
16) Acetophenone	8.693	105	404888	20.252	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.675	70	179714	20.381	ng/u1	99
18) 4-Methylphenol	8.640	108	272476	19.666	ng/u1	98
19) Hexachloroethane	8.940	117	114066	19.870	ng/u1	97
22) Nitrobenzene	9.069	77	299750	20.083	ng/u1	99
23) Isophorone	9.599	82	524211	19.595	ng/u1	99
25) 2-Nitrophenol	9.781	139	144253	20.201	ng/u1	98
26) 2,4-Dimethylphenol	9.846	107	280205	19.785	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.081	93	337909	19.766	ng/u1	99
29) 2,4-Dichlorophenol	10.316	162	239419	19.851	ng/u1	99
30) Naphthalene	10.716	128	888598	19.736	ng/u1	100
32) 4-Chloroaniline	10.834	127	348970	18.788	ng/u1	99
33) Hexachlorobutadiene	10.999	225	141822	19.371	ng/u1	96
34) Caprolactam	11.634	113	72343	18.324	ng/u1	98
35) 4-Chloro-3-methylphenol	11.957	107	236983	19.170	ng/u1	100
36) 2-Methylnaphthalene	12.328	142	563267	19.627	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101022\
 Data File : BP012031.D
 Acq On : 10 Oct 2022 20:08
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV630

Quant Time: Oct 11 01:49:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 01:38:55 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.546	142	558968	19.372	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.699	216	265263	20.214	ng/ul	98
40) Hexachlorocyclopentadiene	12.675	237	129633	21.314	ng/ul	97
41) 2,4,6-Trichlorophenol	12.940	196	167258	20.203	ng/ul	97
42) 2,4,5-Trichlorophenol	13.010	196	177460	20.124	ng/ul	97
43) 1,1'-Biphenyl	13.340	154	696571	20.313	ng/ul	100
44) 2-Chloronaphthalene	13.381	162	554089	20.144	ng/ul	98
45) 2-Nitroaniline	13.593	65	114596	18.280	ng/ul	97
47) Dimethylphthalate	13.969	163	603550	18.805	ng/ul	99
48) 2,6-Dinitrotoluene	14.093	165	99129	18.604	ng/ul	96
50) Acenaphthylene	14.228	152	844870	20.182	ng/ul	100
51) 3-Nitroaniline	14.422	138	116038	17.644	ng/ul	98
52) Acenaphthene	14.575	153	581526	19.640	ng/ul	100
53) 2,4-Dinitrophenol	14.628	184	64645	17.305	ng/ul	94
55) 4-Nitrophenol	14.728	109	83160	17.010	ng/ul	95
56) Dibenzofuran	14.910	168	770051	19.293	ng/ul	99
57) 2,4-Dinitrotoluene	14.881	165	157648	18.418	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.134	232	138564	18.777	ng/ul	96
59) Diethylphthalate	15.334	149	573818	18.282	ng/ul	99
61) Fluorene	15.557	166	624239	19.281	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.551	204	286075	19.186	ng/ul	99
63) 4-Nitroaniline	15.587	138	112720	17.756	ng/ul	97
66) 4,6-Dinitro-2-methylph...	15.640	198	87793	17.328	ng/ul	97
67) N-Nitrosodiphenylamine	15.769	169	502786	20.451	ng/ul	97
68) 4-Bromophenyl-phenylether	16.451	248	160196	20.151	ng/ul	95
69) Hexachlorobenzene	16.563	284	182112	19.705	ng/ul	97
70) Atrazine	16.728	200	143946	17.597	ng/ul	98
71) Pentachlorophenol	16.916	266	101218	17.611	ng/ul	98
72) Phenanthrene	17.310	178	948623	19.730	ng/ul	100
74) Anthracene	17.398	178	949799	19.621	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.304	216	264179	21.929	ng/uL	99
76) Pentachlorobenzene	14.828	250	254619	21.012	ng/uL	99
77) Carbazole	17.675	167	860317	19.024	ng/ul	99
78) Di-n-butylphthalate	18.222	149	891759	18.682	ng/ul	99
80) Fluoranthene	19.275	202	1043416	19.609	ng/ul	98
82) Pyrene	19.628	202	1118212	19.610	ng/ul	99
83) Butylbenzylphthalate	20.504	149	392325	18.449	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.275	252	341016	17.856	ng/ul	98
85) Benzo(a)anthracene	21.339	228	1126840	19.727	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.257	149	568805	18.713	ng/ul	99
87) Chrysene	21.392	228	1059909	19.347	ng/ul	99
89) Di-n-octyl phthalate	22.186	149	1007961	17.495	ng/ul	100
90) Benzo(b)fluoranthene	23.033	252	1179481	19.397	ng/ul	99
91) Benzo(k)fluoranthene	23.080	252	1203254	20.158	ng/ul	99
93) Benzo(a)pyrene	23.669	252	1074730	19.728	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.292	276	1363807	19.820	ng/ul	99
95) Dibenzo(a,h)anthracene	26.310	278	1224839	19.883	ng/ul	98
96) Benzo(g,h,i)perylene	27.074	276	1227603	19.822	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101022\
 Data File : BP012031.D
 Acq On : 10 Oct 2022 20:08
 Operator : CG/JU
 Sample : SSTDICV020
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SICV630

Quant Time: Oct 11 01:49:31 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101022.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 01:38:55 2022
 Response via : Initial Calibration




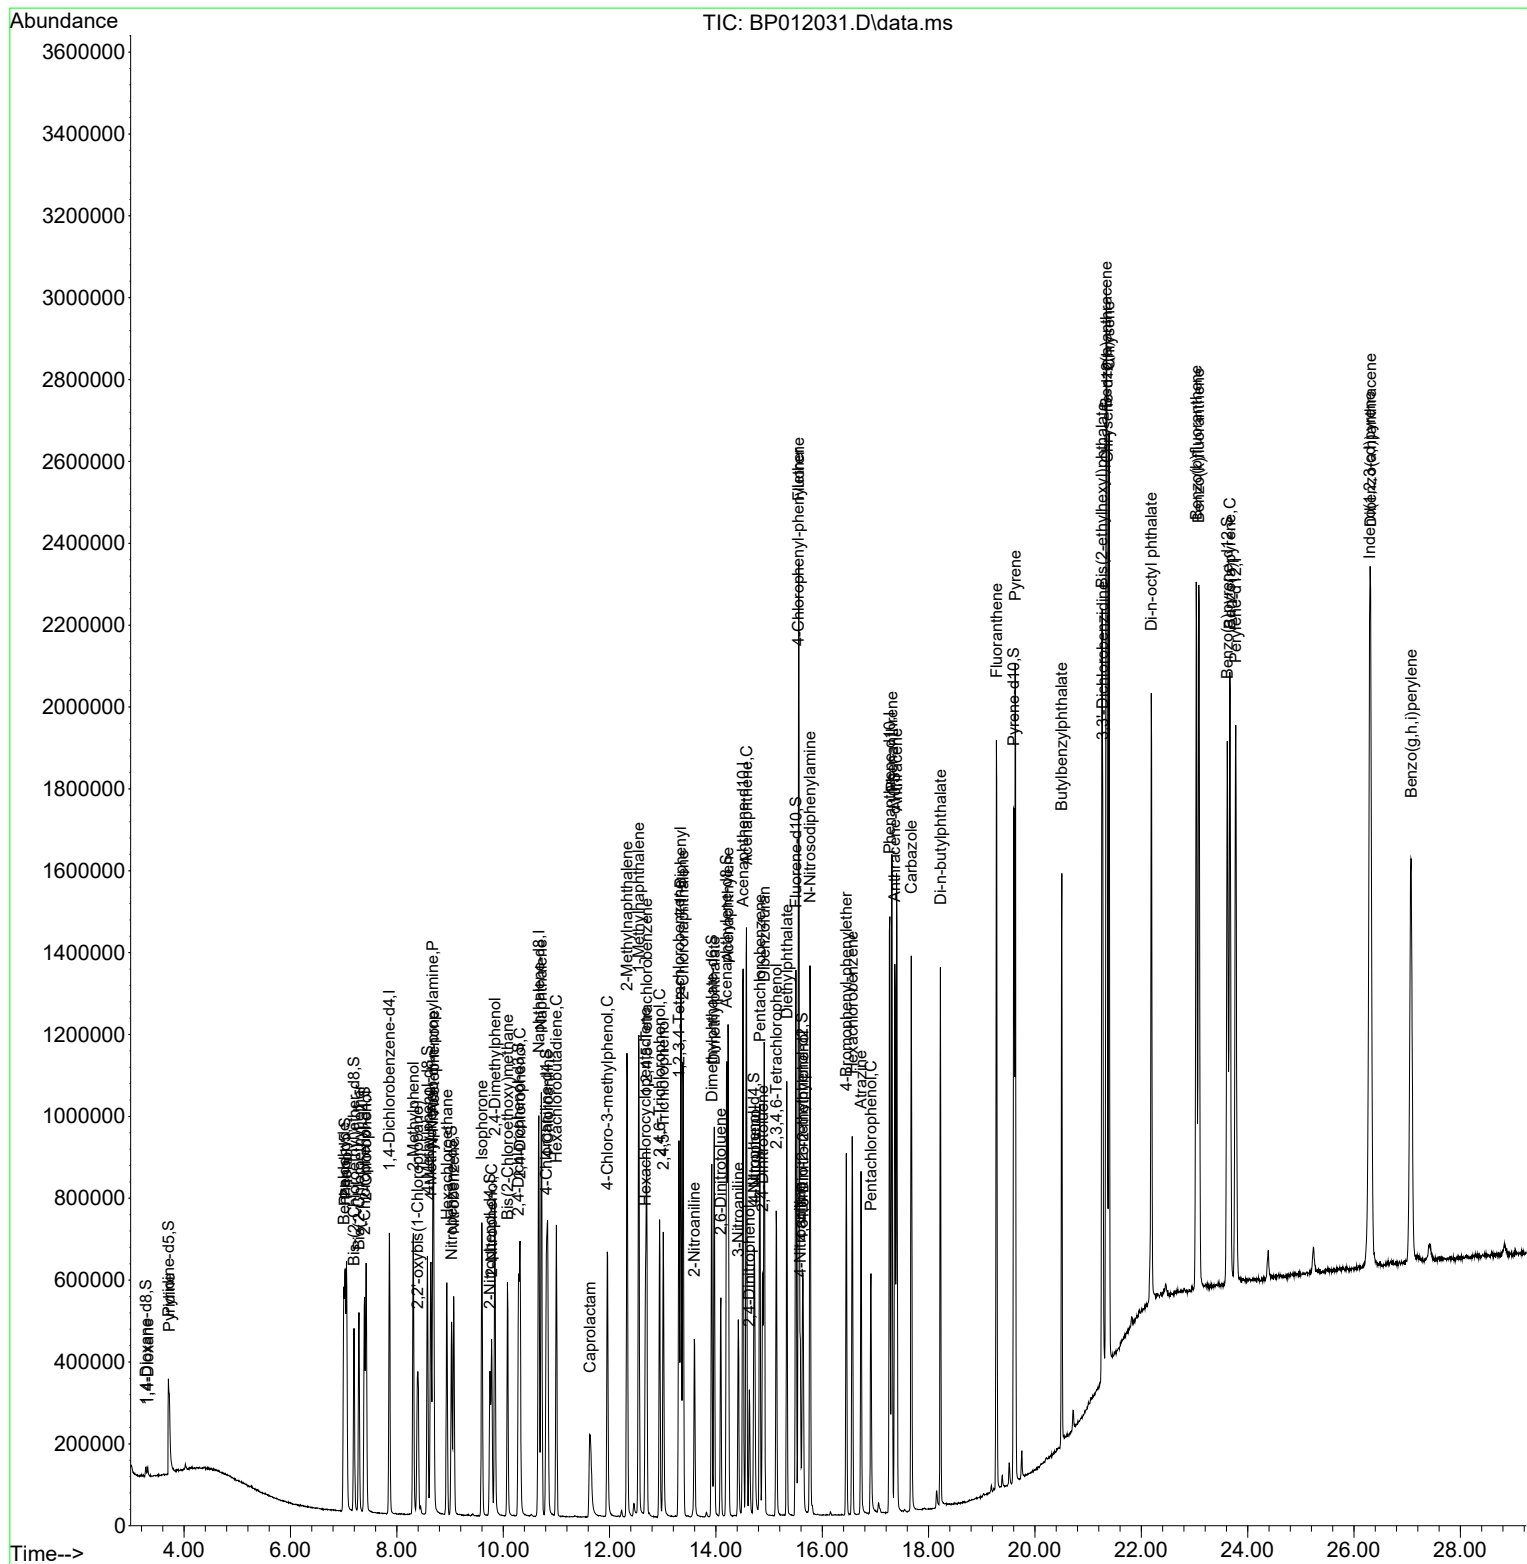


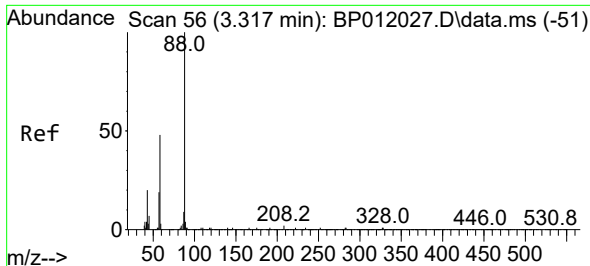

#2
1,4-Dioxane
Concen: 6.003 ng/uL
RT: 3.317 min Scan# 50
Delta R.T. -0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion	Ratio	Lower	Upper
88	100		
43	21.3	17.2	25.8
58	49.4	37.4	56.0

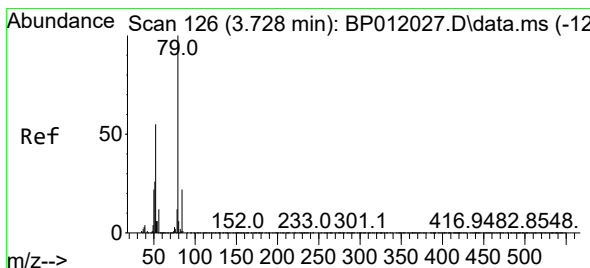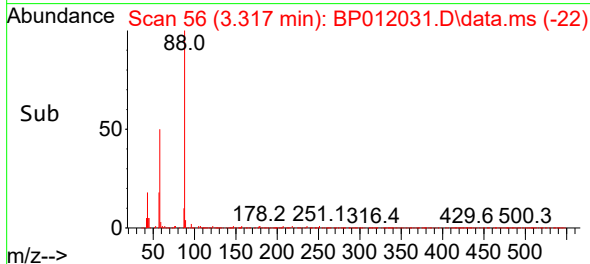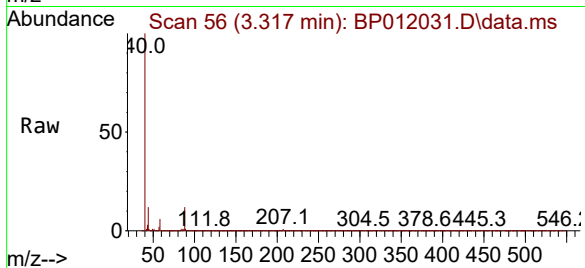

#5
Pyridine
Concen: 15.960 ng/uL
RT: 3.723 min Scan# 125
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion	Ratio	Lower	Upper
79	100		
52	56.3	44.2	66.4
51	28.2	22.9	34.3


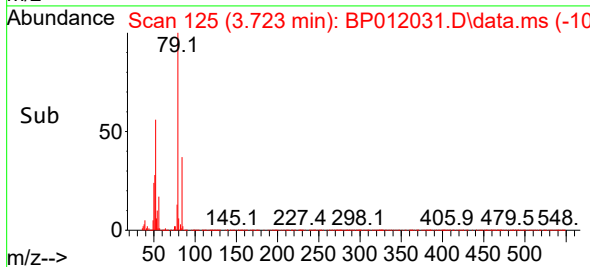

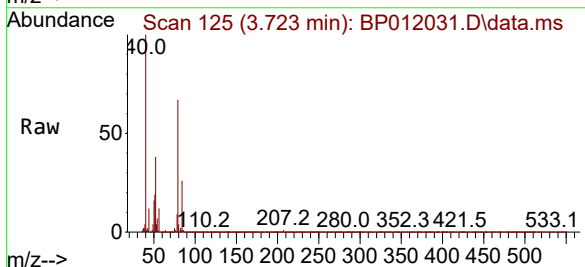




#6
Benzaldehyde
Concen: 24.237 ng/ul
RT: 7.005 min Scan# 61
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion: 77 Resp: 187427
Ion Ratio Lower Upper
77 100
105 101.9 79.8 119.8
106 98.0 77.6 116.4

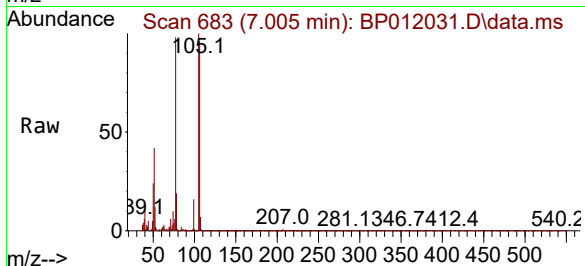

#8
Phenol
Concen: 19.567 ng/ul
RT: 7.052 min Scan# 691
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion: 94 Resp: 343691
Ion Ratio Lower Upper
94 100
65 26.4 20.8 31.2
66 35.0 27.4 41.0



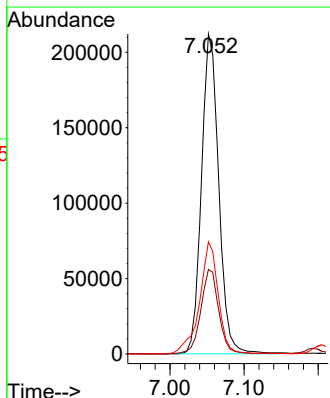
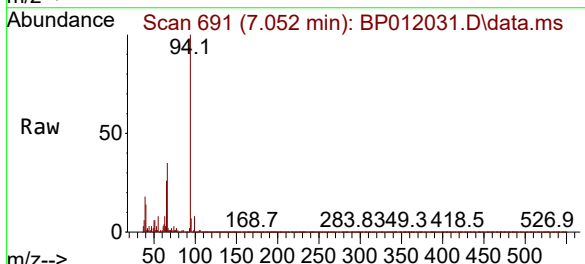




#10
Bis(2-Chloroethyl)ether
Concen: 20.111 ng/ul
RT: 7.287 min Scan# 731
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion: 93 Resp: 276135
Ion Ratio Lower Upper
93 100
63 76.7 61.5 92.3
95 32.4 26.6 40.0



#12
2-Chlorophenol
Concen: 20.139 ng/ul
RT: 7.422 min Scan# 754
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:128 Resp: 279776
Ion Ratio Lower Upper
128 100
64 44.1 34.9 52.3
130 31.9 26.1 39.1





#13

2-Methylphenol

Concen: 19.733 ng/ul

RT: 8.311 min Scan# 905

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :





SICV630

Tgt Ion:108 Resp: 253022

Ion Ratio Lower Upper

108 100

107 88.8 72.4 108.6

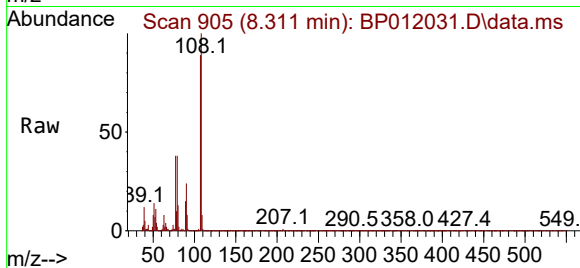

#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.428 ng/ul

RT: 8.393 min Scan# 919

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion: 45 Resp: 328466


Ion Ratio Lower Upper

45 100

77 15.9 13.4 20.0

79 13.0 9.9 14.9



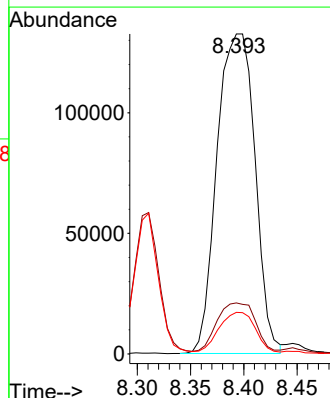
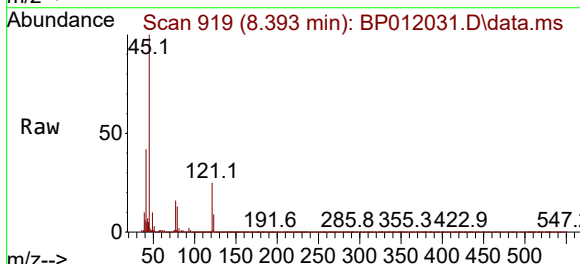




#16
Acetophenone
Concen: 20.252 ng/ul
RT: 8.693 min Scan# 91
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:105 Resp: 404888
Ion Ratio Lower Upper
105 100
77 73.3 59.2 88.8
51 23.7 19.8 29.6



#17
N-Nitroso-di-n-propylamine
Concen: 20.381 ng/ul
RT: 8.675 min Scan# 967
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion: 70 Resp: 179714
Ion Ratio Lower Upper
70 100
42 50.2 39.9 59.9
101 9.7 7.0 10.6
130 19.8 16.8 25.2



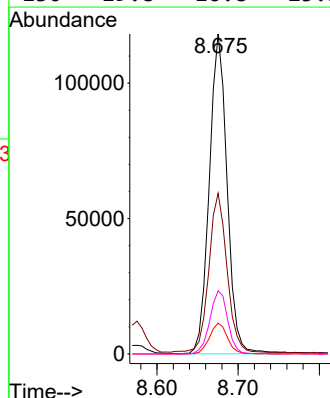





#18
4-Methylphenol
Concen: 19.666 ng/ul
RT: 8.640 min Scan# 961
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:108 Resp: 272476
Ion Ratio Lower Upper
108 100
107 110.4 90.1 135.1



#19
Hexachloroethane
Concen: 19.870 ng/ul
RT: 8.940 min Scan# 1012
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:117 Resp: 114066
Ion Ratio Lower Upper
117 100
201 89.6 74.2 111.4
199 56.0 46.3 69.5









#22
Nitrobenzene
Concen: 20.083 ng/ul
RT: 9.069 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion: 77 Resp: 299750
Ion Ratio Lower Upper
77 100
123 46.4 36.6 54.8
65 12.9 9.6 14.4



#23
Isophorone
Concen: 19.595 ng/ul
RT: 9.599 min Scan# 1124
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion: 82 Resp: 524211
Ion Ratio Lower Upper
82 100
95 6.7 5.2 7.8
138 17.3 14.4 21.6









#25
2-Nitrophenol
Concen: 20.201 ng/ul
RT: 9.781 min Scan# 1155
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:139 Resp: 144253
Ion Ratio Lower Upper
139 100
65 49.3 37.7 56.5
109 26.3 21.2 31.8



#26
2,4-Dimethylphenol
Concen: 19.785 ng/ul
RT: 9.846 min Scan# 1166
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:107 Resp: 280205
Ion Ratio Lower Upper
107 100
121 52.5 41.1 61.7
122 89.8 71.1 106.7

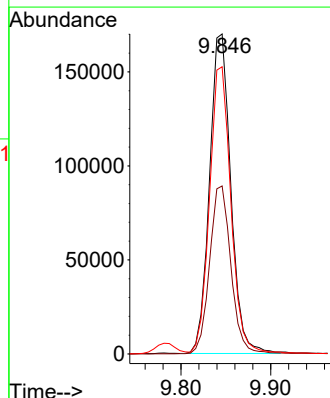



#27

Bis(2-Chloroethoxy)methane

Concen: 19.766 ng/ul

RT: 10.081 min Scan# 1207

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion: 93 Resp: 337909

Ion Ratio Lower Upper

93 100

95 33.0 26.2 39.2

123 11.1 9.2 13.8

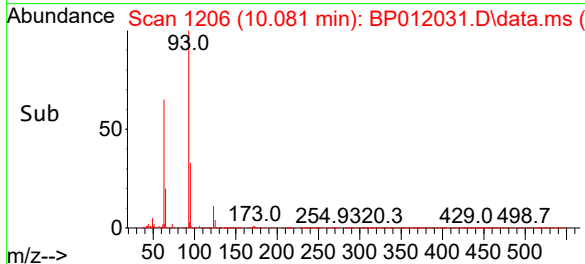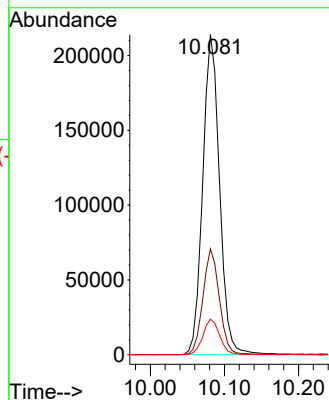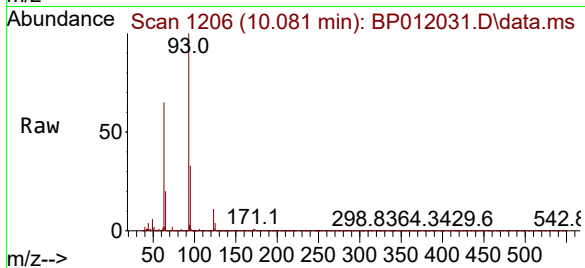

#29

2,4-Dichlorophenol

Concen: 19.851 ng/ul

RT: 10.316 min Scan# 1246

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:162 Resp: 239419


Ion Ratio Lower Upper

162 100

164 64.8 52.5 78.7

98 35.0 27.9 41.9


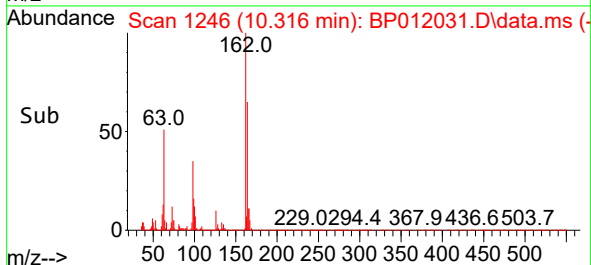
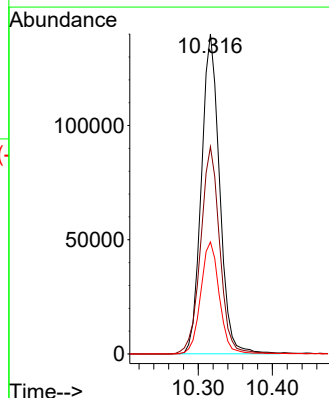
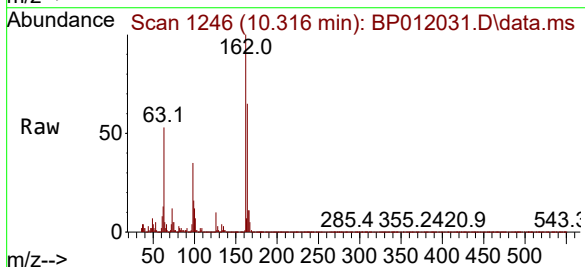




#30
Naphthalene
Concen: 19.736 ng/ul
RT: 10.716 min Scan# 1314
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:128 Resp: 888598
Ion Ratio Lower Upper
128 100
129 10.8 8.8 13.2
127 12.6 10.1 15.1



#32
4-Chloroaniline
Concen: 18.788 ng/ul
RT: 10.834 min Scan# 1334
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:127 Resp: 348970
Ion Ratio Lower Upper
127 100
129 32.8 25.8 38.8

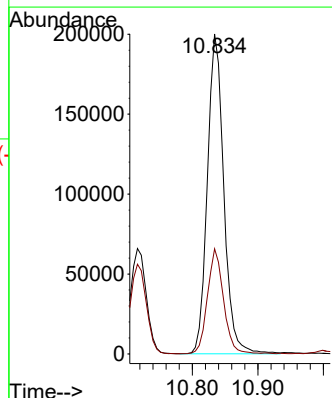



#33

Hexachlorobutadiene

Concen: 19.371 ng/ul

RT: 10.999 min Scan# 11

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:225 Resp: 141822

Ion Ratio Lower Upper

225 100

223 65.9 49.8 74.8

227 65.8 51.0 76.4

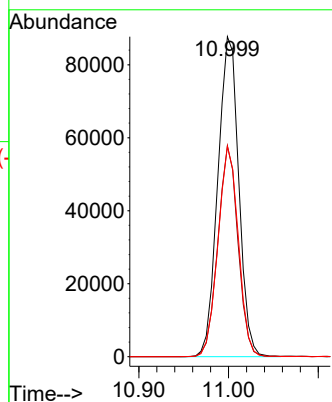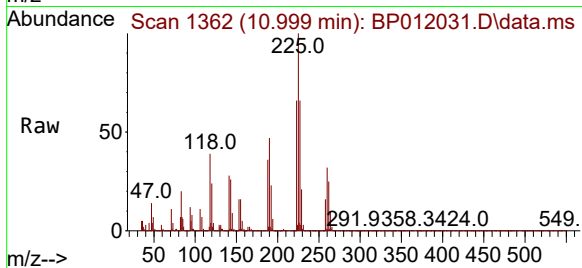

#34

Caprolactam

Concen: 18.324 ng/ul

RT: 11.634 min Scan# 1470

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:113 Resp: 72343


Ion Ratio Lower Upper

113 100

55 162.6 132.9 199.3

56 119.7 97.7 146.5




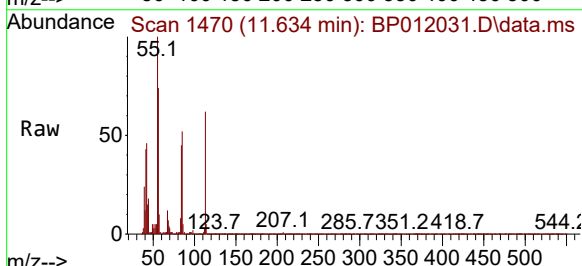


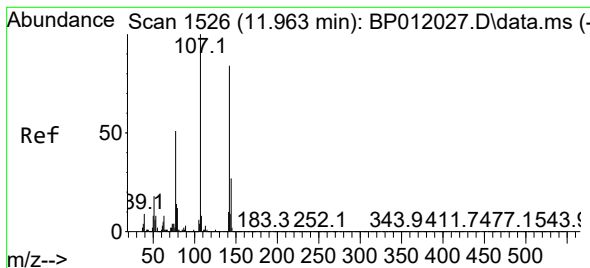

#35
4-Chloro-3-methylphenol
Concen: 19.170 ng/ul
RT: 11.957 min Scan# 11
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:107 Resp: 236983
Ion Ratio Lower Upper
107 100
144 27.3 21.8 32.6
142 84.3 67.1 100.7

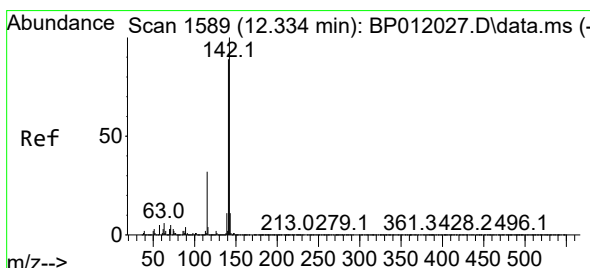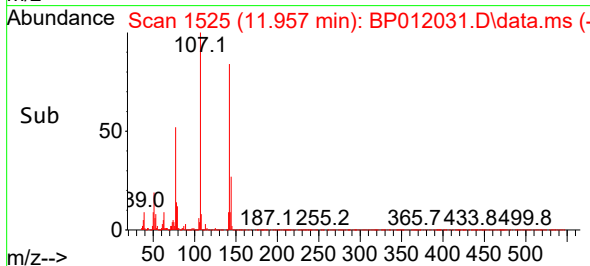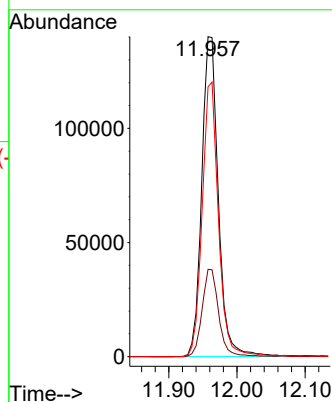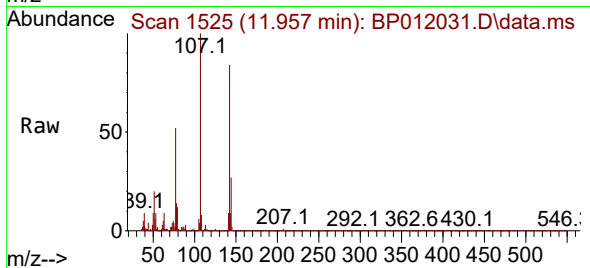

#36
2-Methylnaphthalene
Concen: 19.627 ng/ul
RT: 12.328 min Scan# 1588
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:142 Resp: 563267
Ion Ratio Lower Upper
142 100
141 89.0 71.4 107.0

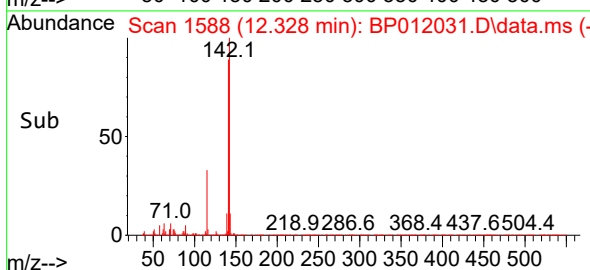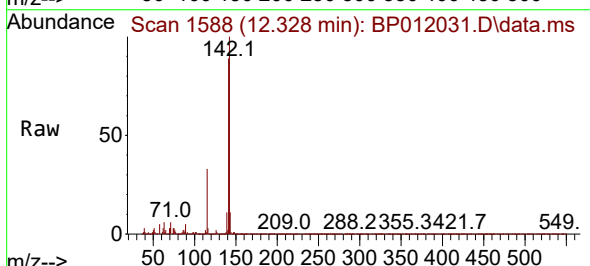



#37

1-Methylnaphthalene

Concen: 19.372 ng/ul

RT: 12.546 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:142 Resp: 558968

Ion Ratio Lower Upper

142 100

141 92.1 74.3 111.5

116 3.7 2.8 4.2

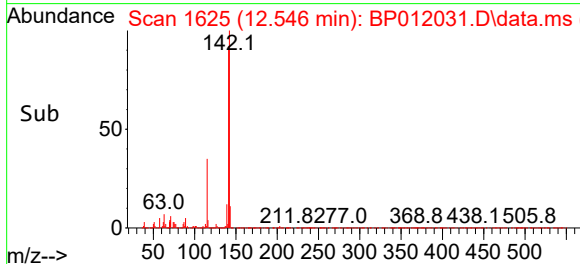

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.214 ng/ul

RT: 12.699 min Scan# 1651

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Tgt Ion:216 Resp: 265263




Ion Ratio Lower Upper


216 100

214 78.0 63.8 95.6

179 21.5 17.3 25.9

108 18.1 15.2 22.8


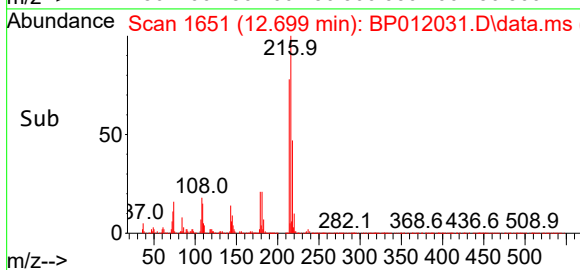

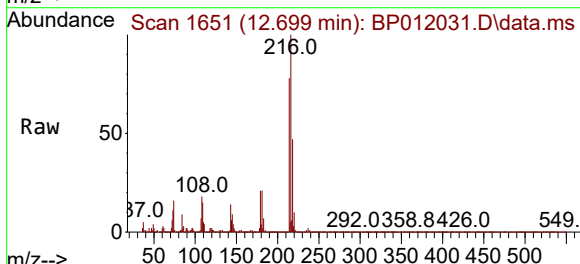




#40
Hexachlorocyclopentadiene
Concen: 21.314 ng/ul
RT: 12.675 min Scan# 1647
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:237 Resp: 129633
Ion Ratio Lower Upper
237 100
235 63.0 52.4 78.6
272 12.8 10.6 16.0



#41
2,4,6-Trichlorophenol
Concen: 20.203 ng/ul
RT: 12.940 min Scan# 1692
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:196 Resp: 167258
Ion Ratio Lower Upper
196 100
198 91.8 75.2 112.8
200 31.4 23.4 35.2









#42
2,4,5-Trichlorophenol
Concen: 20.124 ng/ul
RT: 13.010 min Scan# 1704
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:196 Resp: 177460
Ion Ratio Lower Upper
196 100
198 98.8 76.5 114.7
200 30.9 25.3 37.9



#43
1,1'-Biphenyl
Concen: 20.313 ng/ul
RT: 13.340 min Scan# 1760
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:154 Resp: 696571
Ion Ratio Lower Upper
154 100
153 39.9 31.8 47.8
76 13.9 10.9 16.3




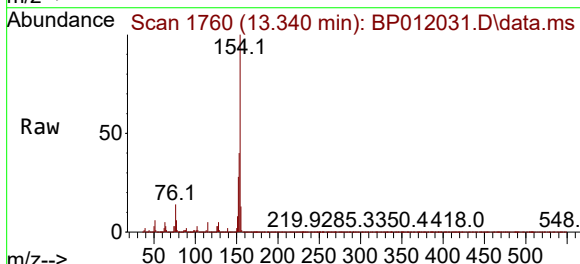




#44
2-Chloronaphthalene
Concen: 20.144 ng/ul
RT: 13.381 min Scan# 1767
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:162 Resp: 554089
Ion Ratio Lower Upper
162 100
164 32.1 26.1 39.1
127 39.2 30.2 45.2



#45
2-Nitroaniline
Concen: 18.280 ng/ul
RT: 13.593 min Scan# 1803
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion: 65 Resp: 114596
Ion Ratio Lower Upper
65 100
92 69.3 57.3 85.9
138 107.5 88.8 133.2




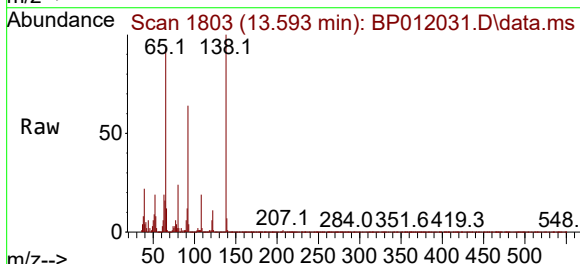




#47
Dimethylphthalate
Concen: 18.805 ng/ul
RT: 13.969 min Scan# 1867
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:163 Resp: 603550
Ion Ratio Lower Upper
163 100
194 3.6 3.1 4.7
164 10.3 8.0 12.0

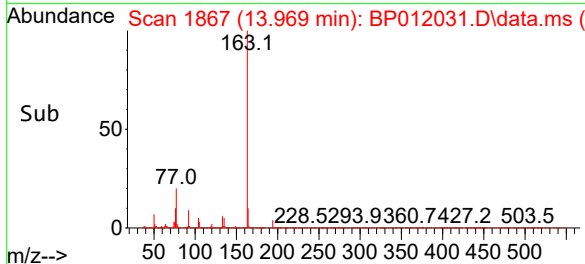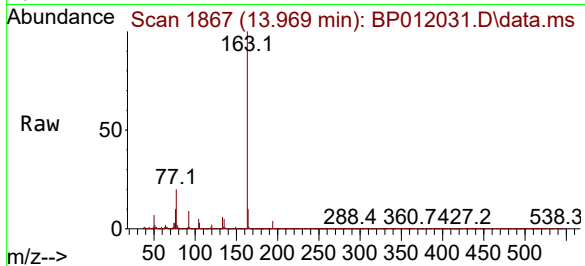

#48
2,6-Dinitrotoluene
Concen: 18.604 ng/ul
RT: 14.093 min Scan# 1888
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:165 Resp: 99129
Ion Ratio Lower Upper
165 100
89 62.7 48.2 72.2
121 26.4 19.3 28.9


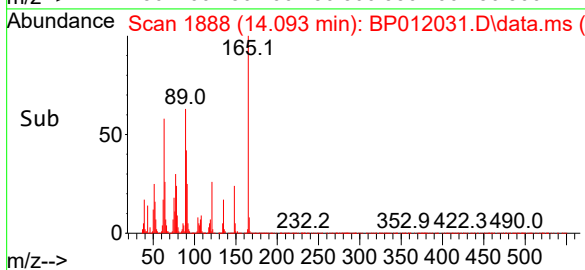

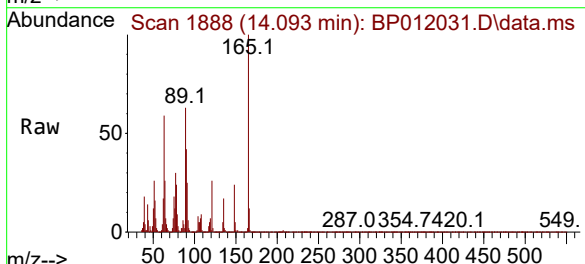




#50
Acenaphthylene
Concen: 20.182 ng/ul
RT: 14.228 min Scan# 1911
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:152 Resp: 844870
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.6
153 13.0 10.5 15.7

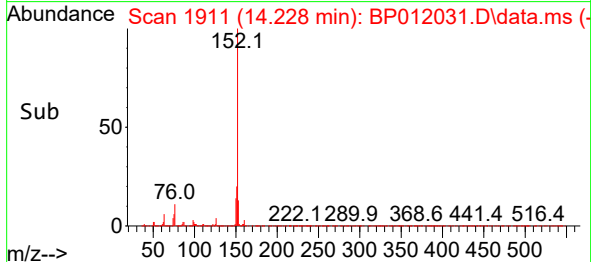

#51
3-Nitroaniline
Concen: 17.644 ng/ul
RT: 14.422 min Scan# 1944
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:138 Resp: 116038
Ion Ratio Lower Upper
138 100
108 11.7 10.2 15.4
92 118.8 96.6 144.8


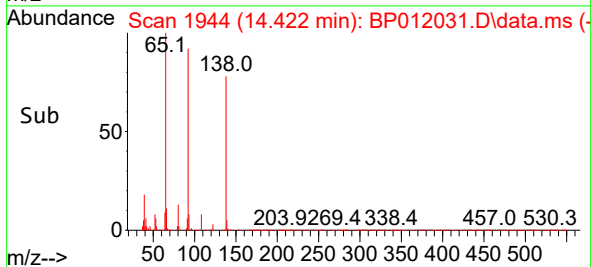

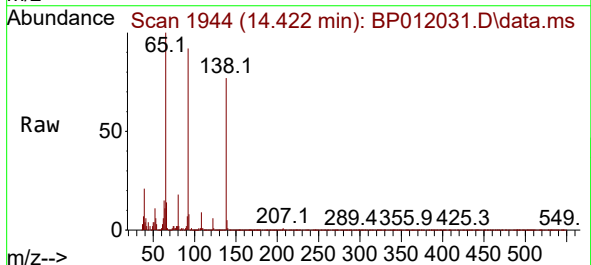




#52
Acenaphthene
Concen: 19.640 ng/ul
RT: 14.575 min Scan# 1970
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:153 Resp: 581526
Ion Ratio Lower Upper
153 100
152 48.9 39.2 58.8
154 88.1 70.4 105.6



#53
2,4-Dinitrophenol
Concen: 17.305 ng/ul
RT: 14.628 min Scan# 1979
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:184 Resp: 64645
Ion Ratio Lower Upper
184 100
63 70.4 52.0 78.0
154 61.8 46.6 70.0




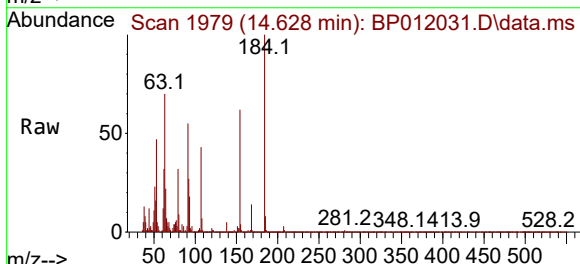




#55
4-Nitrophenol
Concen: 17.010 ng/ul
RT: 14.728 min Scan# 1996
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:109 Resp: 83160
Ion Ratio Lower Upper
109 100
139 149.5 124.5 186.7
65 139.9 107.8 161.6



#56
Dibenzofuran
Concen: 19.293 ng/ul
RT: 14.910 min Scan# 2027
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:168 Resp: 770051
Ion Ratio Lower Upper
168 100
139 37.0 30.0 45.0


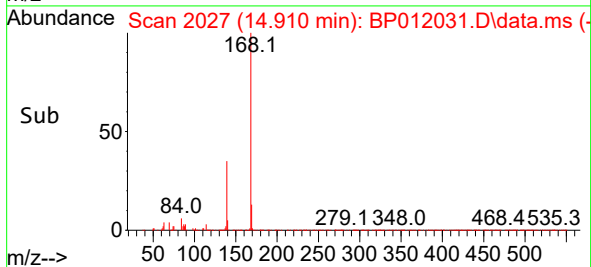

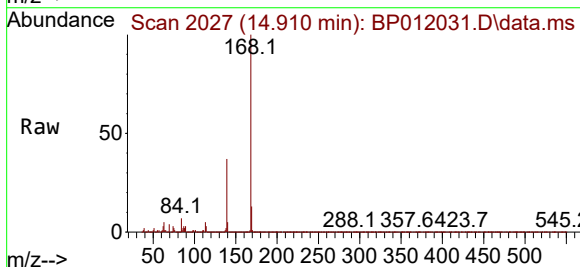




#57
2,4-Dinitrotoluene
Concen: 18.418 ng/ul
RT: 14.881 min Scan# 2022
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:165 Resp: 157648
Ion Ratio Lower Upper
165 100
63 43.1 32.9 49.3
182 2.9 2.1 3.1

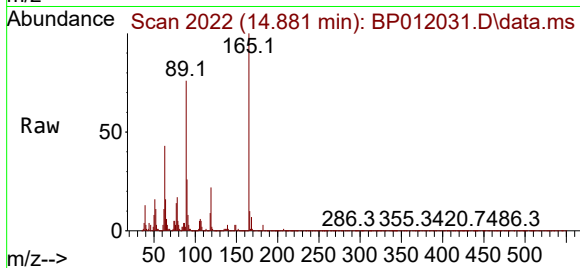

#58
2,3,4,6-Tetrachlorophenol
Concen: 18.777 ng/ul
RT: 15.134 min Scan# 2065
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:232 Resp: 138564
Ion Ratio Lower Upper
232 100
131 52.6 39.3 58.9
130 2.6 1.8 2.8
166 34.0 25.7 38.5



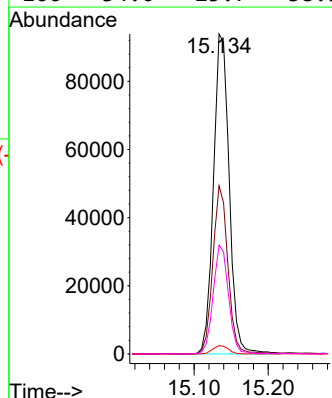





#59
Diethylphthalate
Concen: 18.282 ng/ul
RT: 15.334 min Scan# 2099
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:149 Resp: 573818
Ion Ratio Lower Upper
149 100
177 21.6 16.8 25.2
150 12.1 10.0 15.0



#61
Fluorene
Concen: 19.281 ng/ul
RT: 15.557 min Scan# 2137
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:166 Resp: 624239
Ion Ratio Lower Upper
166 100
165 97.7 79.3 118.9
167 13.5 10.7 16.1









#62
4-Chlorophenyl-phenylether
Concen: 19.186 ng/ul
RT: 15.551 min Scan# 2136
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:204 Resp: 286075
Ion Ratio Lower Upper
204 100
206 32.7 25.9 38.9
141 61.0 47.9 71.9



#63
4-Nitroaniline
Concen: 17.756 ng/ul
RT: 15.587 min Scan# 2142
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:138 Resp: 112720
Ion Ratio Lower Upper
138 100
92 53.6 40.8 61.2
108 76.5 59.5 89.3



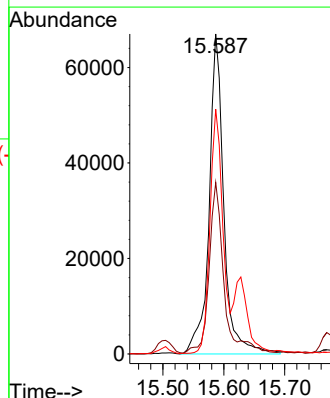
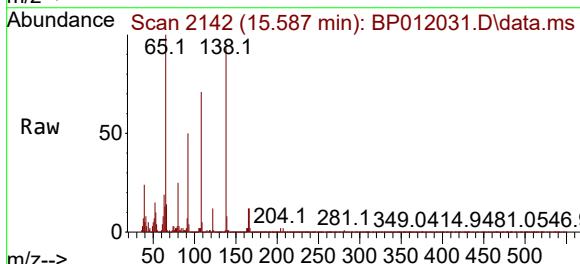




#66
4,6-Dinitro-2-methylphenol
Concen: 17.328 ng/ul
RT: 15.640 min Scan# 2152
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:198 Resp: 87793
Ion Ratio Lower Upper
198 100
182 7.4 5.6 8.4
77 27.3 20.3 30.5



#67
N-Nitrosodiphenylamine
Concen: 20.451 ng/ul
RT: 15.769 min Scan# 2173
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:169 Resp: 502786
Ion Ratio Lower Upper
169 100
168 68.0 52.2 78.2
167 37.1 30.1 45.1









#68
4-Bromophenyl-phenylether
Concen: 20.151 ng/ul
RT: 16.451 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:248 Resp: 160196
Ion Ratio Lower Upper
248 100
250 96.2 75.1 112.7
141 80.0 58.8 88.2



#69
Hexachlorobenzene
Concen: 19.705 ng/ul
RT: 16.563 min Scan# 2308
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:284 Resp: 182112
Ion Ratio Lower Upper
284 100
142 42.5 32.1 48.1
249 31.1 26.0 39.0









#70
 Atrazine
 Concen: 17.597 ng/ul
 RT: 16.728 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BP012031.D
 Acq: 10 Oct 2022 20:08




Instrument :
 BNA_P
 ClientSampleId :
 SICV630


Tgt Ion:200 Resp: 143946
 Ion Ratio Lower Upper
 200 100
 173 26.8 20.9 31.3
 215 47.3 37.0 55.4



#71
 Pentachlorophenol
 Concen: 17.611 ng/ul
 RT: 16.916 min Scan# 2368
 Delta R.T. 0.000 min
 Lab File: BP012031.D
 Acq: 10 Oct 2022 20:08

Tgt Ion:266 Resp: 101218
 Ion Ratio Lower Upper
 266 100
 264 63.8 49.7 74.5
 268 64.0 49.7 74.5

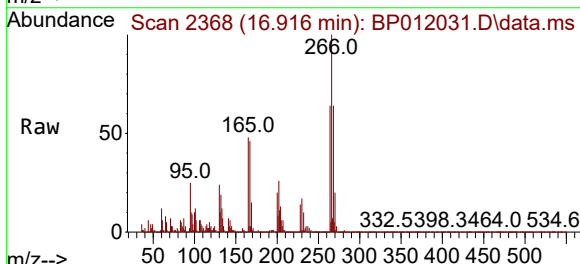

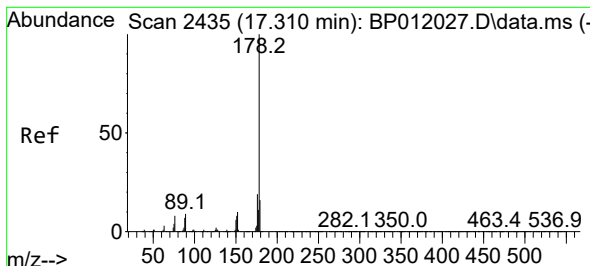

#72

Phenanthrene

Concen: 19.730 ng/ul

RT: 17.310 min Scan# 2435

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:178 Resp: 948623

Ion Ratio Lower Upper

178 100

179 15.6 12.5 18.7

176 19.5 15.5 23.3

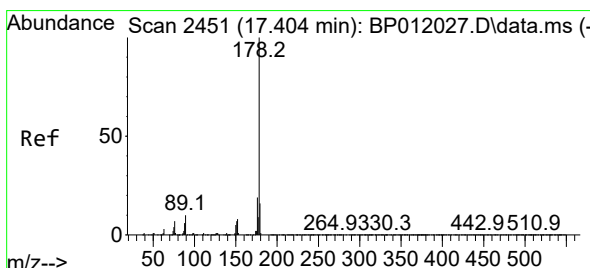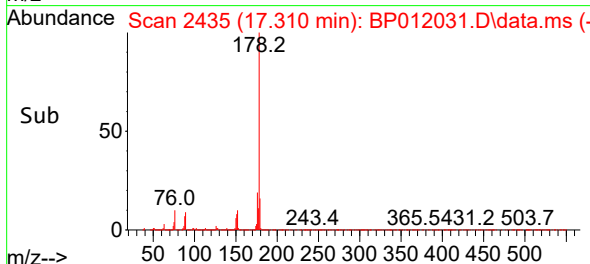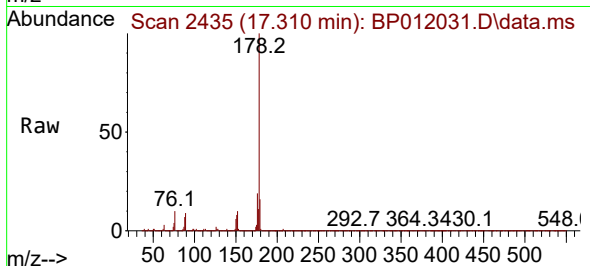

#74

Anthracene

Concen: 19.621 ng/ul

RT: 17.398 min Scan# 2450

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:178 Resp: 949799


Ion Ratio Lower Upper

178 100

179 15.9 12.5 18.7

176 19.0 15.2 22.8

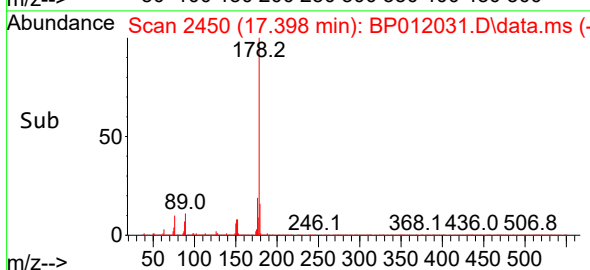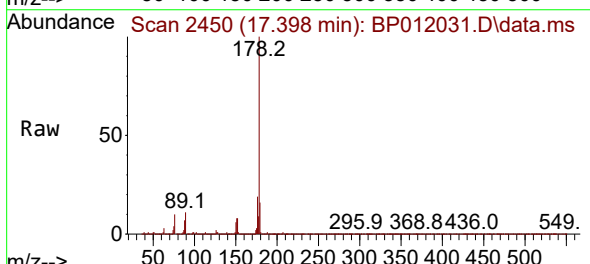



#75

1,2,3,4-Tetrachlorobenzene

Concen: 21.929 ng/uL

RT: 13.304 min Scan# 1754

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:216 Resp: 264179

Ion Ratio Lower Upper

216 100

214 79.4 64.0 96.0

218 46.6 38.2 57.2

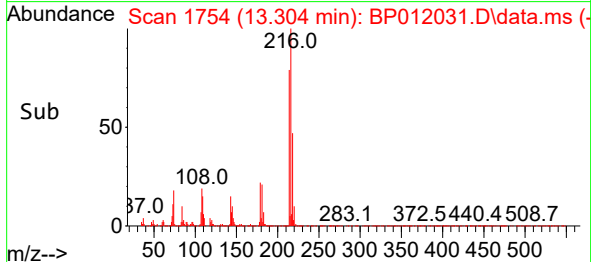

#76

Pentachlorobenzene

Concen: 21.012 ng/uL

RT: 14.828 min Scan# 2013

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:250 Resp: 254619


Ion Ratio Lower Upper

250 100

248 62.9 50.9 76.3

252 63.0 51.5 77.3


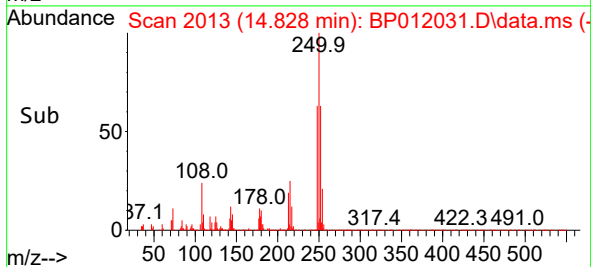

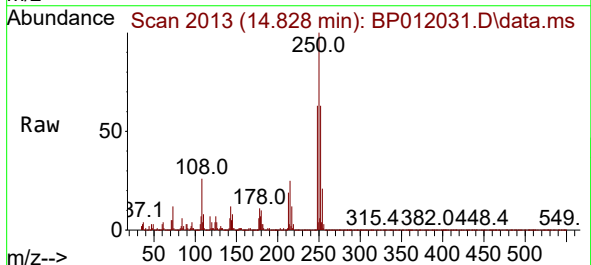




#77
Carbazole
Concen: 19.024 ng/ul
RT: 17.675 min Scan# 2498
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:167 Resp: 860317
Ion Ratio Lower Upper
167 100
166 21.8 17.2 25.8
139 12.9 10.7 16.1



#78
Di-n-butylphthalate
Concen: 18.682 ng/ul
RT: 18.222 min Scan# 2590
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:149 Resp: 891759
Ion Ratio Lower Upper
149 100
150 9.1 7.0 10.6
104 4.8 3.7 5.5

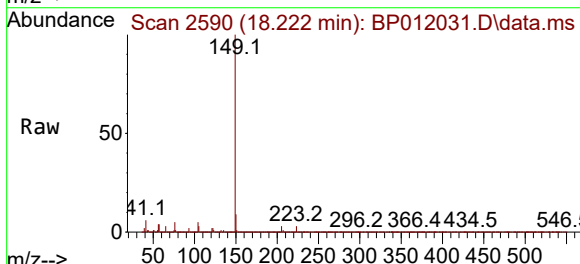



#80

Fluoranthene

Concen: 19.609 ng/u1

RT: 19.275 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:202 Resp: 1043416

Ion Ratio Lower Upper

202 100

101 13.7 10.2 15.2

100 10.1 7.7 11.5



#82

Pyrene

Concen: 19.610 ng/u1

RT: 19.628 min Scan# 2829

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:202 Resp: 1118212


Ion Ratio Lower Upper

202 100

101 15.5 11.6 17.4

100 12.5 9.8 14.8

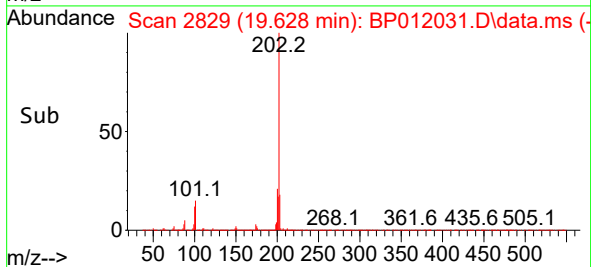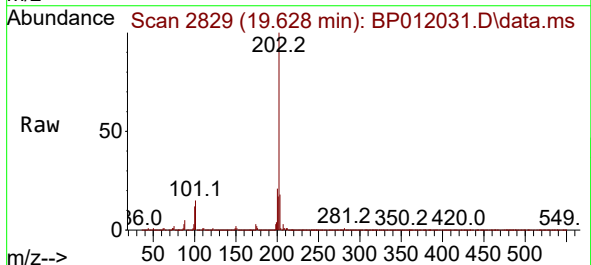



#83

Butylbenzylphthalate

Concen: 18.449 ng/ul

RT: 20.504 min Scan# 2978

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:149 Resp: 392325

Ion Ratio Lower Upper

149 100

91 69.3 56.6 84.8

206 19.4 15.0 22.6

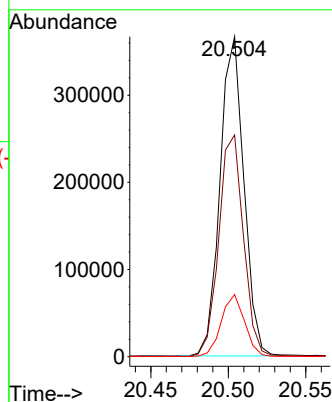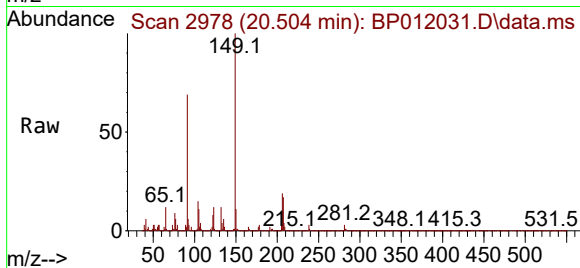

#84

3,3'-Dichlorobenzidine

Concen: 17.856 ng/ul

RT: 21.275 min Scan# 3109

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:252 Resp: 341016


Ion Ratio Lower Upper

252 100

254 65.0 50.5 75.7

126 13.0 11.0 16.4





#85

Benzo(a)anthracene

Concen: 19.727 ng/ul

RT: 21.339 min Scan# 31

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:228 Resp: 1126840

Ion Ratio Lower Upper

228 100

229 19.3 15.5 23.3

226 26.8 21.8 32.6

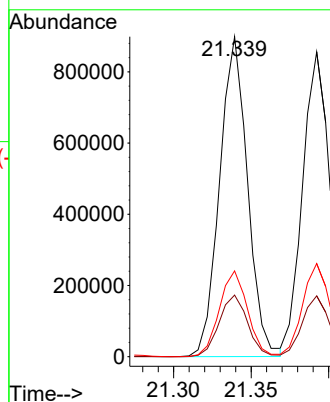

#86

Bis(2-ethylhexyl)phthalate

Concen: 18.713 ng/ul

RT: 21.257 min Scan# 3106

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08




Tgt Ion:149 Resp: 568805


Ion Ratio Lower Upper

149 100

167 25.5 21.0 31.6

279 3.2 2.9 4.3





#87

Chrysene

Concen: 19.347 ng/ul

RT: 21.392 min Scan# 3129

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:228 Resp: 1059909

Ion Ratio Lower Upper

228 100

226 30.6 24.1 36.1

229 20.0 15.8 23.6

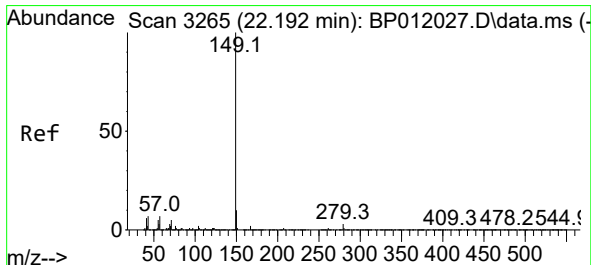

#89

Di-n-octyl phthalate

Concen: 17.495 ng/ul




RT: 22.186 min Scan# 3264


Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Tgt Ion:149 Resp: 1007961


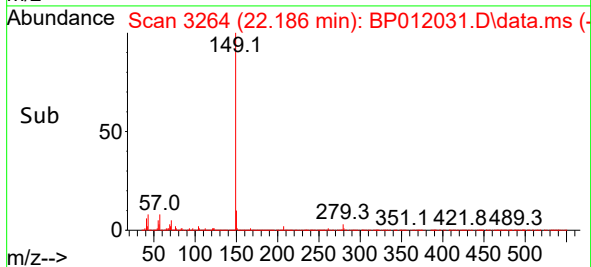

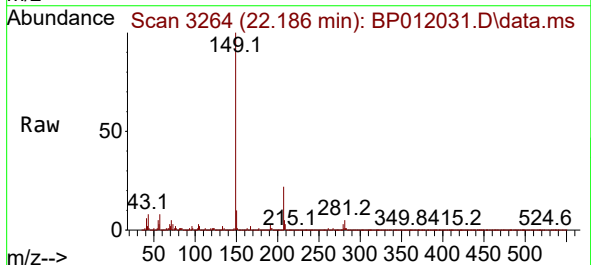




#90
Benzo(b)fluoranthene
Concen: 19.397 ng/ul
RT: 23.033 min Scan# 3409
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:252 Resp: 1179481
Ion Ratio Lower Upper
252 100
253 21.6 17.8 26.8
125 12.1 9.9 14.9

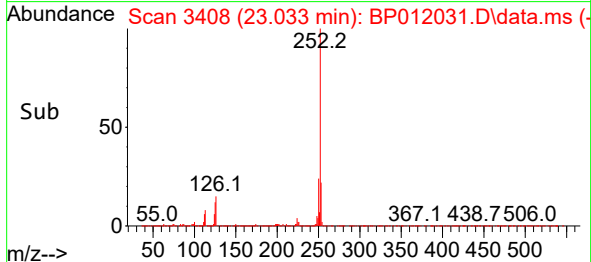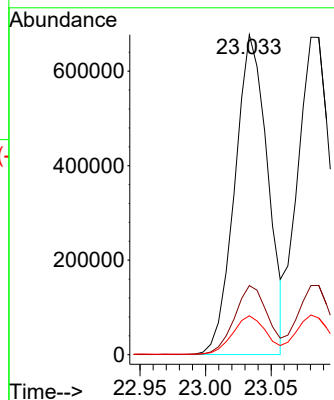

#91
Benzo(k)fluoranthene
Concen: 20.158 ng/ul
RT: 23.080 min Scan# 3416
Delta R.T. -0.006 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:252 Resp: 1203254
Ion Ratio Lower Upper
252 100
253 21.8 17.4 26.0
125 12.5 9.4 14.2


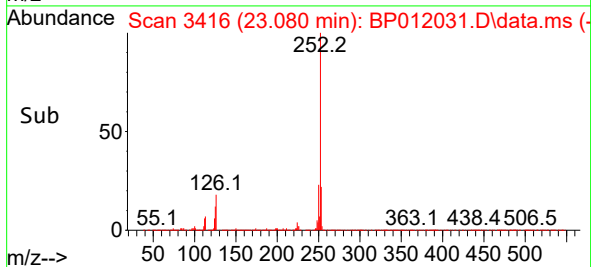
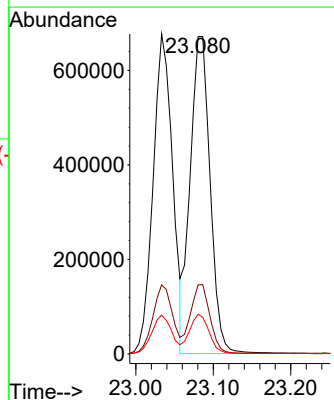
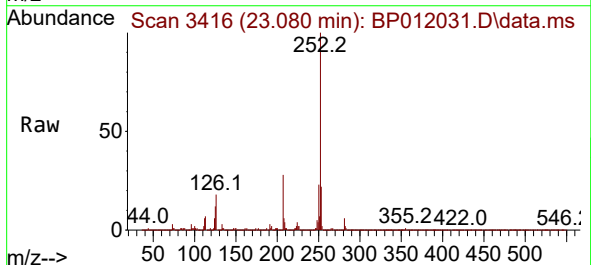




#93
Benzo(a)pyrene
Concen: 19.728 ng/ul
RT: 23.669 min Scan# 3516
Delta R.T. 0.000 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08




Instrument :
BNA_P
ClientSampleId :
SICV630


Tgt Ion:252 Resp: 1074730
Ion Ratio Lower Upper
252 100
253 22.1 17.3 25.9
125 13.1 10.8 16.2



#94
Indeno(1,2,3-cd)pyrene
Concen: 19.820 ng/ul
RT: 26.292 min Scan# 3962
Delta R.T. -0.012 min
Lab File: BP012031.D
Acq: 10 Oct 2022 20:08

Tgt Ion:276 Resp: 1363807
Ion Ratio Lower Upper
276 100
138 29.1 24.1 36.1
277 25.1 20.0 30.0





#95

Dibenzo(a,h)anthracene

Concen: 19.883 ng/ul

RT: 26.310 min Scan# 3966

Delta R.T. -0.006 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Instrument :

BNA_P

ClientSampleId :

SICV630





Tgt Ion:278 Resp: 1224839

Ion Ratio Lower Upper

278 100

139 19.7 15.4 23.0

279 23.5 19.6 29.4

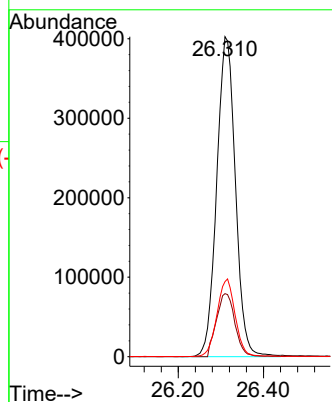

#96

Benzo(g,h,i)perylene

Concen: 19.822 ng/ul

RT: 27.074 min Scan# 4095

Delta R.T. 0.000 min

Lab File: BP012031.D

Acq: 10 Oct 2022 20:08

Tgt Ion:276 Resp: 1227603

Ion Ratio Lower Upper

276 100

138 25.1 20.9 31.3

277 23.6 19.0 28.4

