




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017630.D
Acq On : 10 Oct 2023 10:27
Operator : MA/JU
Sample : PB156061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Manual IntegrationsAPPROVED

Quant Time: Oct 10 23:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 04:45:41 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :mohammad ahmed 10/12/2023

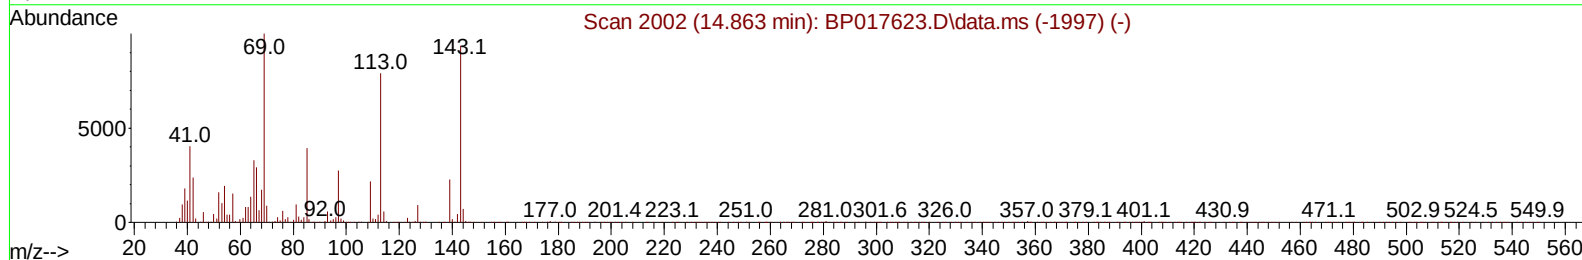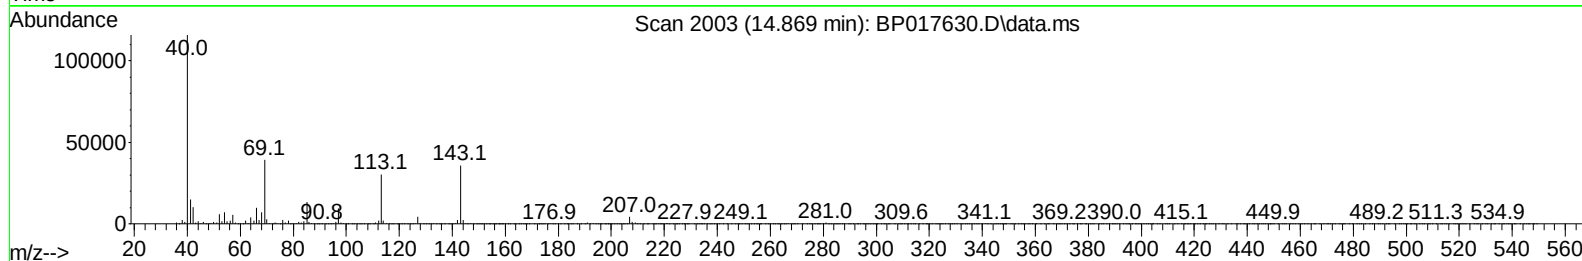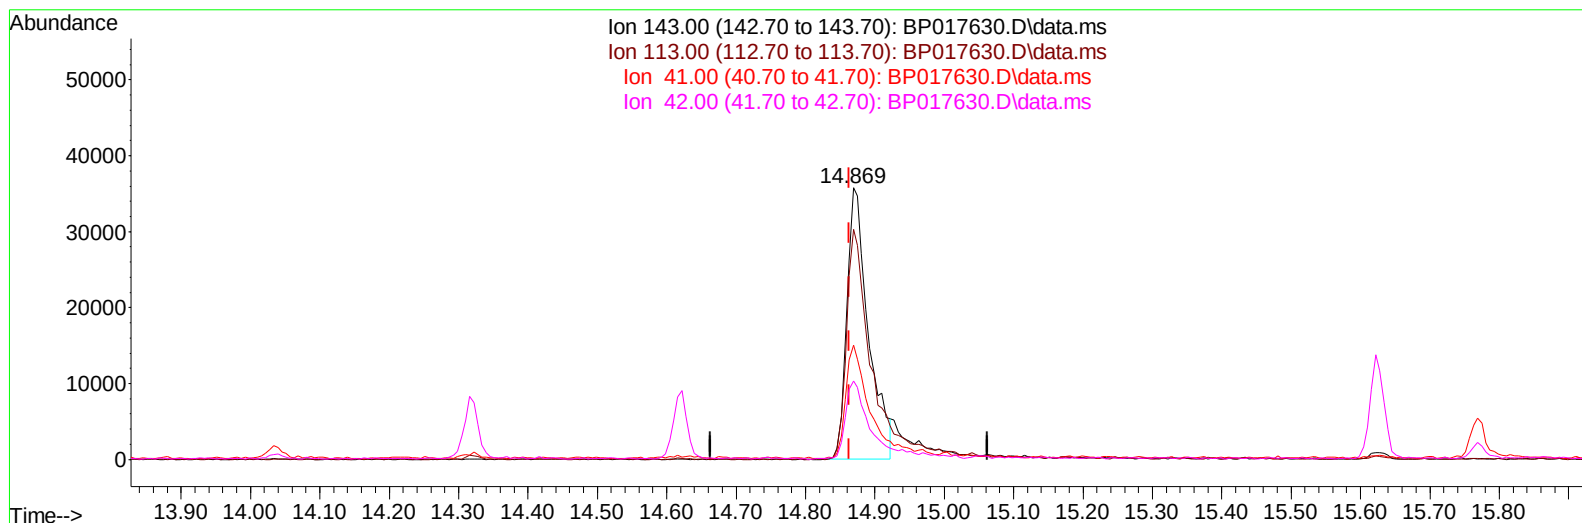

TIC: BP017630.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (+ 0.006) 20.19 ng/ul

response 77718

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	84.70	84.83
41.00	43.90	42.09
42.00	26.40	28.81




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017630.D
Acq On : 10 Oct 2023 10:27
Operator : MA/JU
Sample : PB156061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Manual IntegrationsAPPROVED

Quant Time: Oct 10 23:41:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 04:45:41 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :mohammad ahmed 10/12/2023

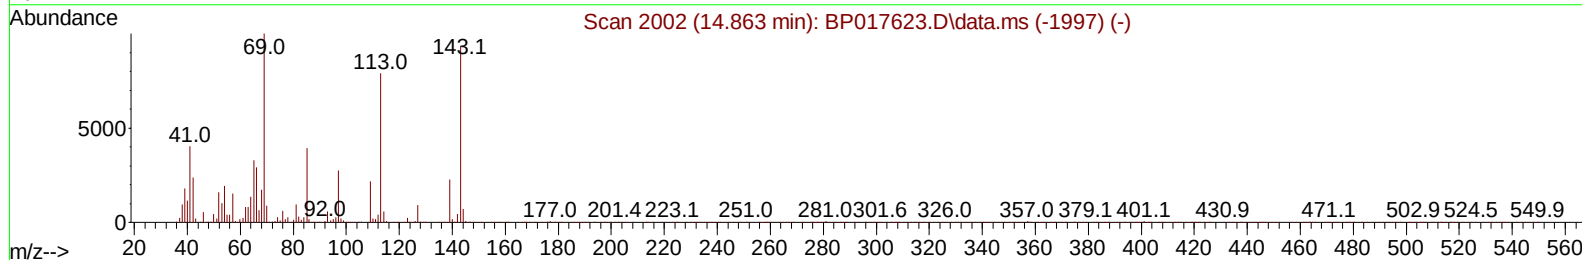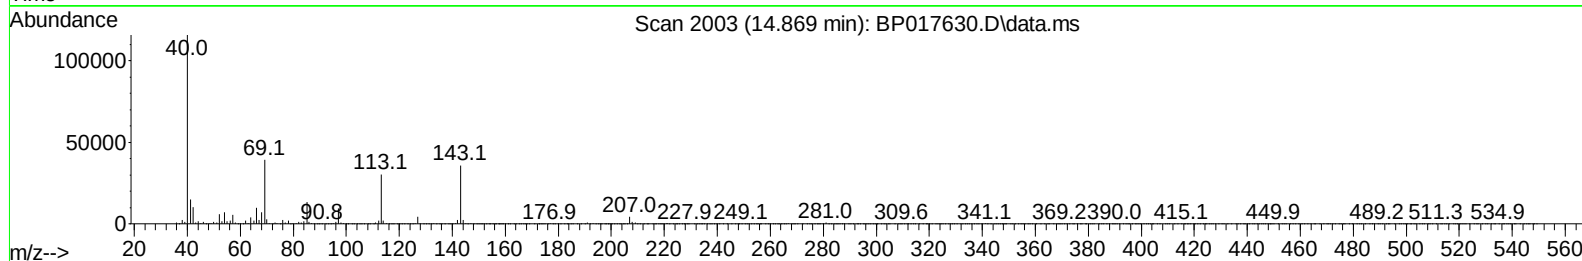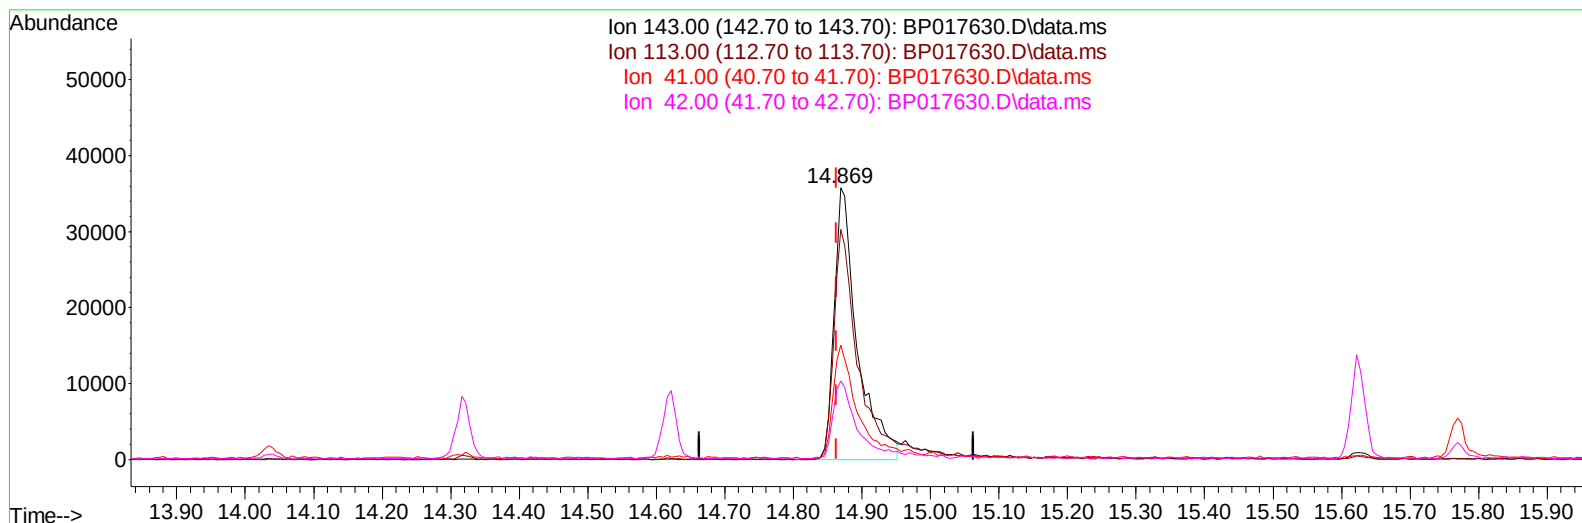

TIC: BP017630.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (+ 0.006) 21.72 ng/ul m

response 83627

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	84.70	84.83
41.00	43.90	42.09
42.00	26.40	28.81

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017630.D
 Acq On : 10 Oct 2023 10:27
 Operator : MA/JU
 Sample : PB156061BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK061

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/11/2023
 Supervised By :mohammad ahmed 10/12/2023

Quant Time: Oct 10 23:53:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 04:45:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.928	152	125197	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136	503896	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.622	164	319939	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	771157	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	773561	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	847143	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	17482	5.665	ng/uL	0.00
4) Pyridine-d5	3.717	84	228899	26.350	ng/ul	0.00
7) Phenol-d5	7.081	99	273326	25.816	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	173840	26.475	ng/ul	0.00
11) 2-Chlorophenol-d4	7.446	132	228367	27.421	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	215419	25.260	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	106294	27.376	ng/ul	0.00
24) 2-Nitrophenol-d4	9.852	143	113045	26.509	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	206589	24.943	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	306186	25.957	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	773283	30.441	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	784088	28.351	ng/ul	0.00
54) 4-Nitrophenol-d4	14.869	143	83627m	21.721	ng/ul	0.00
60) Fluorene-d10	15.622	176	665309	29.948	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	92827	20.294	ng/ul	0.00
73) Anthracene-d10	17.510	188	1128790	30.500	ng/ul	0.00
81) Pyrene-d10	19.769	212	1399980	31.728	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	1353448	30.817	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017630.D
Acq On : 10 Oct 2023 10:27
Operator : MA/JU
Sample : PB156061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/11/2023
Supervised By :mohammad ahmed 10/12/2023

Quant Time: Oct 10 23:53:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 04:45:41 2023
Response via : Initial Calibration

