

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017632.D
 Acq On : 10 Oct 2023 11:43
 Operator : MA/JU
 Sample : 04654-16
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBW5

Quant Time: Oct 10 23:42:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 04:45:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	116694	20.000	ng/ul	0.00
20) Naphthalene-d8	10.769	136	482576	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.628	164	314351	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.422	188	796664	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	895465	20.000	ng/ul	0.00
88) Perylene-d12	24.139	264	1015694	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.287	96	15067	5.238	ng/uL	0.00
4) Pyridine-d5	3.728	84	95305	11.770	ng/ul	0.01
7) Phenol-d5	7.093	99	74989	7.599	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.275	67	239891	39.196	ng/ul	0.00
11) 2-Chlorophenol-d4	7.452	132	241340	31.090	ng/ul	0.00
15) 4-Methylphenol-d8	8.658	113	156078	19.635	ng/ul	0.01
21) Nitrobenzene-d5	9.140	128	151313	40.692	ng/ul	0.00
24) 2-Nitrophenol-d4	9.857	143	161289	39.493	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.387	165	310111	39.097	ng/ul	0.00
31) 4-Chloroaniline-d4	10.940	131	253862	22.472	ng/ul	0.00
46) Dimethylphthalate-d6	14.046	166	1197592	47.983	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	1230401	45.279	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	26867	7.102	ng/ul	0.02
60) Fluorene-d10	15.634	176	1033574	47.352	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.775	200	187280	39.633	ng/ul	0.00
73) Anthracene-d10	17.522	188	1882951	49.249	ng/ul	0.00
81) Pyrene-d10	19.775	212	2519695	49.330	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.968	264	2680391	50.902	ng/ul	0.01
Target Compounds						
71) Pentachlorophenol	17.045	266	10547	1.683	ng/ul	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017632.D
Acq On : 10 Oct 2023 11:43
Operator : MA/JU
Sample : 04654-16
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBW5

Quant Time: Oct 10 23:42:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 04:45:41 2023
Response via : Initial Calibration

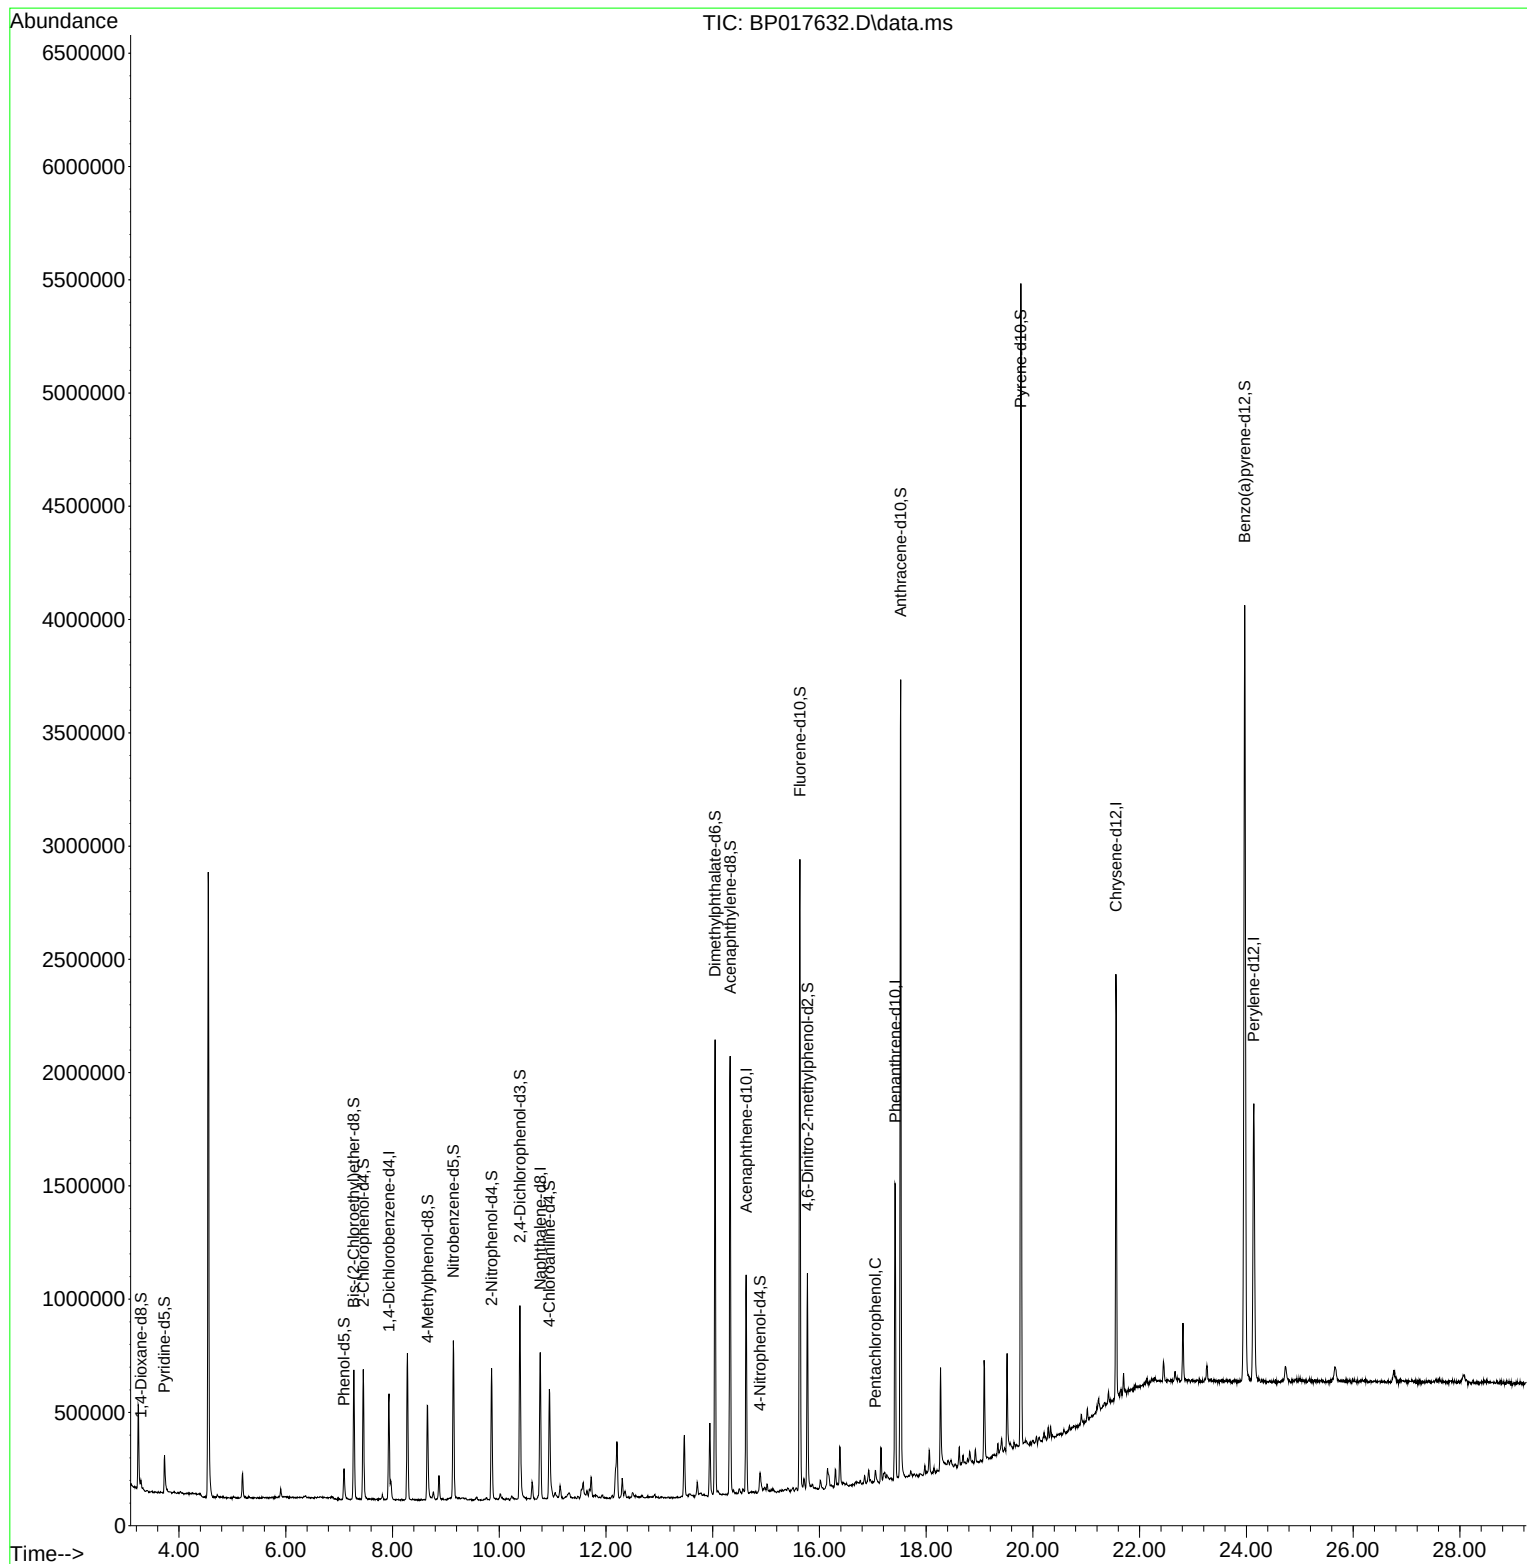

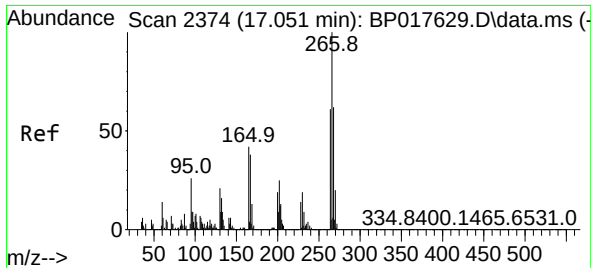

#71
 Pentachlorophenol
 Concen: 1.683 ng/ul
 RT: 17.045 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP017632.D
 Acq: 10 Oct 2023 11:43

Instrument :
 BNA_P
 ClientSampleId :
 BBBW5

Tgt Ion	Ratio	Lower	Upper
266	100		
264	53.7	52.5	78.7
268	58.9	54.6	81.8

