

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017630.D
 Acq On : 10 Oct 2023 10:27
 Operator : MA/JU
 Sample : PB156061BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	41	rVB2	36287	53073	1.50%	0.154%
2	3.717	103	107	119	rBV	414271	641934	18.14%	1.862%
3	4.840	294	298	301	rBV2	6626	10512	0.30%	0.030%
4	5.093	340	341	344	rBV2	5133	5754	0.16%	0.017%
5	5.340	382	383	386	rBV2	5700	5723	0.16%	0.017%
6	5.399	391	393	397	rBV2	5490	7142	0.20%	0.021%
7	6.116	514	515	520	rVB	6789	5917	0.17%	0.017%
8	6.281	542	543	546	rBV	6503	6786	0.19%	0.020%
9	7.081	673	679	691	rBV	489419	811149	22.92%	2.353%
10	7.269	705	711	719	rVB	405112	618789	17.48%	1.795%
11	7.446	734	741	750	rBV	522371	852137	24.07%	2.472%
12	7.922	817	822	830	rBV	468523	768885	21.72%	2.231%
13	8.099	849	852	853	rBV2	7726	7588	0.21%	0.022%
14	8.293	884	885	888	rVB2	6481	5661	0.16%	0.016%
15	8.475	910	916	919	rBV	5996	9689	0.27%	0.028%
16	8.581	930	934	936	rVB2	6304	8229	0.23%	0.024%
17	8.646	938	945	962	rVV	587841	1017665	28.75%	2.952%
18	8.963	995	999	1003	rBV2	4722	6830	0.19%	0.020%
19	9.016	1004	1008	1009	rVB	6618	6795	0.19%	0.020%
20	9.046	1011	1013	1017	rVB	6746	7202	0.20%	0.021%
21	9.093	1017	1021	1022	rBV2	6277	8201	0.23%	0.024%
22	9.134	1022	1028	1041	rVB	466912	809274	22.86%	2.348%
23	9.675	1116	1120	1123	rBV3	5895	9398	0.27%	0.027%
24	9.793	1139	1140	1143	rBV	7505	5775	0.16%	0.017%
25	9.852	1143	1150	1160	rBV	394272	682234	19.27%	1.979%
26	10.381	1233	1240	1252	rBV	551546	1009987	28.53%	2.930%
27	10.616	1276	1280	1282	rBV	6041	8534	0.24%	0.025%
28	10.763	1296	1305	1313	rBV	631438	1074398	30.35%	3.117%
29	10.934	1326	1334	1348	rBV	558790	1042670	29.46%	3.025%
30	11.510	1429	1432	1436	rVB	6641	7880	0.22%	0.023%
31	12.369	1573	1578	1581	rBV3	11474	22547	0.64%	0.065%
32	12.704	1634	1635	1640	rBV2	4807	5645	0.16%	0.016%
33	12.763	1644	1645	1648	rBV	6862	5885	0.17%	0.017%
34	12.798	1648	1651	1654	rVB2	5914	6626	0.19%	0.019%
35	12.922	1669	1672	1675	rBV3	3731	5989	0.17%	0.017%
36	13.457	1759	1763	1767	rBV3	14471	20024	0.57%	0.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017630.D
 Acq On : 10 Oct 2023 10:27
 Operator : MA/JU
 Sample : PB156061BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	13.487	1767	1768	1771	rVB	7233	5760	0.16%	0.017%
38	13.545	1773	1778	1779	rBV5	3740	5689	0.16%	0.017%
39	13.669	1796	1799	1801	rBV	5946	7712	0.22%	0.022%
40	13.845	1822	1829	1831	rVB3	6714	11466	0.32%	0.033%
41	14.034	1855	1861	1873	rBV	1207043	1695020	47.89%	4.918%
42	14.316	1903	1909	1916	rBV	1221782	1806133	51.03%	5.240%
43	14.416	1924	1926	1929	rVB	8168	9005	0.25%	0.026%
44	14.481	1932	1937	1938	rVV2	7766	10927	0.31%	0.032%
45	14.510	1940	1942	1945	rVB	9258	7537	0.21%	0.022%
46	14.622	1954	1961	1970	rBV	1002832	1441147	40.72%	4.181%
47	14.869	1997	2003	2022	rBV	253385	654652	18.50%	1.899%
48	15.322	2077	2080	2082	rVB2	5414	6054	0.17%	0.018%
49	15.469	2103	2105	2110	rVB2	6768	7922	0.22%	0.023%
50	15.622	2125	2131	2139	rBV	1710897	2503215	70.72%	7.262%
51	15.769	2151	2156	2167	rBV2	428510	625079	17.66%	1.813%
52	16.039	2199	2202	2205	rBV2	4983	8618	0.24%	0.025%
53	16.210	2228	2231	2234	rBV2	8510	12182	0.34%	0.035%
54	17.004	2363	2366	2368	rBV2	5916	5862	0.17%	0.017%
55	17.039	2370	2372	2375	rBV	6671	8107	0.23%	0.024%
56	17.063	2375	2376	2378	rBV	7388	6393	0.18%	0.019%
57	17.410	2429	2435	2442	rBV	1350661	1872283	52.90%	5.432%
58	17.510	2446	2452	2466	rBV2	2017575	2909014	82.19%	8.440%
59	19.769	2831	2836	2845	rBV	2851563	3539569	100.00%	10.269%
60	21.551	3134	3139	3146	rBV	1618608	2162091	61.08%	6.273%
61	23.957	3542	3548	3559	rVB2	1658021	3419002	96.59%	9.919%
62	24.127	3572	3577	3588	rVB	1040991	2146040	60.63%	6.226%




Sum of corrected areas: 34469006

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017630.D
Acq On : 10 Oct 2023 10:27
Operator : MA/JU
Sample : PB156061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

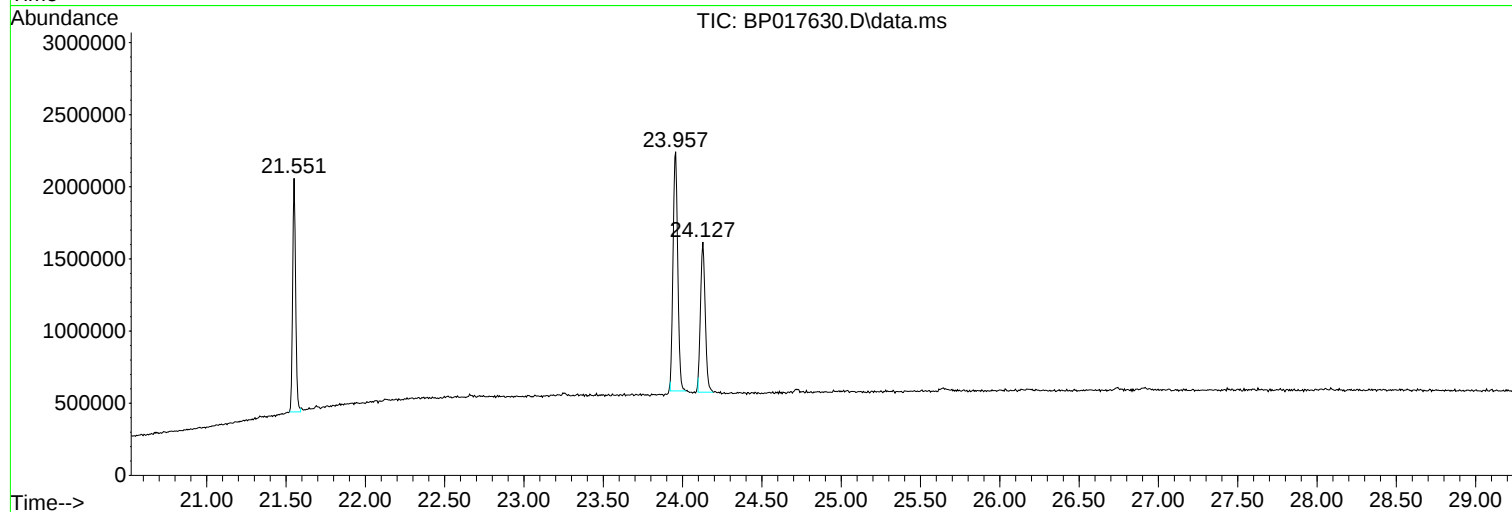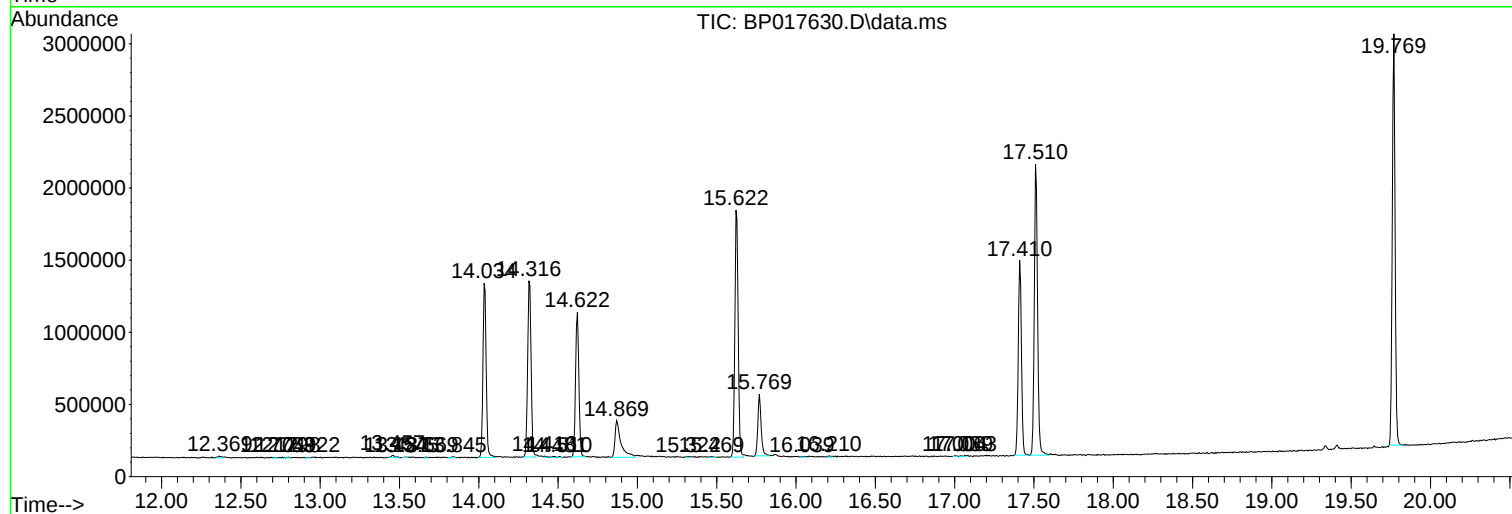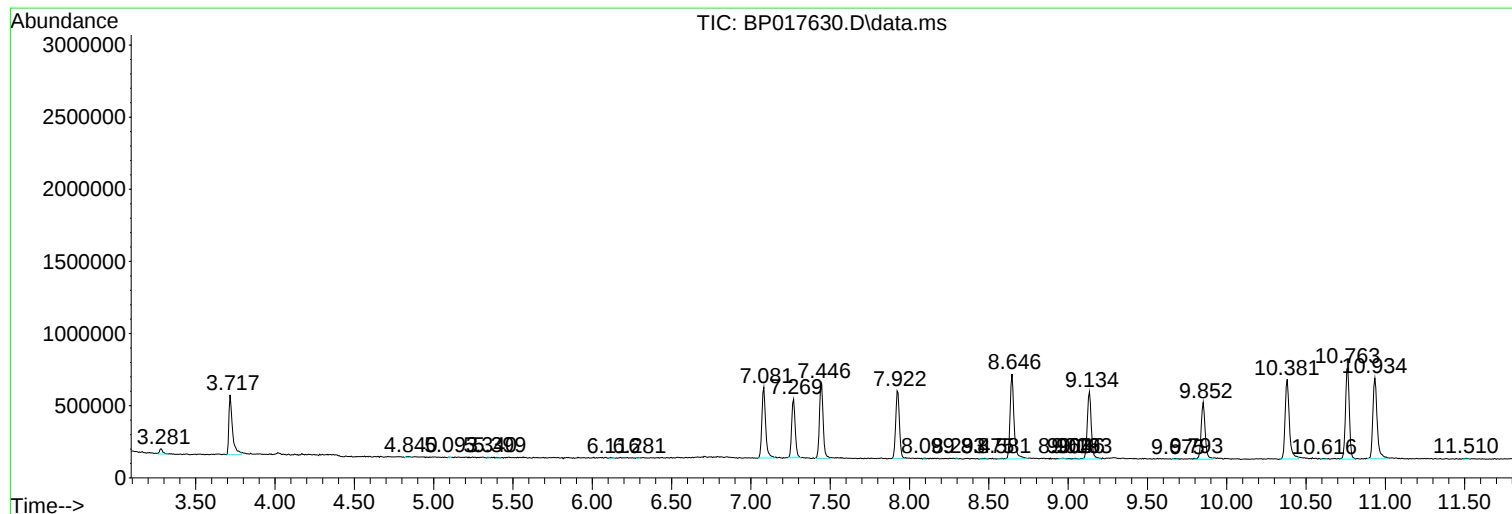

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017630.D
Acq On : 10 Oct 2023 10:27
Operator : MA/JU
Sample : PB156061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017630.D
Acq On : 10 Oct 2023 10:27
Operator : MA/JU
Sample : PB156061BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc