

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017631.D
 Acq On : 10 Oct 2023 11:01
 Operator : MA/JU
 Sample : PB156093BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK093

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	38	rBV	43806	51519	1.35%	0.149%
2	3.505	67	71	73	rBV2	7285	9252	0.24%	0.027%
3	3.716	104	107	121	rBV	463367	720071	18.92%	2.077%
4	3.934	140	144	146	rBV3	7417	10696	0.28%	0.031%
5	4.128	174	177	179	rBV2	6085	7437	0.20%	0.021%
6	5.134	345	348	349	rVB	7079	6205	0.16%	0.018%
7	5.169	349	354	356	rBV2	6619	12768	0.34%	0.037%
8	5.281	369	373	375	rBV4	4323	6582	0.17%	0.019%
9	5.593	425	426	428	rBV2	6342	6048	0.16%	0.017%
10	5.881	470	475	477	rBV3	5211	7771	0.20%	0.022%
11	5.987	491	493	496	rVB	4580	5257	0.14%	0.015%
12	6.022	496	499	500	rBV2	5518	5251	0.14%	0.015%
13	6.134	514	518	521	rVB3	6497	10497	0.28%	0.030%
14	6.316	546	549	553	rVB2	6094	6194	0.16%	0.018%
15	6.428	565	568	571	rVB2	5177	6311	0.17%	0.018%
16	6.599	595	597	601	rVB2	5222	5491	0.14%	0.016%
17	6.634	601	603	607	rBV	8054	8436	0.22%	0.024%
18	6.699	607	614	616	rBV	6657	12291	0.32%	0.035%
19	6.993	663	664	669	rVB2	5890	7101	0.19%	0.020%
20	7.081	672	679	693	rVV	553843	923173	24.26%	2.663%
21	7.269	703	711	720	rBV	456547	706052	18.55%	2.037%
22	7.363	725	727	731	rVB2	6492	8818	0.23%	0.025%
23	7.446	734	741	751	rVV	572551	944847	24.83%	2.725%
24	7.763	793	795	799	rBV2	5554	6945	0.18%	0.020%
25	7.799	799	801	806	rVB2	5301	7419	0.19%	0.021%
26	7.887	812	816	817	rBV	4286	5672	0.15%	0.016%
27	7.922	817	822	829	rVB	341503	543981	14.30%	1.569%
28	8.063	844	846	848	rVB	8565	5532	0.15%	0.016%
29	8.099	850	852	854	rBV	6742	5974	0.16%	0.017%
30	8.646	939	945	958	rVV	644654	1105057	29.04%	3.187%
31	9.057	1011	1015	1018	rBV3	3884	5483	0.14%	0.016%
32	9.134	1021	1028	1036	rBV	536595	889549	23.38%	2.566%
33	9.269	1049	1051	1054	rVV2	5190	6197	0.16%	0.018%
34	9.310	1054	1058	1060	rVB2	4117	6175	0.16%	0.018%
35	9.440	1078	1080	1084	rBV3	5302	7521	0.20%	0.022%
36	9.851	1143	1150	1159	rVV	438649	747305	19.64%	2.156%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017631.D
 Acq On : 10 Oct 2023 11:01
 Operator : MA/JU
 Sample : PB156093BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK093

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	9.987	1171	1173	1176	rVB2	5690	6255	0.16%	0.018%
38	10.057	1181	1185	1186	rBV2	4547	5199	0.14%	0.015%
39	10.163	1201	1203	1206	rVV2	5517	5661	0.15%	0.016%
40	10.210	1208	1211	1214	rVV3	4629	6971	0.18%	0.020%

41	10.281	1220	1223	1226	rBV	4638	5917	0.16%	0.017%
42	10.381	1233	1240	1253	rBV	612154	1134231	29.81%	3.272%
43	10.563	1268	1271	1275	rVV	5497	7327	0.19%	0.021%
44	10.757	1295	1304	1312	rBV	464954	786425	20.67%	2.268%
45	10.840	1316	1318	1321	rVB	7864	5710	0.15%	0.016%

46	10.934	1326	1334	1349	rBV	654380	1173165	30.83%	3.384%
47	11.328	1399	1401	1404	rBV2	5375	5544	0.15%	0.016%
48	11.493	1426	1429	1432	rBV2	5690	6802	0.18%	0.020%
49	11.551	1434	1439	1441	rBV	6921	10115	0.27%	0.029%
50	11.892	1495	1497	1502	rVB3	6154	7740	0.20%	0.022%

51	11.940	1502	1505	1507	rBV2	5218	7635	0.20%	0.022%
52	12.069	1524	1527	1530	rBV	5940	7439	0.20%	0.021%
53	12.269	1559	1561	1564	rBV2	4415	5599	0.15%	0.016%
54	12.363	1573	1577	1578	rBV3	8093	11954	0.31%	0.034%
55	12.922	1667	1672	1673	rBV2	3568	6013	0.16%	0.017%

56	12.987	1679	1683	1684	rBV	6894	6438	0.17%	0.019%
57	13.098	1701	1702	1706	rVB2	5190	5962	0.16%	0.017%
58	13.128	1706	1707	1711	rBV	5778	5970	0.16%	0.017%
59	13.228	1719	1724	1726	rBV	6138	9033	0.24%	0.026%
60	13.463	1758	1764	1767	rBV2	13159	20888	0.55%	0.060%

61	13.498	1767	1770	1773	rVV4	4326	6640	0.17%	0.019%
62	13.692	1801	1803	1806	rVB2	6861	6792	0.18%	0.020%
63	13.734	1806	1810	1811	rBV	7358	8193	0.22%	0.024%
64	13.810	1821	1823	1825	rBV	5682	5904	0.16%	0.017%
65	13.839	1825	1828	1831	rVB2	5147	7654	0.20%	0.022%

66	14.034	1855	1861	1873	rBV	1258116	1831594	48.13%	5.283%
67	14.116	1873	1875	1878	rVB	5826	5413	0.14%	0.016%
68	14.316	1903	1909	1919	rVV	1363546	1996423	52.46%	5.758%
69	14.404	1921	1924	1927	rVV3	7715	12571	0.33%	0.036%
70	14.622	1955	1961	1968	rBV	710935	1049542	27.58%	3.027%

71	14.869	1996	2003	2022	rBV	294799	750264	19.72%	2.164%
72	15.169	2052	2054	2059	rVB2	5852	7976	0.21%	0.023%
73	15.204	2059	2060	2062	rBV	7356	5391	0.14%	0.016%
74	15.322	2077	2080	2082	rBV	5232	6739	0.18%	0.019%
75	15.416	2093	2096	2099	rVB3	4995	5231	0.14%	0.015%

76	15.628	2124	2132	2141	rVV	1823846	2703895	71.06%	7.799%
----	--------	------	------	------	-----	---------	---------	--------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017631.D
 Acq On : 10 Oct 2023 11:01
 Operator : MA/JU
 Sample : PB156093BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK093

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

77	15.698	2141	2144	2147	rVV2	13654	21166	0.56%	0.061%
78	15.769	2150	2156	2170	rVV	481049	758375	19.93%	2.187%
79	15.863	2170	2172	2177	rVV3	14697	26988	0.71%	0.078%
80	15.945	2184	2186	2189	rBV	5209	6342	0.17%	0.018%
81	16.169	2222	2224	2227	rVV	6409	7371	0.19%	0.021%
82	16.210	2229	2231	2234	rVV	7262	7339	0.19%	0.021%
83	16.328	2248	2251	2254	rVV	5818	5859	0.15%	0.017%
84	16.422	2263	2267	2269	rBV	5471	7259	0.19%	0.021%
85	16.563	2288	2291	2293	rBV2	4536	6565	0.17%	0.019%
86	16.798	2330	2331	2336	rVB2	6285	7934	0.21%	0.023%
87	16.845	2336	2339	2342	rBV	5158	6302	0.17%	0.018%
88	17.069	2375	2377	2383	rVB2	6231	11572	0.30%	0.033%
89	17.286	2408	2414	2415	rBV2	5517	9382	0.25%	0.027%
90	17.345	2421	2424	2427	rBV2	5209	6700	0.18%	0.019%
91	17.410	2430	2435	2443	rVV	961206	1355050	35.61%	3.908%
92	17.516	2446	2453	2464	rVV	2131431	3088477	81.16%	8.908%
93	17.833	2505	2507	2510	rBV4	5942	7867	0.21%	0.023%
94	18.022	2537	2539	2542	rBV2	6821	5577	0.15%	0.016%
95	19.339	2759	2763	2769	rBV6	27969	38952	1.02%	0.112%
96	19.410	2772	2775	2781	rVB2	25227	35867	0.94%	0.103%
97	19.769	2830	2836	2845	rBV	2958247	3805289	100.00%	10.976%
98	21.551	3134	3139	3148	rBV	1142063	1606694	42.22%	4.634%
99	23.957	3541	3548	3557	rVB2	1791799	3736294	98.19%	10.777%
100	24.127	3571	3577	3589	rVB	779253	1605257	42.18%	4.630%




Sum of corrected areas: 34669571

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017631.D
Acq On : 10 Oct 2023 11:01
Operator : MA/JU
Sample : PB156093BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

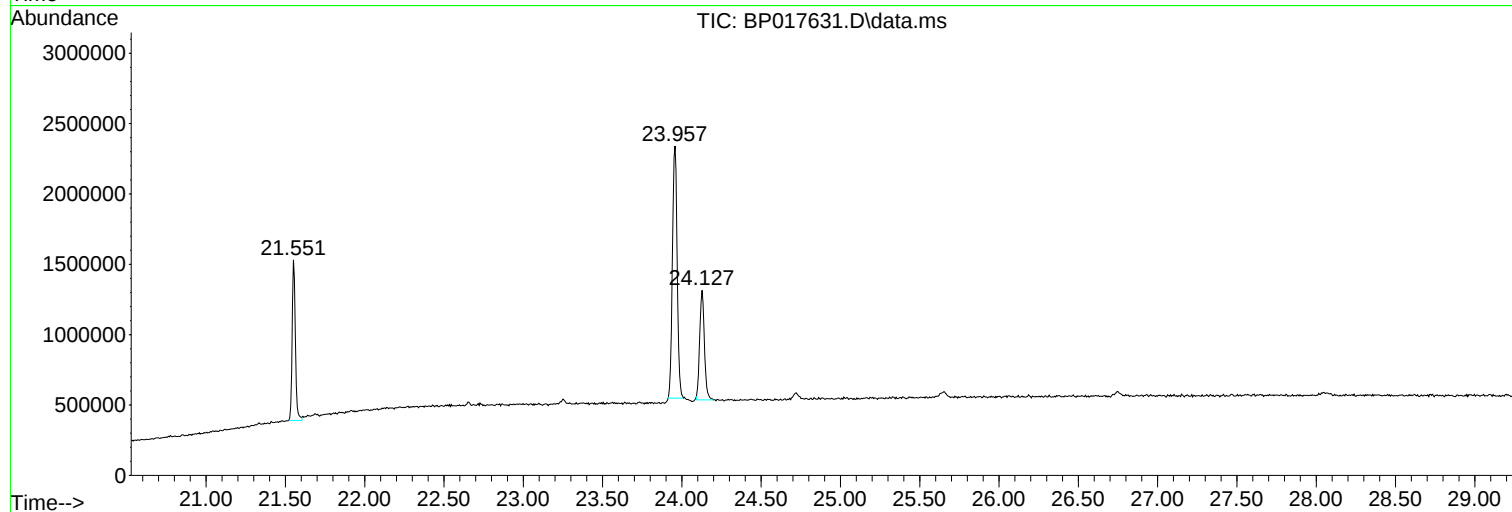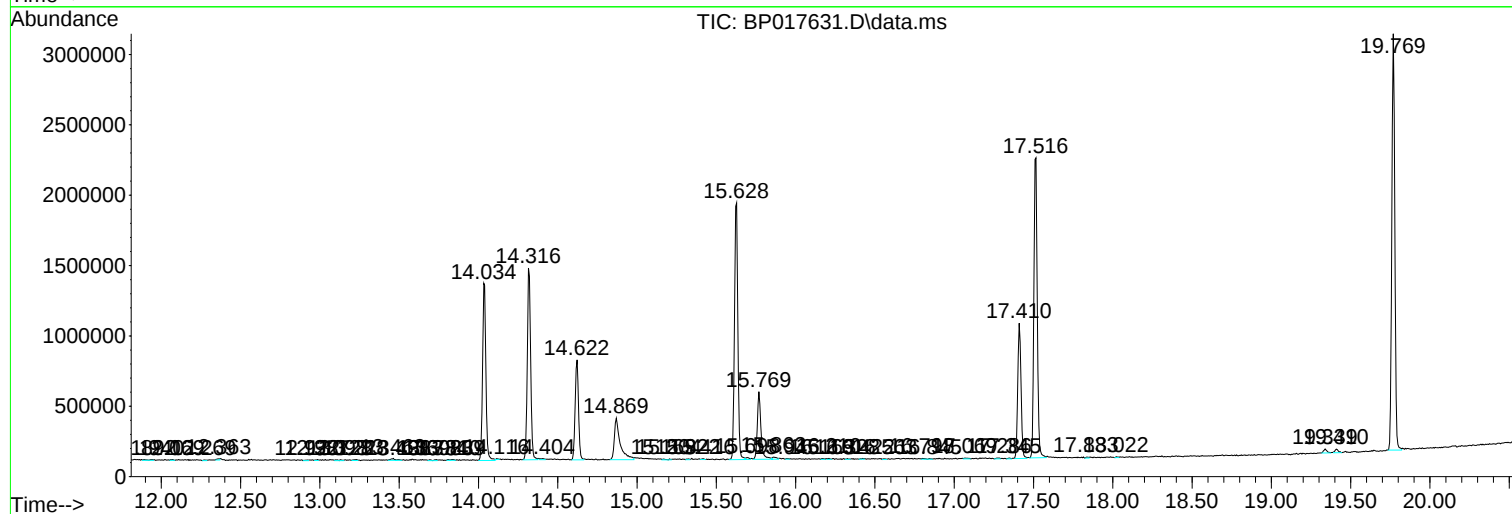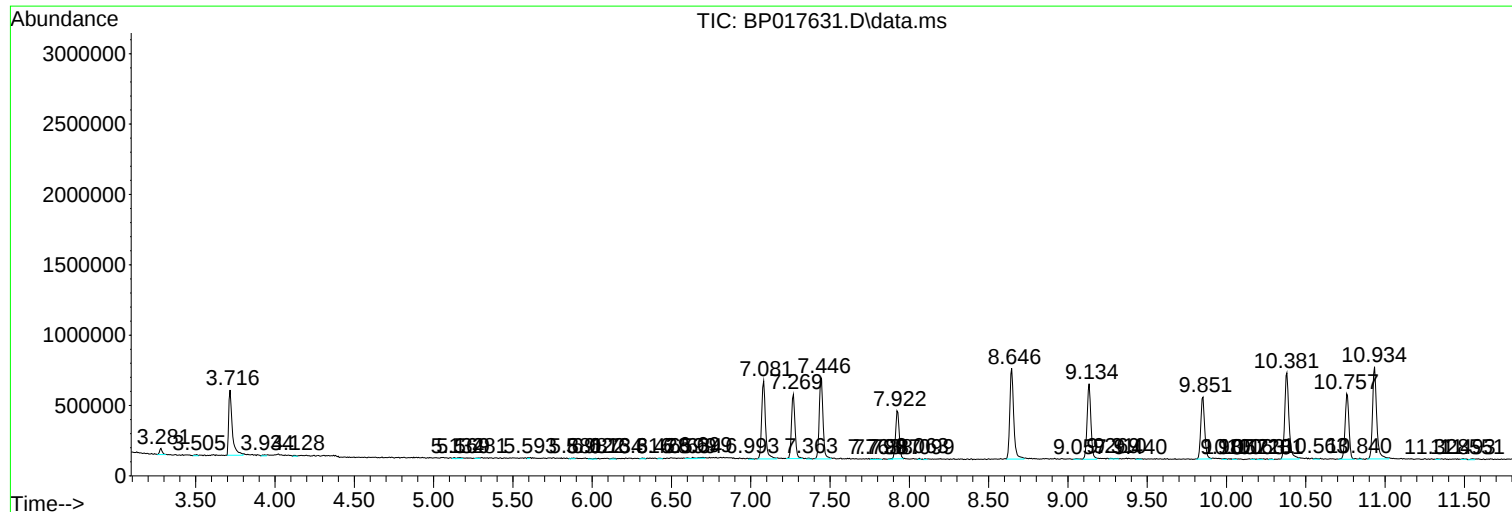

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017631.D
Acq On : 10 Oct 2023 11:01
Operator : MA/JU
Sample : PB156093BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017631.D
Acq On : 10 Oct 2023 11:01
Operator : MA/JU
Sample : PB156093BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------