

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017634.D
 Acq On : 10 Oct 2023 13:14
 Operator : MA/JU
 Sample : 04654-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017634.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	21	25	30	rVV	152900	193103	2.53%	0.373%
2	3.281	30	33	36	rVV2	32063	37933	0.50%	0.073%
3	3.316	36	39	45	rVB3	19385	27692	0.36%	0.054%
4	3.516	71	73	76	rBV3	7536	8607	0.11%	0.017%
5	3.728	106	109	118	rBV2	80101	140360	1.84%	0.271%
6	4.016	155	158	163	rBV	21690	30157	0.39%	0.058%
7	4.352	211	215	218	rBV3	5046	8790	0.12%	0.017%
8	4.540	241	247	262	rBV	5237061	7636357	100.00%	14.767%
9	5.040	329	332	336	rVB	6112	8353	0.11%	0.016%
10	5.181	355	356	360	rVB4	6855	7770	0.10%	0.015%
11	5.228	360	364	365	rBV3	7227	8504	0.11%	0.016%
12	5.634	427	433	434	rBV	5395	8181	0.11%	0.016%
13	6.128	514	517	520	rBV2	5451	8969	0.12%	0.017%
14	6.581	592	594	597	rBV	6740	9164	0.12%	0.018%
15	7.087	674	680	689	rBV2	139715	245651	3.22%	0.475%
16	7.199	698	699	703	rVB	7708	7792	0.10%	0.015%
17	7.269	703	711	720	rBV	567277	909940	11.92%	1.760%
18	7.446	734	741	750	rBV	580075	942852	12.35%	1.823%
19	7.922	816	822	830	rBV	433738	690826	9.05%	1.336%
20	8.046	840	843	847	rVB3	4949	7954	0.10%	0.015%
21	8.275	879	882	885	rBV2	7724	10680	0.14%	0.021%
22	8.587	933	935	938	rBV2	6847	8634	0.11%	0.017%
23	8.646	938	945	958	rVV	431644	736022	9.64%	1.423%
24	8.969	997	1000	1003	rVB	8972	10191	0.13%	0.020%
25	9.010	1003	1007	1009	rBV	6283	8485	0.11%	0.016%
26	9.134	1016	1028	1037	rBV	691198	1177180	15.42%	2.276%
27	9.634	1109	1113	1116	rBV	6114	9191	0.12%	0.018%
28	9.851	1141	1150	1162	rBV	585003	1001549	13.12%	1.937%
29	10.298	1221	1226	1229	rBV2	7237	9780	0.13%	0.019%
30	10.381	1231	1240	1255	rVV	745286	1408609	18.45%	2.724%
31	10.481	1255	1257	1261	rVV2	9448	13755	0.18%	0.027%
32	10.757	1295	1304	1315	rBV	577478	996889	13.05%	1.928%
33	10.934	1326	1334	1346	rBV	591885	1068321	13.99%	2.066%
34	11.116	1362	1365	1368	rBV	6112	7758	0.10%	0.015%
35	11.751	1472	1473	1477	rBV	6718	8257	0.11%	0.016%
36	11.869	1488	1493	1496	rBV	6311	11279	0.15%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017634.D
 Acq On : 10 Oct 2023 13:14
 Operator : MA/JU
 Sample : 04654-18
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BBBW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	12.075	1527	1528	1532	rBV	6593	8156	0.11%	0.016%
38	12.357	1571	1576	1580	rBV4	13213	20721	0.27%	0.040%
39	12.969	1679	1680	1684	rBV2	6291	8779	0.11%	0.017%
40	13.410	1752	1755	1757	rBV2	8548	8445	0.11%	0.016%
41	13.463	1760	1764	1768	rVB4	15457	25906	0.34%	0.050%
42	14.039	1855	1862	1872	rBV	1810962	2573197	33.70%	4.976%
43	14.110	1872	1874	1878	rVB	7233	9648	0.13%	0.019%
44	14.316	1903	1909	1918	rBV	1865560	2797154	36.63%	5.409%
45	14.622	1954	1961	1969	rBV	958888	1369244	17.93%	2.648%
46	14.881	2000	2005	2020	rBV3	60935	188828	2.47%	0.365%
47	15.086	2036	2040	2042	rBV	8649	10249	0.13%	0.020%
48	15.563	2119	2121	2124	rBV2	6453	8396	0.11%	0.016%
49	15.628	2124	2132	2140	rBV	2711498	3826192	50.10%	7.399%
50	15.710	2142	2146	2150	rVV3	30498	55793	0.73%	0.108%
51	15.769	2150	2156	2169	rVV	824648	1198268	15.69%	2.317%
52	15.863	2169	2172	2178	rVB6	17208	33271	0.44%	0.064%
53	16.922	2348	2352	2355	rBV4	13840	19759	0.26%	0.038%
54	17.057	2372	2375	2378	rBV	9107	10947	0.14%	0.021%
55	17.198	2396	2399	2403	rVB2	8323	12424	0.16%	0.024%
56	17.410	2429	2435	2442	rVV	1277198	1764486	23.11%	3.412%
57	17.510	2446	2452	2465	rVV	3143223	4497409	58.89%	8.697%
58	17.827	2502	2506	2508	rBV4	8412	13031	0.17%	0.025%
59	18.263	2576	2580	2587	rBV3	53189	77600	1.02%	0.150%
60	19.339	2759	2763	2768	rBV4	40191	61523	0.81%	0.119%
61	19.410	2772	2775	2779	rVB2	43538	53368	0.70%	0.103%
62	19.504	2788	2791	2797	rBV5	55995	80540	1.05%	0.156%
63	19.769	2830	2836	2845	rBV	4364733	5577316	73.04%	10.785%
64	21.551	3134	3139	3149	rBV	1558409	2073183	27.15%	4.009%
65	23.957	3541	3548	3566	rVB2	2725053	5786555	75.78%	11.190%
66	24.127	3571	3577	3589	rVB	972642	2117200	27.73%	4.094%




Sum of corrected areas: 51713123

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017634.D
Acq On : 10 Oct 2023 13:14
Operator : MA/JU
Sample : 04654-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

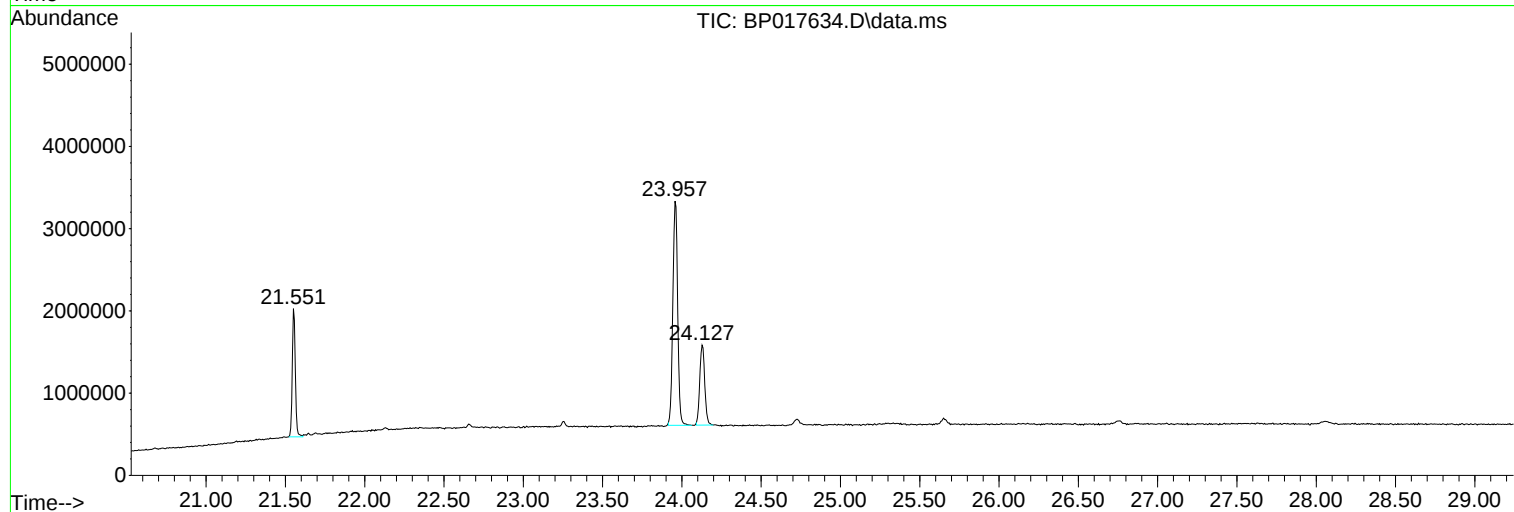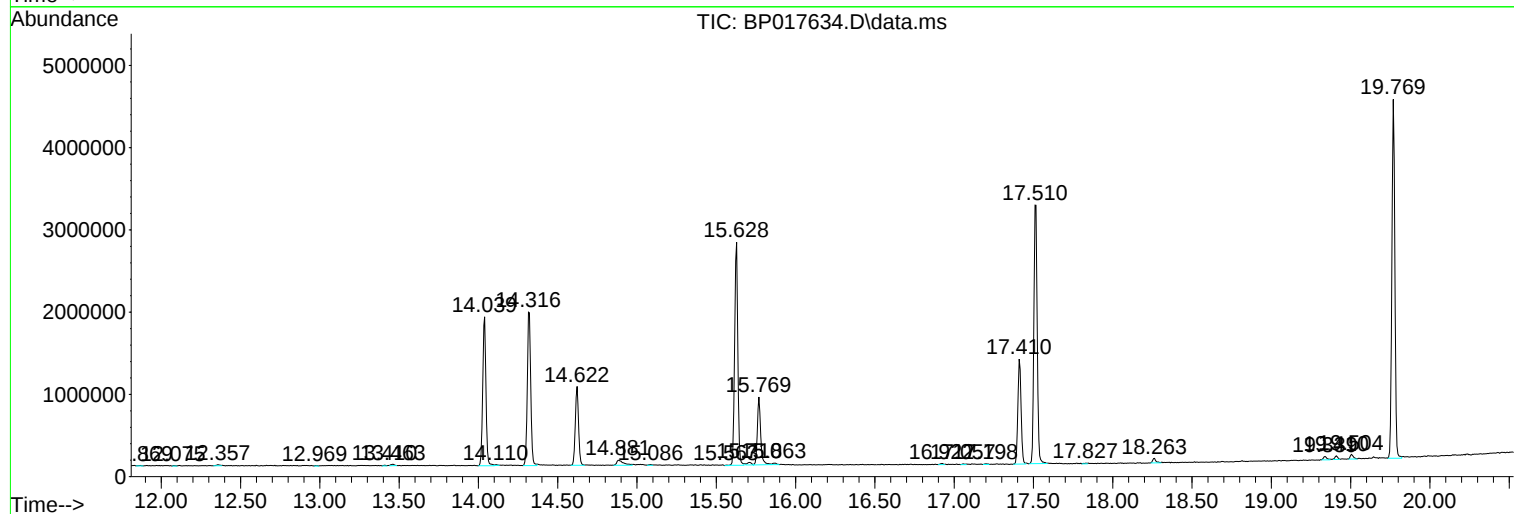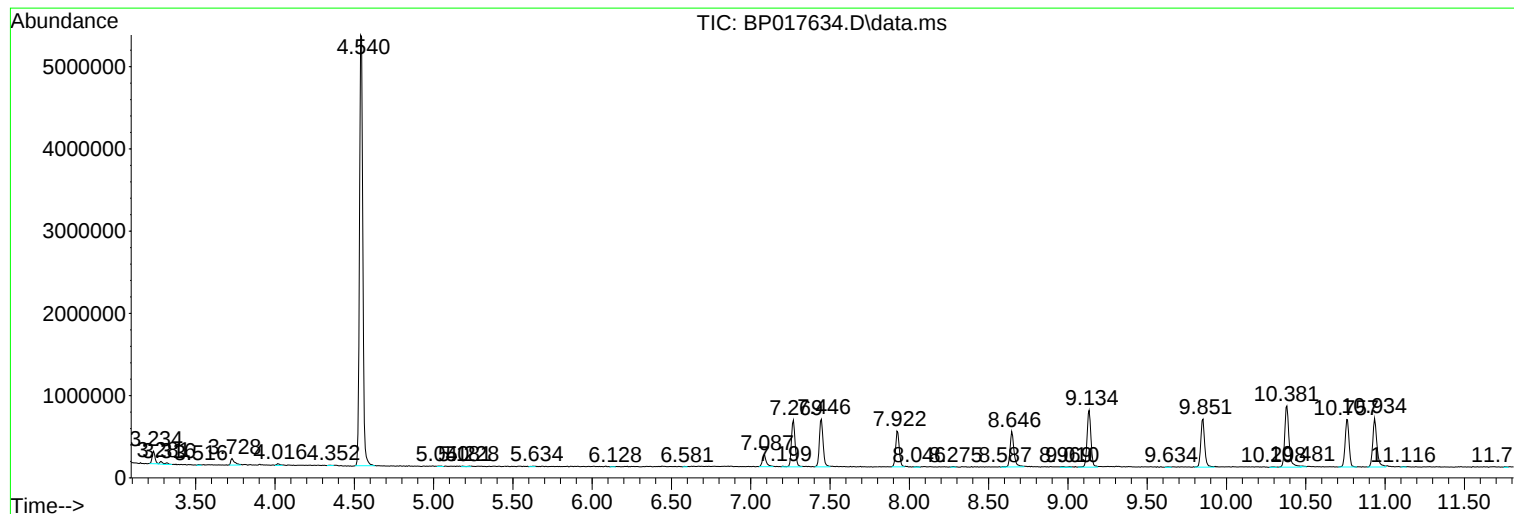

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017634.D
Acq On : 10 Oct 2023 13:14
Operator : MA/JU
Sample : 04654-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017634.D
Acq On : 10 Oct 2023 13:14
Operator : MA/JU
Sample : 04654-18
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BBBW7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc