

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017641.D
 Acq On : 10 Oct 2023 17:22
 Operator : MA/JU
 Sample : 04796-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.363	385	387	390	rBV	6936	7685	0.43%	0.093%
2	5.522	412	414	415	rVB	9202	4885	0.27%	0.059%
3	5.916	479	481	483	rBV	8169	6256	0.35%	0.075%
4	5.969	487	490	491	rBV	6675	7145	0.40%	0.086%
5	6.693	611	613	615	rBV3	5779	6670	0.37%	0.080%
6	7.099	680	682	684	rVB	5645	4491	0.25%	0.054%
7	7.199	697	699	702	rBV2	4119	4901	0.27%	0.059%
8	7.369	726	728	733	rBV3	5995	8360	0.47%	0.101%
9	7.581	759	764	767	rBV3	3962	6393	0.36%	0.077%
10	7.787	797	799	802	rVB3	6516	5591	0.31%	0.067%
11	7.934	818	824	831	rVV	389926	618392	34.61%	7.462%
12	8.440	907	910	911	rBV2	4201	4473	0.25%	0.054%
13	8.593	935	936	940	rVV	6017	5797	0.32%	0.070%
14	8.663	943	948	952	rBV	6676	11000	0.62%	0.133%
15	8.810	971	973	976	rVV	6750	7381	0.41%	0.089%
16	8.846	976	979	980	rVV3	5688	5041	0.28%	0.061%
17	8.875	983	984	987	rVV	5309	4608	0.26%	0.056%
18	8.904	987	989	994	rVB	5156	6061	0.34%	0.073%
19	9.134	1027	1028	1032	rBV	4652	4580	0.26%	0.055%
20	9.310	1055	1058	1061	rVB	5306	6082	0.34%	0.073%
21	9.551	1098	1099	1103	rVB	5753	5182	0.29%	0.063%
22	9.593	1103	1106	1108	rBV2	5325	6371	0.36%	0.077%
23	9.722	1125	1128	1133	rBV3	4413	8546	0.48%	0.103%
24	9.946	1164	1166	1168	rBV3	6654	6338	0.35%	0.076%
25	10.075	1187	1188	1192	rVB	6625	4637	0.26%	0.056%
26	10.228	1210	1214	1216	rVB2	3729	5231	0.29%	0.063%
27	10.246	1216	1217	1220	rBV	4592	4548	0.25%	0.055%
28	10.487	1255	1258	1260	rVB2	6108	5655	0.32%	0.068%
29	10.516	1260	1263	1264	rBV	8887	7566	0.42%	0.091%
30	10.657	1282	1287	1290	rBV	6379	13443	0.75%	0.162%
31	10.769	1299	1306	1316	rBV	496829	856645	47.95%	10.337%
32	10.869	1321	1323	1326	rVV	10132	13389	0.75%	0.162%
33	10.898	1326	1328	1330	rVV	8947	6603	0.37%	0.080%
34	10.922	1330	1332	1335	rVV3	7148	9756	0.55%	0.118%
35	10.969	1338	1340	1343	rVV2	4908	6054	0.34%	0.073%
36	11.034	1349	1351	1353	rVV	7295	5539	0.31%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017641.D
 Acq On : 10 Oct 2023 17:22
 Operator : MA/JU
 Sample : 04796-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	11.198	1376	1379	1381	rBV2	4606	5273	0.30%	0.064%
38	11.428	1415	1418	1420	rVV	4474	5847	0.33%	0.071%
39	11.463	1422	1424	1430	rVB5	3476	5608	0.31%	0.068%
40	11.593	1443	1446	1449	rVB3	4287	5144	0.29%	0.062%
41	11.640	1452	1454	1458	rBV	7366	9942	0.56%	0.120%
42	11.998	1513	1515	1519	rVB2	5504	6063	0.34%	0.073%
43	12.075	1521	1528	1529	rBV2	4777	6947	0.39%	0.084%
44	12.298	1564	1566	1567	rVV	6216	4661	0.26%	0.056%
45	12.334	1571	1572	1575	rVV2	5272	5548	0.31%	0.067%
46	12.363	1575	1577	1580	rVB	4796	5876	0.33%	0.071%
47	12.393	1580	1582	1584	rBV	6218	4584	0.26%	0.055%
48	12.616	1618	1620	1624	rVB2	4008	4719	0.26%	0.057%
49	12.698	1630	1634	1636	rVB4	3362	4336	0.24%	0.052%
50	12.857	1659	1661	1664	rVB	5745	5498	0.31%	0.066%
51	12.892	1664	1667	1670	rBV3	4285	6806	0.38%	0.082%
52	13.022	1683	1689	1693	rVB2	4061	6672	0.37%	0.081%
53	13.104	1702	1703	1708	rVB2	4350	4417	0.25%	0.053%
54	13.222	1717	1723	1725	rBV	5835	9904	0.55%	0.120%
55	13.251	1725	1728	1730	rVB	4749	5077	0.28%	0.061%
56	13.316	1735	1739	1740	rVB2	4693	4873	0.27%	0.059%
57	13.392	1749	1752	1755	rVV	3965	5511	0.31%	0.067%
58	13.445	1755	1761	1762	rVV2	3820	5611	0.31%	0.068%
59	13.481	1762	1767	1769	rVV6	8998	12781	0.72%	0.154%
60	13.498	1769	1770	1775	rVB2	5893	5075	0.28%	0.061%
61	13.540	1775	1777	1779	rBV2	6046	6473	0.36%	0.078%
62	13.569	1781	1782	1787	rVV2	4792	5150	0.29%	0.062%
63	13.745	1810	1812	1814	rVB	6260	4831	0.27%	0.058%
64	13.763	1814	1815	1818	rBV	6483	6725	0.38%	0.081%
65	13.822	1822	1825	1826	rBV	4669	4754	0.27%	0.057%
66	13.845	1826	1829	1830	rBV2	9378	7899	0.44%	0.095%
67	13.922	1836	1842	1844	rVB3	5896	8789	0.49%	0.106%
68	14.022	1857	1859	1861	rBV2	4555	4537	0.25%	0.055%
69	14.110	1869	1874	1876	rBV2	3547	5108	0.29%	0.062%
70	14.263	1897	1900	1902	rBV2	5999	6024	0.34%	0.073%
71	14.398	1919	1923	1925	rVB2	4410	5027	0.28%	0.061%
72	14.463	1931	1934	1935	rBV	6832	6156	0.34%	0.074%
73	14.481	1935	1937	1938	rVB	6872	4658	0.26%	0.056%
74	14.575	1948	1953	1955	rBV2	5510	7029	0.39%	0.085%
75	14.628	1955	1962	1976	rBV	708283	1154007	64.59%	13.926%
76	14.763	1983	1985	1987	rBV2	4272	4623	0.26%	0.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
 Data File : BP017641.D
 Acq On : 10 Oct 2023 17:22
 Operator : MA/JU
 Sample : 04796-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

77	15.004	2025	2026	2030	rVB2	4681	4407	0.25%	0.053%
78	15.045	2030	2033	2038	rBV3	4662	9045	0.51%	0.109%
79	15.110	2042	2044	2046	rVB	6570	5215	0.29%	0.063%
80	15.286	2072	2074	2076	rBV	6646	7149	0.40%	0.086%
81	15.398	2091	2093	2095	rBV	4759	5207	0.29%	0.063%
82	15.422	2095	2097	2100	rVB2	9095	10000	0.56%	0.121%
83	15.504	2109	2111	2113	rBV	5905	4923	0.28%	0.059%
84	15.739	2149	2151	2156	rBV	4548	6700	0.38%	0.081%
85	16.122	2213	2216	2217	rBV	8643	8240	0.46%	0.099%
86	16.181	2222	2226	2230	rVV4	5570	10552	0.59%	0.127%
87	16.216	2230	2232	2235	rVV	6858	6787	0.38%	0.082%
88	16.481	2275	2277	2280	rVB2	5246	5260	0.29%	0.063%
89	16.692	2309	2313	2315	rVB	11283	15031	0.84%	0.181%
90	16.710	2315	2316	2318	rBV2	6430	5837	0.33%	0.070%
91	16.804	2330	2332	2335	rBV2	5149	4306	0.24%	0.052%
92	16.904	2346	2349	2350	rBV	6992	6565	0.37%	0.079%
93	17.033	2368	2371	2372	rVB2	6331	4566	0.26%	0.055%
94	17.086	2376	2380	2383	rVV	6199	9441	0.53%	0.114%
95	17.210	2399	2401	2404	rVB	6962	6783	0.38%	0.082%
96	17.263	2408	2410	2412	rBV	6160	4335	0.24%	0.052%
97	17.422	2429	2437	2450	rBV	963271	1562872	87.48%	18.860%
98	18.039	2540	2542	2546	rVB2	6784	4853	0.27%	0.059%
99	21.557	3136	3140	3152	rBV	1280069	1786546	100.00%	21.559%
100	24.139	3574	3579	3591	rVB	812485	1702385	95.29%	20.543%



Sum of corrected areas: 8286863

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017641.D
Acq On : 10 Oct 2023 17:22
Operator : MA/JU
Sample : 04796-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

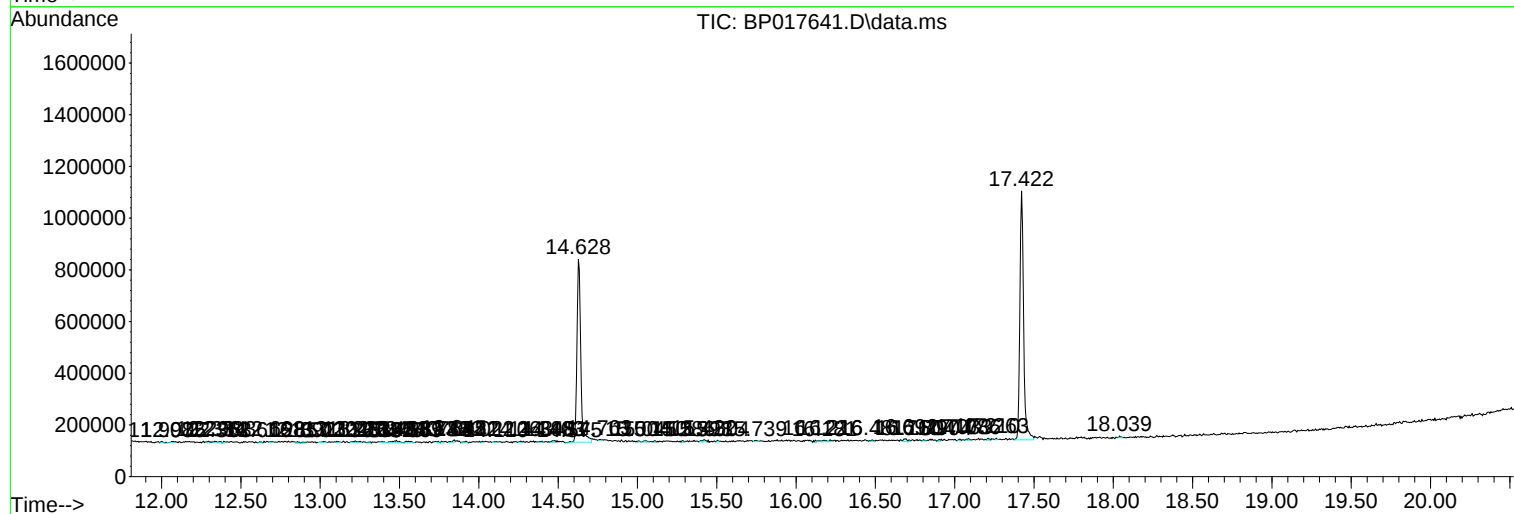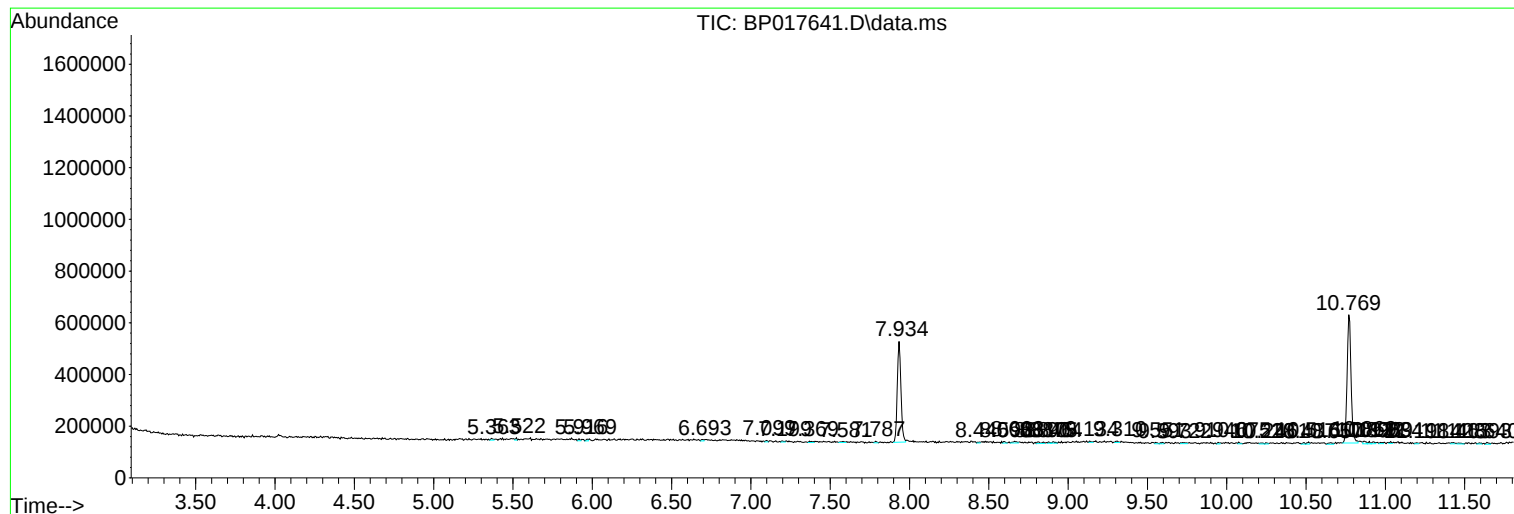

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017641.D
Acq On : 10 Oct 2023 17:22
Operator : MA/JU
Sample : 04796-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101023\
Data File : BP017641.D
Acq On : 10 Oct 2023 17:22
Operator : MA/JU
Sample : 04796-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------