

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101119\
 Data File : BP000633.D
 Acq On : 11 Oct 2019 15:58
 Operator : JU
 Sample : PB123860BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB123860BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	554	559	562	rBV	5242125	5021787	55.79%	8.708%
2	6.387	726	731	734	rBV	4790937	5194411	57.70%	9.007%
3	6.522	749	754	757	rBV	5908466	5418349	60.19%	9.395%
4	6.746	789	792	796	rBV	1712914	1394934	15.50%	2.419%
5	6.905	815	819	822	rBV	5665520	4720062	52.44%	8.185%
6	7.310	883	888	891	rBV	3835250	3357540	37.30%	5.822%
7	8.034	1007	1011	1014	rBV	1971507	1768251	19.64%	3.066%
8	9.116	1190	1195	1198	rBV	8541671	7380013	81.98%	12.797%
9	9.793	1307	1310	1314	rBV	2647087	2232340	24.80%	3.871%
10	10.593	1441	1446	1449	rBV	5214405	4659910	51.77%	8.080%
11	11.293	1561	1565	1568	rBV	3083189	2493786	27.70%	4.324%
12	12.904	1834	1839	1842	rBV	8878640	9001738	100.00%	15.609%
13	13.963	2015	2019	2023	rBV	2853844	2538418	28.20%	4.402%
14	15.439	2264	2270	2276	rBV	2065683	2488615	27.65%	4.315%


Sum of corrected areas: 57670154

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101119\
Data File : BP000633.D
Acq On : 11 Oct 2019 15:58
Operator : JU
Sample : PB123860BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123860BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

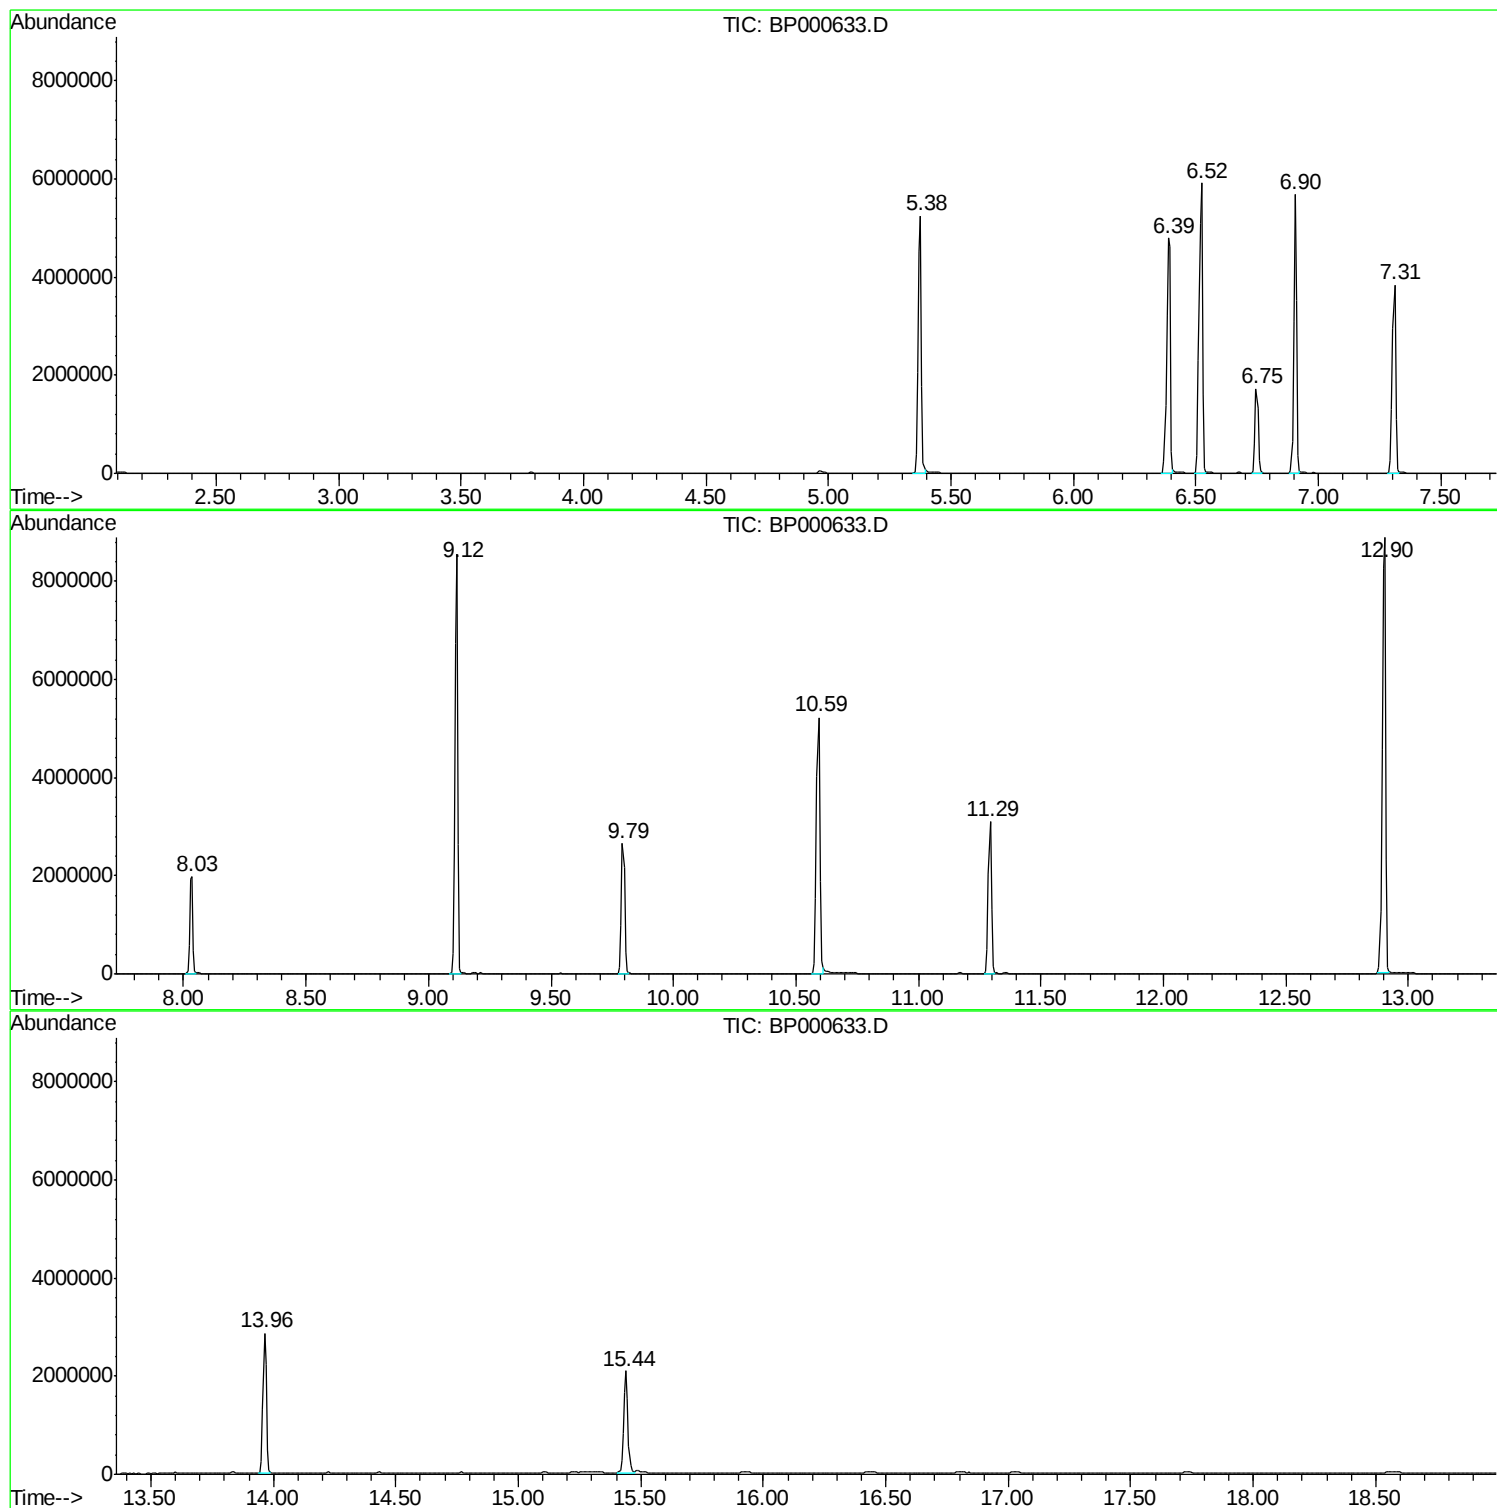

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101119\
Data File : BP000633.D
Acq On : 11 Oct 2019 15:58
Operator : JU
Sample : PB123860BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123860BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	77.69 ng	5418350	1,4-Dichlorobenzene-d4	6.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranvlcvpromine-propionyl	189	C12H15NO	1000123-86-3	16
2		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	12
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
4		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

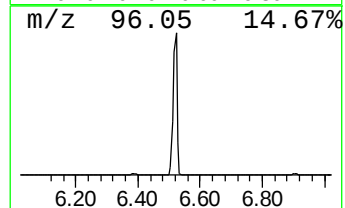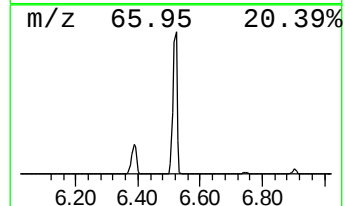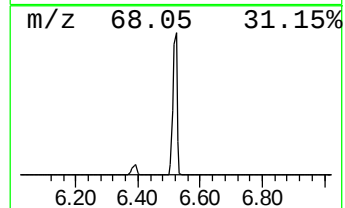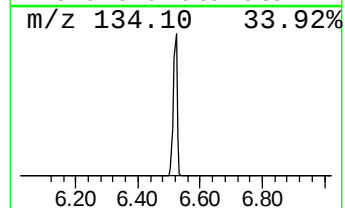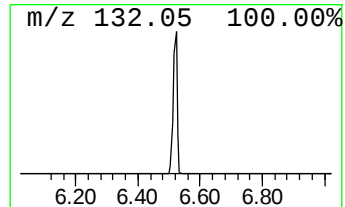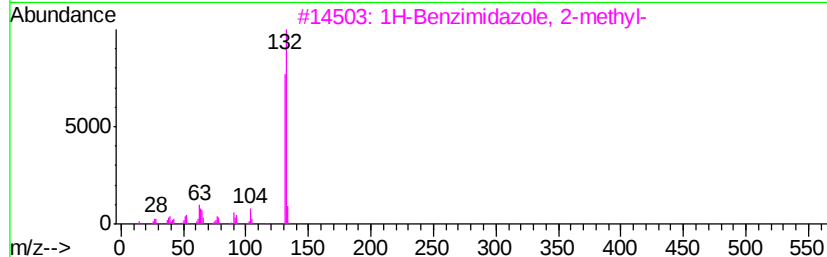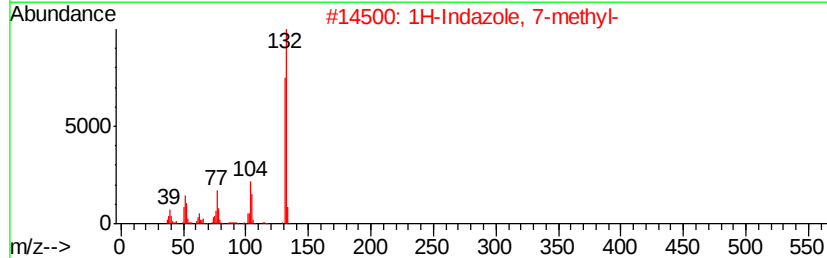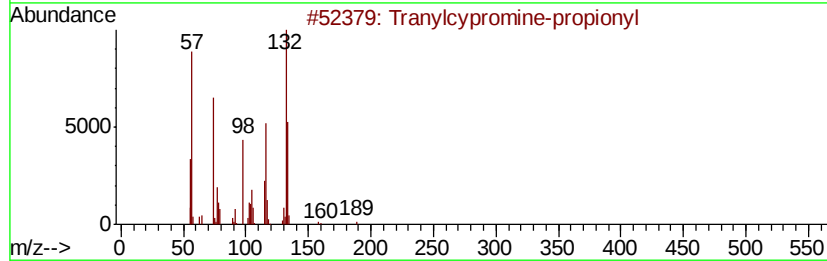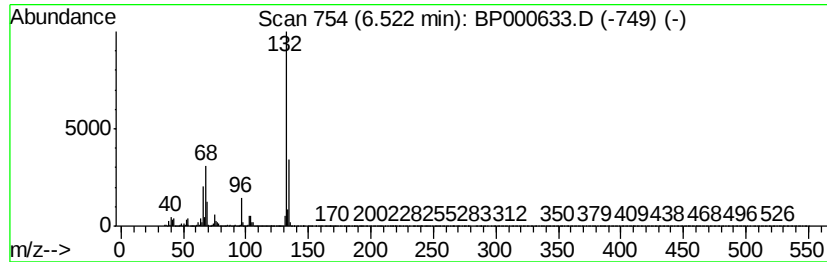

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101119\
Data File : BP000633.D
Acq On : 11 Oct 2019 15:58
Operator : JU
Sample : PB123860BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123860BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.52	6.52	77.7	ng	5418350	1	6.75	1394930	20.0