


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101119\
 Data File : BP000630.D
 Acq On : 11 Oct 2019 14:21
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 01 18:03:42 2019

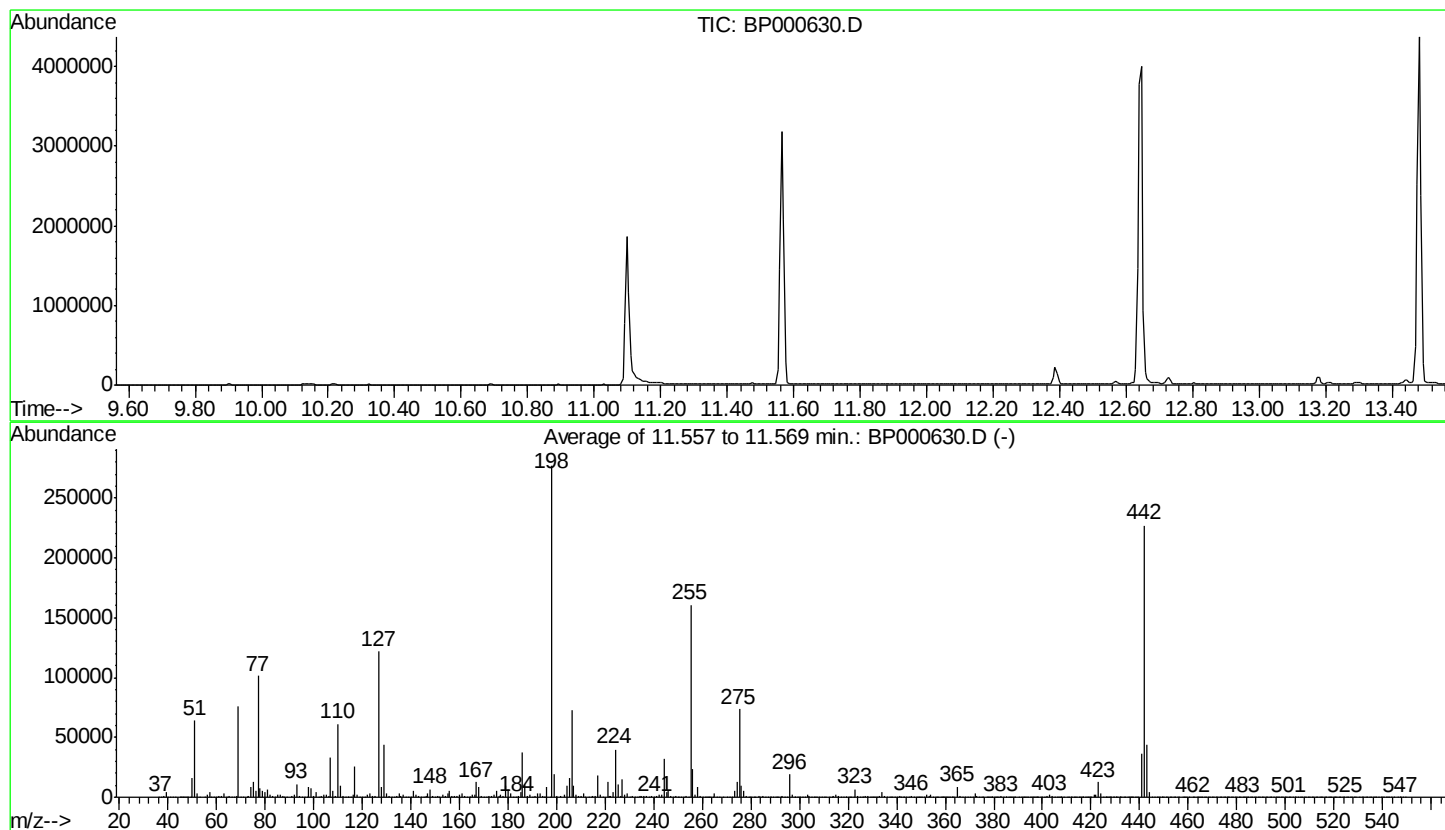

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.0	63684	PASS
68	69	0.00	2	1.8	1372	PASS
69	198	0.00	100	27.5	76284	PASS
70	69	0.00	2	0.5	383	PASS
127	198	10	80	44.0	121785	PASS
197	198	0.00	2	0.2	548	PASS
198	198	100	100	100.0	277034	PASS
199	198	5	9	7.0	19339	PASS
275	198	10	60	26.5	73485	PASS
365	198	1	100	3.2	8825	PASS
441	198	0.01	100	13.0	36100	PASS
442	198	50	100	82.0	227242	PASS
443	442	15	24	19.5	44349	PASS