




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017648.D
 Acq On : 11 Oct 2023 15:47
 Operator : MA/JU
 Sample : 04360-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLDA7

Manual IntegrationsAPPROVED

Quant Time: Oct 12 02:22:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 04:45:41 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/12/2023
 Supervised By :mohammad ahmed 10/13/2023

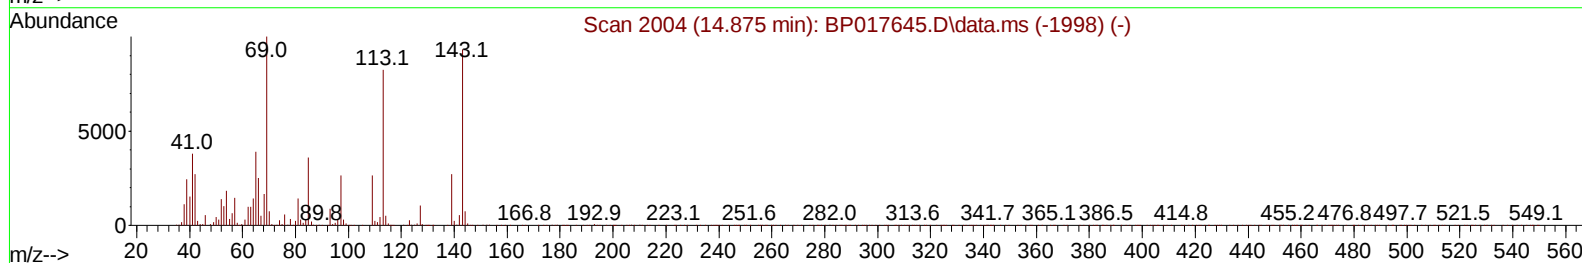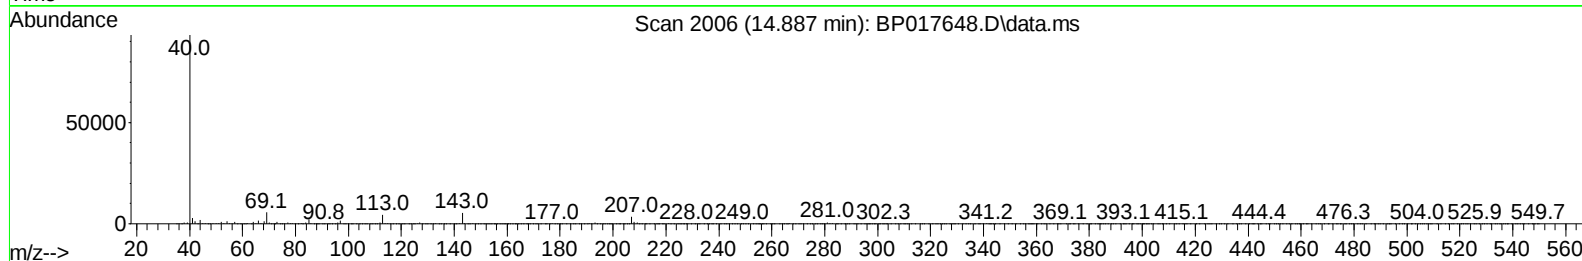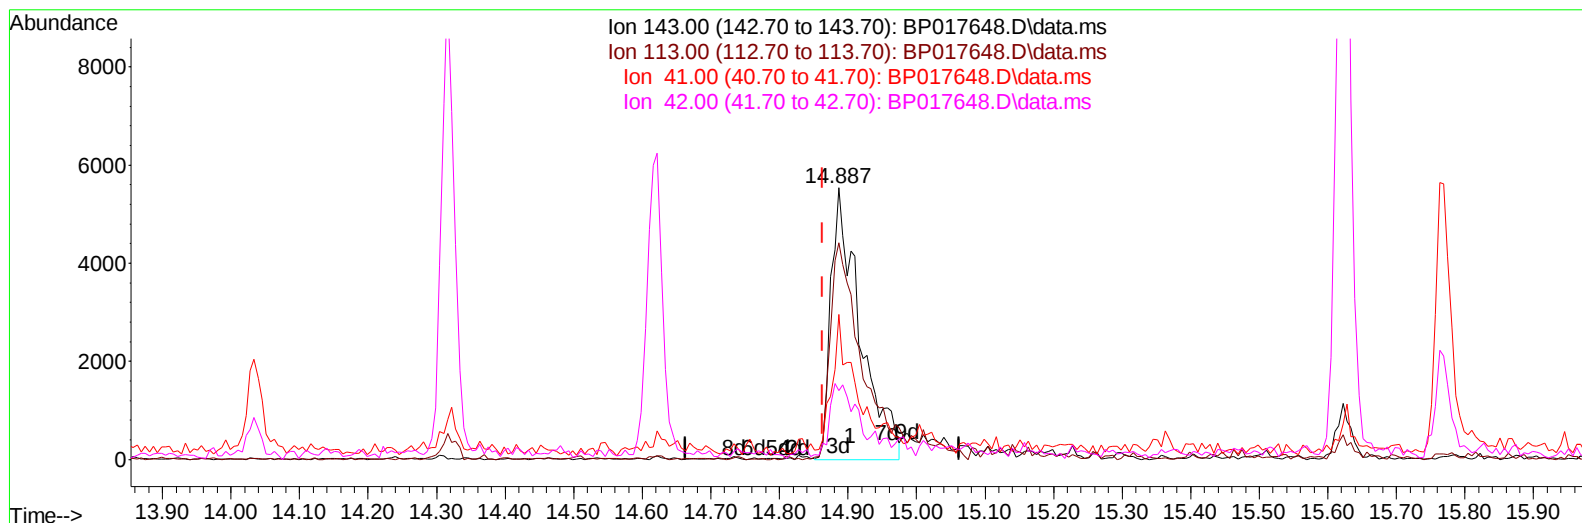

TIC: BP017648.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.887min (+ 0.024) 5.83 ng/ul m

response 16400

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	84.70	79.87
41.00	43.90	53.32#
42.00	26.40	25.48

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017648.D
 Acq On : 11 Oct 2023 15:47
 Operator : MA/JU
 Sample : 04360-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLDA7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/12/2023
 Supervised By :mohammad ahmed 10/13/2023

Quant Time: Oct 12 02:57:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 10 04:45:41 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.922	152	89388	20.000	ng/ul	0.00
20) Naphthalene-d8	10.757	136	360251	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.616	164	233847	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.410	188	551292	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	557606	20.000	ng/ul	0.00
88) Perylene-d12	24.127	264	644678	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	7042	3.196	ng/uL	0.00
4) Pyridine-d5	3.723	84	68941	11.115	ng/ul	0.00
7) Phenol-d5	7.081	99	61649	8.155	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.264	67	175724	37.483	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	173995	29.261	ng/ul	0.00
15) 4-Methylphenol-d8	8.646	113	113216	18.594	ng/ul	0.00
21) Nitrobenzene-d5	9.134	128	104852	37.772	ng/ul	0.00
24) 2-Nitrophenol-d4	9.852	143	109535	35.928	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	194103	32.781	ng/ul	0.00
31) 4-Chloroaniline-d4	10.934	131	258383	30.638	ng/ul	0.00
46) Dimethylphthalate-d6	14.034	166	791190	42.613	ng/ul	0.00
49) Acenaphthylene-d8	14.316	160	809459	40.043	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	16400m	5.828	ng/ul	0.02
60) Fluorene-d10	15.622	176	698724	43.032	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	97507	29.819	ng/ul	0.00
73) Anthracene-d10	17.510	188	1180934	44.635	ng/ul	0.00
81) Pyrene-d10	19.769	212	1469052	46.188	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.957	264	1487618	44.509	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017648.D
Acq On : 11 Oct 2023 15:47
Operator : MA/JU
Sample : 04360-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JLDA7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/12/2023
Supervised By :mohammad ahmed 10/13/2023

Quant Time: Oct 12 02:57:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 10 04:45:41 2023
Response via : Initial Calibration

