

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017646.D
 Acq On : 11 Oct 2023 14:39
 Operator : MA/JU
 Sample : PB156277BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017646.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	31	33	39	rVB2	36976	50002	1.42%	0.145%
2	3.723	104	108	120	rBV	410241	647933	18.42%	1.882%
3	4.887	303	306	308	rBV3	7510	8901	0.25%	0.026%
4	4.946	311	316	319	rVB2	10233	16558	0.47%	0.048%
5	4.993	322	324	327	rBV2	5814	6688	0.19%	0.019%
6	5.428	395	398	401	rBV	6381	7361	0.21%	0.021%
7	5.711	444	446	449	rVB	5925	6802	0.19%	0.020%
8	5.740	449	451	454	rVB3	6860	7575	0.22%	0.022%
9	5.764	454	455	457	rBV	8050	6457	0.18%	0.019%
10	6.093	509	511	513	rBV	8720	8189	0.23%	0.024%
11	6.193	524	528	530	rBV4	6254	8372	0.24%	0.024%
12	6.346	551	554	555	rBV	8879	8348	0.24%	0.024%
13	6.364	555	557	562	rVB2	6655	7199	0.20%	0.021%
14	6.446	569	571	575	rBV2	8395	10388	0.30%	0.030%
15	6.875	641	644	648	rVB	8199	7370	0.21%	0.021%
16	7.093	673	681	694	rVV	501873	851544	24.21%	2.474%
17	7.187	694	697	702	rVV2	8128	14862	0.42%	0.043%
18	7.228	702	704	707	rVV2	6530	6969	0.20%	0.020%
19	7.281	707	713	722	rVB	423316	668334	19.00%	1.941%
20	7.416	732	736	737	rBV	5058	7750	0.22%	0.023%
21	7.452	737	742	752	rVV	525763	855598	24.33%	2.485%
22	7.934	817	824	832	rBV	401689	643754	18.31%	1.870%
23	8.152	859	861	863	rVB2	7337	6786	0.19%	0.020%
24	8.275	878	882	884	rVB3	7221	8519	0.24%	0.025%
25	8.316	884	889	891	rBV	7929	10954	0.31%	0.032%
26	8.658	940	947	959	rBV	615410	1024586	29.13%	2.976%
27	8.822	970	975	977	rVB	6986	7639	0.22%	0.022%
28	8.993	1003	1004	1009	rBV2	5941	9569	0.27%	0.028%
29	9.146	1024	1030	1038	rBV	478608	791850	22.52%	2.300%
30	9.863	1145	1152	1161	rBV	405195	685172	19.48%	1.990%
31	10.205	1208	1210	1215	rVV	5329	8647	0.25%	0.025%
32	10.393	1235	1242	1255	rBV	572510	1042517	29.64%	3.028%
33	10.616	1276	1280	1281	rBV	6552	6638	0.19%	0.019%
34	10.775	1300	1307	1315	rBV	547338	901247	25.63%	2.618%
35	10.946	1327	1336	1348	rBV	549219	1033400	29.39%	3.002%
36	11.163	1370	1373	1374	rBV	8099	8139	0.23%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017646.D
 Acq On : 11 Oct 2023 14:39
 Operator : MA/JU
 Sample : PB156277BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	11.187	1374	1377	1380	rVB2	6366	6806	0.19%	0.020%
38	11.505	1427	1431	1435	rVB2	6319	10487	0.30%	0.030%
39	11.552	1437	1439	1444	rVB2	5745	8405	0.24%	0.024%
40	11.652	1455	1456	1460	rVB2	7477	6684	0.19%	0.019%
41	11.687	1460	1462	1464	rBV	7002	7146	0.20%	0.021%
42	11.940	1501	1505	1506	rBV3	5315	6674	0.19%	0.019%
43	12.252	1555	1558	1560	rBV2	5811	7420	0.21%	0.022%
44	12.322	1568	1570	1573	rBV	8304	7747	0.22%	0.023%
45	12.381	1573	1580	1583	rBV3	14423	25300	0.72%	0.073%
46	12.587	1613	1615	1620	rBV3	5488	8706	0.25%	0.025%
47	12.757	1640	1644	1647	rVV	5841	9266	0.26%	0.027%
48	12.793	1647	1650	1651	rVV3	7083	7232	0.21%	0.021%
49	13.057	1691	1695	1697	rBV2	4712	7120	0.20%	0.021%
50	13.463	1762	1764	1767	rBV	7346	7457	0.21%	0.022%
51	13.604	1780	1788	1790	rBV6	19276	41362	1.18%	0.120%
52	13.899	1836	1838	1841	rVB	7134	7393	0.21%	0.021%
53	14.051	1857	1864	1875	rBV	1174967	1623428	46.16%	4.716%
54	14.334	1904	1912	1921	rBV	1237888	1796916	51.10%	5.220%
55	14.634	1957	1963	1971	rVB	845850	1226246	34.87%	3.562%
56	14.840	1994	1998	1999	rVB	7666	8752	0.25%	0.025%
57	14.887	1999	2006	2021	rBV	245295	641405	18.24%	1.863%
58	15.387	2085	2091	2093	rBV5	47071	83068	2.36%	0.241%
59	15.581	2122	2124	2126	rBV	8389	8760	0.25%	0.025%
60	15.640	2128	2134	2144	rVV	1704286	2442653	69.46%	7.095%
61	15.781	2153	2158	2171	rBV	389901	624789	17.77%	1.815%
62	15.881	2171	2175	2182	rVV4	29762	59135	1.68%	0.172%
63	16.098	2208	2212	2216	rVB5	11399	16325	0.46%	0.047%
64	16.292	2241	2245	2247	rVB4	5571	6733	0.19%	0.020%
65	16.434	2267	2269	2273	rVB	6013	6711	0.19%	0.019%
66	16.481	2273	2277	2283	rBV4	15024	34695	0.99%	0.101%
67	16.540	2283	2287	2291	rVB4	11103	19493	0.55%	0.057%
68	16.687	2306	2312	2318	rBV2	74984	113942	3.24%	0.331%
69	16.881	2342	2345	2348	rBV2	6097	6379	0.18%	0.019%
70	17.034	2366	2371	2372	rBV4	6044	7136	0.20%	0.021%
71	17.087	2377	2380	2386	rVV6	18222	31240	0.89%	0.091%
72	17.187	2393	2397	2400	rVB3	6678	9587	0.27%	0.028%
73	17.269	2409	2411	2414	rBV	6898	8021	0.23%	0.023%
74	17.298	2414	2416	2421	rVB4	13261	16734	0.48%	0.049%
75	17.428	2432	2438	2449	rBV	1164264	1625073	46.21%	4.721%
76	17.528	2449	2455	2467	rVV	1933194	2788645	79.30%	8.101%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017646.D
 Acq On : 11 Oct 2023 14:39
 Operator : MA/JU
 Sample : PB156277BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

77	17.651	2472	2476	2479	rVB5	9411	15134	0.43%	0.044%
78	17.775	2492	2497	2501	rVB2	67086	89920	2.56%	0.261%
79	17.875	2512	2514	2516	rVB	13329	12616	0.36%	0.037%
80	18.051	2541	2544	2550	rVB3	10765	14826	0.42%	0.043%
81	18.122	2554	2556	2563	rVV5	14507	26074	0.74%	0.076%
82	18.175	2563	2565	2567	rVV	6956	6584	0.19%	0.019%
83	18.216	2568	2572	2575	rVV3	7942	11252	0.32%	0.033%
84	18.251	2577	2578	2580	rBV	7421	6572	0.19%	0.019%
85	18.281	2580	2583	2587	rVB4	12250	19716	0.56%	0.057%
86	18.486	2615	2618	2619	rBV	7958	8420	0.24%	0.024%
87	18.598	2634	2637	2646	rBV8	11753	24407	0.69%	0.071%
88	18.698	2649	2654	2658	rVV2	64461	78954	2.25%	0.229%
89	18.828	2672	2676	2685	rBV4	27192	51140	1.45%	0.149%
90	19.351	2762	2765	2770	rVB5	30273	37984	1.08%	0.110%
91	19.422	2774	2777	2780	rVV3	35939	47331	1.35%	0.137%
92	19.475	2783	2786	2793	rVB3	68420	85074	2.42%	0.247%
93	19.781	2833	2838	2845	rBV	2654540	3516718	100.00%	10.215%
94	20.157	2900	2902	2906	rVB2	73151	87892	2.50%	0.255%
95	20.780	3005	3008	3013	rBV2	97440	113839	3.24%	0.331%
96	21.351	3102	3105	3110	rBV2	95142	136443	3.88%	0.396%
97	21.569	3137	3142	3148	rBV	1400123	1851062	52.64%	5.377%
98	21.698	3162	3164	3169	rVB	90960	106308	3.02%	0.309%
99	23.980	3545	3552	3561	rBV2	1642893	3389813	96.39%	9.847%
100	24.151	3575	3581	3592	rVB	877498	1903736	54.13%	5.530%




Sum of corrected areas: 34425503

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017646.D
Acq On : 11 Oct 2023 14:39
Operator : MA/JU
Sample : PB156277BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

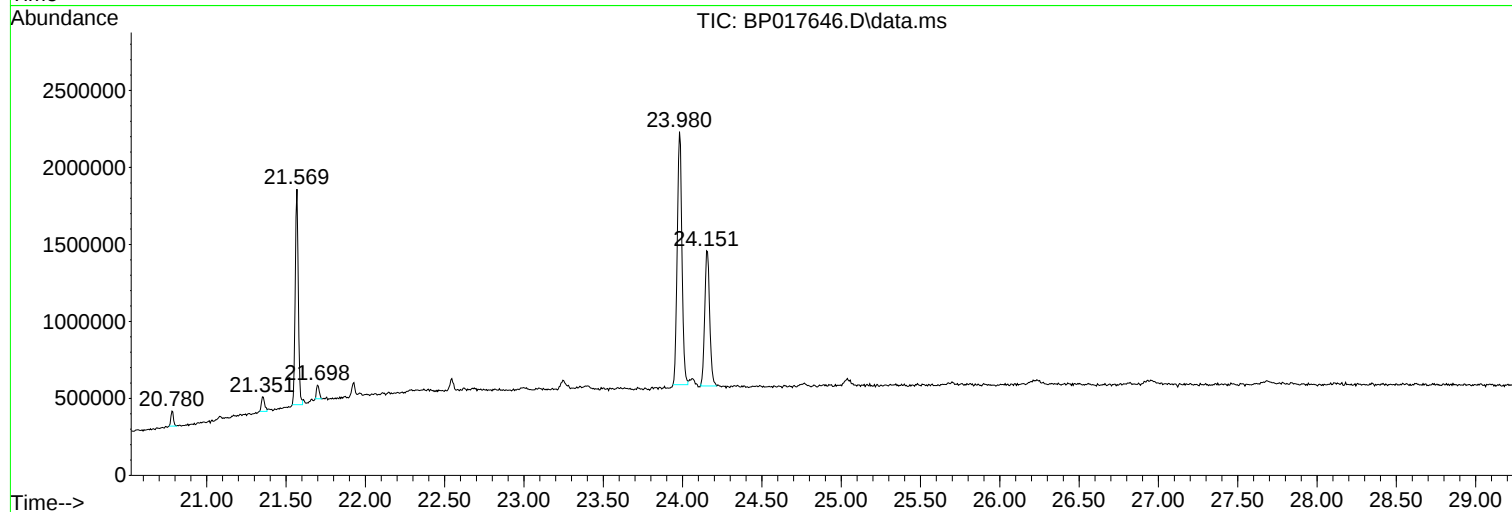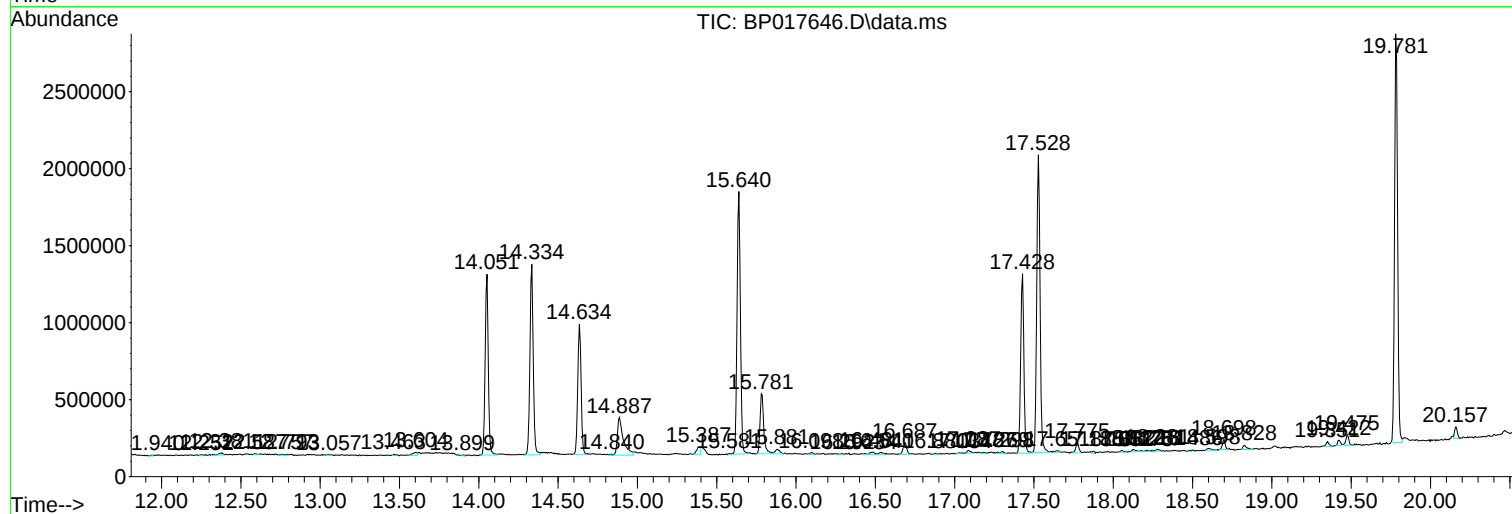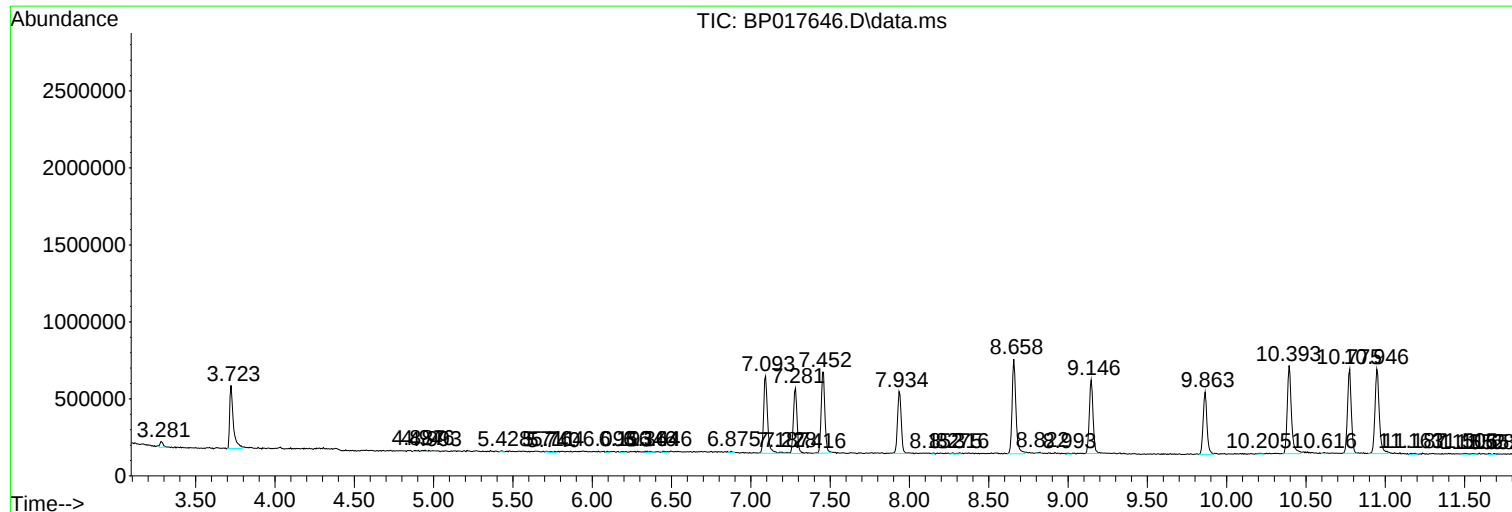

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017646.D
Acq On : 11 Oct 2023 14:39
Operator : MA/JU
Sample : PB156277BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017646.D
Acq On : 11 Oct 2023 14:39
Operator : MA/JU
Sample : PB156277BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK277

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------