

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017647.D
 Acq On : 11 Oct 2023 15:13
 Operator : MA/JU
 Sample : PB156228TB 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB228

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017647.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	30	33	40	rVB	40496	47210	1.42%	0.152%
2	3.716	103	107	121	rBV	388665	621147	18.65%	1.994%
3	6.287	541	544	545	rBV	5208	5775	0.17%	0.019%
4	6.363	556	557	563	rBV2	7022	9383	0.28%	0.030%
5	6.522	582	584	586	rBV	8179	6993	0.21%	0.022%
6	6.869	642	643	647	rVB	8039	5546	0.17%	0.018%
7	6.957	655	658	661	rBV2	5610	6814	0.20%	0.022%
8	7.081	672	679	692	rBV	491589	823438	24.73%	2.644%
9	7.269	705	711	719	rBV	383559	621921	18.68%	1.997%
10	7.440	734	740	748	rBV	528877	835699	25.10%	2.683%
11	7.822	803	805	808	rVB3	4497	5402	0.16%	0.017%
12	7.922	815	822	831	rBV	380872	620901	18.65%	1.993%
13	8.010	835	837	842	rVV	5146	5462	0.16%	0.018%
14	8.093	849	851	854	rVB4	5065	6546	0.20%	0.021%
15	8.399	900	903	906	rBV2	4370	5299	0.16%	0.017%
16	8.646	939	945	961	rBV2	575560	999922	30.03%	3.210%
17	9.134	1019	1028	1037	rBV	465623	803630	24.13%	2.580%
18	9.246	1043	1047	1048	rBV	4606	5365	0.16%	0.017%
19	9.328	1059	1061	1064	rVB	6726	6224	0.19%	0.020%
20	9.357	1064	1066	1068	rBV	6552	6036	0.18%	0.019%
21	9.451	1079	1082	1084	rBV2	6494	8433	0.25%	0.027%
22	9.528	1093	1095	1100	rVB2	6514	10137	0.30%	0.033%
23	9.851	1143	1150	1157	rBV	380248	651714	19.57%	2.092%
24	10.128	1194	1197	1198	rBV	5157	5637	0.17%	0.018%
25	10.163	1199	1203	1204	rBV2	5147	4992	0.15%	0.016%
26	10.216	1209	1212	1213	rBV2	8027	7743	0.23%	0.025%
27	10.304	1226	1227	1230	rBV	6503	5147	0.15%	0.017%
28	10.381	1232	1240	1252	rBV	527594	1023244	30.73%	3.285%
29	10.510	1260	1262	1265	rVB	6467	6293	0.19%	0.020%
30	10.687	1287	1292	1294	rBV	5389	8673	0.26%	0.028%
31	10.757	1296	1304	1312	rVV	507267	836964	25.14%	2.687%
32	10.934	1326	1334	1347	rBV	553523	1040155	31.24%	3.339%
33	11.540	1434	1437	1439	rBV	5204	6085	0.18%	0.020%
34	11.622	1447	1451	1453	rBV2	3479	5588	0.17%	0.018%
35	11.704	1463	1465	1471	rVB	4670	7306	0.22%	0.023%
36	11.898	1495	1498	1500	rBV	6693	6698	0.20%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017647.D
 Acq On : 11 Oct 2023 15:13
 Operator : MA/JU
 Sample : PB156228TB 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB228

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	12.551	1606	1609	1610	rBV3	4858	5147	0.15%	0.017%
38	12.710	1633	1636	1640	rBV	6106	7039	0.21%	0.023%
39	13.004	1684	1686	1689	rVB2	4553	5038	0.15%	0.016%
40	13.028	1689	1690	1693	rVB	6410	5296	0.16%	0.017%
41	13.051	1693	1694	1696	rBV	6994	5668	0.17%	0.018%
42	13.263	1726	1730	1733	rVB2	5346	6852	0.21%	0.022%
43	13.428	1754	1758	1759	rBV2	5265	5791	0.17%	0.019%
44	13.463	1759	1764	1767	rVV2	10312	17804	0.53%	0.057%
45	13.539	1773	1777	1781	rBV2	3510	5332	0.16%	0.017%
46	13.839	1826	1828	1829	rBV	7602	5939	0.18%	0.019%
47	14.039	1854	1862	1872	rBV	1082900	1581554	47.50%	5.077%
48	14.145	1877	1880	1882	rBV	4311	5949	0.18%	0.019%
49	14.257	1896	1899	1901	rVB	7034	7334	0.22%	0.024%
50	14.322	1904	1910	1925	rVV	1161826	1736988	52.16%	5.576%
51	14.528	1943	1945	1947	rBV	5271	5158	0.15%	0.017%
52	14.622	1955	1961	1969	rBV	757107	1110263	33.34%	3.564%
53	14.822	1994	1995	1998	rBV	7707	7291	0.22%	0.023%
54	14.875	1998	2004	2018	rBV	226246	587394	17.64%	1.886%
55	15.628	2126	2132	2142	rBV	1584035	2308686	69.33%	7.412%
56	15.769	2150	2156	2165	rBV	394704	609647	18.31%	1.957%
57	15.857	2169	2171	2172	rBV2	7921	5271	0.16%	0.017%
58	16.198	2227	2229	2232	rBV	6381	7432	0.22%	0.024%
59	16.675	2308	2310	2313	rBV2	6633	6211	0.19%	0.020%
60	17.163	2392	2393	2397	rBV	8046	8726	0.26%	0.028%
61	17.410	2429	2435	2445	rBV	988963	1459245	43.82%	4.685%
62	17.516	2447	2453	2466	rVV	1844379	2675125	80.34%	8.588%
63	19.769	2831	2836	2845	rBV	2502371	3329818	100.00%	10.690%
64	21.557	3135	3140	3149	rBV	1181026	1667506	50.08%	5.353%
65	23.962	3543	3549	3560	rVB2	1544910	3234056	97.12%	10.383%
66	24.133	3573	3578	3587	rVB	804186	1641388	49.29%	5.270%




Sum of corrected areas: 31148470

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017647.D
Acq On : 11 Oct 2023 15:13
Operator : MA/JU
Sample : PB156228TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB228

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

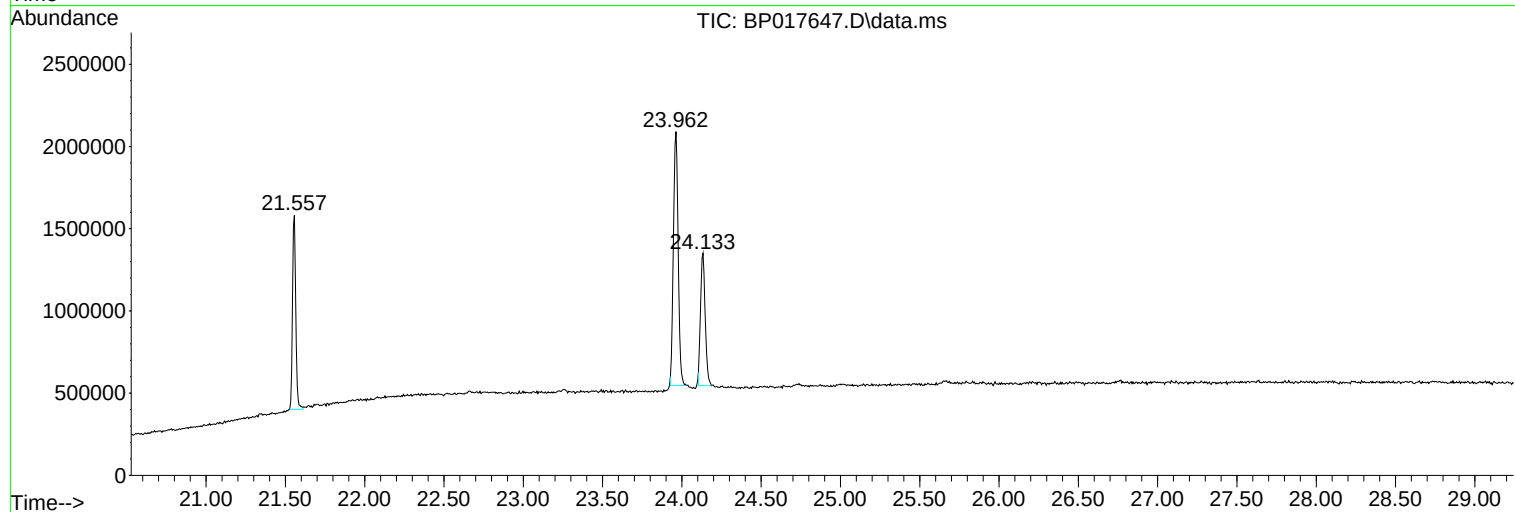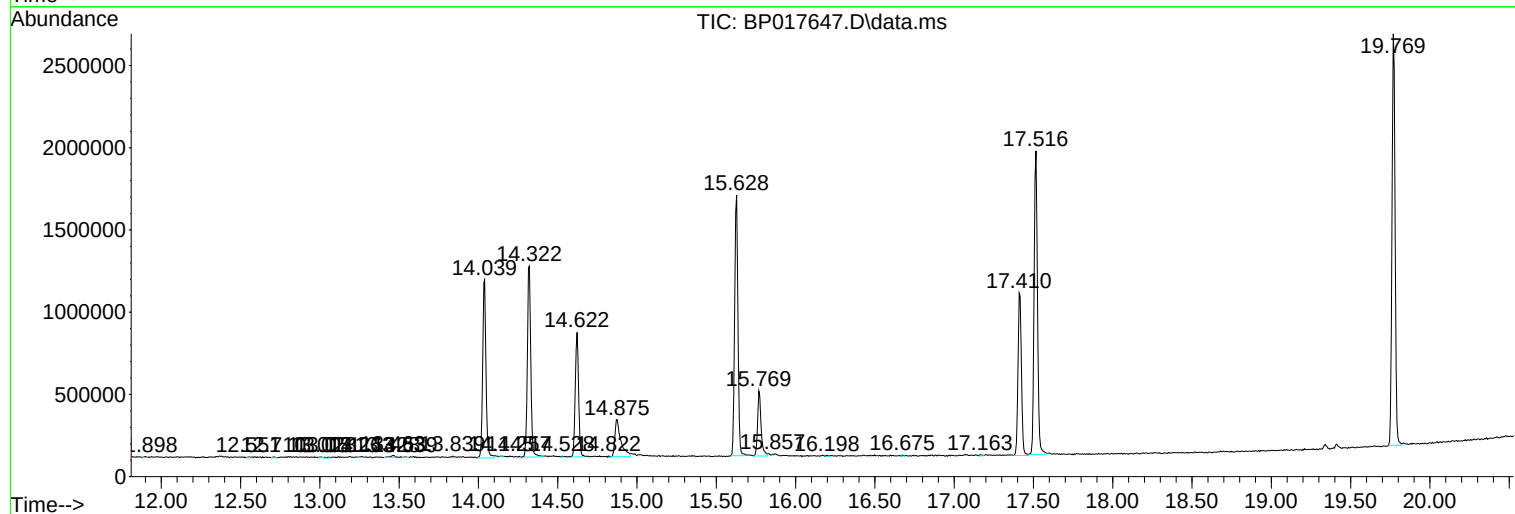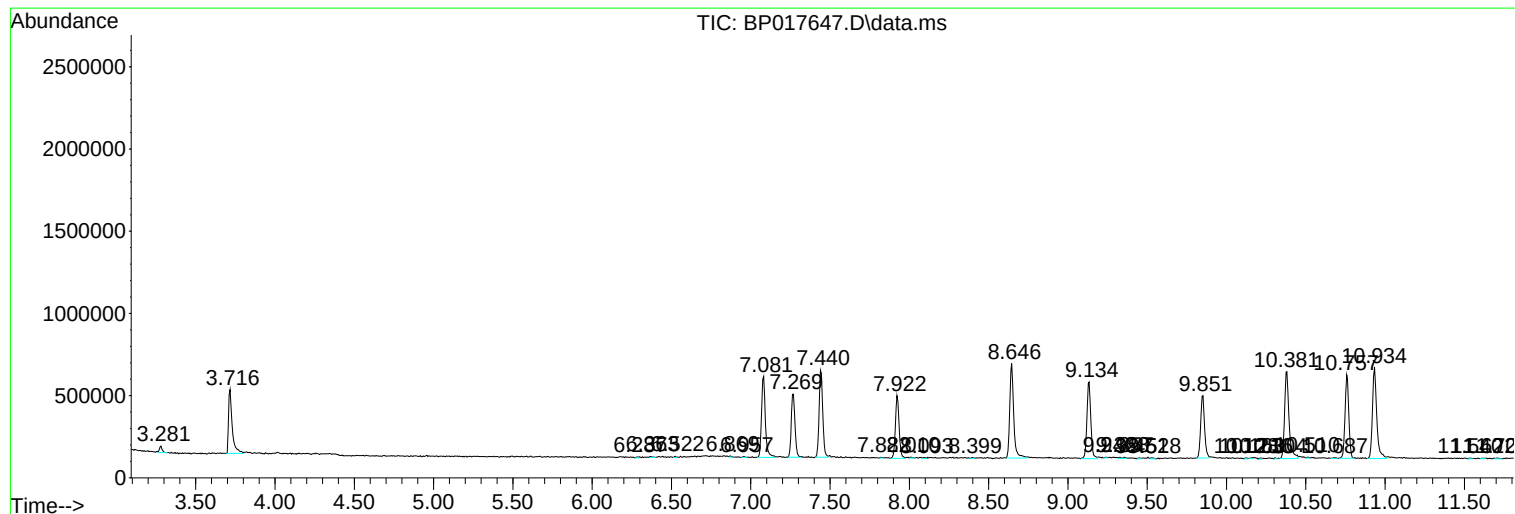

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017647.D
Acq On : 11 Oct 2023 15:13
Operator : MA/JU
Sample : PB156228TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB228

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017647.D
Acq On : 11 Oct 2023 15:13
Operator : MA/JU
Sample : PB156228TB 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB228

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------