

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017648.D
 Acq On : 11 Oct 2023 15:47
 Operator : MA/JU
 Sample : 04360-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLDA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017648.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	11	13	20	rVB2	25682	41501	1.08%	0.131%
2	3.217	20	22	29	rBV2	8102	14754	0.39%	0.047%
3	3.281	30	33	35	rBV2	12657	12536	0.33%	0.040%
4	3.723	105	108	121	rBV	118539	220502	5.76%	0.697%
5	3.905	135	139	142	rBV2	14576	16653	0.43%	0.053%
6	4.017	156	158	162	rVB2	11373	12043	0.31%	0.038%
7	4.281	199	203	208	rVB2	21185	35731	0.93%	0.113%
8	4.370	215	218	220	rBV2	7141	7166	0.19%	0.023%
9	4.540	243	247	251	rVB4	29631	36477	0.95%	0.115%
10	4.811	291	293	297	rBV2	5930	7825	0.20%	0.025%
11	4.846	297	299	302	rVB	8986	7532	0.20%	0.024%
12	4.946	311	316	317	rBV4	5859	8510	0.22%	0.027%
13	4.958	317	318	322	rVB2	9371	9205	0.24%	0.029%
14	5.264	367	370	372	rBV2	5560	6695	0.17%	0.021%
15	5.528	412	415	416	rBV3	6144	6283	0.16%	0.020%
16	5.599	425	427	429	rBV	6659	6060	0.16%	0.019%
17	5.852	469	470	475	rVV	6153	7356	0.19%	0.023%
18	5.899	475	478	481	rVB	6492	7678	0.20%	0.024%
19	5.975	490	491	497	rVB3	6017	6763	0.18%	0.021%
20	6.211	529	531	533	rBV	6881	6335	0.17%	0.020%
21	7.081	674	679	689	rVV	108577	195151	5.09%	0.617%
22	7.264	705	710	720	rVV	403747	647782	16.91%	2.047%
23	7.440	735	740	752	rVV	398304	673104	17.57%	2.127%
24	7.646	770	775	778	rBV2	4089	7575	0.20%	0.024%
25	7.887	813	816	817	rBV2	6258	8114	0.21%	0.026%
26	7.922	817	822	831	rVV	350120	562450	14.68%	1.777%
27	8.052	843	844	849	rBV	7043	10211	0.27%	0.032%
28	8.140	854	859	860	rVV3	4867	6650	0.17%	0.021%
29	8.234	872	875	877	rVV2	6348	7553	0.20%	0.024%
30	8.281	881	883	888	rVB2	5171	8149	0.21%	0.026%
31	8.646	938	945	963	rBV	318177	568196	14.83%	1.795%
32	8.793	965	970	976	rVB2	14434	22789	0.59%	0.072%
33	9.075	1015	1018	1020	rVB	5341	6145	0.16%	0.019%
34	9.134	1020	1028	1035	rBV	479443	821117	21.43%	2.594%
35	9.252	1047	1048	1051	rBV	5850	6526	0.17%	0.021%
36	9.281	1051	1053	1054	rVV2	7355	6536	0.17%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017648.D
 Acq On : 11 Oct 2023 15:47
 Operator : MA/JU
 Sample : 04360-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLDA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

37	9.316	1057	1059	1061	rVB	8134	6243	0.16%	0.020%
38	9.852	1142	1150	1159	rBV	388162	671075	17.52%	2.120%
39	9.910	1159	1160	1163	rVB	6669	6050	0.16%	0.019%
40	9.969	1169	1170	1174	rVB3	7849	6108	0.16%	0.019%
41	10.005	1174	1176	1179	rVB	7454	7387	0.19%	0.023%
42	10.081	1185	1189	1191	rBV4	5472	9236	0.24%	0.029%
43	10.234	1214	1215	1221	rVB5	4831	7031	0.18%	0.022%
44	10.381	1232	1240	1251	rBV	502012	942261	24.60%	2.977%
45	10.757	1296	1304	1314	rVV	472046	784552	20.48%	2.479%
46	10.934	1327	1334	1349	rVV	495691	899986	23.49%	2.843%
47	11.181	1373	1376	1378	rBV	8517	7030	0.18%	0.022%
48	11.263	1383	1390	1396	rBV2	24535	50382	1.32%	0.159%
49	11.322	1396	1400	1406	rVB3	29053	49095	1.28%	0.155%
50	11.569	1441	1442	1445	rVB	6522	5950	0.16%	0.019%
51	11.604	1445	1448	1451	rBV4	5530	7540	0.20%	0.024%
52	11.716	1464	1467	1470	rBV	5450	8003	0.21%	0.025%
53	11.999	1510	1515	1516	rVB	5774	7134	0.19%	0.023%
54	12.357	1572	1576	1580	rBV3	14074	23289	0.61%	0.074%
55	12.493	1595	1599	1600	rBV	6548	6112	0.16%	0.019%
56	12.722	1636	1638	1641	rBV	5800	8177	0.21%	0.026%
57	12.799	1645	1651	1654	rBV4	5560	10828	0.28%	0.034%
58	12.993	1681	1684	1687	rBV2	4376	5905	0.15%	0.019%
59	13.028	1687	1690	1694	rBV	4171	5911	0.15%	0.019%
60	13.093	1699	1701	1704	rVB	7694	7539	0.20%	0.024%
61	13.451	1758	1762	1769	rBV4	22037	45258	1.18%	0.143%
62	13.728	1806	1809	1812	rBV	5582	7574	0.20%	0.024%
63	14.034	1855	1861	1873	rBV	1276017	1782191	46.52%	5.631%
64	14.316	1902	1909	1918	rBV	1365172	1943838	50.74%	6.141%
65	14.622	1954	1961	1970	rVV	721671	1067643	27.87%	3.373%
66	14.822	1991	1995	1998	rBV2	4671	6723	0.18%	0.021%
67	14.887	2001	2006	2013	rBV4	41999	112121	2.93%	0.354%
68	15.457	2100	2103	2104	rVV2	6412	7744	0.20%	0.024%
69	15.622	2125	2131	2144	rVV	1898765	2686637	70.13%	8.488%
70	15.728	2146	2149	2150	rVV	5924	6404	0.17%	0.020%
71	15.769	2150	2156	2167	rVV	487879	708811	18.50%	2.239%
72	15.869	2169	2173	2179	rVB4	15997	31622	0.83%	0.100%
73	15.916	2179	2181	2184	rBV	7076	5957	0.16%	0.019%
74	16.010	2193	2197	2200	rVB2	5405	8835	0.23%	0.028%
75	16.063	2202	2206	2207	rBV	5281	7589	0.20%	0.024%
76	16.128	2215	2217	2220	rVB	7082	7173	0.19%	0.023%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
 Data File : BP017648.D
 Acq On : 11 Oct 2023 15:47
 Operator : MA/JU
 Sample : 04360-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 JLDA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
 Title : SVOA CALIBRATION

77	16.163	2220	2223	2225	rBV	7442	8184	0.21%	0.026%
78	16.204	2225	2230	2233	rVV2	5043	8343	0.22%	0.026%
79	16.498	2276	2280	2283	rBV2	7697	10566	0.28%	0.033%
80	16.522	2283	2284	2288	rVB2	5833	6226	0.16%	0.020%
81	16.622	2298	2301	2303	rBV	7880	9342	0.24%	0.030%
82	16.675	2306	2310	2311	rVV3	6253	6965	0.18%	0.022%
83	16.839	2335	2338	2343	rBV2	5608	10847	0.28%	0.034%
84	17.092	2379	2381	2385	rVV	5485	6582	0.17%	0.021%
85	17.204	2395	2400	2403	rVB5	5553	7657	0.20%	0.024%
86	17.245	2406	2407	2410	rBV	5359	6269	0.16%	0.020%
87	17.410	2429	2435	2444	rVV	976356	1359929	35.50%	4.297%
88	17.510	2446	2452	2463	rBV2	2212894	3064131	79.99%	9.681%
89	17.834	2504	2507	2511	rBV3	6158	7160	0.19%	0.023%
90	17.986	2529	2533	2534	rBV	8167	9494	0.25%	0.030%
91	18.257	2575	2579	2587	rBV2	65017	90624	2.37%	0.286%
92	18.686	2650	2652	2655	rBV4	7177	6764	0.18%	0.021%
93	19.239	2744	2746	2748	rBV	9301	10411	0.27%	0.033%
94	19.333	2759	2762	2767	rBV3	34158	49873	1.30%	0.158%
95	19.410	2771	2775	2779	rVB2	27664	43015	1.12%	0.136%
96	19.504	2788	2791	2797	rVB6	31647	43182	1.13%	0.136%
97	19.769	2830	2836	2843	rBV	2969680	3804601	99.32%	12.020%
98	21.551	3134	3139	3145	rBV	1216577	1599720	41.76%	5.054%
99	23.957	3541	3548	3557	rBV2	1866785	3830790	100.00%	12.103%
100	24.127	3571	3577	3587	rVB	814185	1636018	42.71%	5.169%




Sum of corrected areas: 31651290

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017648.D
Acq On : 11 Oct 2023 15:47
Operator : MA/JU
Sample : 04360-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JLDA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

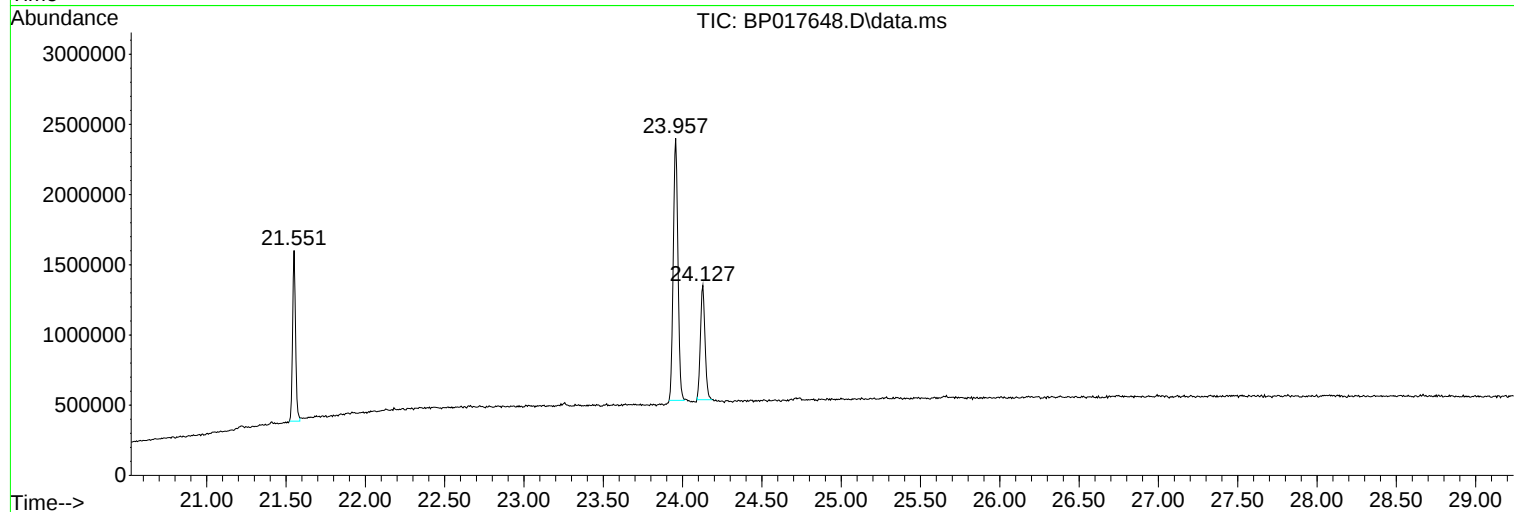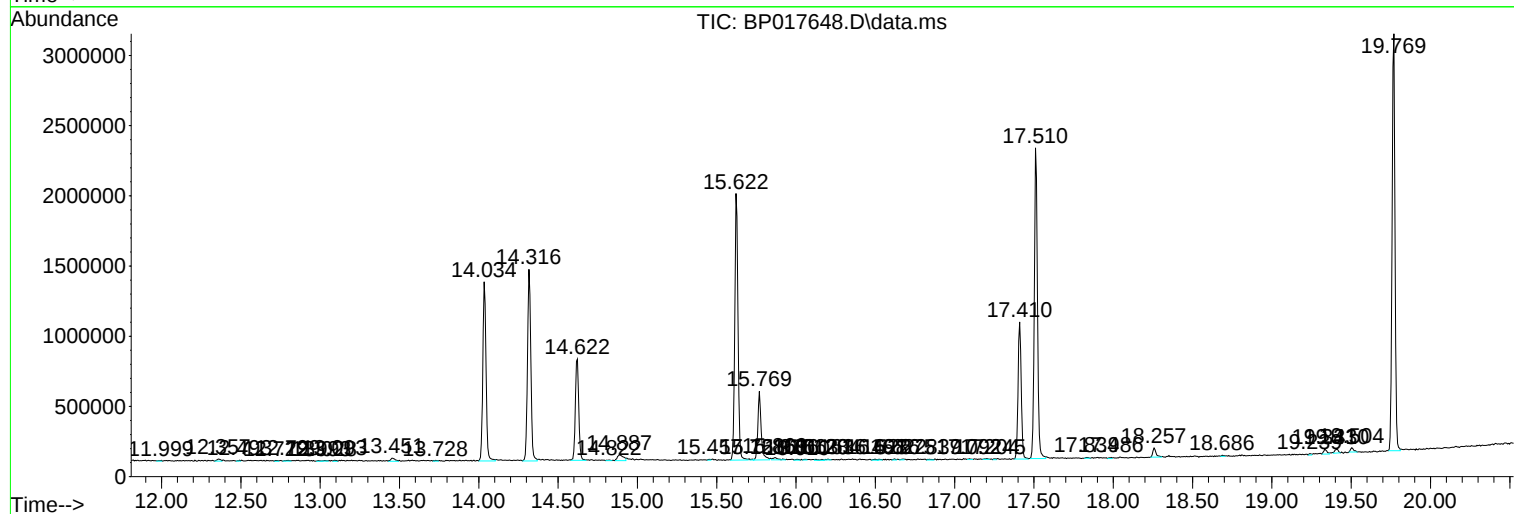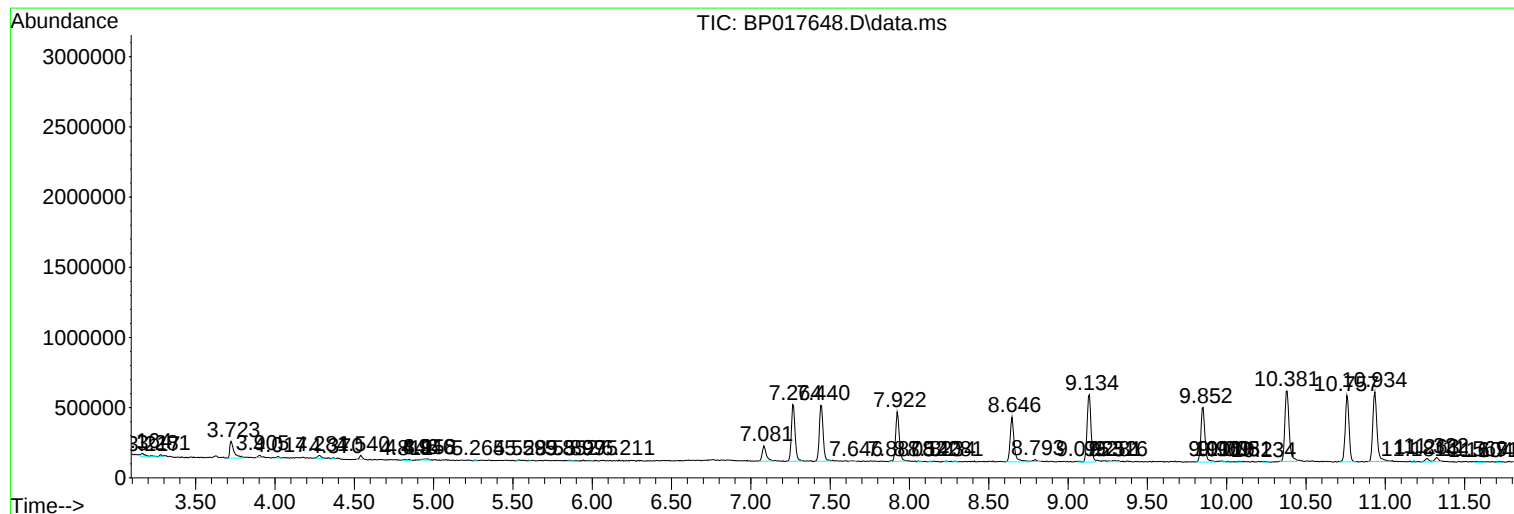

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017648.D
Acq On : 11 Oct 2023 15:47
Operator : MA/JU
Sample : 04360-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JLDA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101123\
Data File : BP017648.D
Acq On : 11 Oct 2023 15:47
Operator : MA/JU
Sample : 04360-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
JLDA7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP100923.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc