

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101219\
 Data File : BP000669.D
 Acq On : 12 Oct 2019 15:55
 Operator : JU
 Sample : PB123660BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Oct 12 21:47:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	174586	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	662438	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	370670	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	687163	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	619993	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	691443	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.36	96	31266	7.43	ng/uL	-0.01
5) Phenol-d5	6.38	99	505796	37.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	258701	38.42	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	422369	37.23	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	394898	38.38	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	194945	38.71	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	210786	39.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	368796	35.94	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	518771	45.45	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1005086	38.73	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	1206316	37.79	ng/ul	0.00
52) 4-Nitrophenol-d4	9.90	143	145188	36.33	ng/ul	0.00
58) Fluorene-d10	10.32	176	839822	37.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	88735	27.12	ng/ul	0.00
71) Anthracene-d10	11.35	188	1259319	39.56	ng/ul	0.00
79) Pyrene-d10	12.73	212	1319773	37.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1353687	39.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	7.13	70	7812	1.142	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101219\
Data File : BP000669.D
Acq On : 12 Oct 2019 15:55
Operator : JU
Sample : PB123660BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Oct 12 21:47:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration

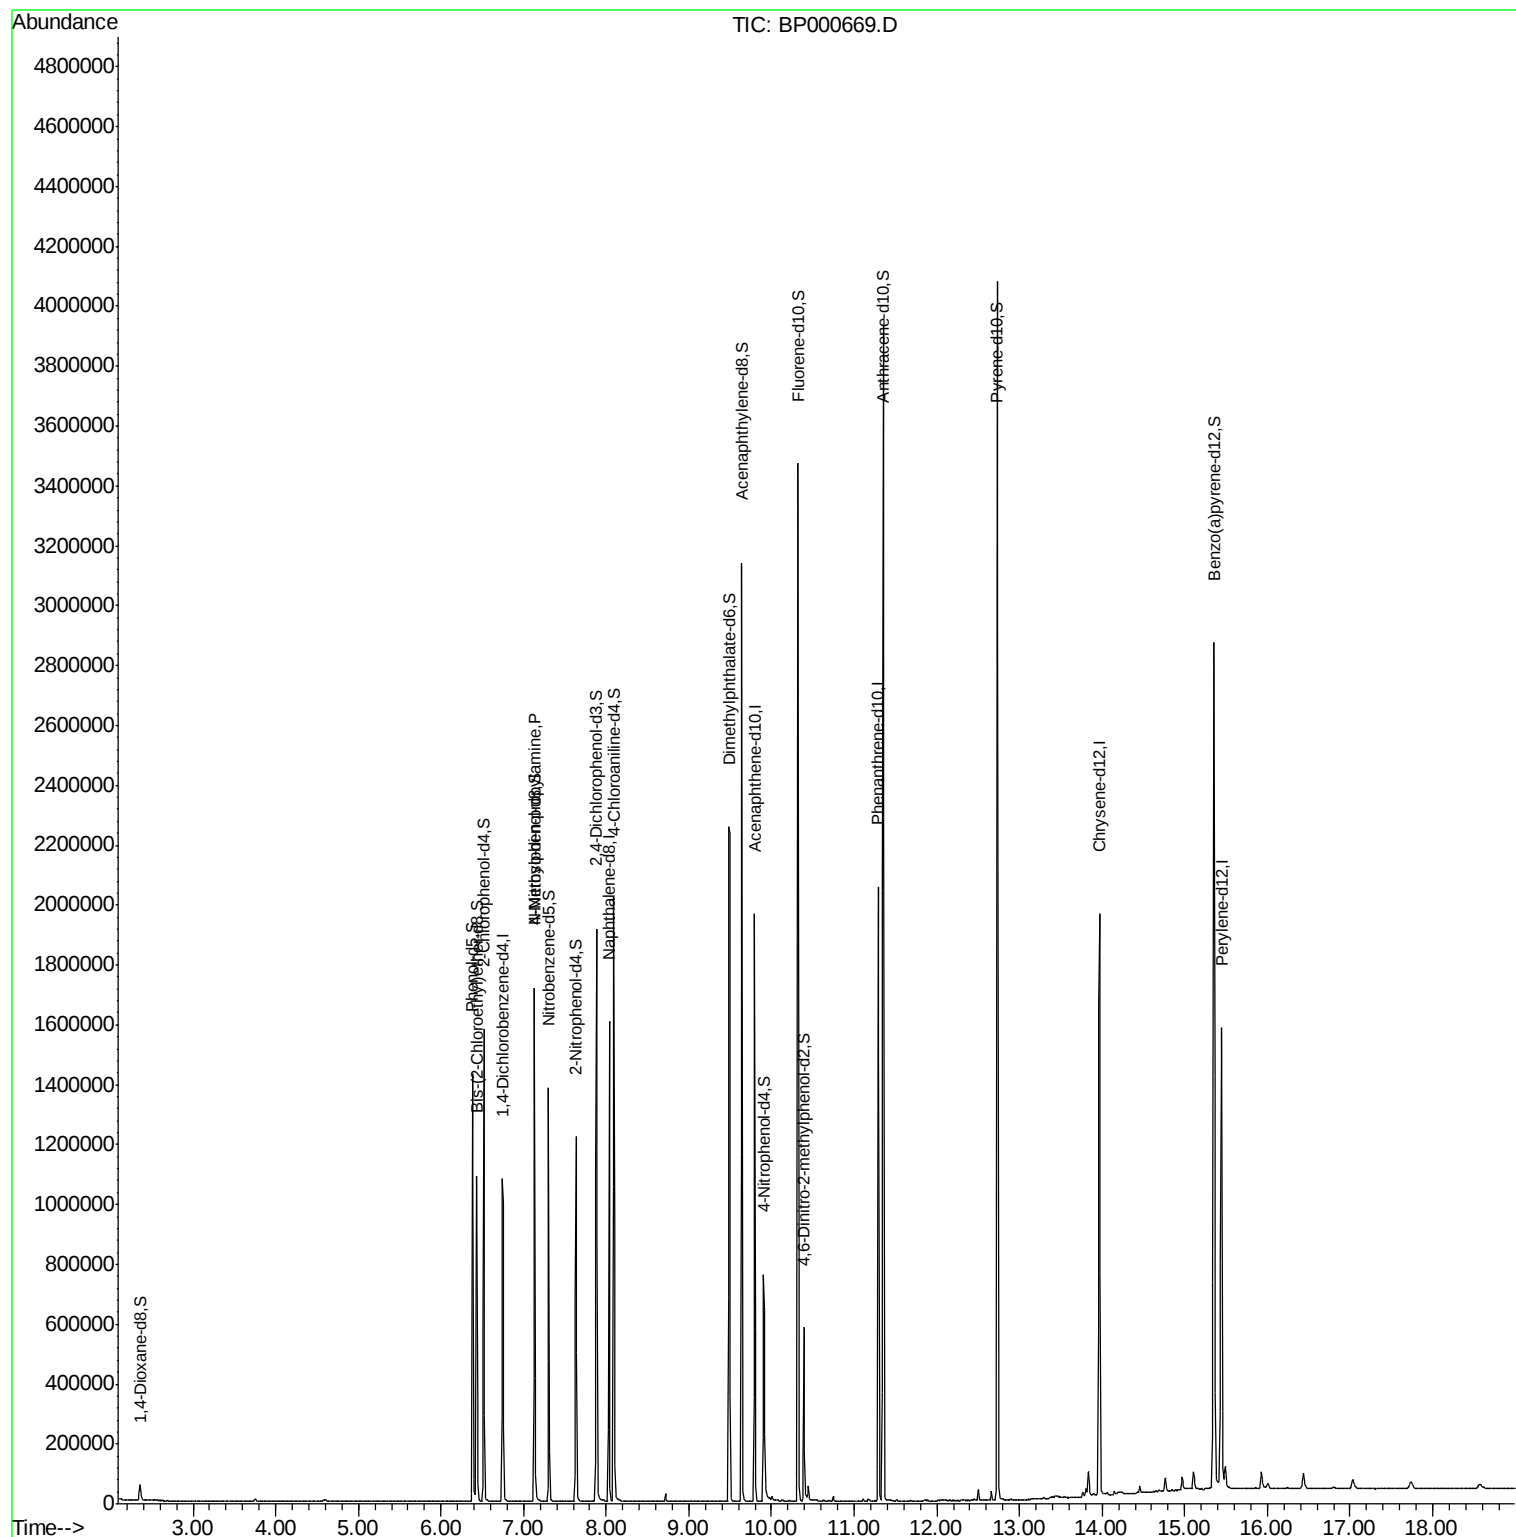

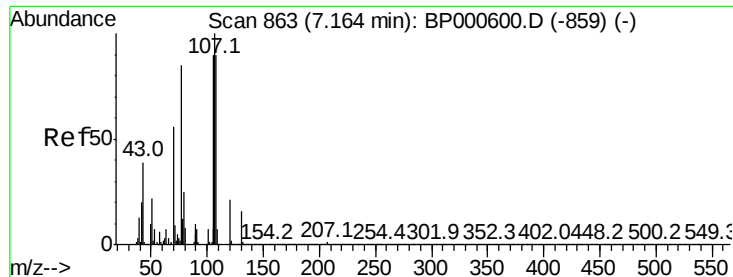

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.142 ng/ul
 RT: 7.13 min Scan# 857
 Delta R.T. -0.04 min
 Lab File: BP000669.D
 Acq: 12 Oct 2019 15:55

Instrument :
 BNA_P
 ClientSampleId :

Tot Ion:	70	Resp:	7812
Ion Ratio	Lower	Upper	
70	100		
42	298.7	33.5	50.3#
101	0.0	9.6	14.4#
130	0.5	21.8	32.8#

