

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101219\
 Data File : BP000670.D
 Acq On : 12 Oct 2019 16:19
 Operator : JU
 Sample : PB123733BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Oct 12 21:47:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	185371	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	718172	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	406453	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	761857	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	662378	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	748993	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.35	96	31354	7.02	ng/uL	-0.02
5) Phenol-d5	6.38	99	508611	35.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	258364	36.14	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	422547	35.07	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	396848	36.33	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	196393	35.97	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	211746	36.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	371994	33.43	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	525150	42.44	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	1040480	36.57	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	1234055	35.26	ng/ul	0.00
52) 4-Nitrophenol-d4	9.90	143	152483	34.79	ng/ul	0.00
58) Fluorene-d10	10.32	176	867076	35.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	92889	25.60	ng/ul	0.00
71) Anthracene-d10	11.35	188	1298837	36.81	ng/ul	0.00
79) Pyrene-d10	12.73	212	1363382	36.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1370189	37.06	ng/ul	0.00

Target Compounds


				Ovalue	
15) N-Nitroso-di-n-propylamine	7.13	70	7872	1.083 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101219\
Data File : BP000670.D
Acq On : 12 Oct 2019 16:19
Operator : JU
Sample : PB123733BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Oct 12 21:47:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration

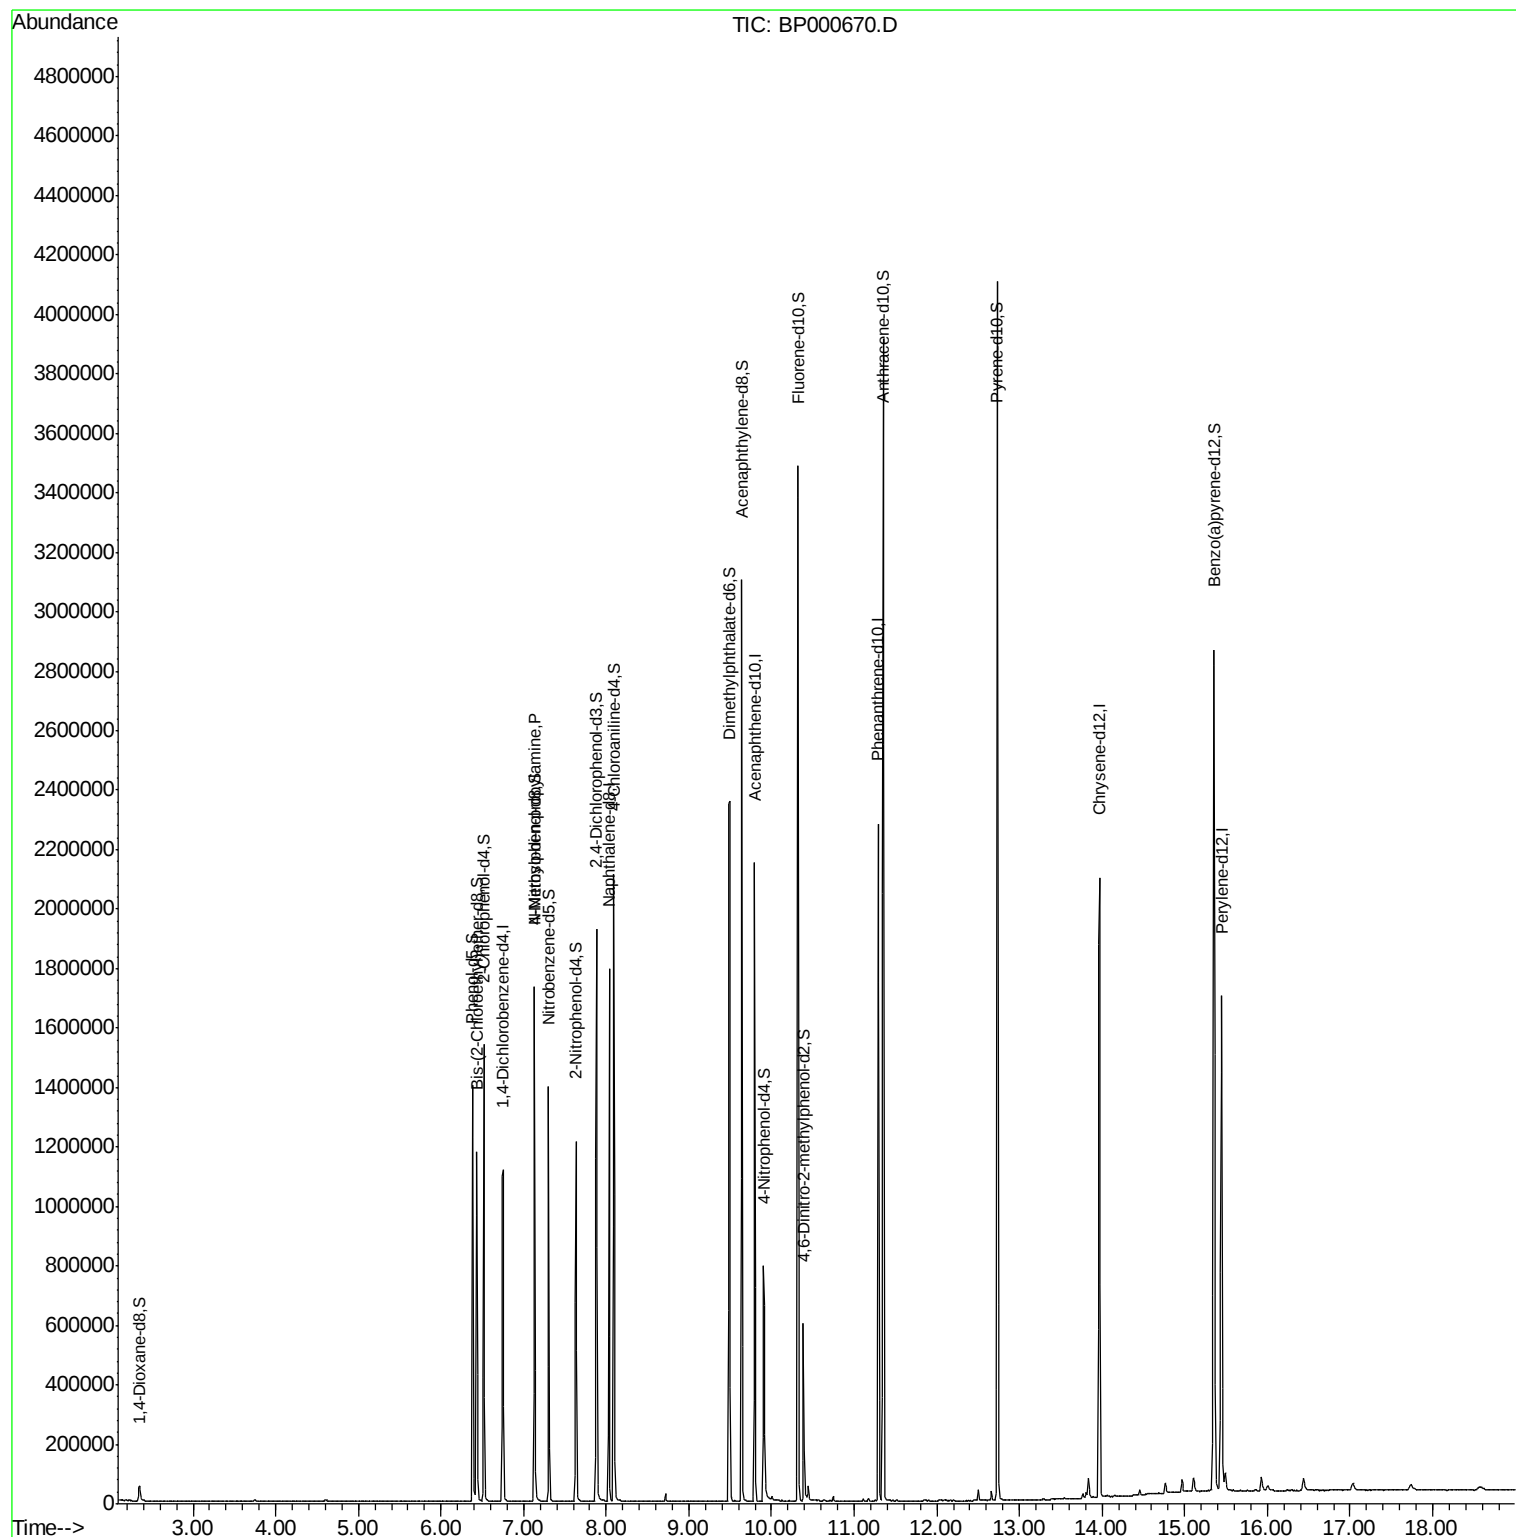

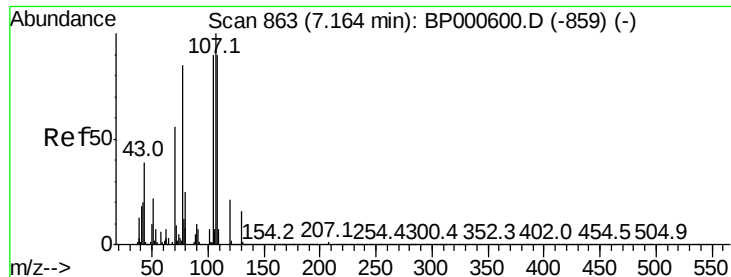

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.083 ng/ul
 RT: 7.13 min Scan# 857
 Delta R.T. -0.04 min
 Lab File: BP000670.D
 Acq: 12 Oct 2019 16:19

Instrument :
 BNA_P
 ClientSampleId :

Tot Ion:	70	Resp:	7872
Ion Ratio	Lower	Upper	
70	100		
42	304.4	33.5	50.3#
101	0.2	9.6	14.4#
130	0.1	21.8	32.8#

