

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101219\
 Data File : BP000662.D
 Acq On : 12 Oct 2019 13:07
 Operator : JU
 Sample : K5199-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BEP75

Quant Time: Oct 12 21:46:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 09 17:20:45 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.75	152	210981	20.00	ng/ul	0.00
18) Naphthalene-d8	8.03	136	824951	20.00	ng/ul	0.00
36) Acenaphthene-d10	9.80	164	470296	20.00	ng/ul	0.00
62) Phenanthrene-d10	11.29	188	867848	20.00	ng/ul	0.00
78) Chrysene-d12	13.97	240	746785	20.00	ng/ul	0.00
86) Perylene-d12	15.45	264	806792	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.36	96	21434	4.21	ng/uL	0.00
5) Phenol-d5	6.38	99	373031	22.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.43	67	202712	24.91	ng/ul	0.00
9) 2-Chlorophenol-d4	6.52	132	325572	23.74	ng/ul	0.00
13) 4-Methylphenol-d8	7.13	113	265878	21.38	ng/ul	0.00
19) Nitrobenzene-d5	7.30	128	152917	24.39	ng/ul	0.00
22) 2-Nitrophenol-d4	7.63	143	162636	24.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	7.88	165	291320	22.79	ng/ul	0.00
29) 4-Chloroaniline-d4	8.09	131	348919	24.55	ng/ul	0.00
44) Dimethylphthalate-d6	9.49	166	818004	24.85	ng/ul	0.00
47) Acenaphthylene-d8	9.64	160	976859	24.12	ng/ul	0.00
52) 4-Nitrophenol-d4	9.91	143	103360	20.38	ng/ul	0.00
58) Fluorene-d10	10.32	176	691317	24.54	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	10.39	200	75067	18.16	ng/ul	0.00
71) Anthracene-d10	11.35	188	1011886	25.17	ng/ul	0.00
79) Pyrene-d10	12.73	212	1080569	25.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	15.36	264	1038272	26.07	ng/ul	0.00
Target Compounds						
6) Phenol	6.39	94	17263	1.052	ng/ul#	80
45) Dimethylphthalate	9.51	163	202469	6.172	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101219\
Data File : BP000662.D
Acq On : 12 Oct 2019 13:07
Operator : JU
Sample : K5199-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BEP75

Quant Time: Oct 12 21:46:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 09 17:20:45 2019
Response via : Initial Calibration




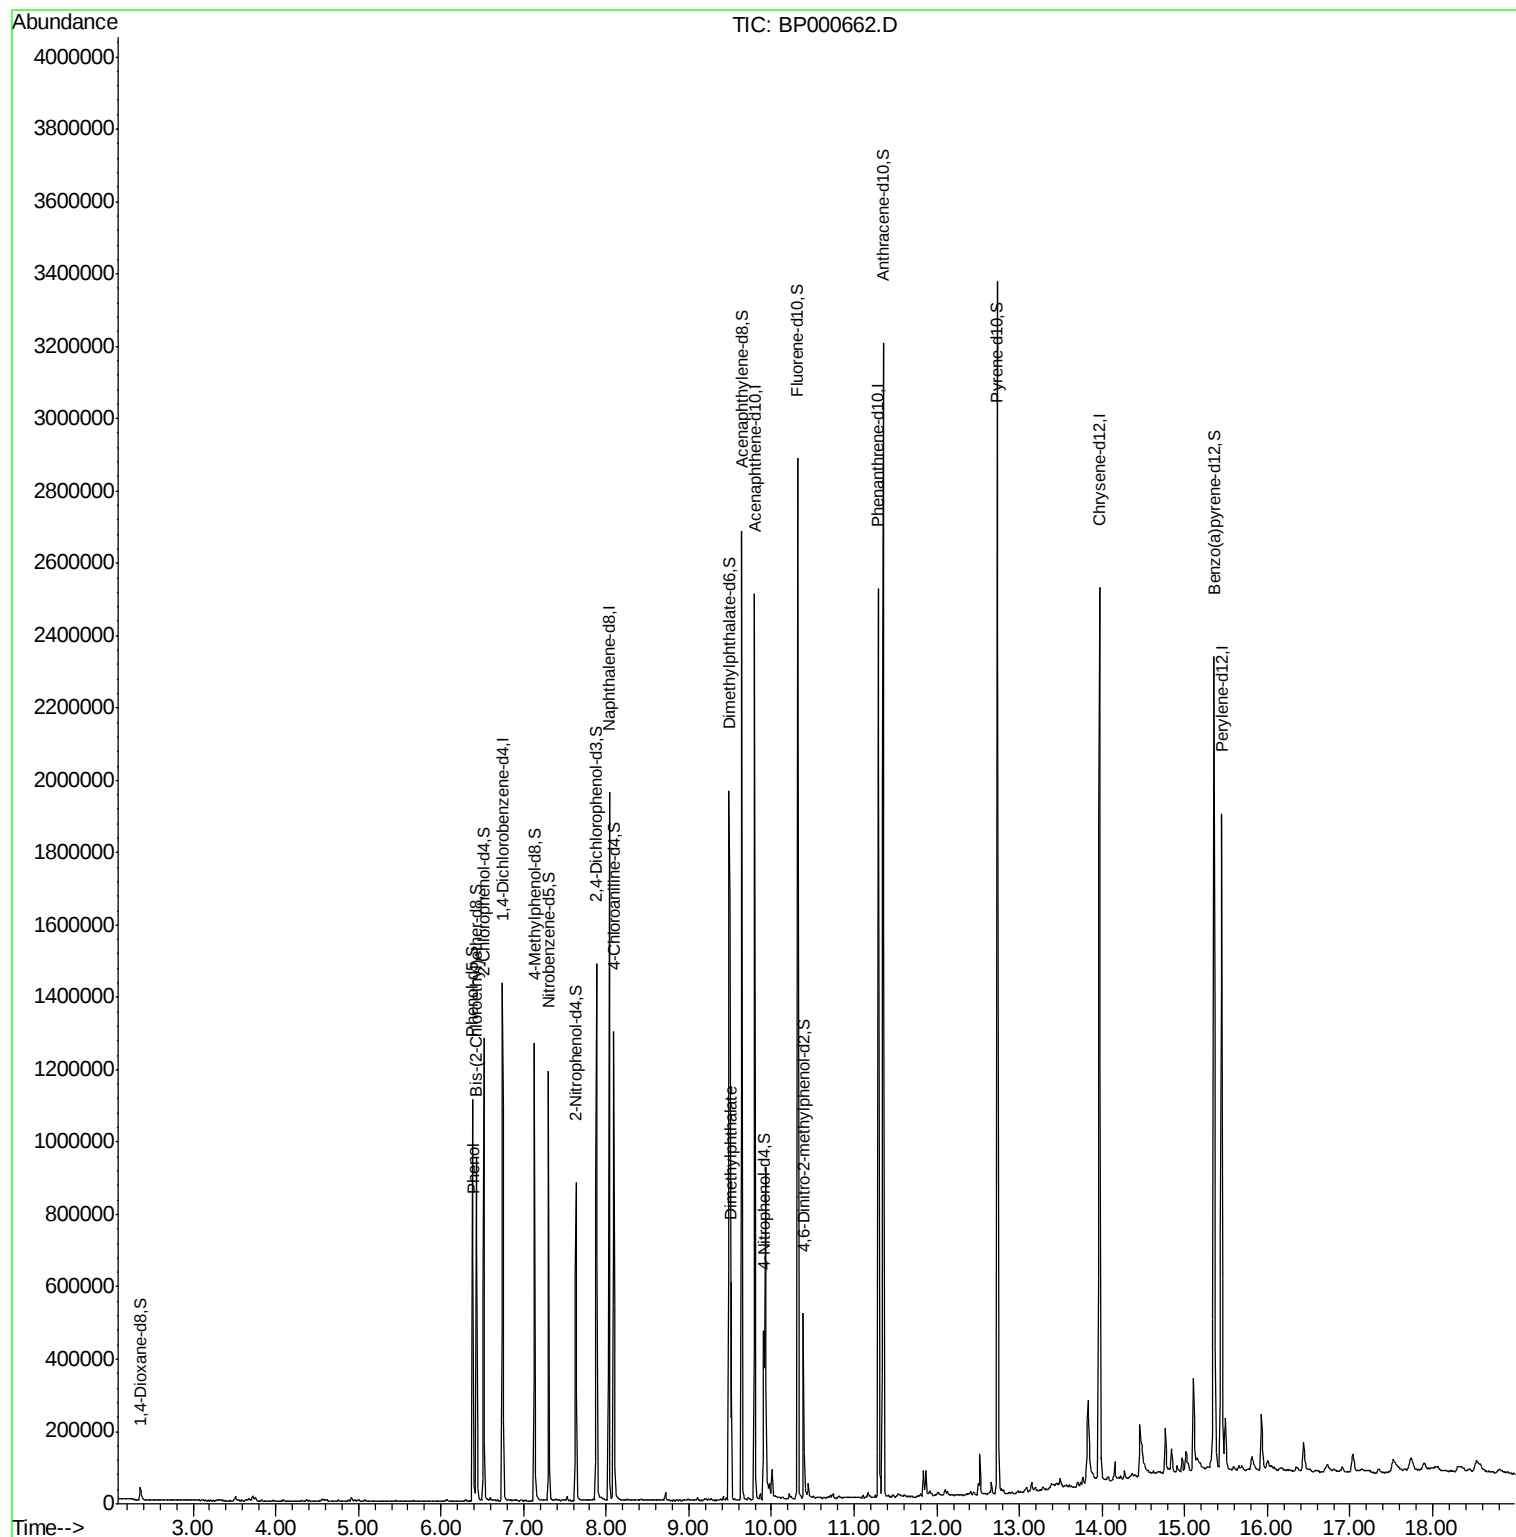


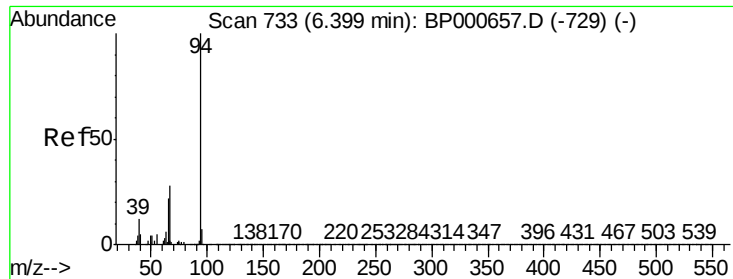

#6
Phenol
Concen: 1.052 ng/ul
RT: 6.39 min Scan# 732
Delta R.T. -0.01 min
Lab File: BP000662.D
Acq: 12 Oct 2019 13:07

Instrument :
BNA_P
ClientSampleId :
BEP75

Tot Ion: 94 Resp: 17263
Ion Ratio Lower Upper
94 100
65 28.1 19.2 28.8
66 48.5 25.7 38.5#

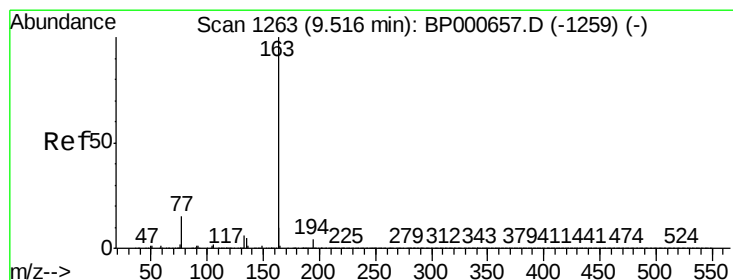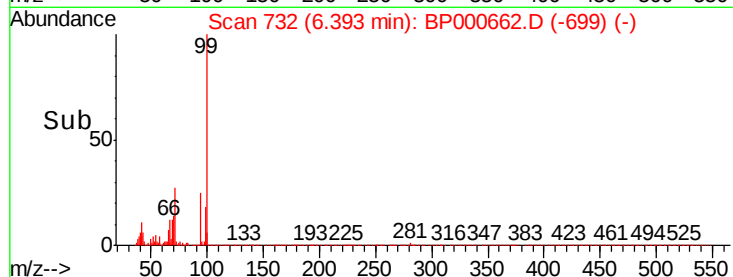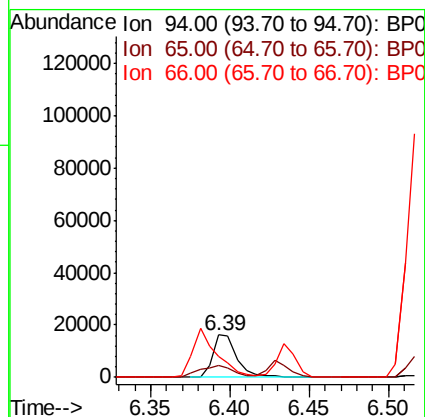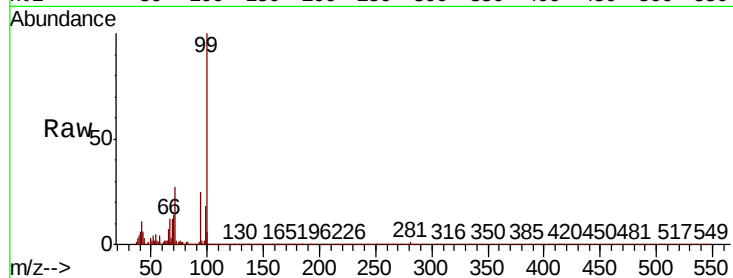

#45
Dimethylphthalate
Concen: 6.172 ng/ul
RT: 9.51 min Scan# 1262
Delta R.T. -0.01 min
Lab File: BP000662.D
Acq: 12 Oct 2019 13:07

Tgt Ion: 163 Resp: 202469
Ion Ratio Lower Upper
163 100
194 4.0 3.3 4.9
164 10.2 8.1 12.1

