

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101319\
Data File : BP000675.D
Acq On : 12 Oct 2019 18:21
Operator : JU
Sample : PB123900BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123900BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.375	555	559	562	rBV	4369597	3959093	55.68%	8.315%
2	6.387	727	731	734	rBV	4102208	4067918	57.21%	8.544%
3	6.522	750	754	757	rBV	4857448	4323811	60.81%	9.081%
4	6.746	789	792	796	rBV	1507141	1323745	18.62%	2.780%
5	6.905	815	819	822	rBV	4575151	3767995	52.99%	7.914%
6	7.311	883	888	891	rBV	3104621	2617371	36.81%	5.497%
7	8.034	1007	1011	1014	rBV	1924254	1686993	23.73%	3.543%
8	9.116	1191	1195	1198	rBV	7096428	5840929	82.15%	12.268%
9	9.799	1307	1311	1314	rBV	2375643	2135171	30.03%	4.485%
10	10.593	1442	1446	1449	rBV	4086124	3550920	49.94%	7.458%
11	11.293	1561	1565	1569	rBV	2802938	2328856	32.75%	4.891%
12	12.904	1834	1839	1842	rBV	7853875	7110312	100.00%	14.934%
13	13.969	2016	2020	2030	rBV	2772835	2425060	34.11%	5.093%
14	15.445	2265	2271	2276	rBV	2083333	2473342	34.79%	5.195%


Sum of corrected areas: 47611516

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101319\
Data File : BP000675.D
Acq On : 12 Oct 2019 18:21
Operator : JU
Sample : PB123900BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123900BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

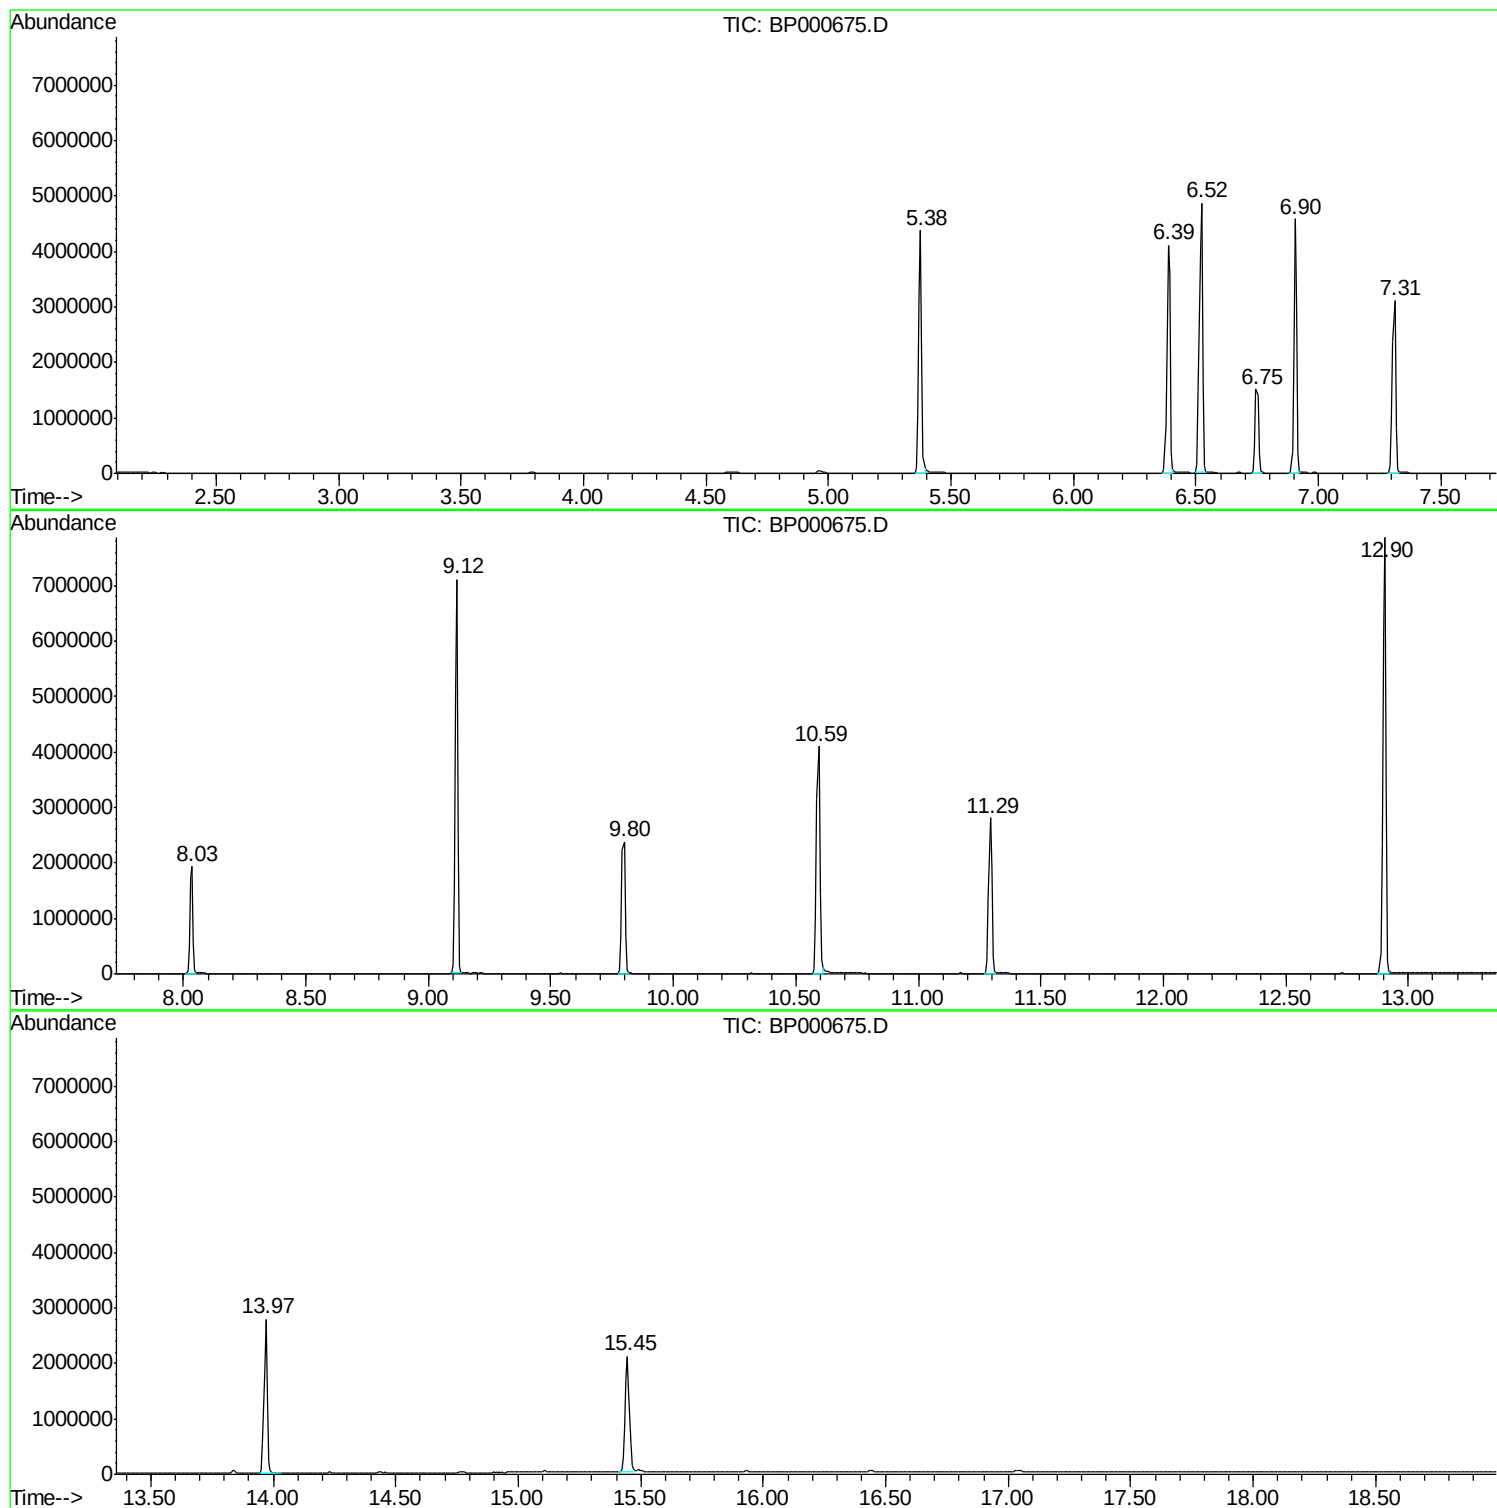

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101319\
Data File : BP000675.D
Acq On : 12 Oct 2019 18:21
Operator : JU
Sample : PB123900BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123900BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.52 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.52	65.33 ng	4323810	1,4-Dichlorobenzene-d4	6.75

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
4		1H-Indazole, 7-methyl-	132	C8H8N2	1000316-00-7	12
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

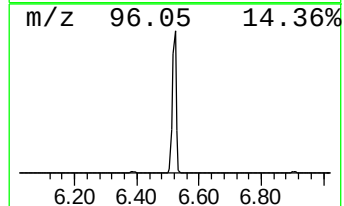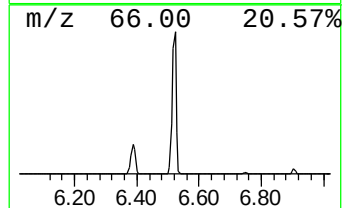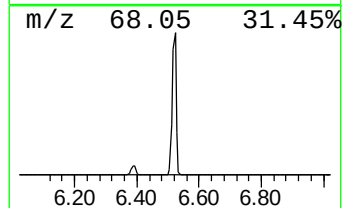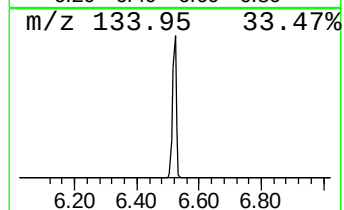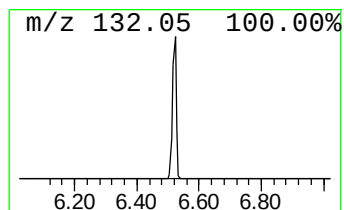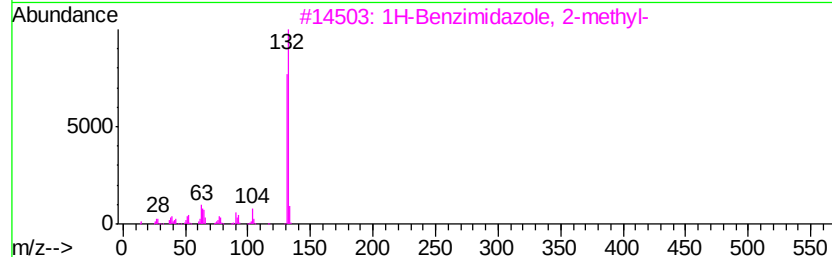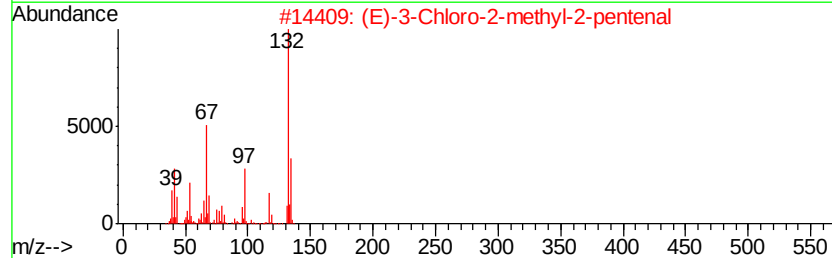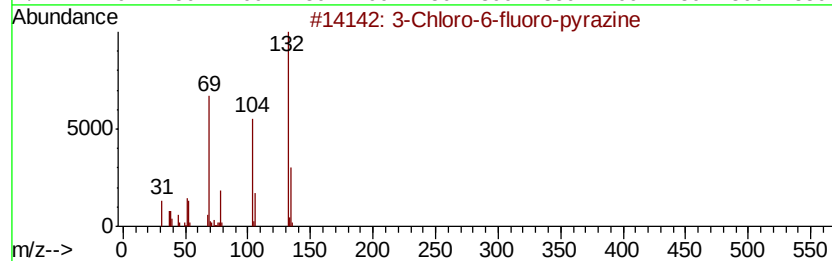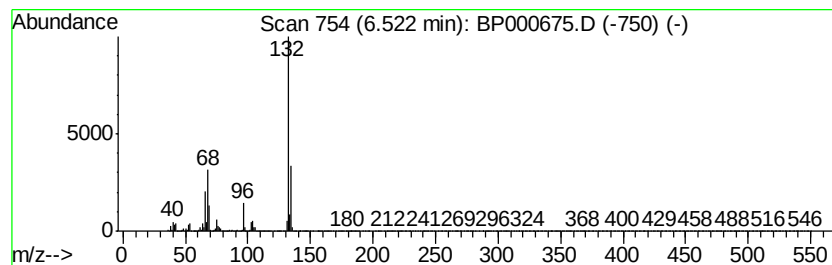

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101319\
Data File : BP000675.D
Acq On : 12 Oct 2019 18:21
Operator : JU
Sample : PB123900BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB123900BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.52	6.52	65.3	ng	4323810	1	6.75	1323750	20.0