


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101319\
Data File : BP000672.D
Acq On : 12 Oct 2019 17:09
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 01 18:03:42 2019

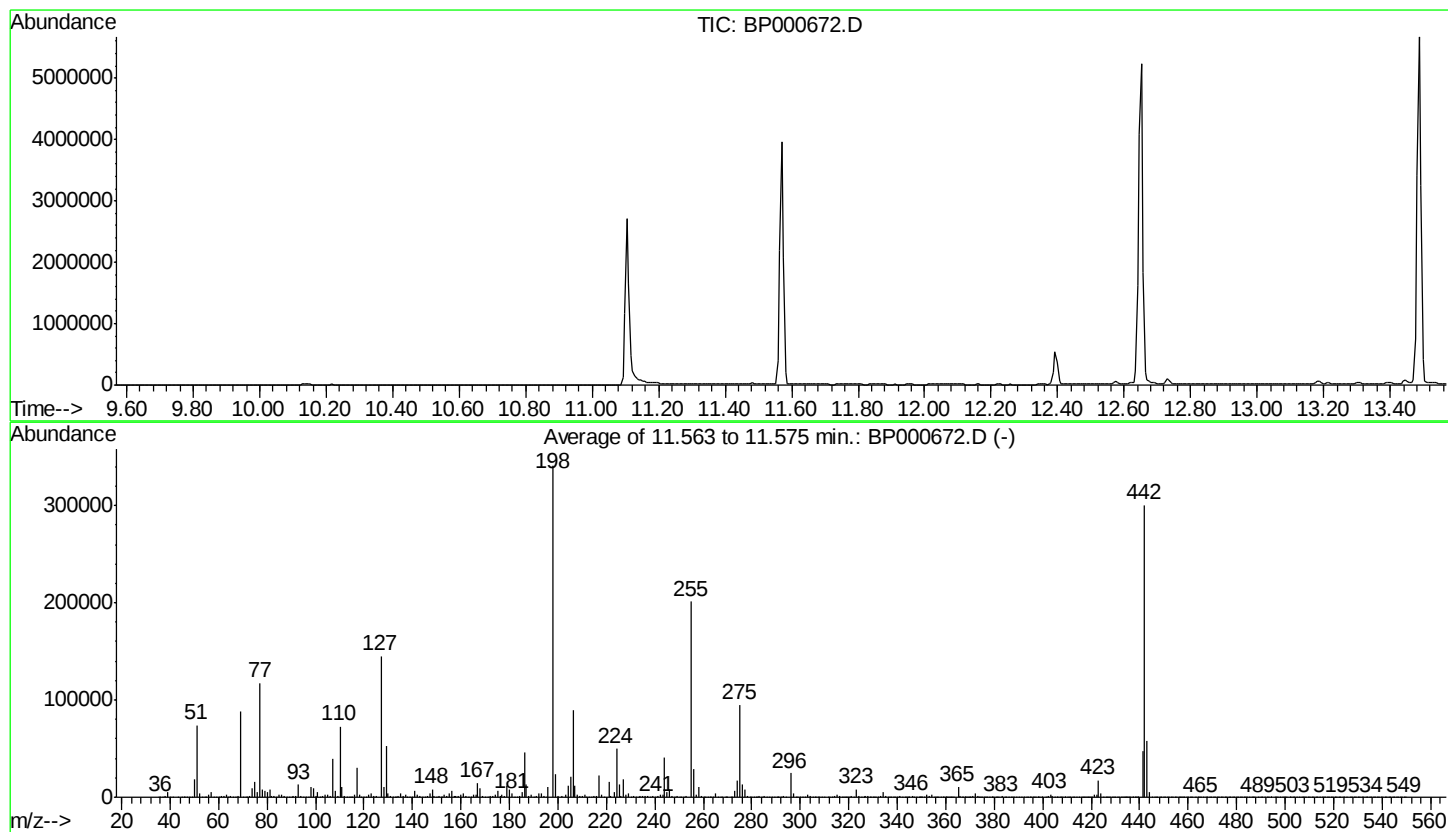

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.8	74306	PASS
68	69	0.00	2	1.9	1674	PASS
69	198	0.00	100	26.0	88743	PASS
70	69	0.00	2	0.6	520	PASS
127	198	10	80	42.5	144872	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	341011	PASS
199	198	5	9	6.8	23319	PASS
275	198	10	60	27.9	94989	PASS
365	198	1	100	3.2	11043	PASS
441	198	0.01	100	13.8	46890	PASS
442	198	50	100	88.0	300234	PASS
443	442	15	24	19.4	58156	PASS