

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
 Data File : BP017669.D
 Acq On : 13 Oct 2023 17:02
 Operator : MA/JU
 Sample : PB156222BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK222

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	27	30	36	rVB	45459	54742	1.32%	0.145%
2	3.699	100	104	127	rBV	497839	793536	19.06%	2.100%
3	3.881	133	135	138	rBV3	4624	4464	0.11%	0.012%
4	4.005	153	156	158	rBV3	8075	9849	0.24%	0.026%
5	5.205	352	360	366	rBV3	3932	13249	0.32%	0.035%
6	7.058	668	675	689	rBV	612003	996266	23.94%	2.636%
7	7.246	701	707	718	rVB	494239	763677	18.35%	2.021%
8	7.422	731	737	749	rBV	651662	1020859	24.53%	2.701%
9	7.905	812	819	830	rBV	438380	719611	17.29%	1.904%
10	8.622	935	941	958	rBV	714629	1205508	28.96%	3.190%
11	8.811	970	973	979	rBV8	2991	6663	0.16%	0.018%
12	9.111	1017	1024	1039	rBV	574670	962690	23.13%	2.547%
13	9.828	1138	1146	1156	rBV	498534	821057	19.73%	2.173%
14	10.358	1228	1236	1253	rVV	643427	1218740	29.28%	3.225%
15	10.487	1257	1258	1264	rVB6	3841	5255	0.13%	0.014%
16	10.740	1291	1301	1309	rBV	601452	988387	23.75%	2.615%
17	10.910	1323	1330	1353	rBV	713694	1273225	30.59%	3.369%
18	12.340	1569	1573	1579	rBV5	8424	16238	0.39%	0.043%
19	13.440	1756	1760	1765	rBV4	11576	19205	0.46%	0.051%
20	14.022	1852	1859	1874	rBV	1320906	1894186	45.51%	5.012%
21	14.299	1900	1906	1925	rBV	1432262	2099048	50.43%	5.555%
22	14.604	1950	1958	1968	rBV	885652	1298130	31.19%	3.435%
23	14.728	1978	1979	1986	rVB7	3385	5080	0.12%	0.013%
24	14.857	1993	2001	2027	rBV	320852	860371	20.67%	2.277%
25	15.610	2122	2129	2143	rBV	1905987	2779782	66.78%	7.356%
26	15.751	2148	2153	2166	rVV	482898	774295	18.60%	2.049%
27	15.851	2168	2170	2180	rVB9	13630	22670	0.54%	0.060%
28	16.398	2261	2263	2268	rBV6	2803	4274	0.10%	0.011%
29	16.463	2270	2274	2280	rVB9	2700	5147	0.12%	0.014%
30	16.857	2338	2341	2345	rBV6	2240	4617	0.11%	0.012%
31	17.398	2426	2433	2441	rBV	1142913	1640323	39.41%	4.341%
32	17.498	2443	2450	2464	rVV	2122893	3119960	74.96%	8.256%
33	18.251	2572	2578	2583	rBV10	22595	41908	1.01%	0.111%
34	19.210	2738	2741	2745	rBV5	6328	12410	0.30%	0.033%
35	19.328	2757	2761	2767	rBV4	23925	35208	0.85%	0.093%
36	19.398	2769	2773	2779	rVV2	26802	36419	0.87%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
Data File : BP017669.D
Acq On : 13 Oct 2023 17:02
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK222

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Title : SVOA CALIBRATION

37	19.498	2788	2790	2795	rBV6	11480	16549	0.40%	0.044%
38	19.757	2828	2834	2847	rBV	2904899	3853459	92.58%	10.197%
39	21.539	3132	3137	3147	rBV	1508027	2059351	49.48%	5.449%
40	23.939	3538	3545	3557	rBV2	1991552	4162378	100.00%	11.015%
41	24.110	3568	3574	3590	rVB	980666	2171036	52.16%	5.745%




Sum of corrected areas: 37789822

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
Data File : BP017669.D
Acq On : 13 Oct 2023 17:02
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

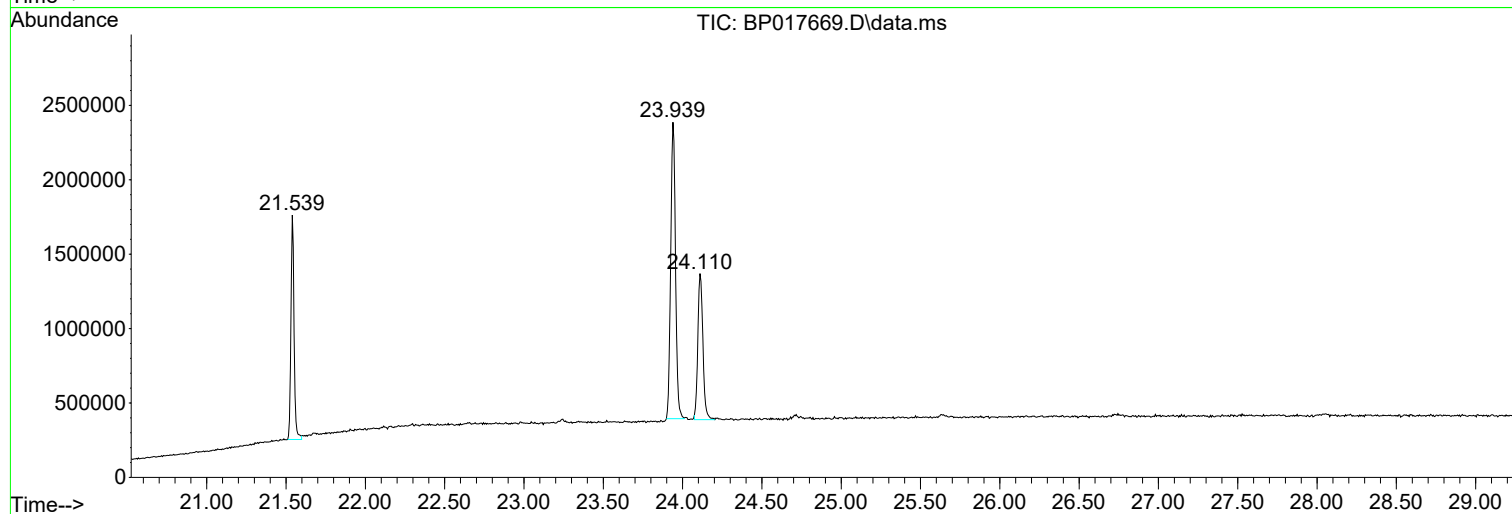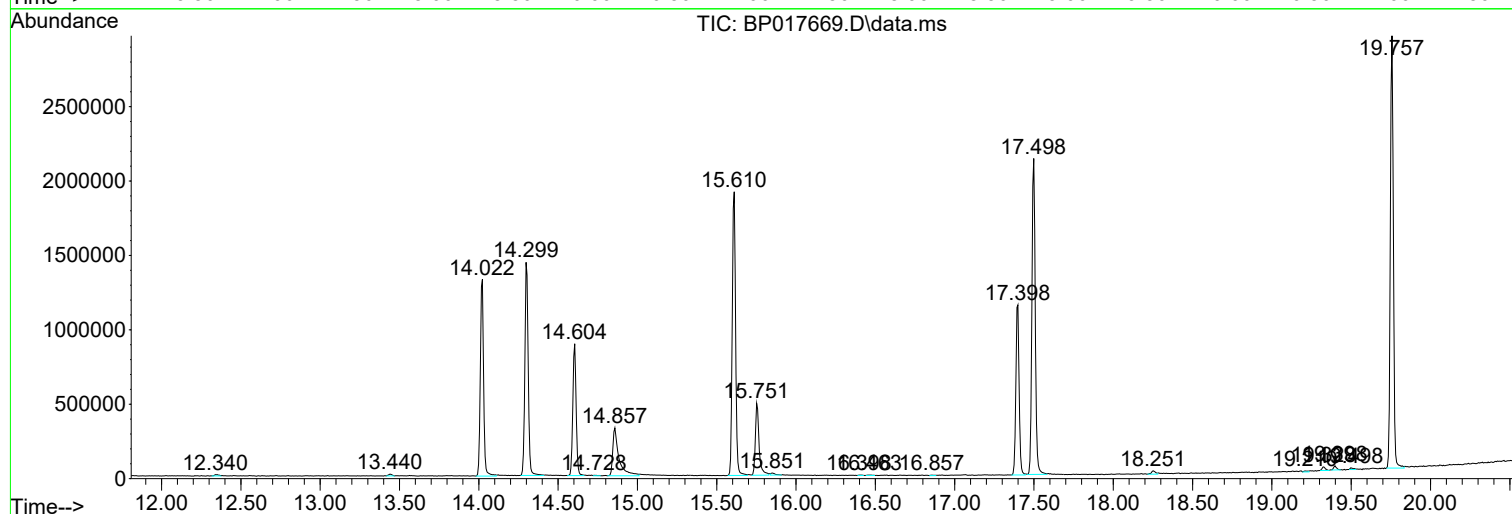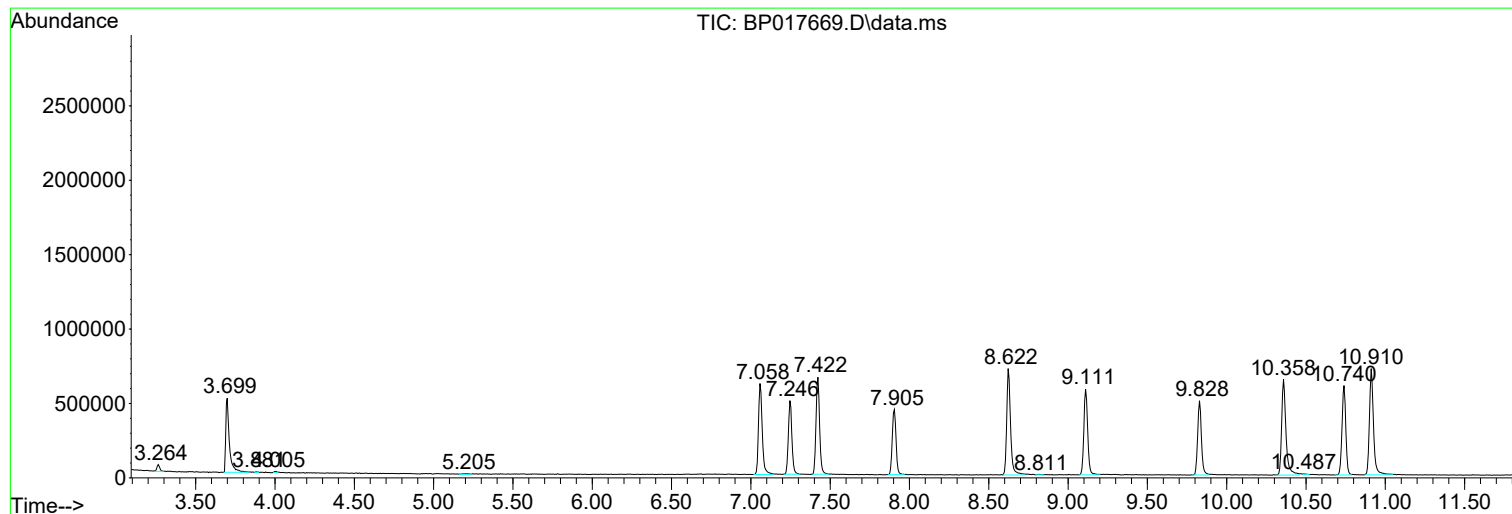

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
Data File : BP017669.D
Acq On : 13 Oct 2023 17:02
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
Data File : BP017669.D
Acq On : 13 Oct 2023 17:02
Operator : MA/JU
Sample : PB156222BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc