

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
 Data File : BP017670.D
 Acq On : 13 Oct 2023 17:36
 Operator : MA/JU
 Sample : PB156223BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP017670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	26	30	38	rVB	38242	54508	1.40%	0.164%
2	3.699	101	104	123	rBV	406658	653050	16.71%	1.961%
3	4.005	152	156	159	rBV4	7058	10584	0.27%	0.032%
4	4.222	191	193	195	rBV2	4812	5796	0.15%	0.017%
5	4.669	266	269	271	rBV4	3892	4755	0.12%	0.014%
6	6.599	595	597	603	rBV7	1828	4002	0.10%	0.012%
7	7.058	668	675	688	rBV	492380	819567	20.97%	2.460%
8	7.246	701	707	716	rBV	423844	657010	16.81%	1.972%
9	7.422	730	737	748	rBV	552226	885571	22.66%	2.659%
10	7.905	812	819	829	rBV	402040	659862	16.89%	1.981%
11	8.552	926	929	932	rBV5	3120	4270	0.11%	0.013%
12	8.622	934	941	960	rBV	573552	1029449	26.35%	3.090%
13	9.110	1017	1024	1037	rBV	496574	830949	21.27%	2.495%
14	9.828	1138	1146	1163	rBV	413935	699031	17.89%	2.099%
15	9.999	1172	1175	1179	rVB6	3226	4138	0.11%	0.012%
16	10.134	1194	1198	1199	rBV4	2785	4014	0.10%	0.012%
17	10.357	1226	1236	1257	rBV	533887	1031430	26.40%	3.096%
18	10.604	1276	1278	1284	rVB7	3457	4522	0.12%	0.014%
19	10.740	1294	1301	1309	rBV	532378	898369	22.99%	2.697%
20	10.910	1323	1330	1350	rBV	581606	1068046	27.33%	3.206%
21	11.169	1371	1374	1378	rVB5	2391	4032	0.10%	0.012%
22	11.234	1381	1385	1390	rBV8	2782	6222	0.16%	0.019%
23	12.351	1568	1575	1585	rVB8	10097	22730	0.58%	0.068%
24	13.440	1756	1760	1768	rVB3	18358	30146	0.77%	0.091%
25	14.022	1852	1859	1869	rBV	1130841	1614777	41.33%	4.848%
26	14.298	1900	1906	1923	rBV	1197678	1799898	46.06%	5.403%
27	14.604	1951	1958	1969	rBV	822820	1190746	30.47%	3.575%
28	14.857	1993	2001	2021	rBV	291423	735199	18.82%	2.207%
29	15.057	2034	2035	2041	rVB6	4558	6356	0.16%	0.019%
30	15.557	2115	2120	2122	rBV6	2624	4858	0.12%	0.015%
31	15.610	2122	2129	2141	rBV	1629201	2375538	60.80%	7.132%
32	15.757	2147	2154	2166	rBV	415696	661324	16.93%	1.985%
33	15.851	2166	2170	2177	rVB5	11261	23754	0.61%	0.071%
34	16.516	2280	2283	2288	rVB5	3179	4373	0.11%	0.013%
35	17.039	2369	2372	2374	rBV4	3663	4488	0.11%	0.013%
36	17.398	2425	2433	2443	rBV	1048134	1529238	39.14%	4.591%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
 Data File : BP017670.D
 Acq On : 13 Oct 2023 17:36
 Operator : MA/JU
 Sample : PB156223BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
 Title : SVOA CALIBRATION

37	17.498	2444	2450	2464	rVV	1933211	2670150	68.34%	8.016%
38	18.251	2572	2578	2584	rBV8	25292	52692	1.35%	0.158%
39	18.563	2628	2631	2633	rBV4	5048	5970	0.15%	0.018%
40	18.804	2669	2672	2677	rBV7	5938	8879	0.23%	0.027%
41	19.322	2757	2760	2764	rVB5	27972	35697	0.91%	0.107%
42	19.398	2769	2773	2777	rVB	25018	32808	0.84%	0.098%
43	19.498	2787	2790	2797	rBV8	15837	23189	0.59%	0.070%
44	19.757	2828	2834	2844	rBV	2544485	3387229	86.69%	10.169%
45	21.539	3132	3137	3147	rBV	1433377	1877596	48.05%	5.637%
46	23.939	3537	3545	3557	rBV2	1815359	3907378	100.00%	11.730%
47	24.110	3567	3574	3586	rVB	931682	1966188	50.32%	5.903%




Sum of corrected areas: 33310378

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP017670\
Data File : BP017670.D
Acq On : 13 Oct 2023 17:36
Operator : MA/JU
Sample : PB156223BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

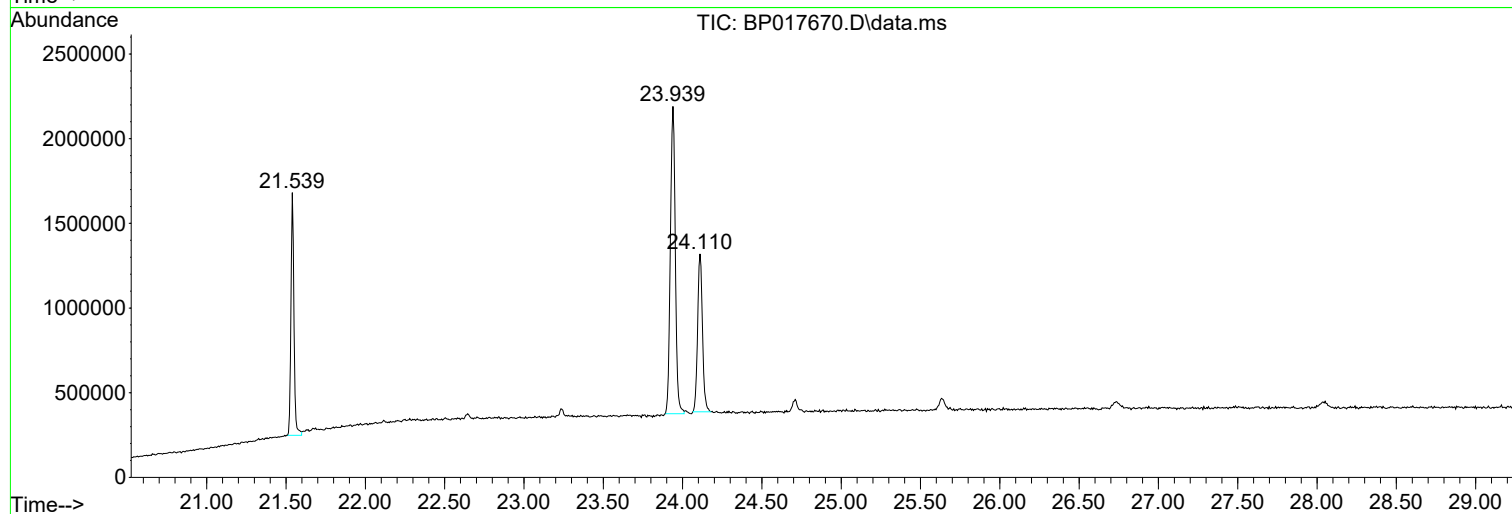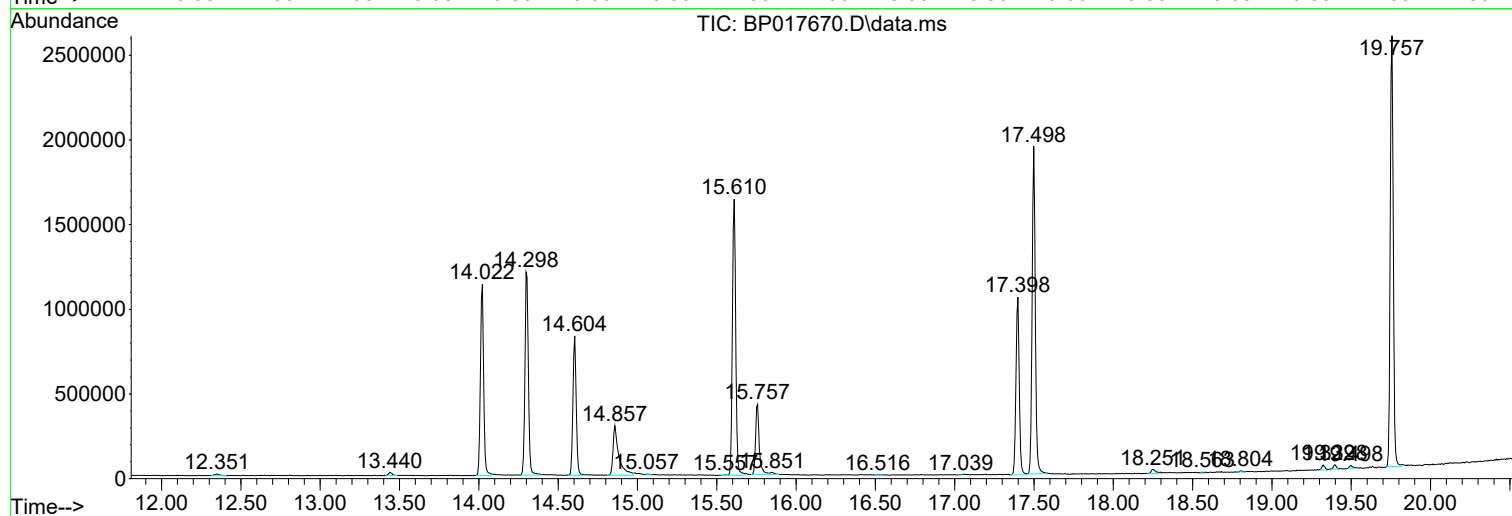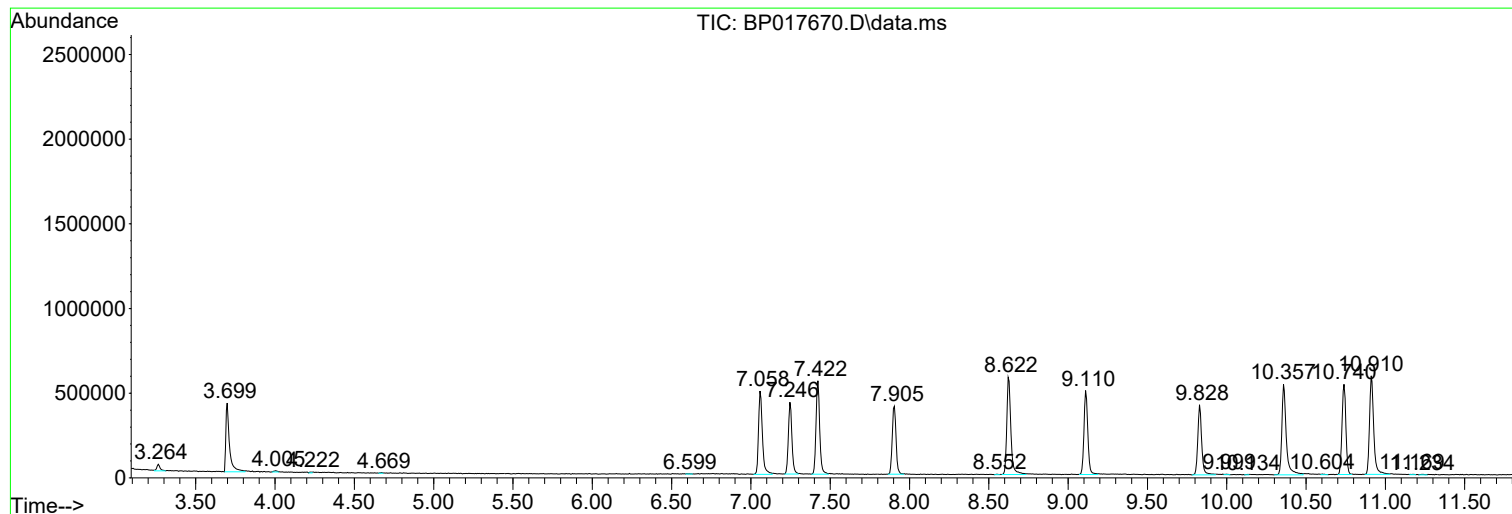

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
Data File : BP017670.D
Acq On : 13 Oct 2023 17:36
Operator : MA/JU
Sample : PB156223BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101323\
Data File : BP017670.D
Acq On : 13 Oct 2023 17:36
Operator : MA/JU
Sample : PB156223BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP101223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
