

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\  
 Data File : BP000709.D  
 Acq On : 14 Oct 2019 14:41  
 Operator : JU  
 Sample : K5348-05  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :

Quant Time: Oct 15 02:42:29 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Oct 01 18:03:42 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 6.75  | 152  | 207252   | 20.00 | ng    | -0.02    |
| 21) Naphthalene-d8        | 8.03  | 136  | 746272   | 20.00 | ng    | -0.02    |
| 39) Acenaphthene-d10      | 9.80  | 164  | 405439   | 20.00 | ng    | -0.02    |
| 64) Phenanthrene-d10      | 11.30 | 188  | 745614   | 20.00 | ng    | -0.01    |
| 76) Chrysene-d12          | 13.97 | 240  | 637792   | 20.00 | ng    | 0.00     |
| 87) Perylene-d12          | 15.45 | 264  | 747718   | 20.00 | ng    | 0.00     |

|                             |       |     |         |       |    |       |
|-----------------------------|-------|-----|---------|-------|----|-------|
| System Monitoring Compounds |       |     |         |       |    |       |
| 5) 2-Fluorophenol           | 5.38  | 112 | 230547  | 17.88 | ng | -0.02 |
| 7) Phenol-d6                | 6.39  | 99  | 1177848 | 75.81 | ng | -0.02 |
| 23) Nitrobenzene-d5         | 7.31  | 82  | 749657  | 61.35 | ng | -0.02 |
| 42) 2,4,6-Tribromophenol    | 10.59 | 330 | 24377   | 5.64  | ng | -0.02 |
| 45) 2-Fluorobiphenyl        | 9.12  | 172 | 1320235 | 52.69 | ng | -0.02 |
| 79) Terphenyl-d14           | 12.90 | 244 | 1567632 | 49.77 | ng | -0.01 |


|                                |       |     |        |        |    |      |
|--------------------------------|-------|-----|--------|--------|----|------|
| Target Compounds               |       |     |        | Qvalue |    |      |
| 9) Benzaldehyde                | 6.30  | 77  | 35128  | 4.341  | ng | 95   |
| 10) Phenol                     | 6.40  | 94  | 68287  | 4.293  | ng | 92   |
| 19) n-Nitroso-di-n-propylamine | 7.31  | 70  | 95251  | 13.300 | ng | # 73 |
| 25) Isophorone                 | 7.31  | 82  | 748995 | 34.538 | ng | # 61 |
| 41) Hexachlorocyclopentadiene  | 8.93  | 237 | 17     | 7.300  | ng | # 11 |
| 50) Dimethylphthalate          | 9.51  | 163 | 287938 | 10.221 | ng | 99   |
| 57) 2,4-Dinitrotoluene         | 9.80  | 165 | 53170  | 6.527  | ng | # 32 |
| 71) Phenanthrene               | 11.32 | 178 | 104462 | 2.790  | ng | 99   |
| 75) Fluoranthene               | 12.52 | 202 | 361272 | 8.590  | ng | 99   |
| 78) Pyrene                     | 12.76 | 202 | 376865 | 8.567  | ng | 99   |
| 81) Benzo(a)anthracene         | 13.96 | 228 | 240129 | 6.171  | ng | # 78 |
| 83) Chrysene                   | 14.00 | 228 | 222324 | 5.821  | ng | 97   |
| 84) Bis(2-ethylhexyl)phthalate | 13.96 | 149 | 128889 | 5.346  | ng | 99   |
| 86) Indeno(1,2,3-cd)pyrene     | 16.92 | 276 | 164511 | 3.448  | ng | 96   |
| 88) Benzo(b)fluoranthene       | 15.02 | 252 | 424754 | 10.013 | ng | # 93 |
| 89) Benzo(k)fluoranthene       | 15.02 | 252 | 424754 | 10.517 | ng | # 95 |
| 90) Benzo(a)pyrene             | 15.39 | 252 | 264217 | 6.682  | ng | # 93 |
| 92) Benzo(g,h,i)perylene       | 17.36 | 276 | 173422 | 4.450  | ng | 100  |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\  
Data File : BP000709.D  
Acq On : 14 Oct 2019 14:41  
Operator : JU  
Sample : K5348-05  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :

Quant Time: Oct 15 02:42:29 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Oct 01 18:03:42 2019  
Response via : Initial Calibration

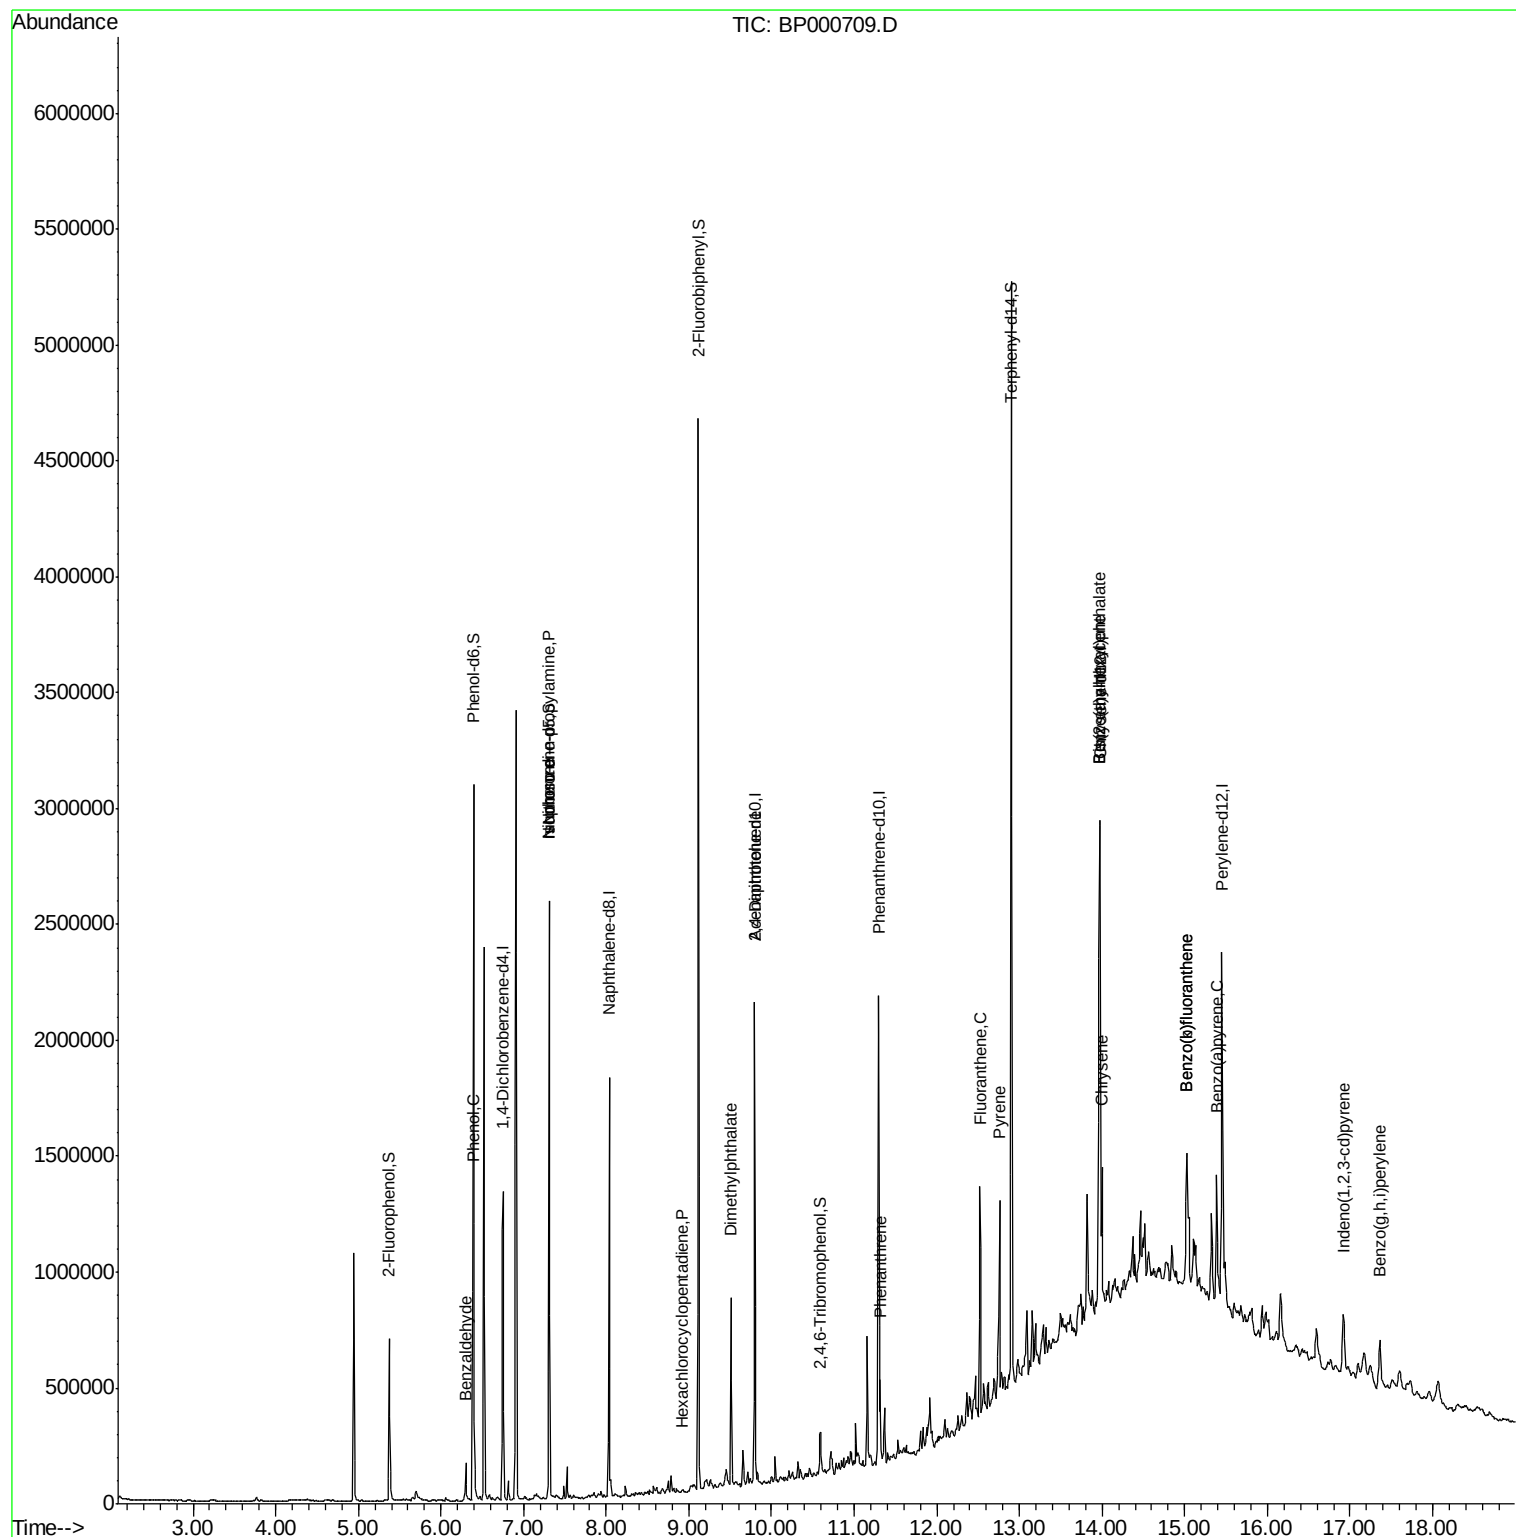




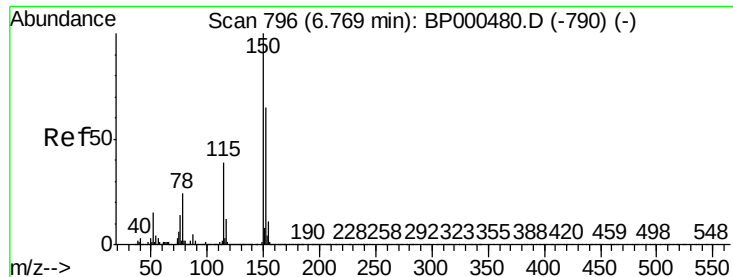


#1

1,4-Dichlorobenzene-d4  
Concen: 20.000 ng  
RT: 6.75 min Scan# 793  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

Instrument :  
BNA\_P  
ClientSampled :




| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 152     | 100   |       |       |
| 150     | 153.1 | 124.1 | 186.1 |
| 115     | 56.3  | 48.7  | 73.1  |

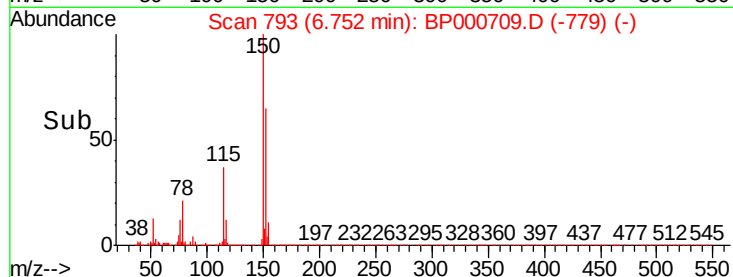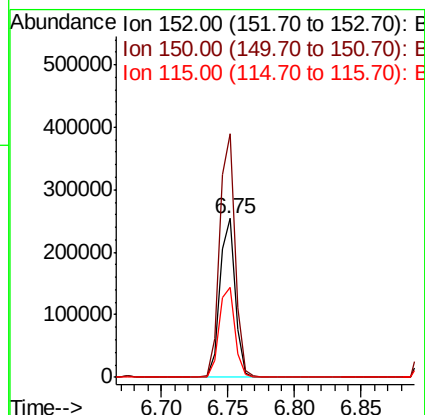


#5

2-Fluorophenol  
Concen: 17.881 ng  
RT: 5.38 min Scan# 559  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 112     | 100   |       |       |
| 64      | 44.6  | 34.2  | 51.4  |
| 63      | 22.6  | 17.9  | 26.9  |

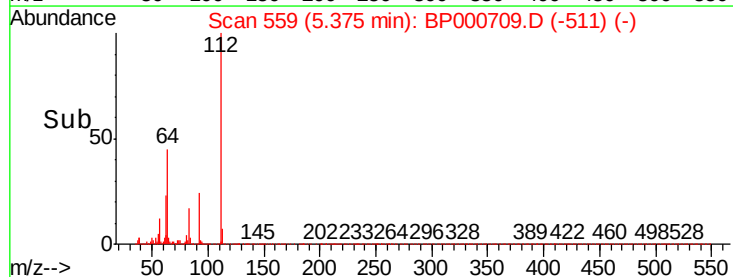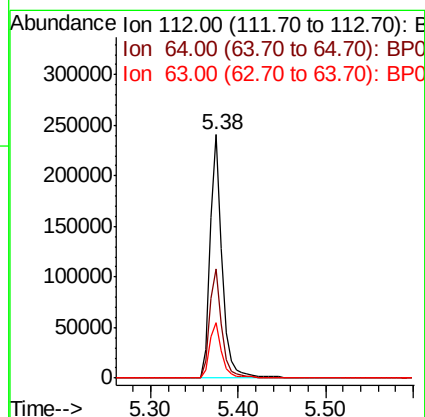

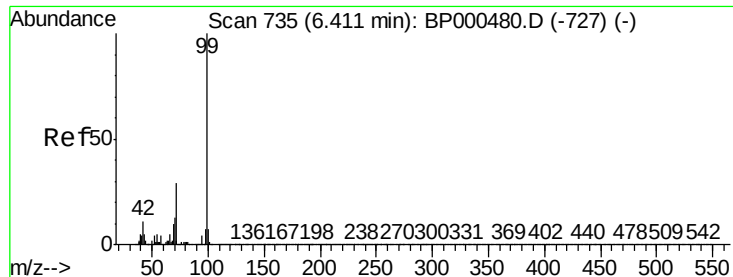

#7

Phenol-d6

Concen: 75.809 ng

RT: 6.39 min Scan# 732

Delta R.T. -0.02 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampleId :





Tot Ion: 99 Resp: 1177848

Ion Ratio Lower Upper

99 100

42 10.7 8.6 12.8

71 28.7 23.0 34.4

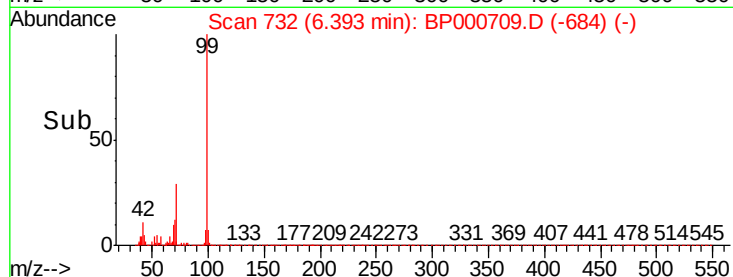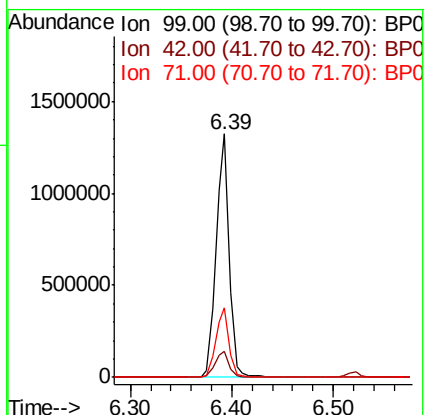

#9

Benzaldehyde

Concen: 4.341 ng

RT: 6.30 min Scan# 716

Delta R.T. -0.02 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41




Tgt Ion: 77 Resp: 35128


Ion Ratio Lower Upper

77 100

105 113.6 88.3 128.3

106 109.8 85.7 125.7

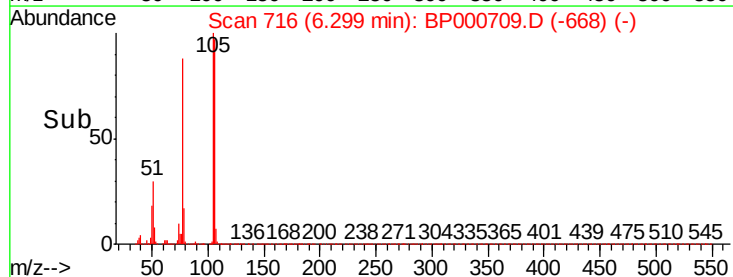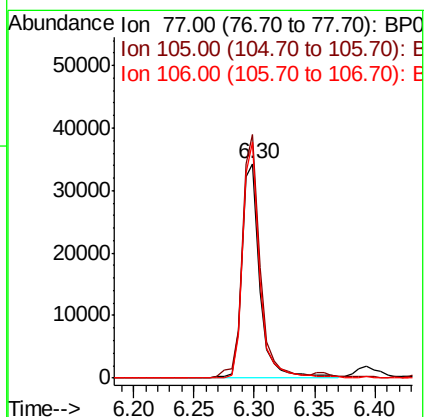

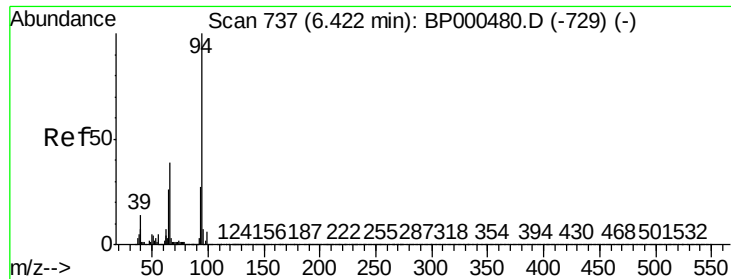

#10

Phenol

Concen: 4.293 ng

RT: 6.40 min Scan# 734

Delta R.T. -0.02 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampleId :


Tot Ion: 94 Resp: 68287

Ion Ratio Lower Upper

94 100

65 23.3 5.9 45.9




66 33.0 18.8 58.8



Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

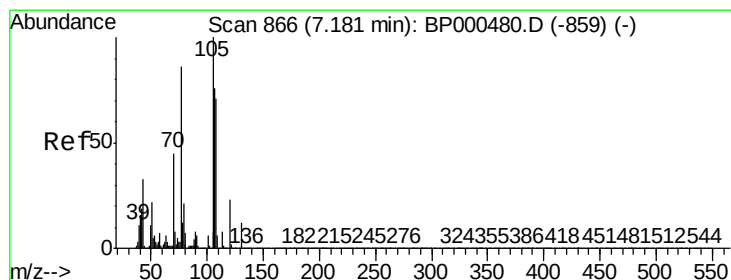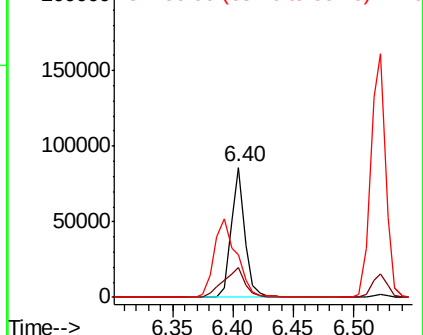

#19

n-Nitroso-di-n-propylamine

Concen: 13.300 ng

RT: 7.31 min Scan# 888

Delta R.T. 0.13 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Tgt Ion: 70 Resp: 95251


Ion Ratio Lower Upper

70 100

42 33.4 33.2 49.8

101 0.1 9.9 14.9#

130 2.6 21.8 32.8#


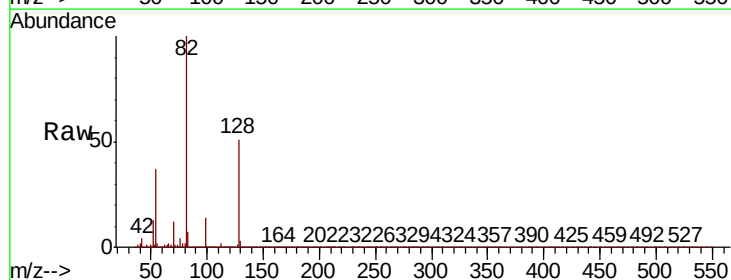



Abundance Ion 70.00 (69.70 to 70.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

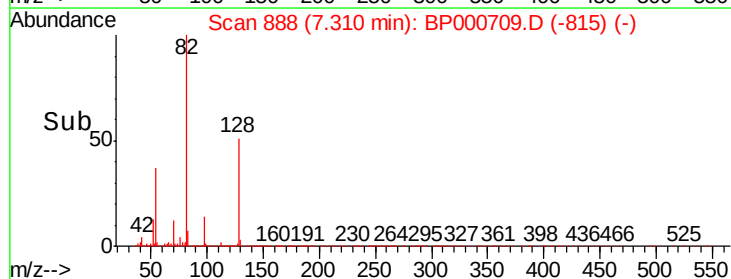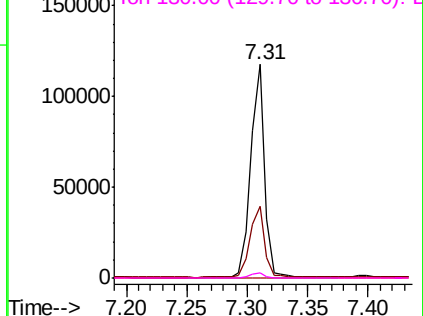







#21  
Naphthalene-d8  
Concen: 20.000 ng  
RT: 8.03 min Scan# 1011  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

Instrument :  
BNA\_P  
ClientSampled :

|             |       |        |
|-------------|-------|--------|
| Tot Ion:136 | Resp: | 746272 |
| Ion Ratio   | Lower | Upper  |
| 136 100     |       |        |
| 137 11.0    | 8.2   | 12.4   |
| 54 5.3      | 4.1   | 6.1    |
| 68 5.4      | 4.1   | 6.1    |

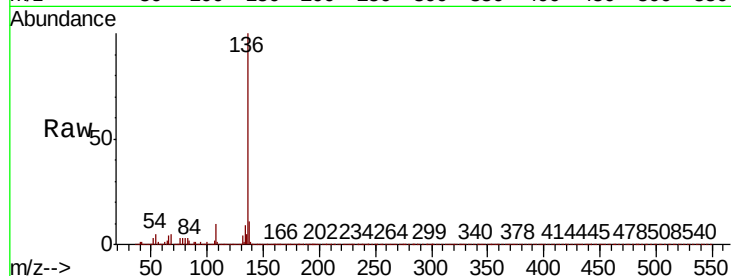


Abundance Ion 136.00 (135.70 to 136.70): E  
1500000  
Ion 137.00 (136.70 to 137.70): E  
Ion 54.00 (53.70 to 54.70): BP0  
Ion 68.00 (67.70 to 68.70): BP0

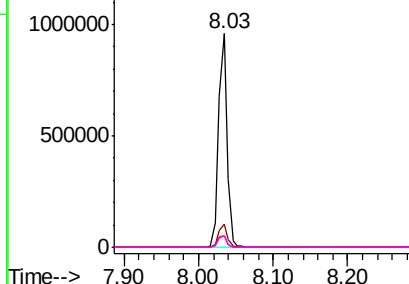




#23  
Nitrobenzene-d5  
Concen: 61.352 ng  
RT: 7.31 min Scan# 888  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

|     |         |       |        |
|-----|---------|-------|--------|
| Tgt | Ion: 82 | Resp: | 749657 |
| Ion | Ratio   | Lower | Upper  |
| 82  | 100     |       |        |
| 128 | 50.6    | 40.9  | 61.3   |
| 54  | 37.2    | 29.4  | 44.2   |



Abundance Ion 82.00 (81.70 to 82.70): BP0  
1200000  
Ion 128.00 (127.70 to 128.70): E  
Ion 54.00 (53.70 to 54.70): BP0

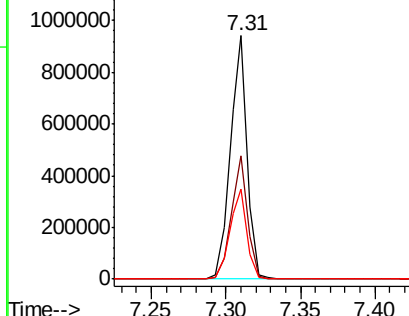



#25

Isophorone

Concen: 34.538 ng

RT: 7.31 min Scan# 888

Delta R.T. -0.28 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampleId :


Tot Ion: 82 Resp: 748995

Ion Ratio Lower Upper

82 100

95 0.0 5.8 8.6#

138 0.0 17.0 25.4#



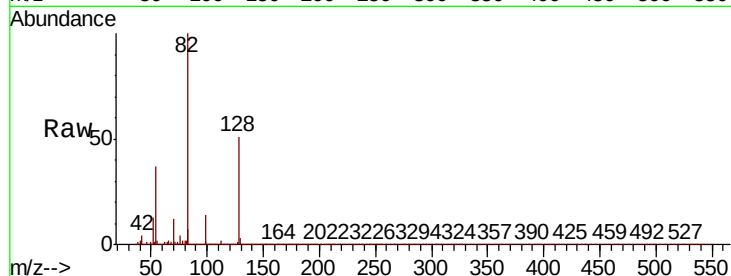


Abundance Ion 82.00 (81.70 to 82.70): BP000480.D (-930) (-)

Ion 95.00 (94.70 to 95.70): BP000480.D (-930) (-)

Ion 138.00 (137.70 to 138.70): BP000480.D (-930) (-)

Time-->

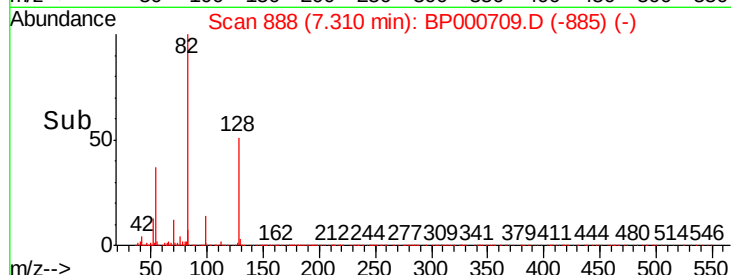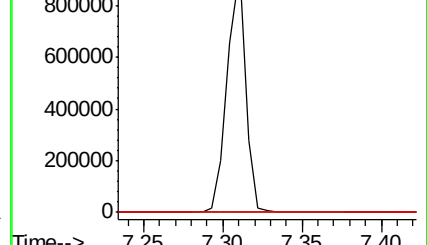

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.80 min Scan# 1311

Delta R.T. -0.02 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41


Tgt Ion: 164 Resp: 405439

Ion Ratio Lower Upper

164 100

162 100.5 82.2 123.2

160 44.9 37.6 56.4






Abundance Ion 164.00 (163.70 to 164.70): BP000480.D (-1307) (-)

Ion 162.00 (161.70 to 162.70): BP000480.D (-1307) (-)

Ion 160.00 (159.70 to 160.70): BP000480.D (-1307) (-)

Time-->

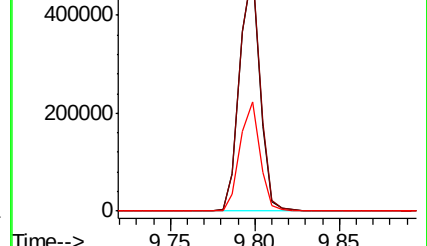



#41

Hexachlorocyclopentadiene

Concen: 7.300 ng

RT: 8.93 min Scan# 1163

Delta R.T. -0.00 min

Lab File: BP000709.D





Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampled :

|           |       |       |       |
|-----------|-------|-------|-------|
| Tot Ion:  | 237   | Resp: | 17    |
| Ion Ratio | Lower | Upper |       |
| 237       | 100   |       |       |
| 235       | 0.0   | 42.9  | 82.9# |
| 272       | 63.2  | 0.0   | 32.4# |

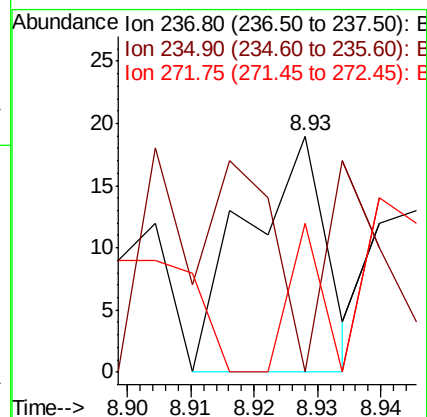

#42

2,4,6-Tribromophenol

Concen: 5.642 ng




RT: 10.59 min Scan# 1446

Delta R.T. -0.02 min


Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 330   | Resp: | 24377 |
| Ion Ratio | Lower | Upper |       |
| 330       | 100   |       |       |
| 332       | 95.8  | 77.1  | 115.7 |
| 141       | 34.1  | 26.0  | 39.0  |

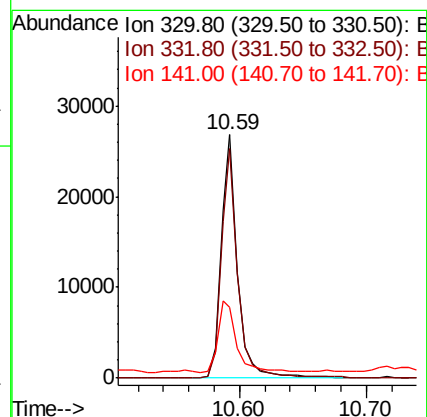







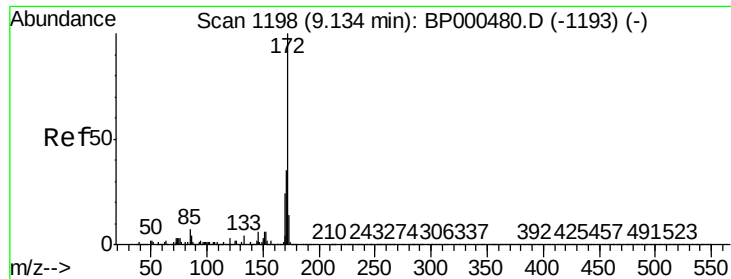

#45  
2-Fluorobiphenyl  
Concen: 52.687 ng  
RT: 9.12 min Scan# 1195  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41




Instrument :  
BNA\_P  
ClientSampleId :


Tot Ion:172 Resp: 1320235  
Ion Ratio Lower Upper  
172 100  
171 35.9 28.4 42.6  
170 23.8 19.1 28.7

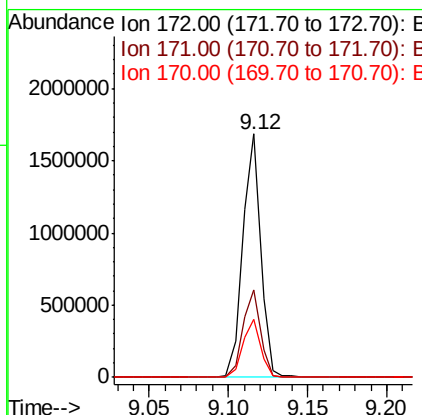

#50  
Dimethylphthalate  
Concen: 10.221 ng  
RT: 9.51 min Scan# 1262  
Delta R.T. -0.03 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

Tgt Ion:163 Resp: 287938  
Ion Ratio Lower Upper  
163 100  
194 4.6 3.4 5.2  
164 10.3 8.0 12.0


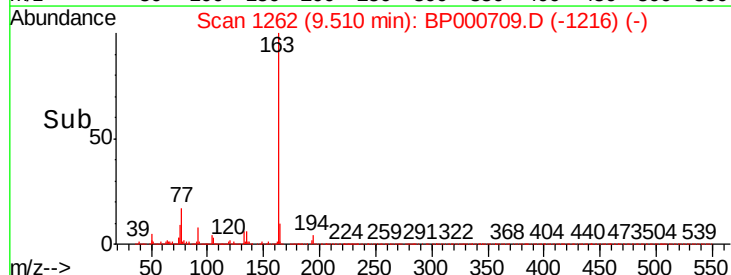
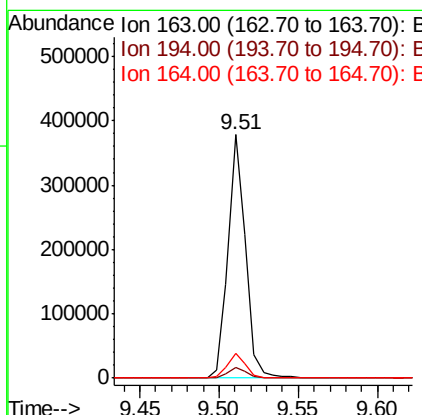



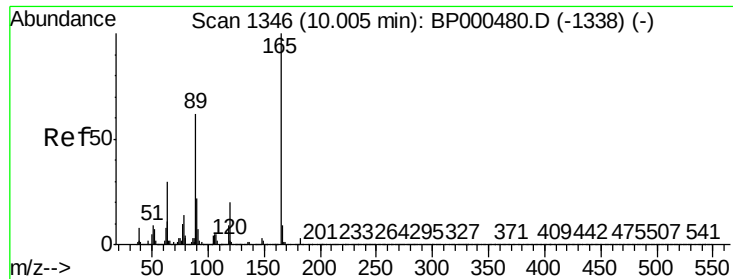

#57  
2,4-Dinitrotoluene  
Concen: 6.527 ng  
RT: 9.80 min Scan# 1311  
Delta R.T. -0.21 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41




Instrument :  
BNA\_P  
ClientSampleId :


|             |       |            |
|-------------|-------|------------|
| Tot Ion:165 | Resp: | 53170      |
| Ion Ratio   | Lower | Upper      |
| 165         | 100   |            |
| 63          | 0.9   | 24.2 36.4# |
| 89          | 1.4   | 49.4 74.0# |
| 182         | 0.4   | 2.5 3.7#   |

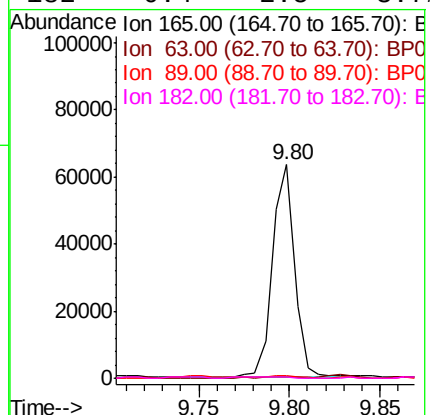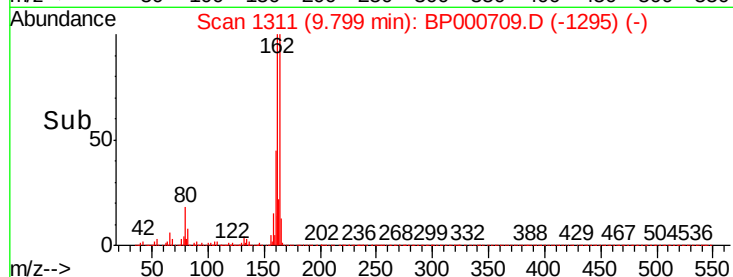

#64  
Phenanthrene-d10  
Concen: 20.000 ng  
RT: 11.30 min Scan# 1566  
Delta R.T. -0.01 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

|             |       |          |
|-------------|-------|----------|
| Tgt Ion:188 | Resp: | 745614   |
| Ion Ratio   | Lower | Upper    |
| 188         | 100   |          |
| 94          | 8.8   | 8.2 12.2 |
| 80          | 8.8   | 8.3 12.5 |


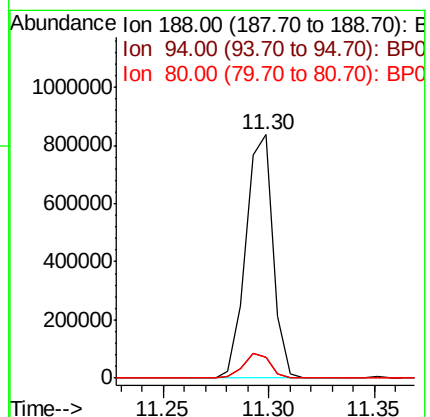
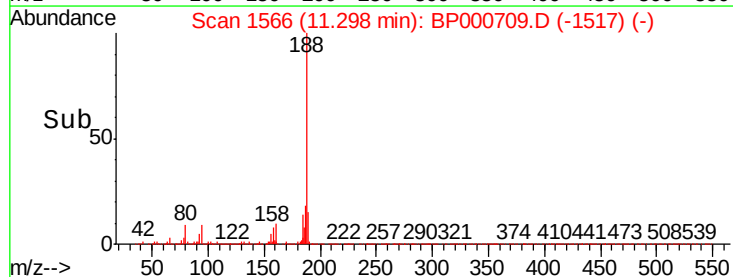



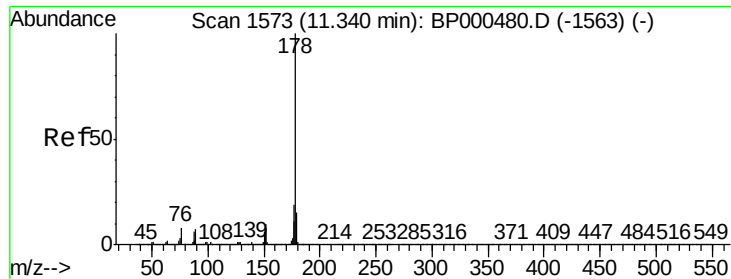

#71  
Phenanthrene  
Concen: 2.790 ng  
RT: 11.32 min Scan# 1569  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41




Instrument :  
BNA\_P  
ClientSampleId :


Tot Ion:178 Resp: 104462  
Ion Ratio Lower Upper  
178 100  
176 19.1 15.4 23.2  
179 16.3 12.2 18.4

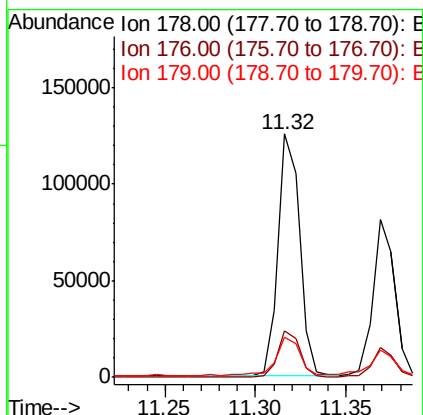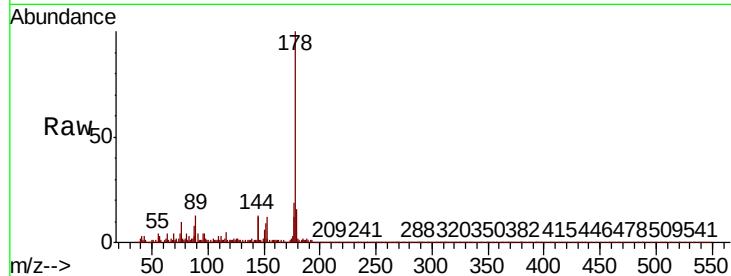

#75  
Fluoranthene  
Concen: 8.590 ng  
RT: 12.52 min Scan# 1774  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

Tgt Ion:202 Resp: 361272  
Ion Ratio Lower Upper  
202 100  
101 12.2 0.0 31.3  
203 17.7 0.0 38.1

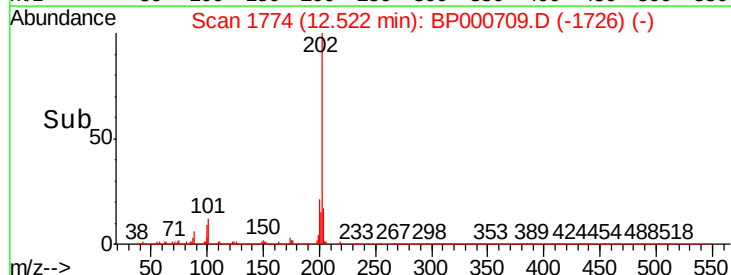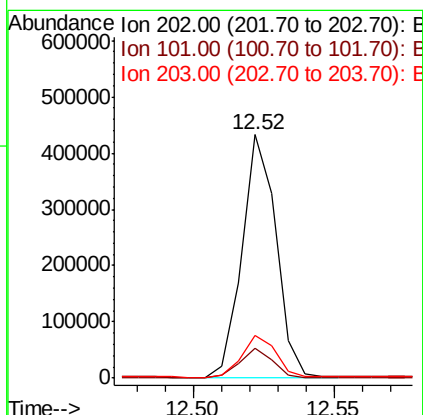



#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.97 min Scan# 2021

Delta R.T. -0.01 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampleId :


Tot Ion:240 Resp: 637792

Ion Ratio Lower Upper

240 100

120 10.8 10.1 15.1




236 26.6 22.7 34.1



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

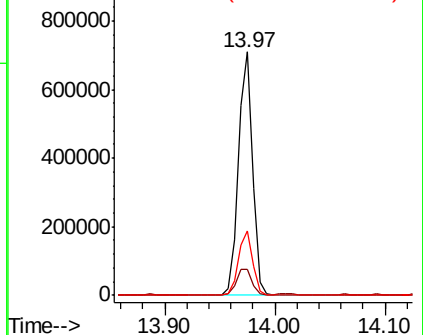

#78

Pyrene

Concen: 8.567 ng

RT: 12.76 min Scan# 1814

Delta R.T. -0.01 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41


Tgt Ion:202 Resp: 376865

Ion Ratio Lower Upper

202 100

200 20.8 17.1 25.7



203 17.5 14.6 21.8




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

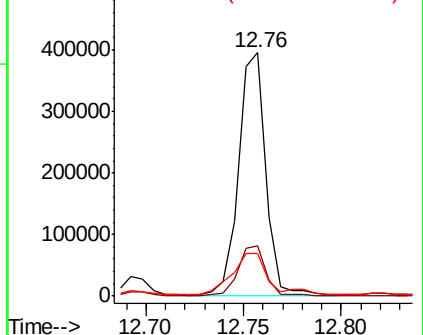

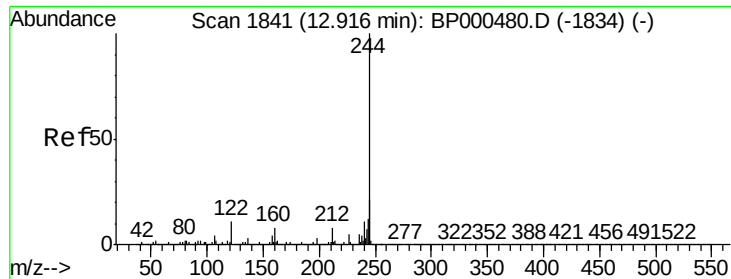

#79

Terphenyl-d14

Concen: 49.766 ng

RT: 12.90 min Scan# 1839

Delta R.T. -0.01 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampled :


Tot Ion:244 Resp: 1567632

Ion Ratio Lower Upper

244 100

212 7.1 6.0 9.0




122 10.7 8.9 13.3

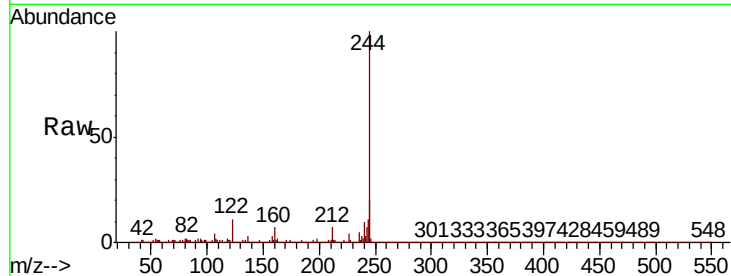

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

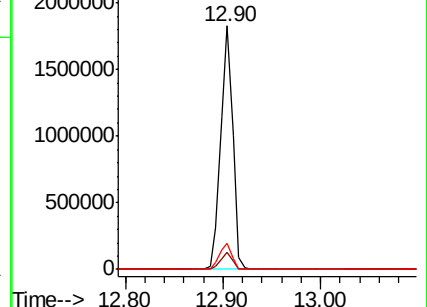

#81

Benzo(a)anthracene

Concen: 6.171 ng

RT: 13.96 min Scan# 2019

Delta R.T. -0.01 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41


Tgt Ion:228 Resp: 240129

Ion Ratio Lower Upper

228 100

226 43.1 21.4 32.2#



229 21.8 14.7 22.1




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

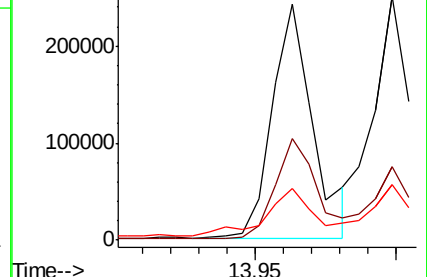

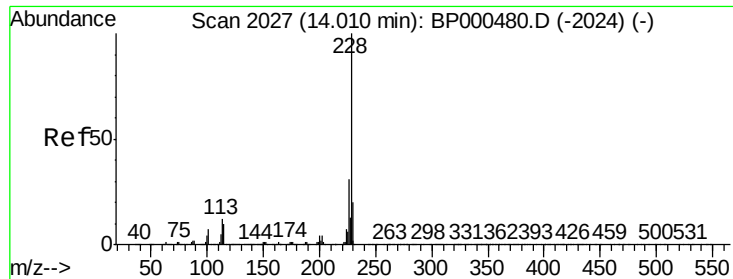

#83

Chrysene

Concen: 5.821 ng

RT: 14.00 min Scan# 2025

Delta R.T. -0.01 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41

Instrument :

BNA\_P

ClientSampleId :





Tot Ion:228 Resp: 222324

Ion Ratio Lower Upper

228 100

226 30.1 24.7 37.1

229 22.6 16.3 24.5

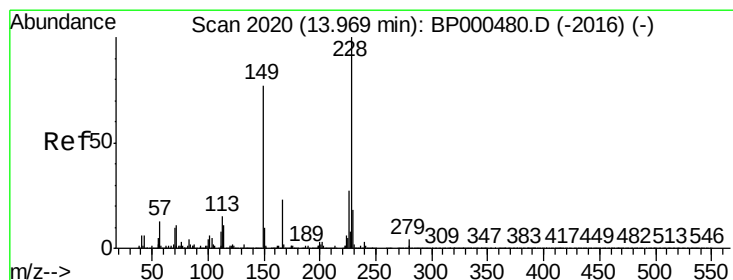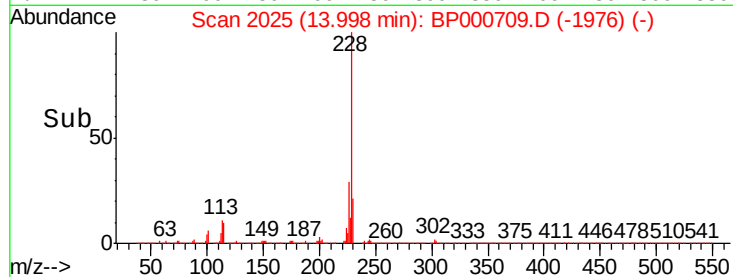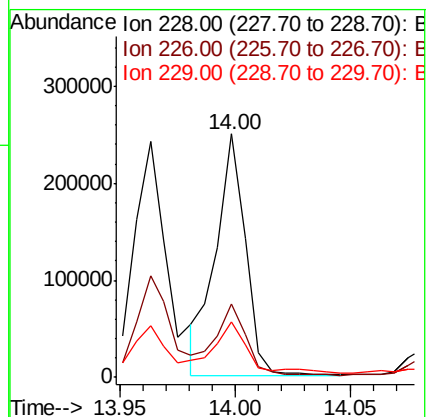

#84

Bis(2-ethylhexyl)phthalate

Concen: 5.346 ng

RT: 13.96 min Scan# 2019

Delta R.T. -0.01 min

Lab File: BP000709.D

Acq: 14 Oct 2019 14:41




Tgt Ion:149 Resp: 128889


Ion Ratio Lower Upper

149 100

167 28.8 23.6 35.4

279 5.1 3.9 5.9


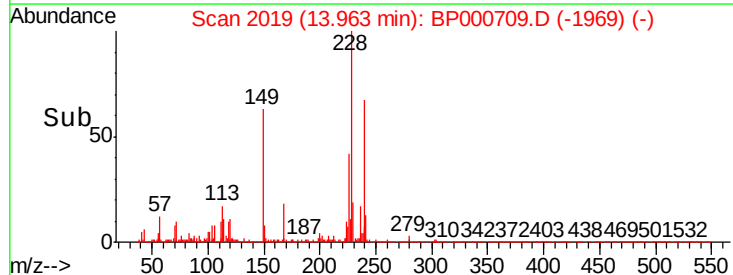
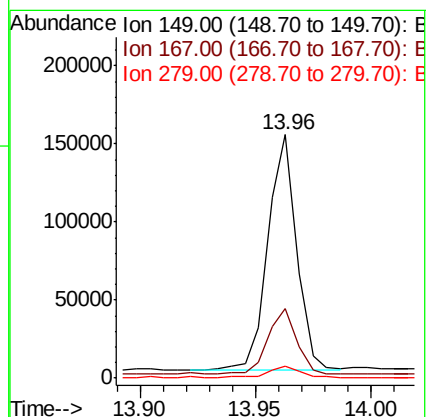





#86  
 Indeno(1,2,3-cd)pyrene  
 Concen: 3.448 ng  
 RT: 16.92 min Scan# 2522  
 Delta R.T. -0.01 min  
 Lab File: BP000709.D  
 Acq: 14 Oct 2019 14:41




Instrument :  
 BNA\_P  
 ClientSampleId :


| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 276     | 100   |       |       |
| 138     | 22.5  | 20.9  | 31.3  |
| 277     | 24.9  | 20.6  | 30.8  |

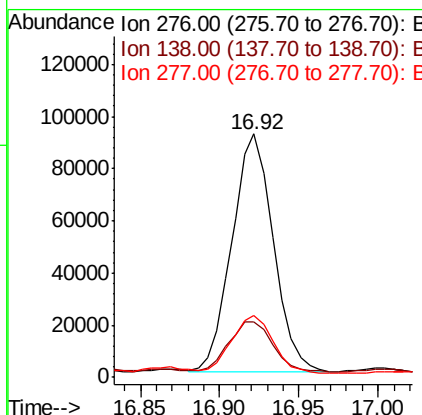

#87  
 Perylene-d12  
 Concen: 20.000 ng  
 RT: 15.45 min Scan# 2272  
 Delta R.T. -0.01 min  
 Lab File: BP000709.D  
 Acq: 14 Oct 2019 14:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 264     | 100   |       |       |
| 260     | 23.8  | 20.3  | 30.5  |
| 265     | 22.0  | 18.0  | 27.0  |


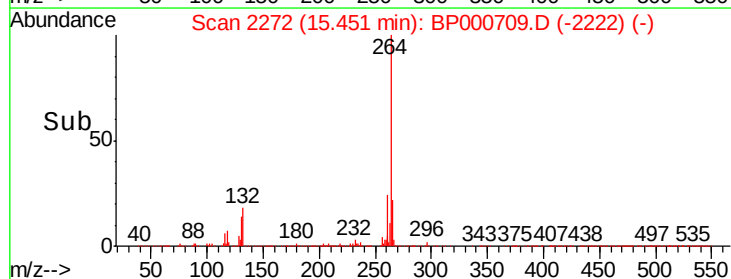
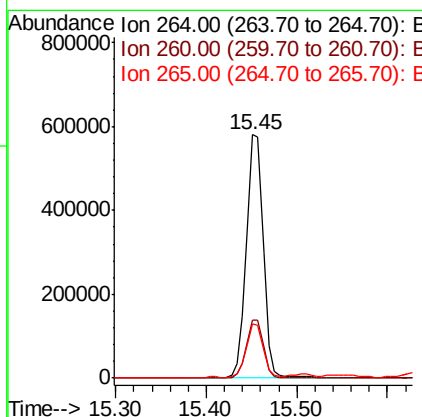



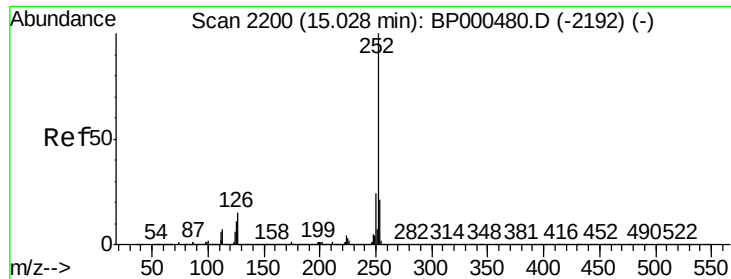

#88  
Benzo(b)fluoranthene  
Concen: 10.013 ng  
RT: 15.02 min Scan# 2199  
Delta R.T. -0.01 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41




Instrument :  
BNA\_P  
ClientSampled :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 23.3  | 17.0  | 25.4  |
| 125     | 15.7  | 8.9   | 13.3# |

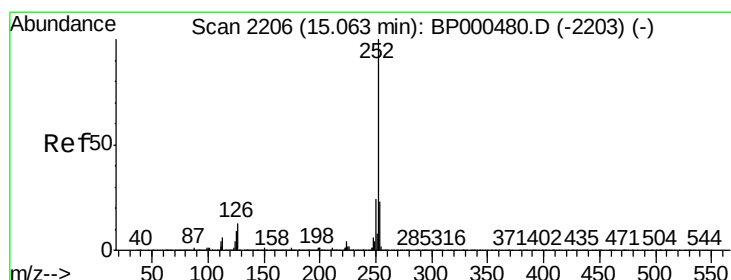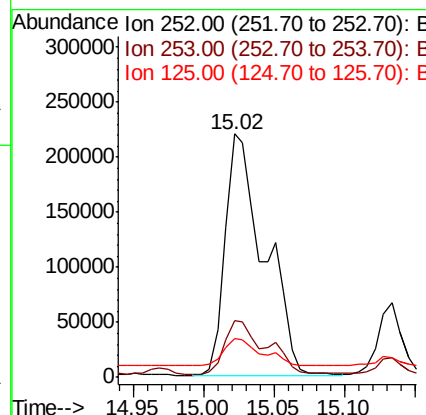


#89  
Benzo(k)fluoranthene  
Concen: 10.517 ng  
RT: 15.02 min Scan# 2199  
Delta R.T. -0.04 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 23.3  | 18.4  | 27.6  |
| 125     | 15.7  | 7.8   | 11.8# |

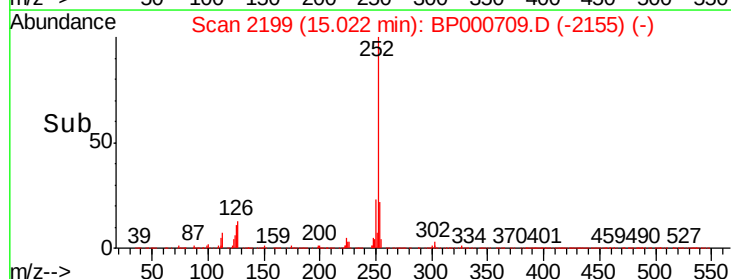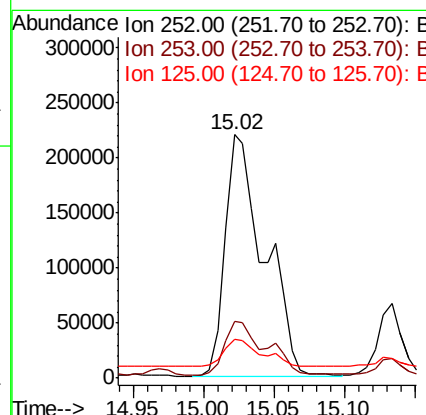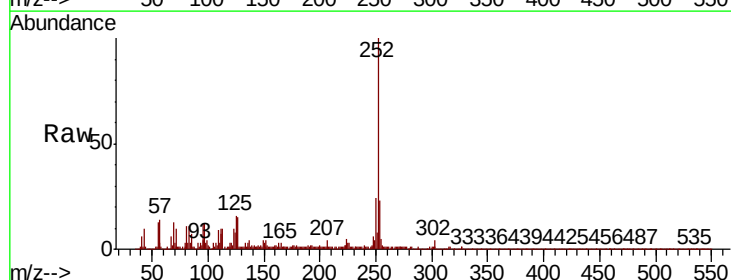







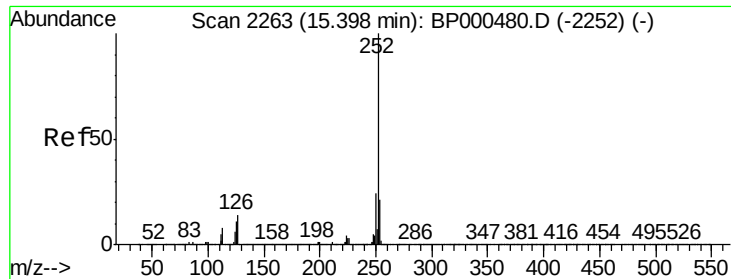

#90  
Benzo(a)pyrene  
Concen: 6.682 ng  
RT: 15.39 min Scan# 2261  
Delta R.T. -0.01 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

Instrument :  
BNA\_P  
ClientSampleId :

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 23.4  | 17.0  | 25.6  |
| 125     | 15.3  | 8.4   | 12.6  |

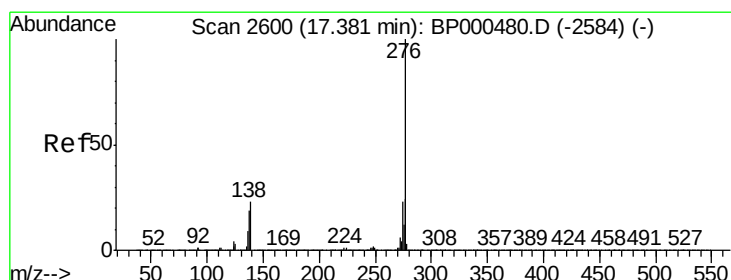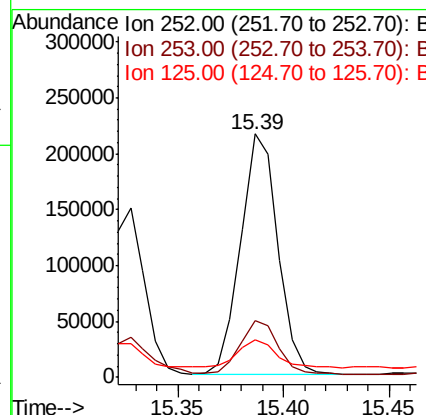

#92  
Benzo(g,h,i)perylene  
Concen: 4.450 ng  
RT: 17.36 min Scan# 2597  
Delta R.T. -0.02 min  
Lab File: BP000709.D  
Acq: 14 Oct 2019 14:41

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 276     | 100   |       |       |
| 277     | 24.3  | 19.4  | 29.2  |
| 138     | 23.4  | 18.5  | 27.7  |

