


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN101419\
 Data File : BN008133.D
 Acq On : 14 Oct 2019 14:26
 Operator : JU
 Sample : DFTPP03
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN101019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 14 17:19:29 2019

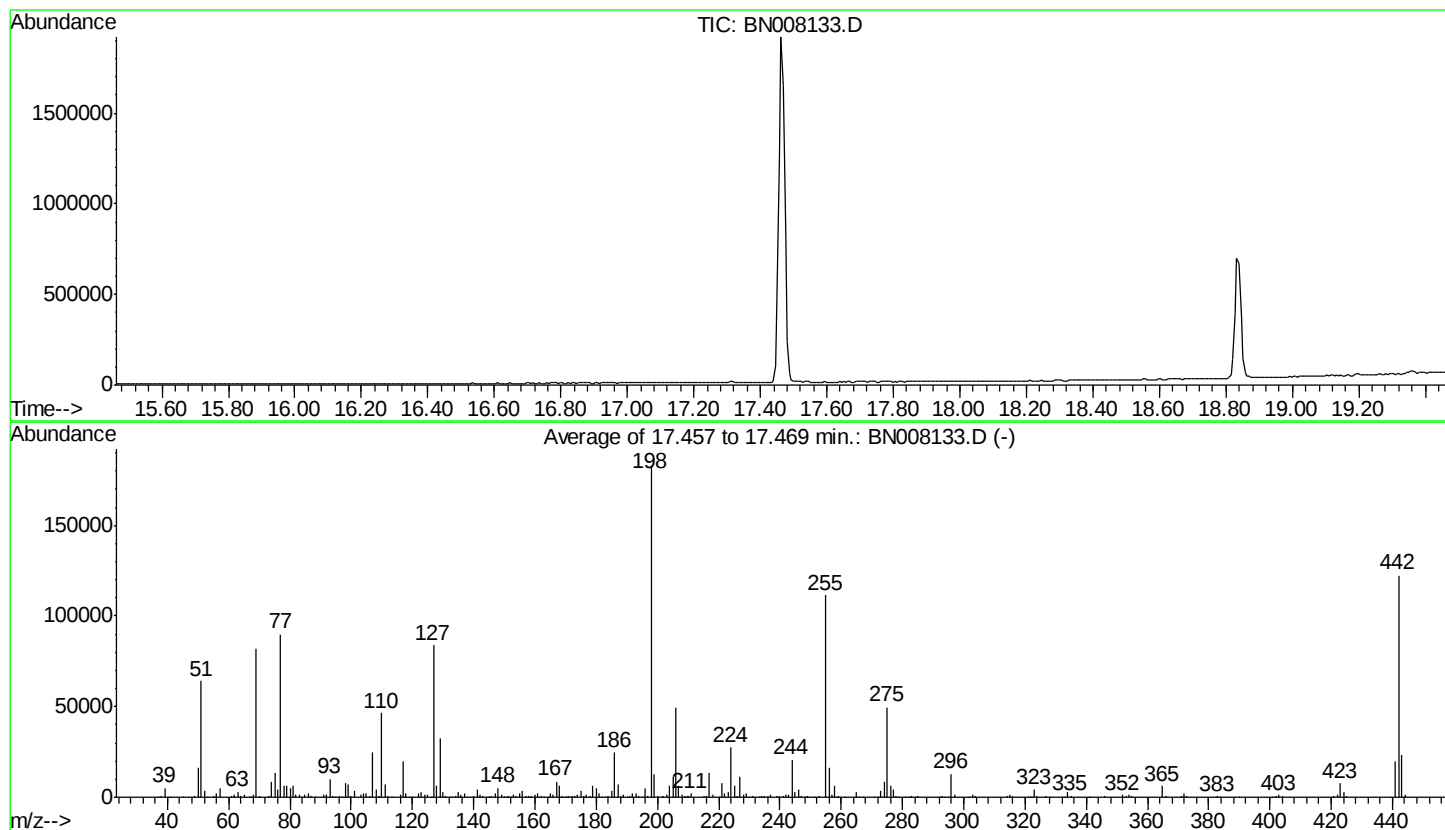

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	64082	PASS
68	69	0.00	2	1.5	1207	PASS
69	198	0.00	100	45.0	82293	PASS
70	69	0.00	2	0.5	447	PASS
127	198	10	80	45.9	83973	PASS
197	198	0.00	2	0.3	532	PASS
198	198	100	100	100.0	182997	PASS
199	198	5	9	6.9	12572	PASS
275	198	10	60	27.1	49602	PASS
365	198	1	100	3.3	6084	PASS
441	198	0.01	100	10.7	19661	PASS
442	198	50	100	66.9	122384	PASS
443	442	15	24	18.9	23184	PASS