
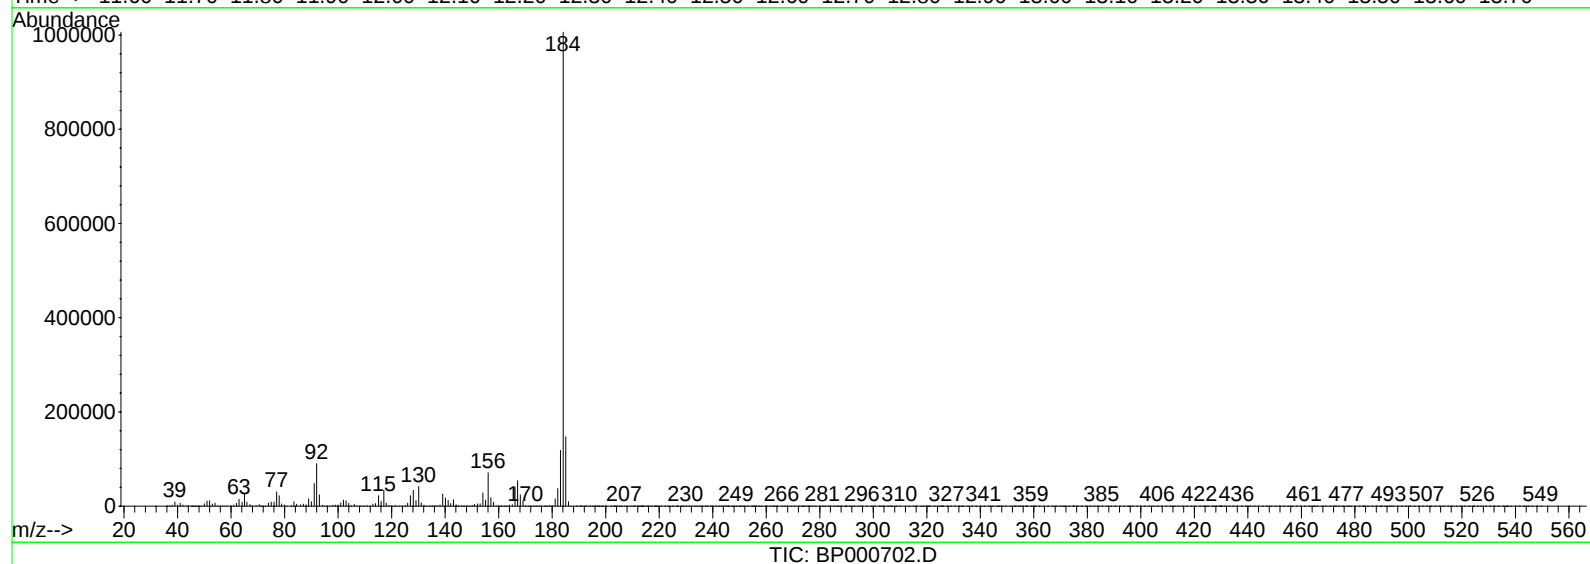


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101419\
 Data File : BP000702.D
 Acq On : 14 Oct 2019 11:28
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 09:16:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 01 18:03:42 2019
 Response via : Initial Calibration

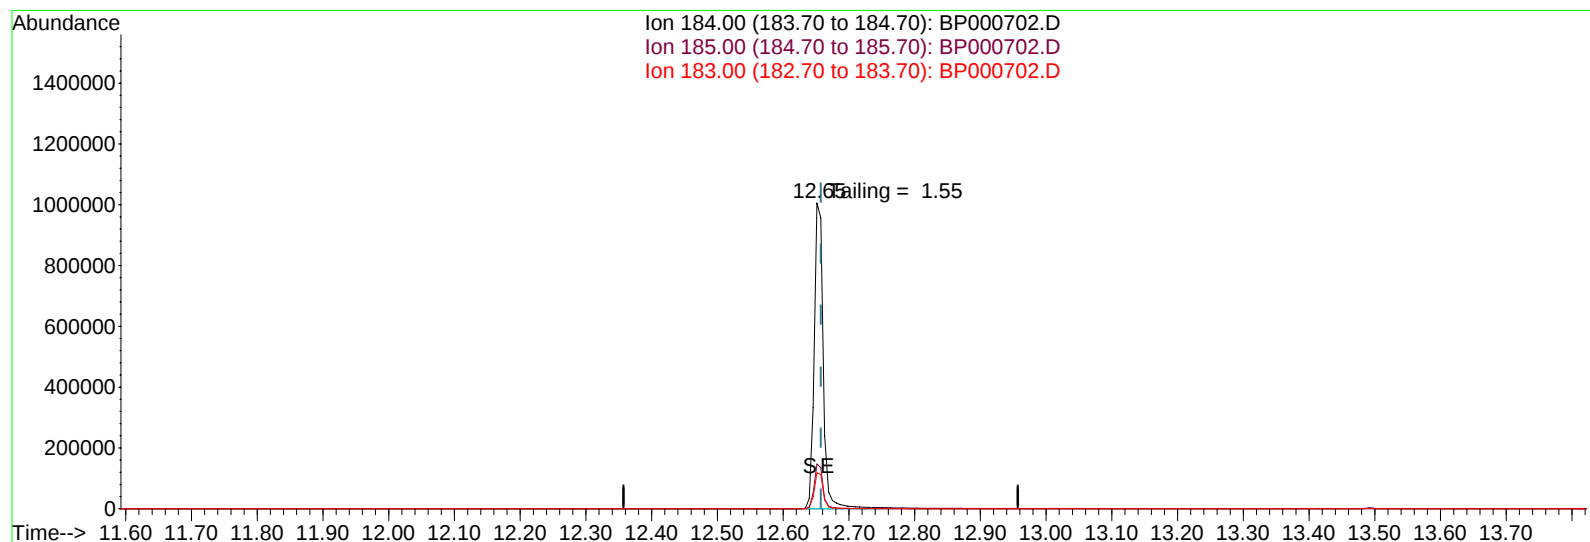

(77) Benzidine



12.651min (-0.006) 433433.72ng

response 978992

Ion	Exp%	Act%
184.00	100	100
185.00	15.90	14.66
183.00	12.10	11.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP101419\
Data File : BP000702.D
Acq On : 14 Oct 2019 11:28
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 15 09:16:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 01 18:03:42 2019
Response via : Initial Calibration

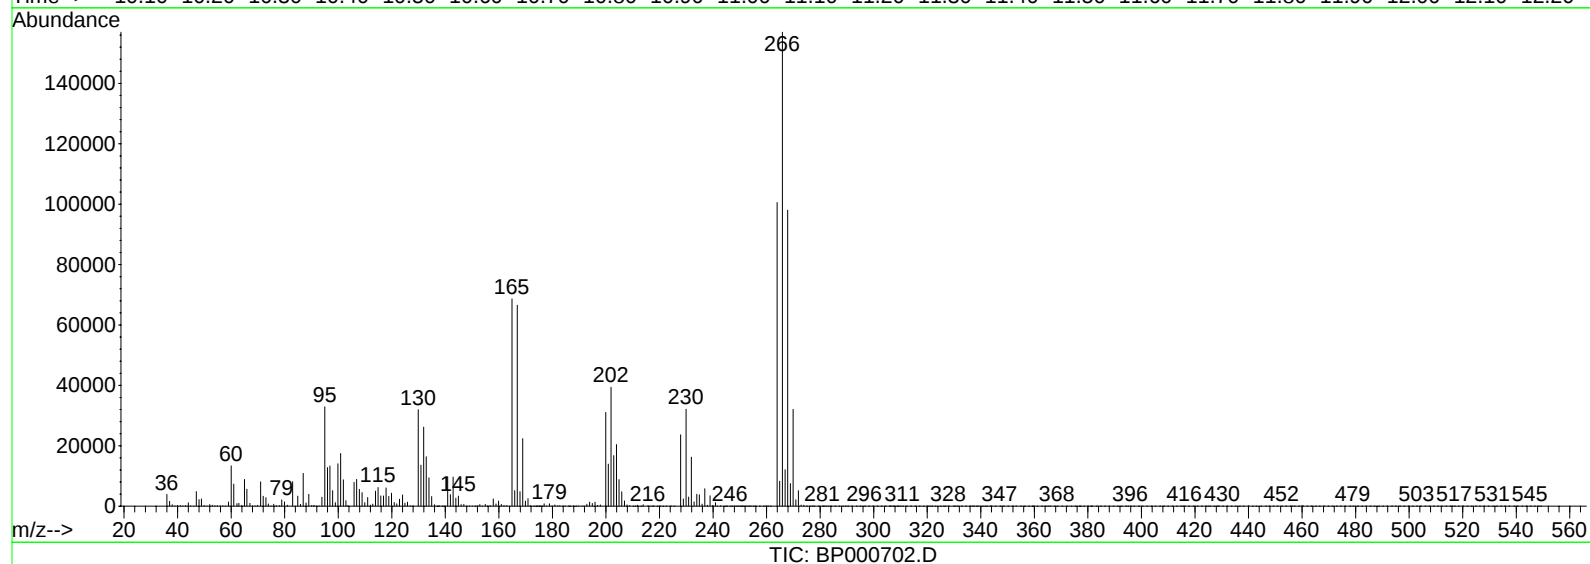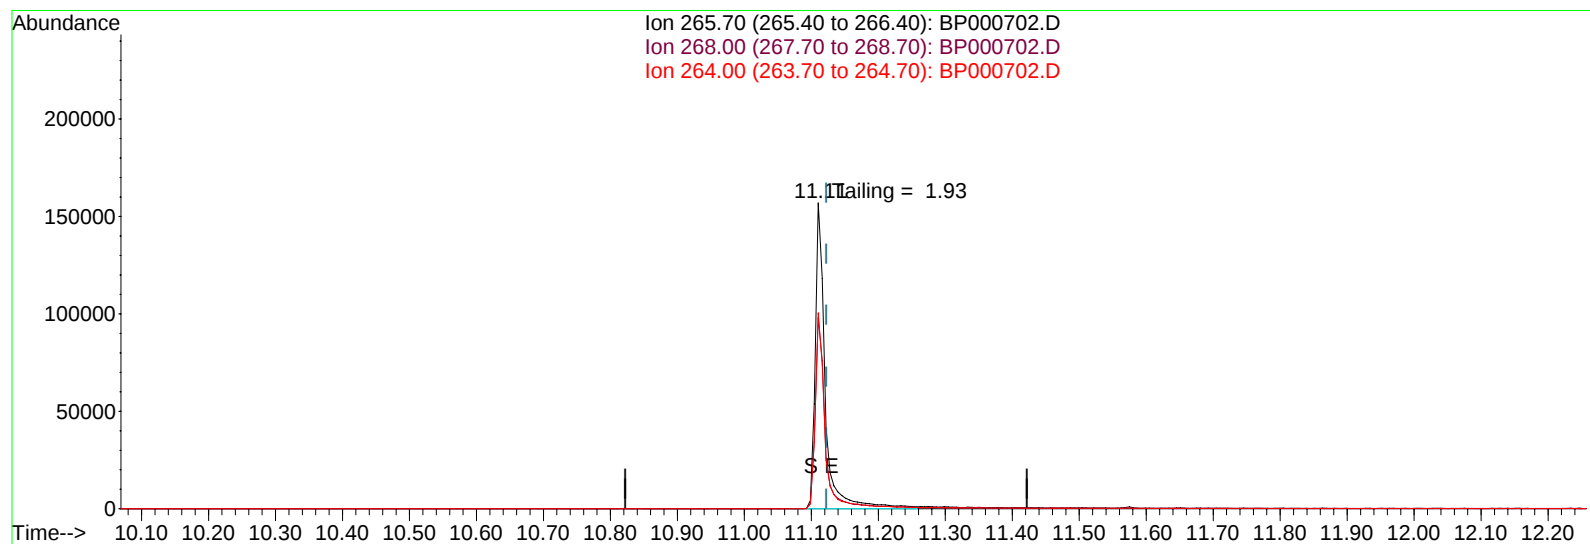

(70) Pentachlorophenol (C)

11.110min (-0.012) 2895226.76ng

response 163626

Ion	Exp%	Act%
265.70	100	100
268.00	66.50	62.46
264.00	61.20	64.08
0.00	0.00	0.00