

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000705.D
 Acq On : 14 Oct 2019 13:04
 Operator : JU
 Sample : K5348-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190825-COMPOSITE-ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.952	481	487	490	rBV	1259082	1423104	33.78%	3.107%
2	5.375	555	559	570	rVB	504226	493516	11.72%	1.077%
3	5.681	609	611	623	rVB2	36731	73568	1.75%	0.161%
4	6.299	711	716	720	rBV	178326	185696	4.41%	0.405%
5	6.393	727	732	742	rBV	2981936	3085396	73.24%	6.735%
6	6.522	750	754	757	rBV	2034053	1781238	42.28%	3.888%
7	6.752	789	793	801	rVB	1311682	1183237	28.09%	2.583%
8	6.816	801	804	811	rBV	104379	88362	2.10%	0.193%
9	6.905	815	819	823	rBV	3705163	3014399	71.56%	6.580%
10	7.310	884	888	891	rBV	2726112	2199506	52.21%	4.802%
11	7.487	915	918	921	rBV	66388	51314	1.22%	0.112%
12	7.528	921	925	928	rVV	154150	136880	3.25%	0.299%
13	7.852	977	980	987	rVB2	39586	50444	1.20%	0.110%
14	8.034	1007	1011	1013	rBV	1727239	1454949	34.54%	3.176%
15	8.052	1013	1014	1018	rVB	87861	55764	1.32%	0.122%
16	8.781	1135	1138	1142	rBV2	78134	71196	1.69%	0.155%
17	9.116	1191	1195	1198	rBV	4617228	3774848	89.61%	8.241%
18	9.216	1205	1212	1215	rBV5	45321	99867	2.37%	0.218%
19	9.510	1259	1262	1267	rBV	902035	724449	17.20%	1.581%
20	9.657	1284	1287	1292	rBV	157429	161036	3.82%	0.352%
21	9.710	1293	1296	1299	rVB3	59949	61794	1.47%	0.135%
22	9.799	1307	1311	1314	rVB	2008197	1749953	41.54%	3.820%
23	10.040	1349	1352	1355	rVB	111513	98599	2.34%	0.215%
24	10.322	1397	1400	1402	rBV	96397	83082	1.97%	0.181%
25	10.346	1402	1404	1411	rVB2	51144	68494	1.63%	0.150%
26	10.593	1443	1446	1452	rVB2	139279	201181	4.78%	0.439%
27	10.716	1464	1467	1475	rVB4	97762	167933	3.99%	0.367%
28	10.781	1475	1478	1481	rBV	60647	66695	1.58%	0.146%
29	10.957	1505	1508	1512	rVB4	69553	70638	1.68%	0.154%
30	11.022	1516	1519	1521	rBV	191645	164398	3.90%	0.359%
31	11.157	1539	1542	1546	rBV	619101	565607	13.43%	1.235%
32	11.293	1562	1565	1568	rBV	2106081	1971540	46.80%	4.304%
33	11.316	1568	1569	1572	rVV	405145	263883	6.26%	0.576%
34	11.369	1574	1578	1581	rVB	272483	285825	6.79%	0.624%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
 Data File : BP000705.D
 Acq On : 14 Oct 2019 13:04
 Operator : JU
 Sample : K5348-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190825-COMPOSITE-ARE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.404	1582	1584	1588	rBV2	43092	49418	1.17%	0.108%
36	11.528	1603	1605	1608	rBV	93306	94081	2.23%	0.205%
37	11.804	1649	1652	1654	rBV	92771	85511	2.03%	0.187%
38	11.834	1654	1657	1660	rVV	97727	84098	2.00%	0.184%
39	11.881	1662	1665	1666	rBV	72448	60828	1.44%	0.133%
40	11.898	1666	1668	1669	rVV	90439	73671	1.75%	0.161%
41	11.916	1669	1671	1674	rVB	158612	136197	3.23%	0.297%
42	12.098	1699	1702	1705	rVB3	102330	106250	2.52%	0.232%
43	12.257	1727	1729	1731	rVB	82126	61355	1.46%	0.134%
44	12.287	1732	1734	1736	rBV	51202	51425	1.22%	0.112%
45	12.363	1744	1747	1749	rBV	130384	135914	3.23%	0.297%
46	12.440	1758	1760	1762	rBV2	75265	86144	2.04%	0.188%
47	12.463	1762	1764	1767	rVV	160876	158696	3.77%	0.346%
48	12.522	1771	1774	1777	rBV	1179134	942070	22.36%	2.057%
49	12.569	1779	1782	1784	rVV2	108439	95163	2.26%	0.208%
50	12.616	1788	1790	1793	rBV	115301	106888	2.54%	0.233%
51	12.693	1801	1803	1807	rVB	75347	63307	1.50%	0.138%
52	12.751	1808	1813	1816	rBV	1012154	1048167	24.88%	2.288%
53	12.781	1816	1818	1821	rVB2	63215	59701	1.42%	0.130%
54	12.875	1832	1834	1835	rBV	64559	49074	1.16%	0.107%
55	12.904	1835	1839	1842	rVV	4749438	4212538	100.00%	9.196%
56	13.063	1864	1866	1868	rBV2	69119	78547	1.86%	0.171%
57	13.087	1868	1870	1874	rVB	328649	275354	6.54%	0.601%
58	13.157	1878	1882	1885	rBV	259429	250538	5.95%	0.547%
59	13.193	1886	1888	1891	rVV2	137370	112178	2.66%	0.245%
60	13.287	1902	1904	1907	rVB	121361	100787	2.39%	0.220%
61	13.316	1907	1909	1914	rBV	132152	139763	3.32%	0.305%
62	13.498	1937	1940	1942	rBV2	99774	97255	2.31%	0.212%
63	13.816	1991	1994	2001	rVB3	440746	537062	12.75%	1.172%
64	13.969	2015	2020	2023	rBV2	2358301	3028356	71.89%	6.611%
65	13.998	2023	2025	2028	rVB	544454	444758	10.56%	0.971%
66	14.151	2048	2051	2055	rVB4	106826	116845	2.77%	0.255%
67	14.363	2085	2087	2090	rVB	178406	149499	3.55%	0.326%
68	14.463	2101	2104	2106	rBV2	235246	237413	5.64%	0.518%
69	14.510	2110	2112	2116	rVB	227077	229264	5.44%	0.500%
70	14.839	2166	2168	2175	rVB2	219742	259872	6.17%	0.567%
71	15.022	2195	2199	2207	rBV	626347	1112699	26.41%	2.429%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000705.D
Acq On : 14 Oct 2019 13:04
Operator : JU
Sample : K5348-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190825-COMPOSITE-ARE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	15.110	2211	2214	2216	rBV2	178184	224596	5.33%	0.490%
73	15.322	2246	2250	2256	rVB	431878	576346	13.68%	1.258%
74	15.381	2257	2260	2267	rBV	569841	730464	17.34%	1.595%
75	15.451	2267	2272	2275	rBV	1574932	1960443	46.54%	4.280%
76	15.934	2350	2354	2357	rBV	152944	215287	5.11%	0.470%
77	16.157	2388	2392	2405	rVB5	163972	367032	8.71%	0.801%
78	16.916	2516	2521	2527	rBV2	258102	446948	10.61%	0.976%
79	17.357	2591	2596	2607	rVB	206610	428278	10.17%	0.935%


Sum of corrected areas: 45808471

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000705.D
Acq On : 14 Oct 2019 13:04
Operator : JU
Sample : K5348-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190825-COMPOSITE-ARE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

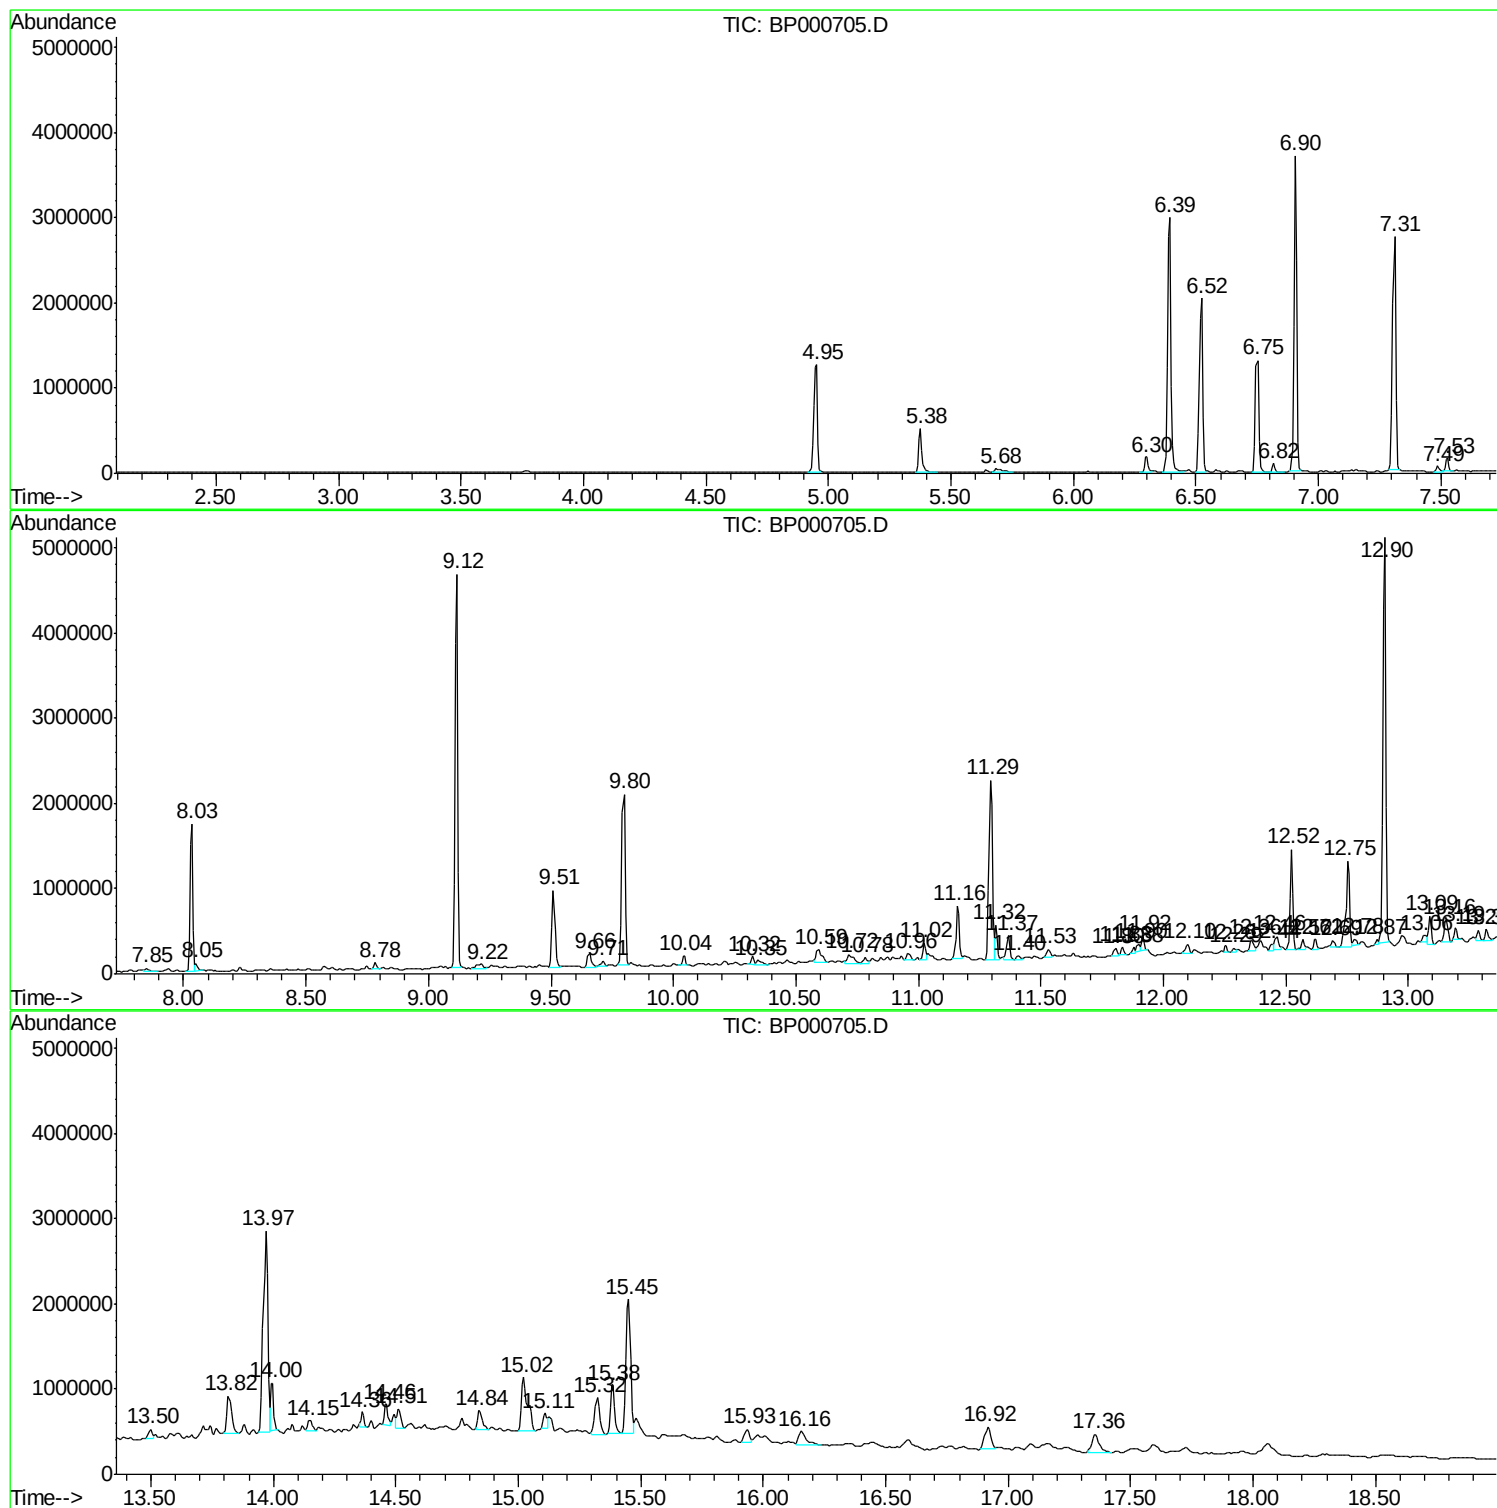

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000705.D
Acq_On : 14 Oct 2019 13:044
Operator : JUJ
Sample : K5348-01REE
Misc :
ALS_Vial : 4 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190825-COMPOSITE-ARE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
