

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000706.D
 Acq On : 14 Oct 2019 13:28
 Operator : JU
 Sample : K5348-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190826-COMPOSITE-BRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	481	486	490	rBV	1231762	1332355	35.86%	3.390%
2	5.375	555	559	569	rBV	718664	727825	19.59%	1.852%
3	5.675	608	610	622	rVB2	41514	84530	2.27%	0.215%
4	6.299	711	716	721	rBV	158030	161128	4.34%	0.410%
5	6.393	728	732	741	rBV	2778208	2732952	73.55%	6.953%
6	6.522	750	754	761	rBV	2270583	1909033	51.38%	4.857%
7	6.751	789	793	796	rBV	1305877	1118363	30.10%	2.845%
8	6.816	801	804	808	rBV	92172	71088	1.91%	0.181%
9	6.904	815	819	823	rBV	3192322	2578077	69.38%	6.559%
10	7.310	884	888	891	rBV	2310905	1868662	50.29%	4.754%
11	7.487	915	918	921	rBV	59798	46866	1.26%	0.119%
12	7.528	921	925	928	rVV	121768	105504	2.84%	0.268%
13	7.851	977	980	987	rVB3	26788	48709	1.31%	0.124%
14	8.034	1007	1011	1013	rBV	1684502	1416501	38.12%	3.604%
15	8.051	1013	1014	1018	rVB	68474	48163	1.30%	0.123%
16	8.234	1042	1045	1052	rVB	44856	45255	1.22%	0.115%
17	8.751	1127	1133	1135	rBV2	46863	53309	1.43%	0.136%
18	8.781	1135	1138	1141	rBV2	72946	61099	1.64%	0.155%
19	9.116	1191	1195	1198	rBV	4003642	3326396	89.52%	8.463%
20	9.257	1216	1219	1226	rVB2	33164	46691	1.26%	0.119%
21	9.457	1247	1253	1255	rBV7	33096	50144	1.35%	0.128%
22	9.510	1259	1262	1268	rBV	820666	641852	17.27%	1.633%
23	9.657	1283	1287	1292	rBV	113504	123616	3.33%	0.314%
24	9.716	1294	1297	1299	rVB2	43074	46142	1.24%	0.117%
25	9.798	1307	1311	1314	rVB	2060821	1707634	45.96%	4.344%
26	10.045	1350	1353	1355	rVB	106044	86820	2.34%	0.221%
27	10.322	1397	1400	1402	rVV	66349	57601	1.55%	0.147%
28	10.345	1402	1404	1411	rVB	40420	52087	1.40%	0.133%
29	10.592	1442	1446	1453	rBV2	120832	145505	3.92%	0.370%
30	10.716	1464	1467	1475	rVB4	76492	126894	3.42%	0.323%
31	10.781	1475	1478	1481	rBV	41072	47426	1.28%	0.121%
32	10.957	1506	1508	1512	rVB3	53688	55387	1.49%	0.141%
33	11.022	1516	1519	1521	rBV	189774	157400	4.24%	0.400%
34	11.157	1538	1542	1546	rBV	612633	563631	15.17%	1.434%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000706.D
 Acq On : 14 Oct 2019 13:28
 Operator : JU
 Sample : K5348-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190826-COMPOSITE-BRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.292	1562	1565	1568	rBV	2218749	1907681	51.34%	4.853%
36	11.316	1568	1569	1572	rVV	317835	196471	5.29%	0.500%
37	11.369	1574	1578	1581	rVB2	199899	226105	6.09%	0.575%
38	11.528	1602	1605	1608	rBV	72925	75768	2.04%	0.193%
39	11.804	1649	1652	1654	rBV	68024	59711	1.61%	0.152%
40	11.834	1654	1657	1659	rBV	73523	67166	1.81%	0.171%
41	11.881	1662	1665	1666	rBV2	43108	42793	1.15%	0.109%
42	11.898	1666	1668	1669	rVV	86823	74772	2.01%	0.190%
43	11.916	1669	1671	1674	rVB	127360	108672	2.92%	0.276%
44	12.098	1699	1702	1705	rBV2	68635	68710	1.85%	0.175%
45	12.357	1744	1746	1749	rBV	91395	101725	2.74%	0.259%
46	12.463	1761	1764	1766	rVB	100305	87333	2.35%	0.222%
47	12.522	1771	1774	1777	rBV	824657	662097	17.82%	1.684%
48	12.569	1779	1782	1784	rBV	70254	62379	1.68%	0.159%
49	12.616	1788	1790	1793	rBV	76378	70096	1.89%	0.178%
50	12.751	1808	1813	1816	rBV	784839	766214	20.62%	1.949%
51	12.898	1835	1838	1842	rBV	3892789	3715765	100.00%	9.453%
52	13.039	1860	1862	1864	rBV2	64921	58525	1.58%	0.149%
53	13.086	1868	1870	1873	rVB	226216	190033	5.11%	0.483%
54	13.151	1878	1881	1884	rVB	184192	173765	4.68%	0.442%
55	13.192	1885	1888	1891	rBV2	122134	118259	3.18%	0.301%
56	13.286	1902	1904	1907	rVB	94232	72289	1.95%	0.184%
57	13.316	1907	1909	1913	rBV	102526	108375	2.92%	0.276%
58	13.816	1991	1994	2002	rBV3	480524	614606	16.54%	1.564%
59	13.969	2015	2020	2023	rBV2	2304357	2743434	73.83%	6.979%
60	13.992	2023	2024	2028	rVB	382450	313580	8.44%	0.798%
61	14.463	2101	2104	2107	rBV2	198727	181210	4.88%	0.461%
62	14.845	2166	2169	2175	rVB2	143765	177515	4.78%	0.452%
63	15.022	2195	2199	2208	rBV	435261	774821	20.85%	1.971%
64	15.110	2211	2214	2216	rBV2	170524	184311	4.96%	0.469%
65	15.322	2247	2250	2256	rVB	308711	407192	10.96%	1.036%
66	15.386	2257	2261	2267	rBV	428540	582953	15.69%	1.483%
67	15.451	2267	2272	2276	rBV	1662622	1983640	53.38%	5.046%
68	15.933	2351	2354	2358	rBV	110594	137675	3.71%	0.350%
69	16.916	2517	2521	2528	rVB2	152800	255415	6.87%	0.650%
70	17.357	2592	2596	2607	rVB	156417	291731	7.85%	0.742%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000706.D
Acq On : 14 Oct 2019 13:28
Operator : JU
Sample : K5348-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190826-COMPOSITE-BRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 39307432

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000706.D
Acq On : 14 Oct 2019 13:28
Operator : JU
Sample : K5348-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190826-COMPOSITE-BRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

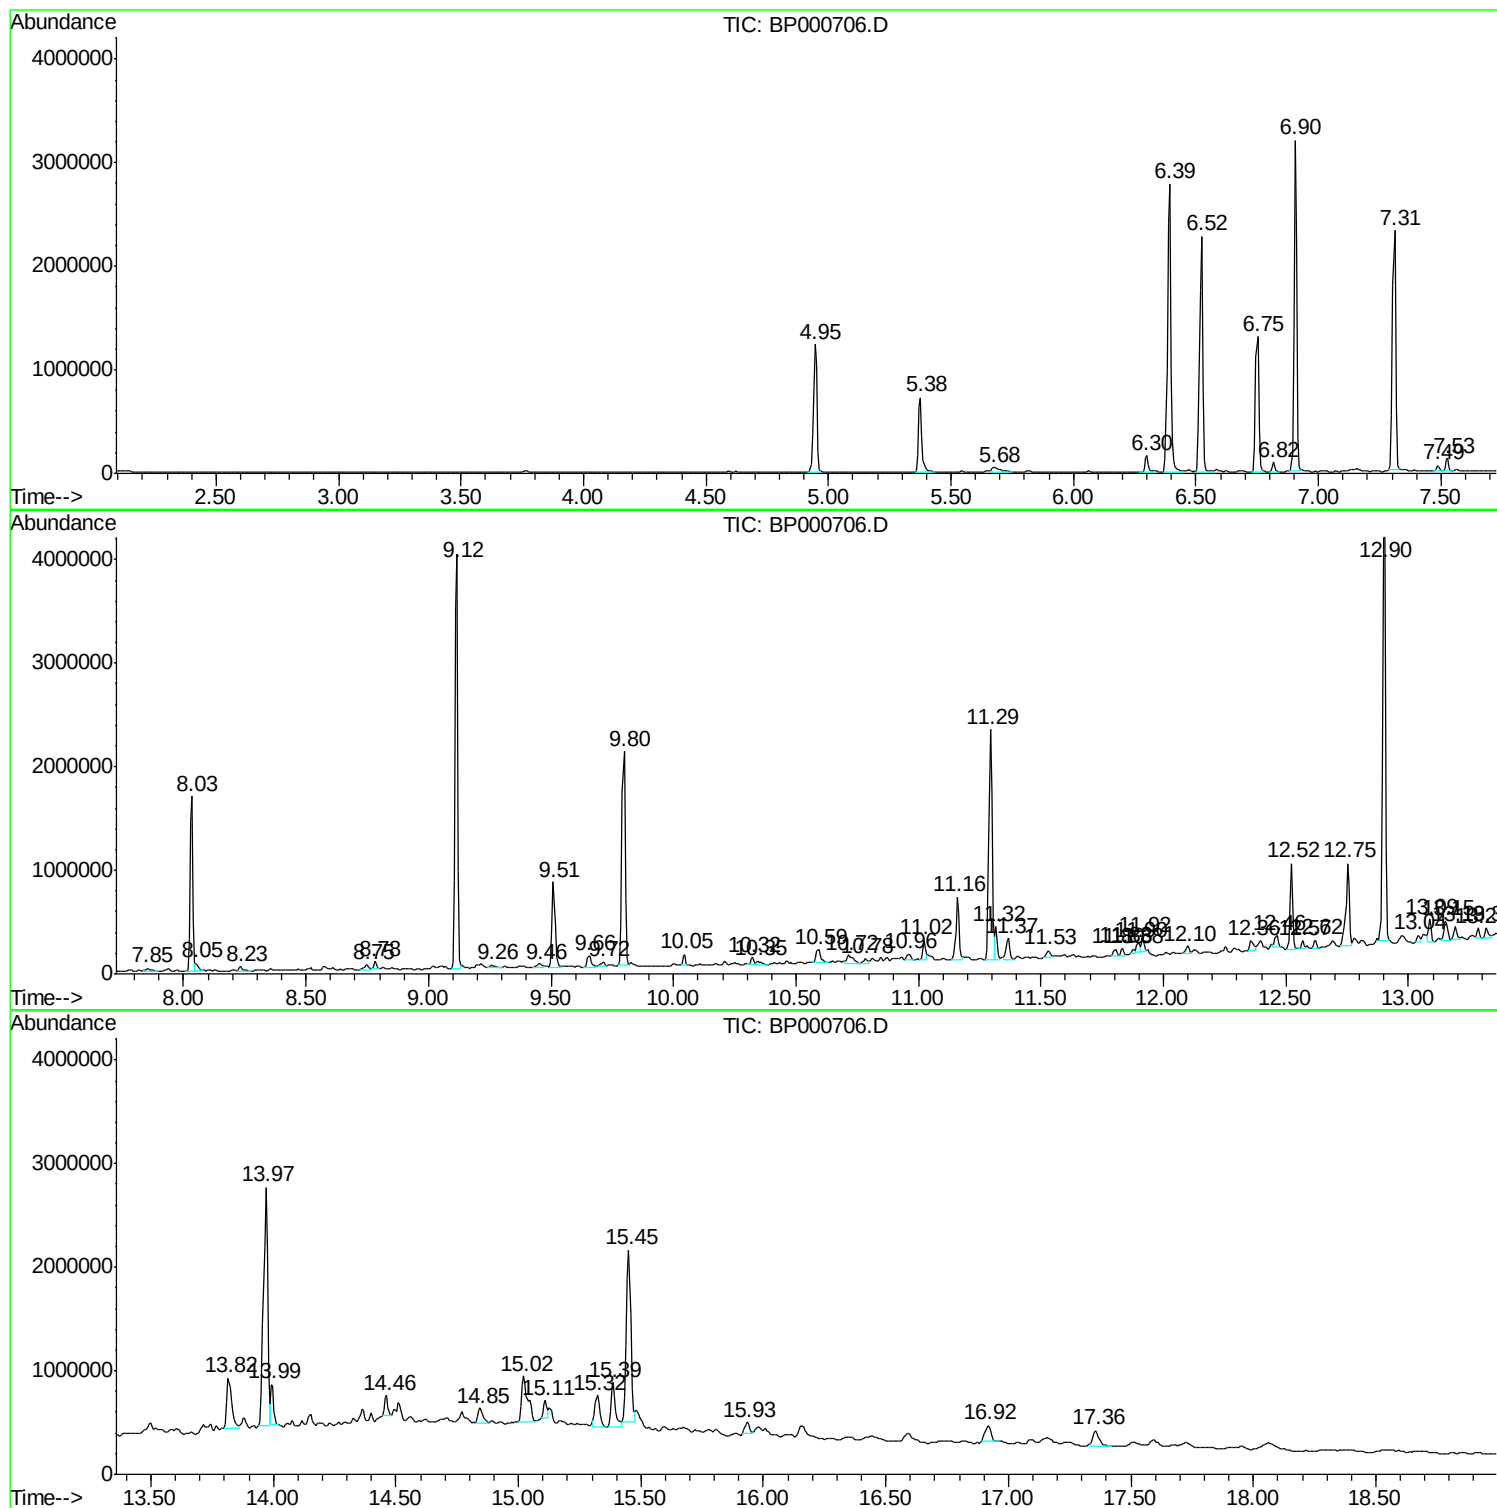

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000706.D
Acq_On : 14 Oct 2019 13:288
Operator : JUJ
Sample : K5348-02REE
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190826-COMPOSITE-BRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
