

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000708.D
 Acq On : 14 Oct 2019 14:17
 Operator : JU
 Sample : K5348-04RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190828-COMPOSITE-DRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	481	486	499	rBV	1065383	1114249	25.87%	2.583%
2	5.375	555	559	571	rBV	1228092	1156494	26.85%	2.681%
3	5.699	610	614	627	rVB2	41232	86178	2.00%	0.200%
4	6.299	710	716	720	rBV	147899	153487	3.56%	0.356%
5	6.393	727	732	743	rBV	3340912	3178307	73.80%	7.368%
6	6.522	750	754	757	rBV	2775216	2359318	54.78%	5.470%
7	6.752	789	793	801	rBV	1261267	1117388	25.94%	2.591%
8	6.816	801	804	808	rBV	79307	62189	1.44%	0.144%
9	6.904	815	819	823	rBV	3557457	3007866	69.84%	6.973%
10	7.310	884	888	891	rBV	2664140	2133421	49.54%	4.946%
11	7.528	921	925	928	rBV	148517	137942	3.20%	0.320%
12	7.851	977	980	987	rVB2	37759	51464	1.19%	0.119%
13	8.034	1007	1011	1013	rBV	1670463	1377015	31.97%	3.192%
14	8.781	1135	1138	1141	rBV3	75989	62573	1.45%	0.145%
15	9.116	1191	1195	1198	rBV	5177122	4096123	95.11%	9.496%
16	9.210	1205	1211	1216	rBV5	42227	100164	2.33%	0.232%
17	9.257	1216	1219	1226	rVB2	38261	58653	1.36%	0.136%
18	9.451	1247	1252	1255	rBV2	41044	75986	1.76%	0.176%
19	9.510	1259	1262	1267	rBV	785909	611707	14.20%	1.418%
20	9.657	1284	1287	1291	rBV	144401	137007	3.18%	0.318%
21	9.798	1307	1311	1314	rVB	2031975	1656101	38.45%	3.839%
22	10.046	1350	1353	1355	rVB	106576	89028	2.07%	0.206%
23	10.322	1397	1400	1402	rVB	68676	53072	1.23%	0.123%
24	10.593	1442	1446	1453	rBV	495171	500854	11.63%	1.161%
25	10.716	1464	1467	1475	rVB4	90161	161724	3.76%	0.375%
26	10.781	1475	1478	1481	rBV	51067	56808	1.32%	0.132%
27	10.963	1506	1509	1513	rVB3	63220	67562	1.57%	0.157%
28	11.022	1517	1519	1521	rBV	186857	147516	3.43%	0.342%
29	11.157	1539	1542	1546	rBV	547938	522090	12.12%	1.210%
30	11.293	1562	1565	1568	rBV	1914437	1860747	43.20%	4.314%
31	11.316	1568	1569	1572	rVV	316932	221277	5.14%	0.513%
32	11.369	1574	1578	1581	rVB2	255344	287169	6.67%	0.666%
33	11.528	1603	1605	1608	rBV	72031	63819	1.48%	0.148%
34	11.804	1649	1652	1654	rBV	73792	67971	1.58%	0.158%

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000708.D
Acq On : 14 Oct 2019 14:17
Operator : JU
Sample : K5348-04RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190828-COMPOSITE-DRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.834	1654	1657	1660	rVV	70724	67387	1.56%	0.156%
36	11.898	1666	1668	1669	rBV	82083	55435	1.29%	0.129%
37	11.916	1669	1671	1674	rVB	130870	108155	2.51%	0.251%
38	12.098	1699	1702	1705	rBV3	73631	75667	1.76%	0.175%
39	12.363	1744	1747	1749	rBV	125101	128571	2.99%	0.298%
40	12.463	1761	1764	1767	rVB2	158838	130699	3.03%	0.303%
41	12.522	1771	1774	1778	rBV	809747	711102	16.51%	1.649%
42	12.569	1780	1782	1784	rBV	97379	74329	1.73%	0.172%
43	12.622	1788	1791	1793	rBV	96468	79434	1.84%	0.184%
44	12.757	1808	1814	1816	rBV	782123	843915	19.59%	1.957%
45	12.904	1835	1839	1842	rBV	5009227	4306824	100.00%	9.985%
46	13.087	1868	1870	1874	rVB	243537	222910	5.18%	0.517%
47	13.157	1879	1882	1885	rVB	191452	177522	4.12%	0.412%
48	13.192	1886	1888	1891	rBV	120248	115180	2.67%	0.267%
49	13.287	1902	1904	1907	rVB	117231	95781	2.22%	0.222%
50	13.316	1907	1909	1913	rBV	116905	129064	3.00%	0.299%
51	13.816	1991	1994	2002	rBV4	309917	433576	10.07%	1.005%
52	13.969	2015	2020	2023	rBV2	2178317	2774576	64.42%	6.432%
53	13.998	2023	2025	2028	rVB	456519	361900	8.40%	0.839%
54	14.463	2101	2104	2107	rBV2	231418	207393	4.82%	0.481%
55	14.845	2166	2169	2172	rBV2	140219	162515	3.77%	0.377%
56	15.022	2195	2199	2207	rBV	508941	922181	21.41%	2.138%
57	15.110	2211	2214	2216	rBV	173194	201828	4.69%	0.468%
58	15.322	2247	2250	2256	rVB	384770	503924	11.70%	1.168%
59	15.386	2257	2261	2267	rBV	523410	684926	15.90%	1.588%
60	15.451	2267	2272	2275	rBV	1583202	1909934	44.35%	4.428%
61	15.933	2351	2354	2358	rBV	122677	158994	3.69%	0.369%
62	16.916	2517	2521	2527	rVB2	184631	308677	7.17%	0.716%
63	17.357	2592	2596	2608	rVB	183702	348165	8.08%	0.807%


Sum of corrected areas: 43133833

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000708.D
Acq On : 14 Oct 2019 14:17
Operator : JU
Sample : K5348-04RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190828-COMPOSITE-DRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

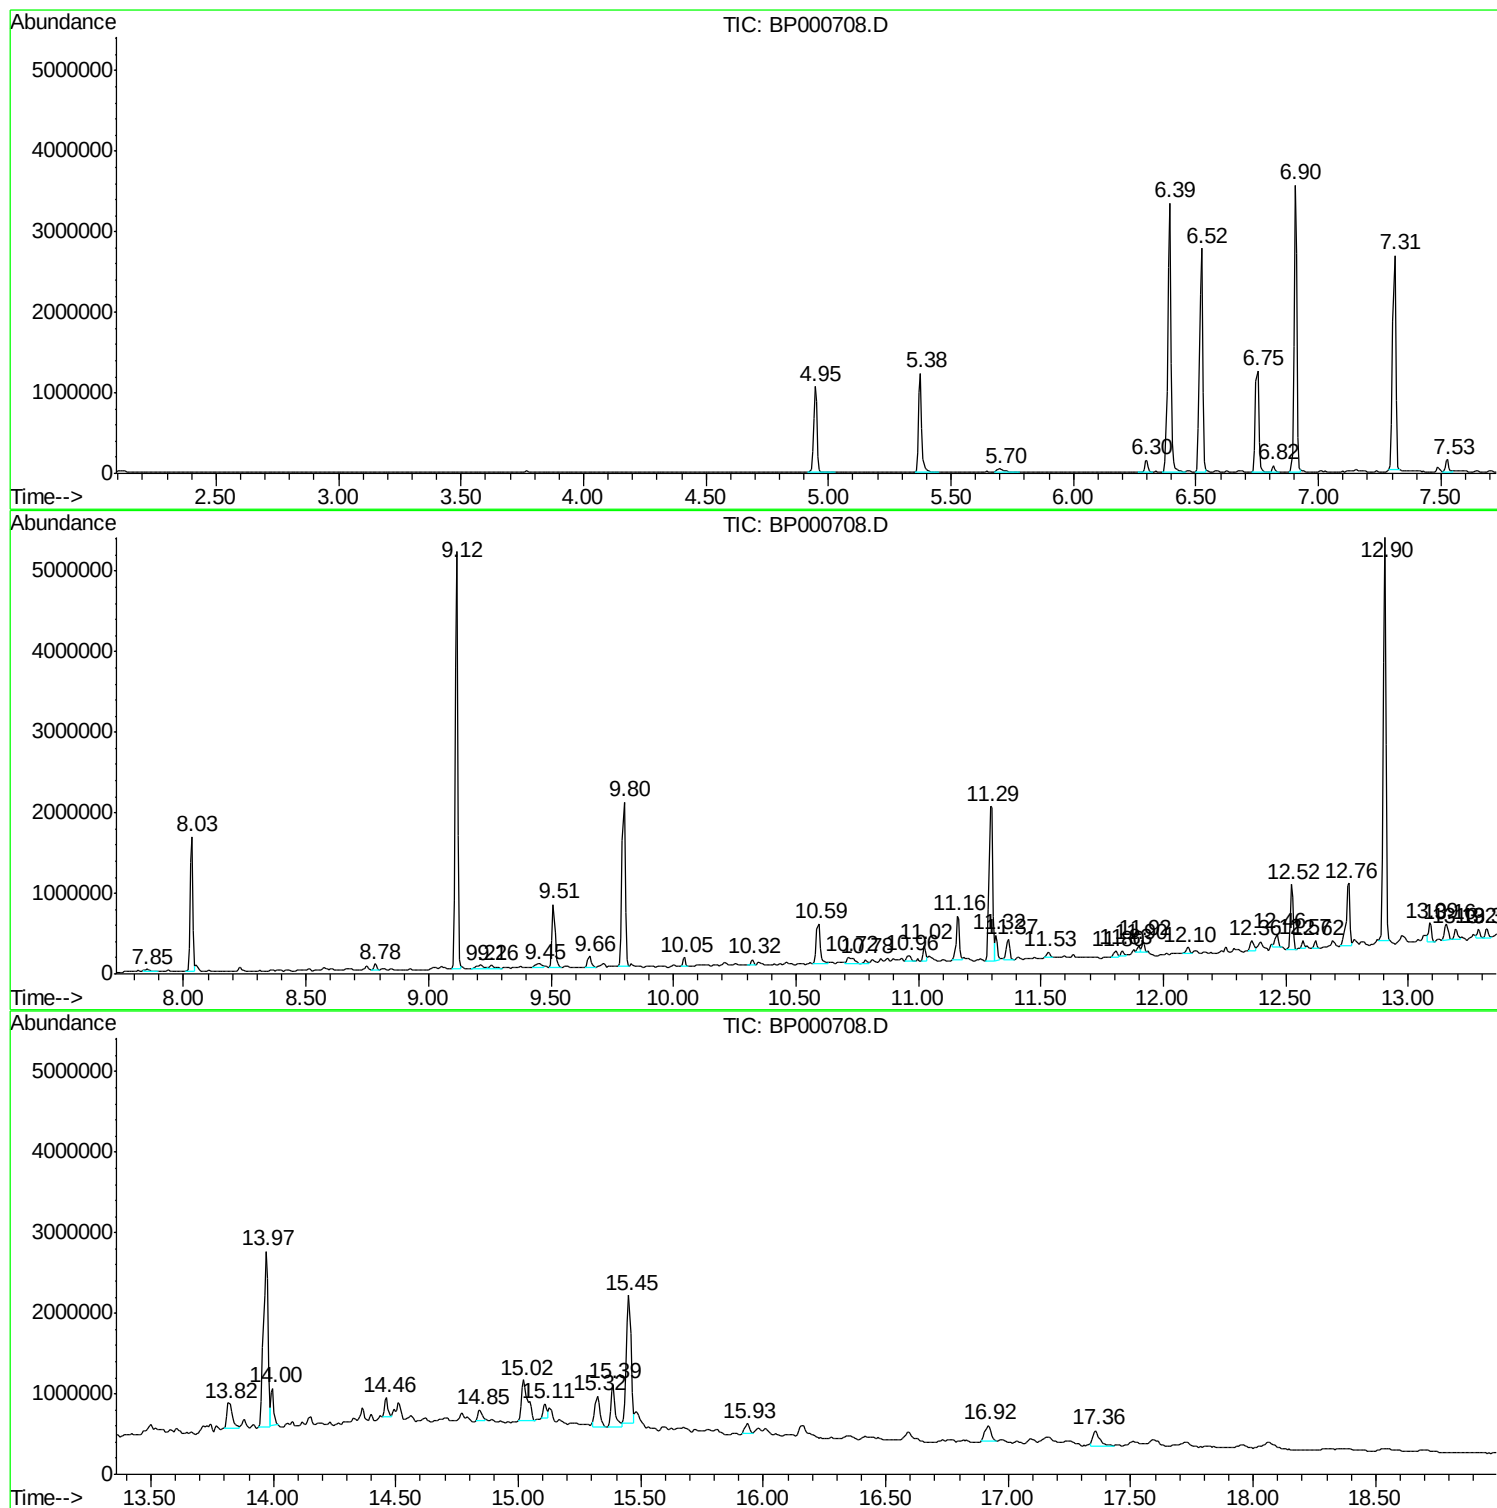

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000708.D
Acq_On : 14 Oct 2019 14:177
Operator : JUJ
Sample : K5348-04REE
Misc :
ALS_Vial : 7 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190828-COMPOSITE-DRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
