

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000710.D
 Acq On : 14 Oct 2019 15:05
 Operator : JU
 Sample : K5348-06RE
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190830-COMPOSITE-FRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	482	486	497	rVB	1017744	1056225	25.33%	2.713%
2	5.375	555	559	571	rBV	1097091	1030039	24.70%	2.646%
3	5.716	612	617	632	rVB2	22031	61983	1.49%	0.159%
4	6.299	712	716	720	rBV	178350	172075	4.13%	0.442%
5	6.393	728	732	743	rBV	3269784	3113630	74.67%	7.998%
6	6.522	750	754	757	rBV	2552037	2066375	49.56%	5.308%
7	6.752	789	793	796	rBV	1373458	1139842	27.34%	2.928%
8	6.816	801	804	808	rBV	100203	78232	1.88%	0.201%
9	6.905	815	819	823	rBV	3549685	3050058	73.15%	7.835%
10	7.311	884	888	891	rBV	2727481	2216649	53.16%	5.694%
11	7.528	921	925	928	rVB	149767	128350	3.08%	0.330%
12	8.034	1007	1011	1014	rBV	1783460	1443608	34.62%	3.708%
13	9.116	1191	1195	1198	rBV	4876154	3869597	92.80%	9.940%
14	9.205	1206	1210	1217	rBV5	39529	90663	2.17%	0.233%
15	9.510	1259	1262	1267	rBV	809152	649987	15.59%	1.670%
16	9.657	1284	1287	1292	rBV	132377	140964	3.38%	0.362%
17	9.799	1307	1311	1314	rVB	2147390	1710373	41.02%	4.393%
18	10.046	1350	1353	1355	rVB2	79924	65590	1.57%	0.168%
19	10.346	1402	1404	1411	rVB3	40252	58478	1.40%	0.150%
20	10.593	1442	1446	1453	rBV	504027	507717	12.18%	1.304%
21	10.716	1465	1467	1475	rVB4	94965	158632	3.80%	0.407%
22	10.781	1475	1478	1481	rBV	62441	66135	1.59%	0.170%
23	10.957	1506	1508	1512	rVB3	68584	70796	1.70%	0.182%
24	11.022	1517	1519	1521	rBV	123108	100921	2.42%	0.259%
25	11.157	1539	1542	1546	rBV	417749	378777	9.08%	0.973%
26	11.293	1562	1565	1568	rBV	1935588	1892222	45.38%	4.861%
27	11.316	1568	1569	1572	rVV	295130	215447	5.17%	0.553%
28	11.369	1574	1578	1581	rVB3	234469	257653	6.18%	0.662%
29	11.528	1603	1605	1608	rBV	95373	87459	2.10%	0.225%
30	11.834	1654	1657	1661	rBV2	90023	101638	2.44%	0.261%
31	11.916	1669	1671	1674	rVB	111936	91284	2.19%	0.234%
32	12.363	1744	1747	1749	rBV	109212	117523	2.82%	0.302%
33	12.446	1758	1761	1762	rBV	86393	102109	2.45%	0.262%
34	12.522	1771	1774	1777	rBV	845381	718858	17.24%	1.847%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000710.D
Acq On : 14 Oct 2019 15:05
Operator : JU
Sample : K5348-06RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190830-COMPOSITE-FRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.622	1789	1791	1794	rBV	97525	86800	2.08%	0.223%
36	12.751	1809	1813	1816	rBV	735707	758296	18.19%	1.948%
37	12.904	1835	1839	1842	rBV	4856368	4169722	100.00%	10.711%
38	13.087	1868	1870	1873	rVB	248951	237491	5.70%	0.610%
39	13.822	1992	1995	2003	rBV2	456881	590786	14.17%	1.518%
40	13.969	2016	2020	2023	rBV2	1976983	2539871	60.91%	6.524%
41	13.998	2023	2025	2028	rVB	406578	317936	7.62%	0.817%
42	15.028	2197	2200	2207	rVB	519030	1003599	24.07%	2.578%
43	15.392	2259	2262	2268	rVB	406143	540898	12.97%	1.389%
44	15.457	2269	2273	2276	rBV	1433358	1674666	40.16%	4.302%


Sum of corrected areas: 38929954

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000710.D
Acq On : 14 Oct 2019 15:05
Operator : JU
Sample : K5348-06RE
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190830-COMPOSITE-FRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

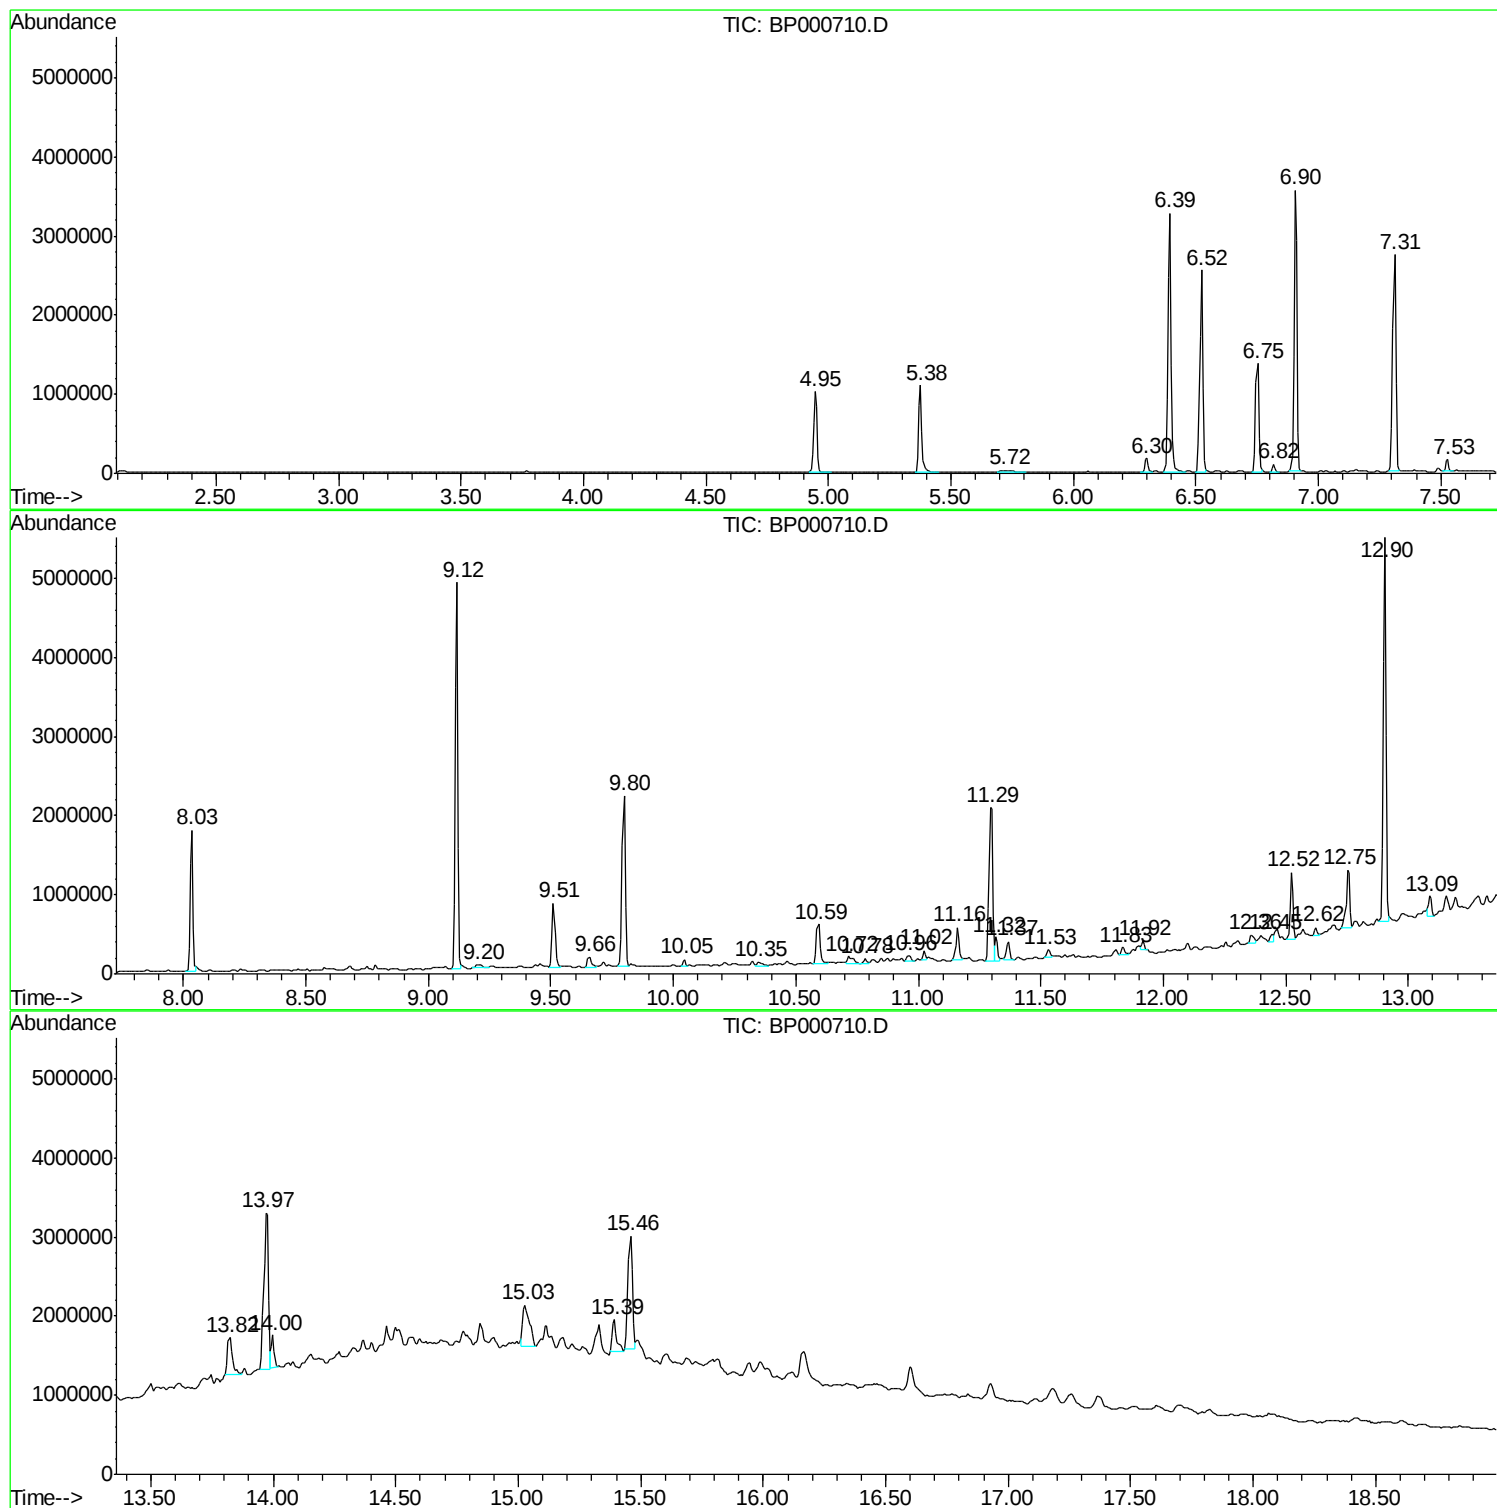

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000710.D
Acq_On : 14 Oct 2019 15:055
Operator : JUJ
Sample : K5348-06REE
Misc :
ALS_Vial : 9 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190830-COMPOSITE-FRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
