

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000712.D
 Acq On : 14 Oct 2019 15:53
 Operator : JU
 Sample : K5348-08RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190832-COMPOSITE-HRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.946	481	486	495	rBV	665643	694589	17.25%	1.776%
2	5.375	555	559	574	rVB	1208625	1182038	29.36%	3.022%
3	6.299	710	716	720	rBV	106807	101692	2.53%	0.260%
4	6.393	728	732	743	rBV	3357179	3175350	78.86%	8.118%
5	6.522	750	754	758	rBV	3145448	2531288	62.87%	6.471%
6	6.752	789	793	796	rBV	1387811	1096974	27.24%	2.804%
7	6.816	801	804	808	rBV	68030	53579	1.33%	0.137%
8	6.905	816	819	823	rBV	3290688	2830485	70.30%	7.236%
9	7.310	884	888	891	rBV	2652663	2065597	51.30%	5.281%
10	7.528	921	925	928	rBV	112628	95511	2.37%	0.244%
11	8.034	1007	1011	1014	rBV	1798276	1398807	34.74%	3.576%
12	9.116	1191	1195	1198	rBV	4862346	3805635	94.52%	9.729%
13	9.510	1259	1262	1268	rBV	791823	639379	15.88%	1.635%
14	9.657	1284	1287	1291	rBV	129442	122793	3.05%	0.314%
15	9.799	1307	1311	1315	rBV	2098910	1663674	41.32%	4.253%
16	10.593	1442	1446	1453	rBV	375338	372036	9.24%	0.951%
17	10.716	1465	1467	1469	rBV3	44836	52532	1.30%	0.134%
18	10.963	1506	1509	1512	rVB3	56165	61673	1.53%	0.158%
19	11.022	1517	1519	1521	rBV	84518	70695	1.76%	0.181%
20	11.157	1539	1542	1546	rBV3	78652	92300	2.29%	0.236%
21	11.299	1562	1566	1568	rBV	1960913	1816684	45.12%	4.644%
22	11.316	1568	1569	1572	rVV	287348	218985	5.44%	0.560%
23	11.369	1574	1578	1581	rVB	209601	219671	5.46%	0.562%
24	11.410	1582	1585	1588	rBV2	40281	54444	1.35%	0.139%
25	11.528	1603	1605	1608	rBV	72450	69622	1.73%	0.178%
26	11.804	1649	1652	1654	rBV	68703	64500	1.60%	0.165%
27	11.834	1654	1657	1661	rVV2	98284	113329	2.81%	0.290%
28	11.916	1669	1671	1674	rVB	115722	98909	2.46%	0.253%
29	12.363	1744	1747	1749	rBV	105795	103991	2.58%	0.266%
30	12.445	1758	1761	1762	rBV2	83012	82954	2.06%	0.212%
31	12.522	1771	1774	1778	rBV	981012	838078	20.81%	2.143%
32	12.569	1780	1782	1784	rBV2	79485	65642	1.63%	0.168%
33	12.622	1789	1791	1795	rVB	85769	78651	1.95%	0.201%
34	12.757	1809	1814	1817	rBV	1050407	1051440	26.11%	2.688%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000712.D
Acq On : 14 Oct 2019 15:53
Operator : JU
Sample : K5348-08RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190832-COMPOSITE-HRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.904	1835	1839	1842	rBV	4728465	4026359	100.00%	10.294%
36	13.093	1868	1871	1874	rVB	234433	220348	5.47%	0.563%
37	13.157	1879	1882	1885	rVB2	199101	212445	5.28%	0.543%
38	13.193	1886	1888	1894	rVV2	137433	181578	4.51%	0.464%
39	13.822	1992	1995	2002	rBV2	581537	762767	18.94%	1.950%
40	13.975	2016	2021	2023	rBV2	2049700	2631520	65.36%	6.728%
41	13.998	2023	2025	2028	rVB	585647	439395	10.91%	1.123%
42	14.463	2102	2104	2107	rBV	266687	204399	5.08%	0.523%
43	15.028	2197	2200	2203	rBV	668075	902396	22.41%	2.307%
44	15.392	2259	2262	2268	rBV	611702	835976	20.76%	2.137%
45	15.457	2269	2273	2277	rBV	1374362	1714786	42.59%	4.384%


Sum of corrected areas: 39115496

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000712.D
Acq On : 14 Oct 2019 15:53
Operator : JU
Sample : K5348-08RE
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190832-COMPOSITE-HRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

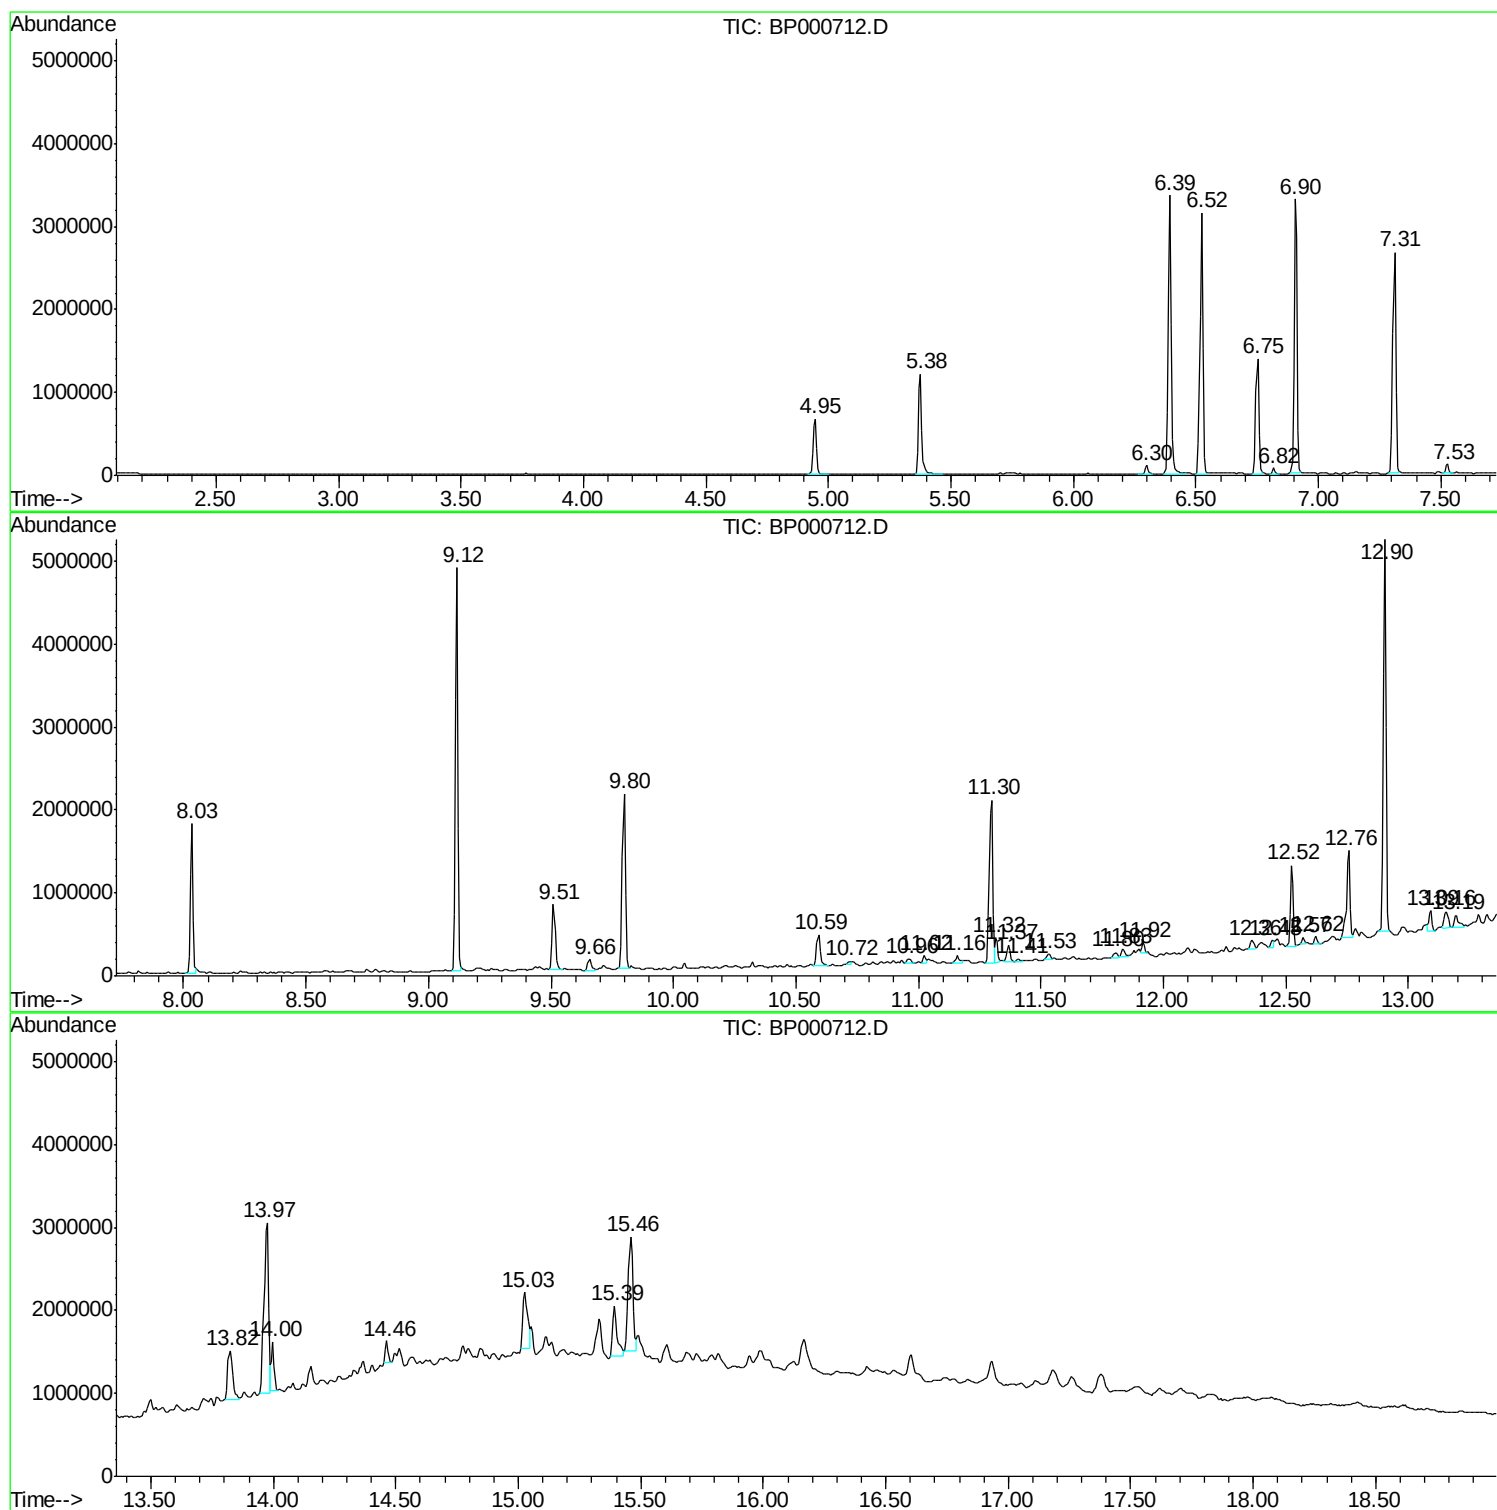

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000712.D
Acq_On : 14 Oct 2019 15:533
Operator : JUJ
Sample : K5348-08REE
Misc :
ALS_Vial : 11 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190832-COMPOSITE-HRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
