

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000713.D
 Acq On : 14 Oct 2019 16:18
 Operator : JU
 Sample : K5348-09RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190833-COMPOSITE-IRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.957	482	488	491	rBV	1726993	1961440	45.95%	4.706%
2	5.375	556	559	577	rVB	615209	600069	14.06%	1.440%
3	5.699	611	614	623	rBV	33987	53659	1.26%	0.129%
4	6.299	712	716	720	rBV	273837	242411	5.68%	0.582%
5	6.393	728	732	742	rBV	3148926	3105207	72.74%	7.449%
6	6.522	750	754	762	rVB	2222595	1784925	41.81%	4.282%
7	6.752	789	793	796	rBV	1403436	1102257	25.82%	2.644%
8	6.816	801	804	808	rBV	124947	95215	2.23%	0.228%
9	6.910	816	820	823	rBV	3401661	3075863	72.05%	7.379%
10	7.310	884	888	891	rBV	2705142	2192883	51.37%	5.261%
11	7.528	921	925	928	rBV	197591	158924	3.72%	0.381%
12	8.034	1007	1011	1014	rBV	1751225	1392075	32.61%	3.340%
13	8.681	1116	1121	1127	rBV2	70283	80400	1.88%	0.193%
14	8.787	1136	1139	1142	rBV2	57971	54476	1.28%	0.131%
15	9.116	1191	1195	1198	rBV	5383297	4214948	98.73%	10.112%
16	9.216	1206	1212	1217	rBV6	54032	114160	2.67%	0.274%
17	9.510	1259	1262	1268	rBV	814676	732670	17.16%	1.758%
18	9.657	1284	1287	1292	rBV	181328	171546	4.02%	0.412%
19	9.798	1308	1311	1315	rVB	2144492	1648252	38.61%	3.954%
20	10.045	1350	1353	1355	rBV	109136	77182	1.81%	0.185%
21	10.351	1402	1405	1411	rVB3	46116	63086	1.48%	0.151%
22	10.592	1443	1446	1449	rBV2	72683	75698	1.77%	0.182%
23	10.716	1465	1467	1469	rBV2	80818	83900	1.97%	0.201%
24	10.781	1476	1478	1482	rBV	56236	71231	1.67%	0.171%
25	10.851	1487	1490	1492	rBV	55215	52862	1.24%	0.127%
26	10.963	1506	1509	1512	rVB3	76484	79825	1.87%	0.192%
27	11.022	1517	1519	1522	rBV	142774	147173	3.45%	0.353%
28	11.163	1539	1543	1547	rBV	543665	495990	11.62%	1.190%
29	11.298	1562	1566	1568	rBV	2187066	1806944	42.33%	4.335%
30	11.322	1568	1570	1572	rVV	352739	286311	6.71%	0.687%
31	11.369	1574	1578	1582	rVB2	278753	322633	7.56%	0.774%
32	11.534	1603	1606	1609	rBV	74134	70444	1.65%	0.169%
33	11.804	1650	1652	1655	rVB	67209	59081	1.38%	0.142%
34	11.834	1655	1657	1662	rBV	86823	90972	2.13%	0.218%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000713.D
Acq On : 14 Oct 2019 16:18
Operator : JU
Sample : K5348-09RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190833-COMPOSITE-IRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.881	1663	1665	1667	rBV	62975	60346	1.41%	0.145%
36	11.922	1669	1672	1674	rVB	128819	132223	3.10%	0.317%
37	12.257	1727	1729	1732	rVB	75976	53233	1.25%	0.128%
38	12.363	1744	1747	1750	rBV	149518	169444	3.97%	0.406%
39	12.463	1762	1764	1767	rVB	177894	140097	3.28%	0.336%
40	12.528	1771	1775	1778	rBV	920378	798787	18.71%	1.916%
41	12.569	1780	1782	1784	rBV2	87958	78581	1.84%	0.189%
42	12.622	1789	1791	1794	rBV	111429	90206	2.11%	0.216%
43	12.757	1809	1814	1817	rBV	1011326	950532	22.27%	2.280%
44	12.904	1836	1839	1843	rBV	4618829	4269092	100.00%	10.242%
45	13.092	1869	1871	1874	rVB	298728	225227	5.28%	0.540%
46	13.157	1880	1882	1885	rVB	240037	205490	4.81%	0.493%
47	13.198	1887	1889	1891	rVB2	141370	109872	2.57%	0.264%
48	13.822	1992	1995	2002	rBV	605010	720091	16.87%	1.728%
49	13.975	2016	2021	2024	rBV2	2180877	2827088	66.22%	6.782%
50	13.998	2024	2025	2028	rVB	566924	387844	9.08%	0.930%
51	14.463	2102	2104	2107	rVB2	277476	229976	5.39%	0.552%
52	15.028	2197	2200	2203	rBV	575992	795461	18.63%	1.908%
53	15.328	2249	2251	2257	rVB	411790	502309	11.77%	1.205%
54	15.392	2259	2262	2268	rBV	513757	593071	13.89%	1.423%
55	15.457	2269	2273	2277	rBV2	1453798	1780083	41.70%	4.270%


Sum of corrected areas: 41683765

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000713.D
Acq On : 14 Oct 2019 16:18
Operator : JU
Sample : K5348-09RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190833-COMPOSITE-IRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

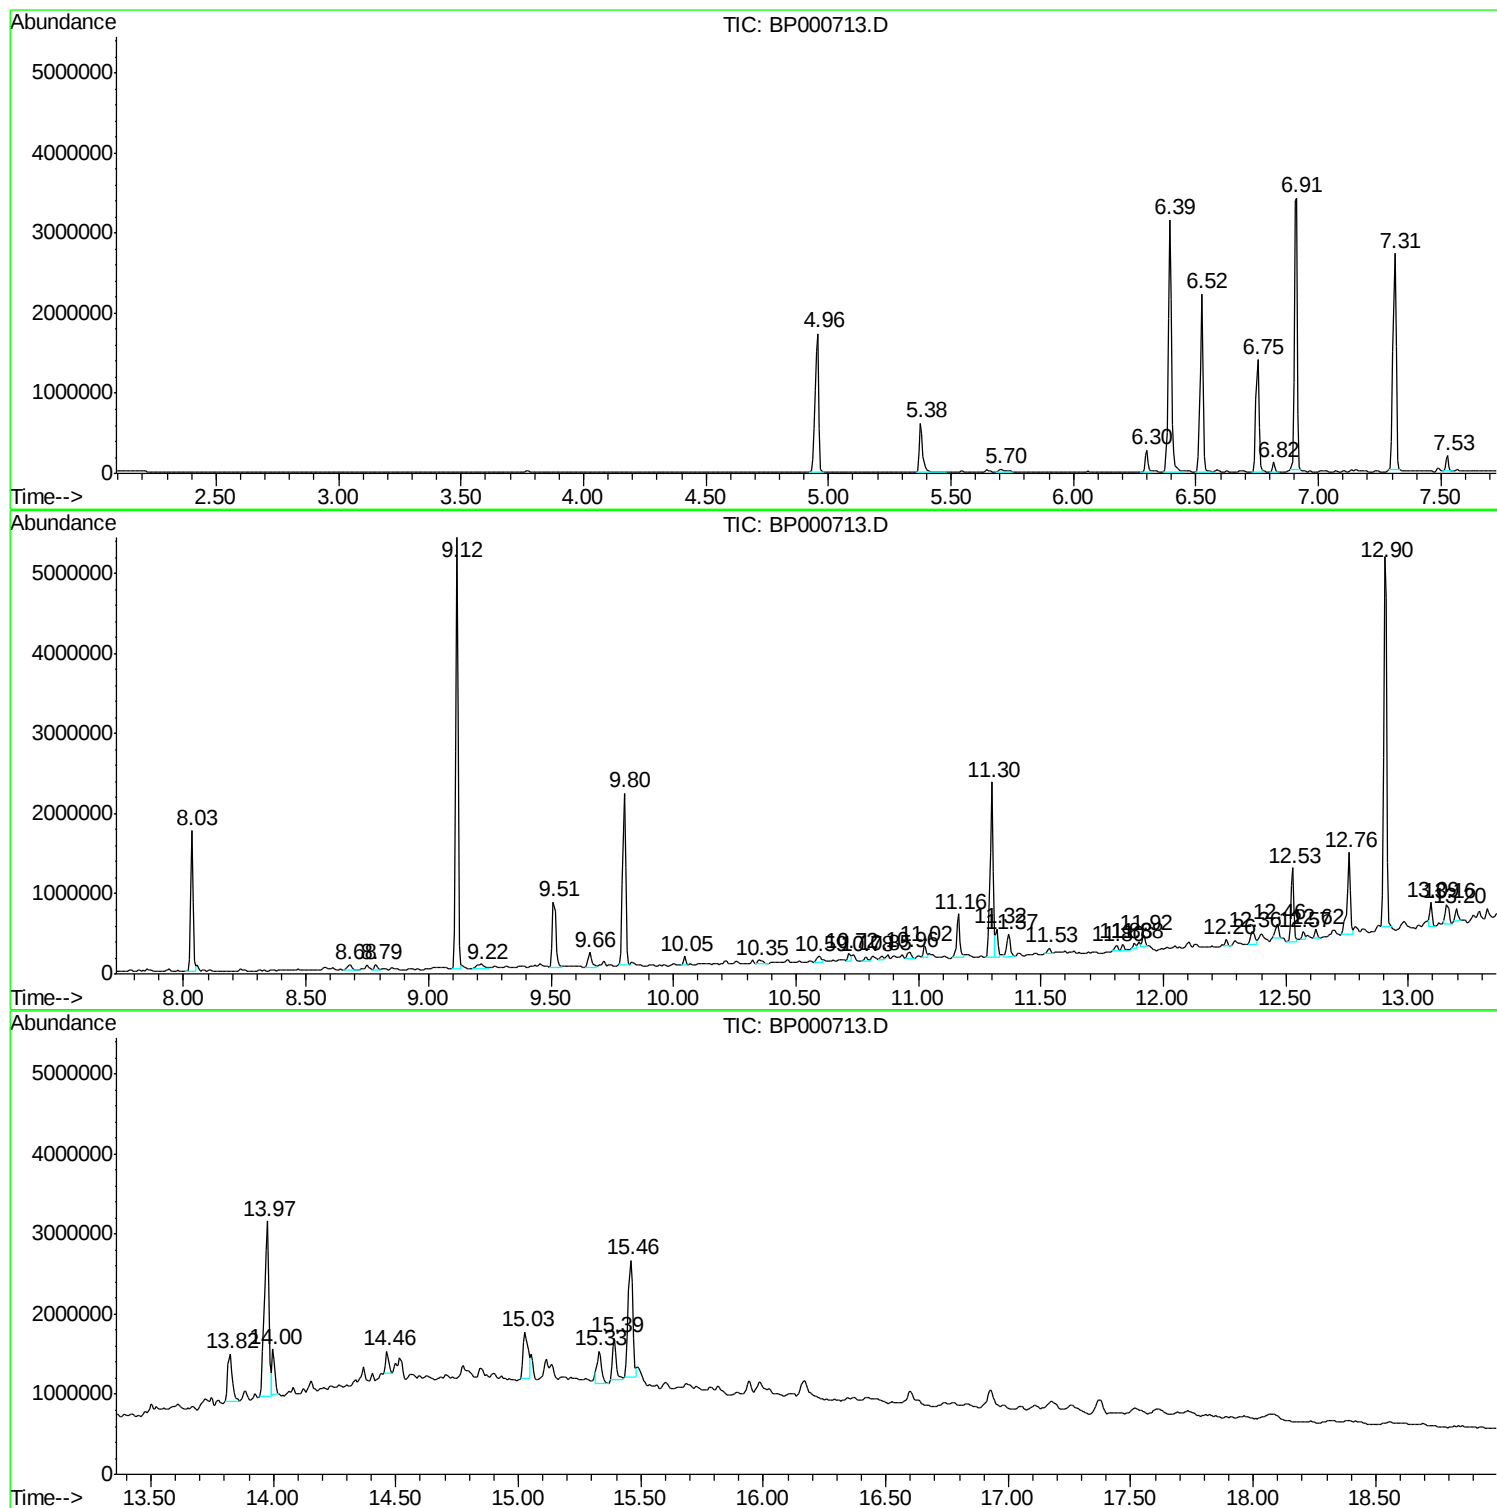

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000713.D
Acq_On : 14 Oct 2019 16:188
Operator : JUJ
Sample : K5348-09REE
Misc :
ALS_Vial : 12 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190833-COMPOSITE-IRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
