

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000714.D
 Acq On : 14 Oct 2019 16:42
 Operator : JU
 Sample : K5348-10RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190834-COMPOSITE-JRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.952	481	487	490	rBV	1133896	1227061	29.58%	2.835%
2	5.375	556	559	572	rVB	597929	579667	13.98%	1.339%
3	5.699	611	614	632	rVB	45476	96231	2.32%	0.222%
4	6.299	712	716	720	rBV	303407	267060	6.44%	0.617%
5	6.393	728	732	743	rBV2	3150595	3343816	80.62%	7.726%
6	6.522	750	754	762	rVB	2517481	2032339	49.00%	4.696%
7	6.752	789	793	796	rBV	1413049	1120697	27.02%	2.589%
8	6.816	801	804	808	rBV	92122	71451	1.72%	0.165%
9	6.911	812	820	823	rBV	3381326	3111981	75.03%	7.190%
10	7.311	884	888	891	rBV	2673822	2173539	52.40%	5.022%
11	7.528	921	925	928	rBV	173190	146682	3.54%	0.339%
12	8.034	1007	1011	1014	rBV	1847286	1421084	34.26%	3.283%
13	8.675	1116	1120	1126	rBV	106271	117101	2.82%	0.271%
14	8.752	1130	1133	1136	rVV	65910	57191	1.38%	0.132%
15	8.781	1136	1138	1142	rVV2	60600	57870	1.40%	0.134%
16	9.116	1191	1195	1198	rBV	4986861	3890020	93.79%	8.988%
17	9.216	1206	1212	1217	rBV6	58594	118659	2.86%	0.274%
18	9.510	1259	1262	1268	rBV	834823	715319	17.25%	1.653%
19	9.658	1284	1287	1292	rBV	203210	187295	4.52%	0.433%
20	9.799	1307	1311	1314	rBV	2211362	1681496	40.54%	3.885%
21	10.046	1350	1353	1355	rVB	113928	83313	2.01%	0.192%
22	10.352	1402	1405	1411	rVB3	44649	66124	1.59%	0.153%
23	10.593	1443	1446	1449	rBV2	76746	76924	1.85%	0.178%
24	10.716	1465	1467	1475	rVB4	95453	171338	4.13%	0.396%
25	10.781	1476	1478	1482	rBV	56889	71403	1.72%	0.165%
26	10.963	1506	1509	1512	rVB4	76529	77649	1.87%	0.179%
27	11.022	1517	1519	1522	rBV2	165384	169159	4.08%	0.391%
28	11.163	1539	1543	1546	rBV	474325	456251	11.00%	1.054%
29	11.299	1562	1566	1568	rBV	2228045	1842404	44.42%	4.257%
30	11.322	1568	1570	1573	rVV	390956	329097	7.93%	0.760%
31	11.369	1574	1578	1582	rVB2	272560	318614	7.68%	0.736%
32	11.410	1582	1585	1588	rBV2	49330	55751	1.34%	0.129%
33	11.534	1603	1606	1608	rBV	75076	69227	1.67%	0.160%
34	11.804	1650	1652	1655	rBV	82208	70789	1.71%	0.164%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000714.D
Acq On : 14 Oct 2019 16:42
Operator : JU
Sample : K5348-10RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190834-COMPOSITE-JRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 3 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.834	1655	1657	1660	rBV	100351	80002	1.93%	0.185%
36	11.881	1663	1665	1667	rBV	70338	59200	1.43%	0.137%
37	11.922	1669	1672	1674	rVB	157303	151778	3.66%	0.351%
38	12.257	1727	1729	1732	rVB	85021	63207	1.52%	0.146%
39	12.363	1744	1747	1750	rBV	152758	162987	3.93%	0.377%
40	12.463	1762	1764	1767	rVB	171176	127310	3.07%	0.294%
41	12.528	1771	1775	1778	rBV	1185491	1018744	24.56%	2.354%
42	12.569	1780	1782	1785	rBV2	109357	108967	2.63%	0.252%
43	12.622	1789	1791	1794	rBV	148592	120570	2.91%	0.279%
44	12.757	1808	1814	1817	rBV	1169323	1199831	28.93%	2.772%
45	12.904	1836	1839	1843	rVB	4678784	4147618	100.00%	9.583%
46	13.093	1868	1871	1874	rVB	327896	303150	7.31%	0.700%
47	13.157	1879	1882	1885	rVB2	307807	291507	7.03%	0.674%
48	13.199	1886	1889	1892	rBV2	173731	176358	4.25%	0.407%
49	13.322	1908	1910	1914	rBV	132788	132535	3.20%	0.306%
50	13.499	1938	1940	1943	rBV2	138015	115860	2.79%	0.268%
51	13.822	1992	1995	2003	rVB2	564536	676966	16.32%	1.564%
52	13.975	2016	2021	2024	rBV2	2267903	3044291	73.40%	7.034%
53	13.998	2024	2025	2028	rVB	583954	441299	10.64%	1.020%
54	14.151	2049	2051	2056	rBV2	183384	161443	3.89%	0.373%
55	14.463	2102	2104	2107	rVB2	361891	293411	7.07%	0.678%
56	15.028	2197	2200	2203	rBV	667116	891888	21.50%	2.061%
57	15.328	2248	2251	2258	rVB	467789	646837	15.60%	1.494%
58	15.393	2259	2262	2268	rBV	650540	785128	18.93%	1.814%
59	15.457	2269	2273	2277	rBV	1476034	1806696	43.56%	4.174%


Sum of corrected areas: 43282185

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000714.D
Acq On : 14 Oct 2019 16:42
Operator : JU
Sample : K5348-10RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190834-COMPOSITE-JRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

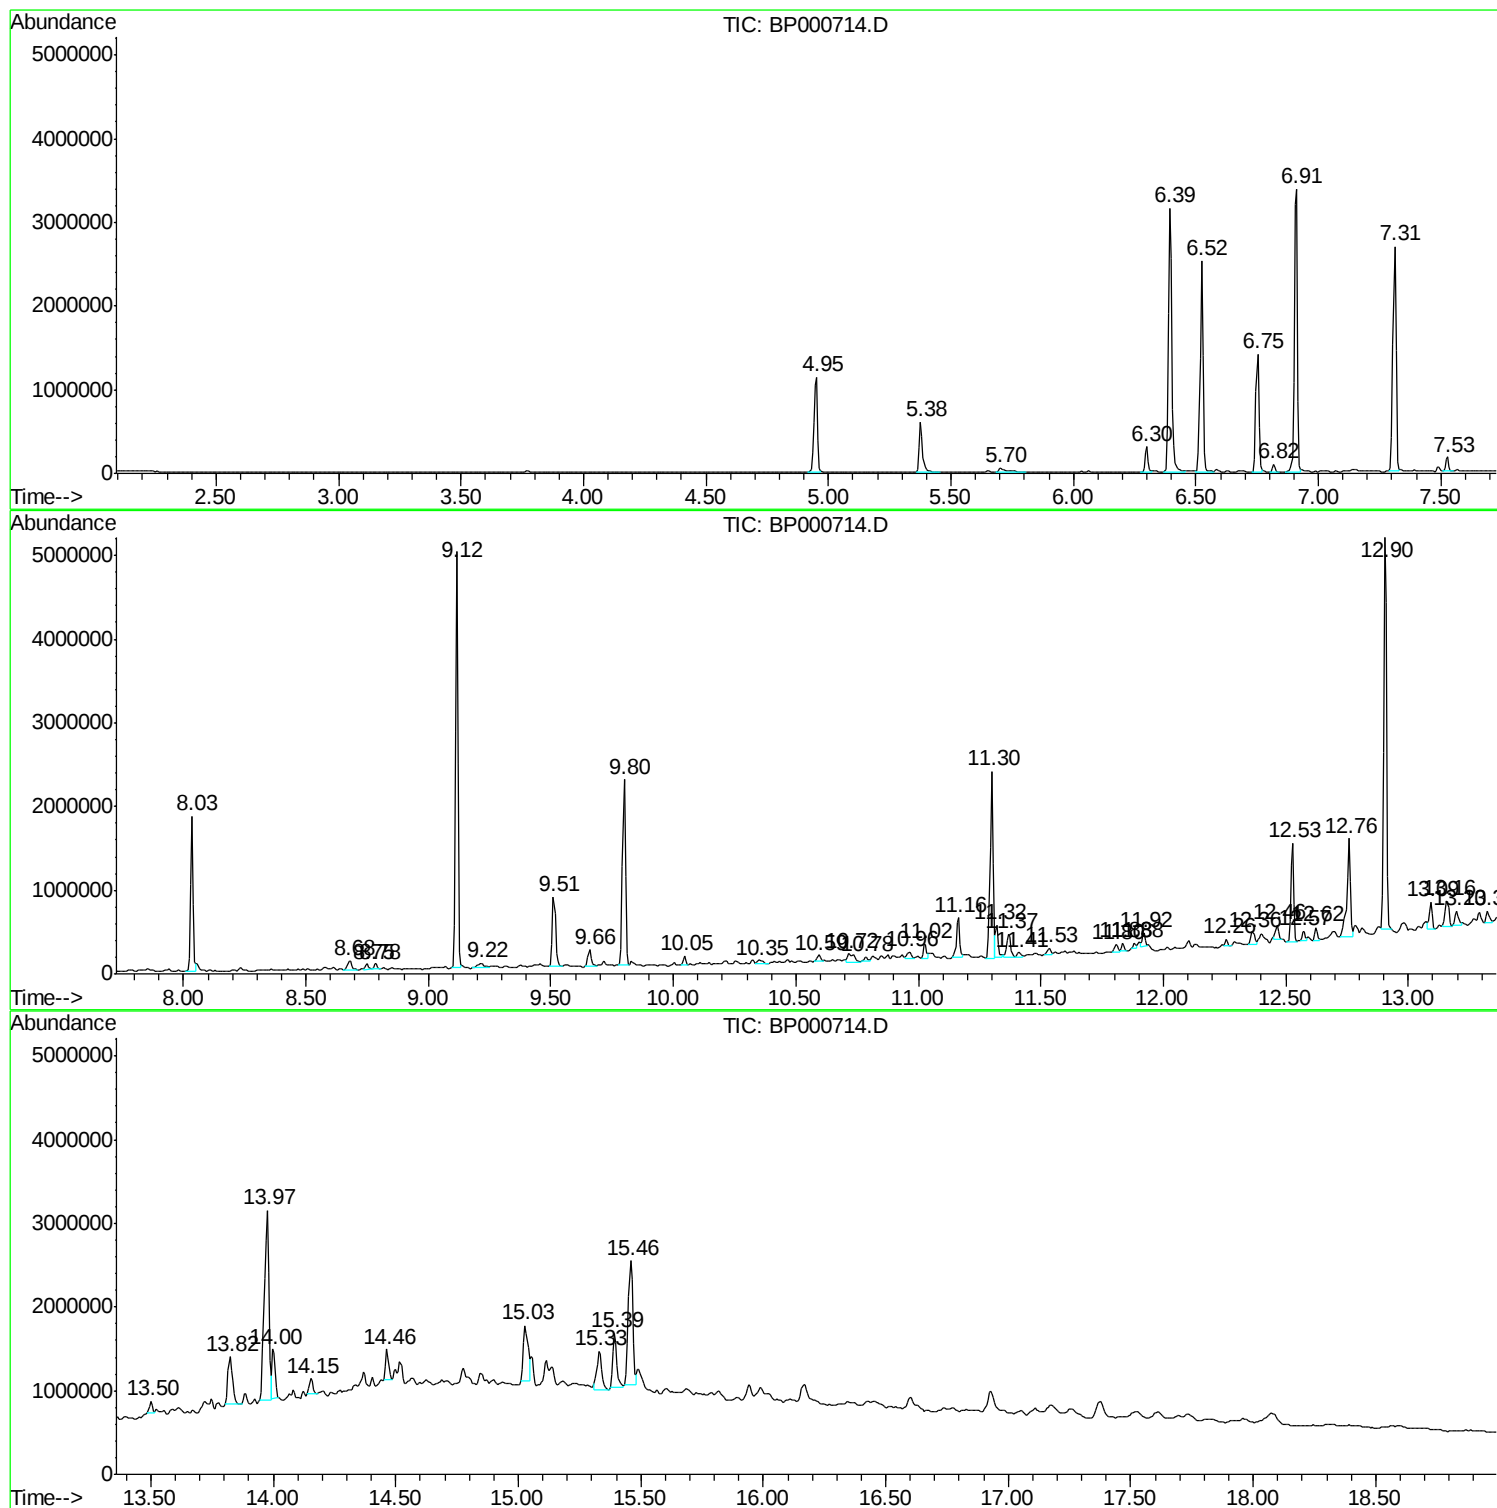

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000714.D
Acq_On : 14 Oct 2019 16:422
Operator : JUJ
Sample : K5348-10REE
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190834-COMPOSITE-JRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
