

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000715.D
 Acq On : 14 Oct 2019 17:06
 Operator : JU
 Sample : K5348-12RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190880-COMPOSITE-LRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.958	481	488	491	rBV	2023751	2443242	46.16%	6.381%
2	5.375	555	559	572	rVB	863148	807404	15.25%	2.109%
3	6.393	728	732	743	rBV	2692741	2566177	48.48%	6.702%
4	6.522	750	754	762	rBV	1847236	1487561	28.10%	3.885%
5	6.752	789	793	796	rBV	1430281	1106834	20.91%	2.891%
6	6.816	801	804	811	rVV	90031	69013	1.30%	0.180%
7	6.910	816	820	823	rBV	3591000	3215090	60.74%	8.396%
8	7.310	884	888	891	rBV	2792120	2289393	43.25%	5.979%
9	7.528	922	925	928	rVB	90739	75339	1.42%	0.197%
10	8.034	1007	1011	1014	rBV	1832195	1386434	26.19%	3.621%
11	9.116	1191	1195	1198	rBV	6106385	4844975	91.54%	12.653%
12	9.428	1242	1248	1256	rBV	94128	182409	3.45%	0.476%
13	9.510	1259	1262	1268	rBV	825004	687878	13.00%	1.796%
14	9.657	1284	1287	1292	rBV	64154	62641	1.18%	0.164%
15	9.799	1307	1311	1315	rBV	2198977	1694018	32.01%	4.424%
16	10.322	1397	1400	1402	rVB	86351	70409	1.33%	0.184%
17	10.593	1443	1446	1453	rBV	628130	539540	10.19%	1.409%
18	10.716	1464	1467	1476	rVB5	59540	93607	1.77%	0.244%
19	11.022	1517	1519	1522	rBV	78959	72226	1.36%	0.189%
20	11.157	1539	1542	1547	rBV	381492	369010	6.97%	0.964%
21	11.299	1562	1566	1569	rBV	2179982	1862598	35.19%	4.864%
22	11.369	1574	1578	1582	rVB3	186474	189252	3.58%	0.494%
23	11.534	1603	1606	1609	rBV2	53230	58347	1.10%	0.152%
24	12.528	1772	1775	1778	rBV	299693	250902	4.74%	0.655%
25	12.757	1811	1814	1817	rVB	306211	253295	4.79%	0.661%
26	12.904	1835	1839	1843	rBV	5682981	5292921	100.00%	13.823%
27	13.093	1869	1871	1874	rVB	93379	69611	1.32%	0.182%
28	13.157	1879	1882	1885	rVB2	80719	91535	1.73%	0.239%
29	13.816	1991	1994	2002	rBV	588525	776210	14.67%	2.027%
30	13.975	2016	2021	2024	rBV	2174055	2233327	42.19%	5.832%
31	13.998	2024	2025	2028	rVB	175375	95445	1.80%	0.249%
32	14.151	2049	2051	2056	rVB2	103150	81165	1.53%	0.212%
33	14.463	2101	2104	2107	rBV2	180036	172525	3.26%	0.451%
34	14.769	2154	2156	2164	rVB2	144239	206446	3.90%	0.539%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000715.D
Acq On : 14 Oct 2019 17:06
Operator : JU
Sample : K5348-12RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190880-COMPOSITE-LRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.028	2197	2200	2203	rBV	152990	213809	4.04%	0.558%
36	15.110	2212	2214	2223	rVB3	171880	274330	5.18%	0.716%
37	15.387	2259	2261	2266	rVB	154851	157814	2.98%	0.412%
38	15.451	2268	2272	2276	rBV	1510968	1948745	36.82%	5.089%


Sum of corrected areas: 38291477

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000715.D
Acq On : 14 Oct 2019 17:06
Operator : JU
Sample : K5348-12RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190880-COMPOSITE-LRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

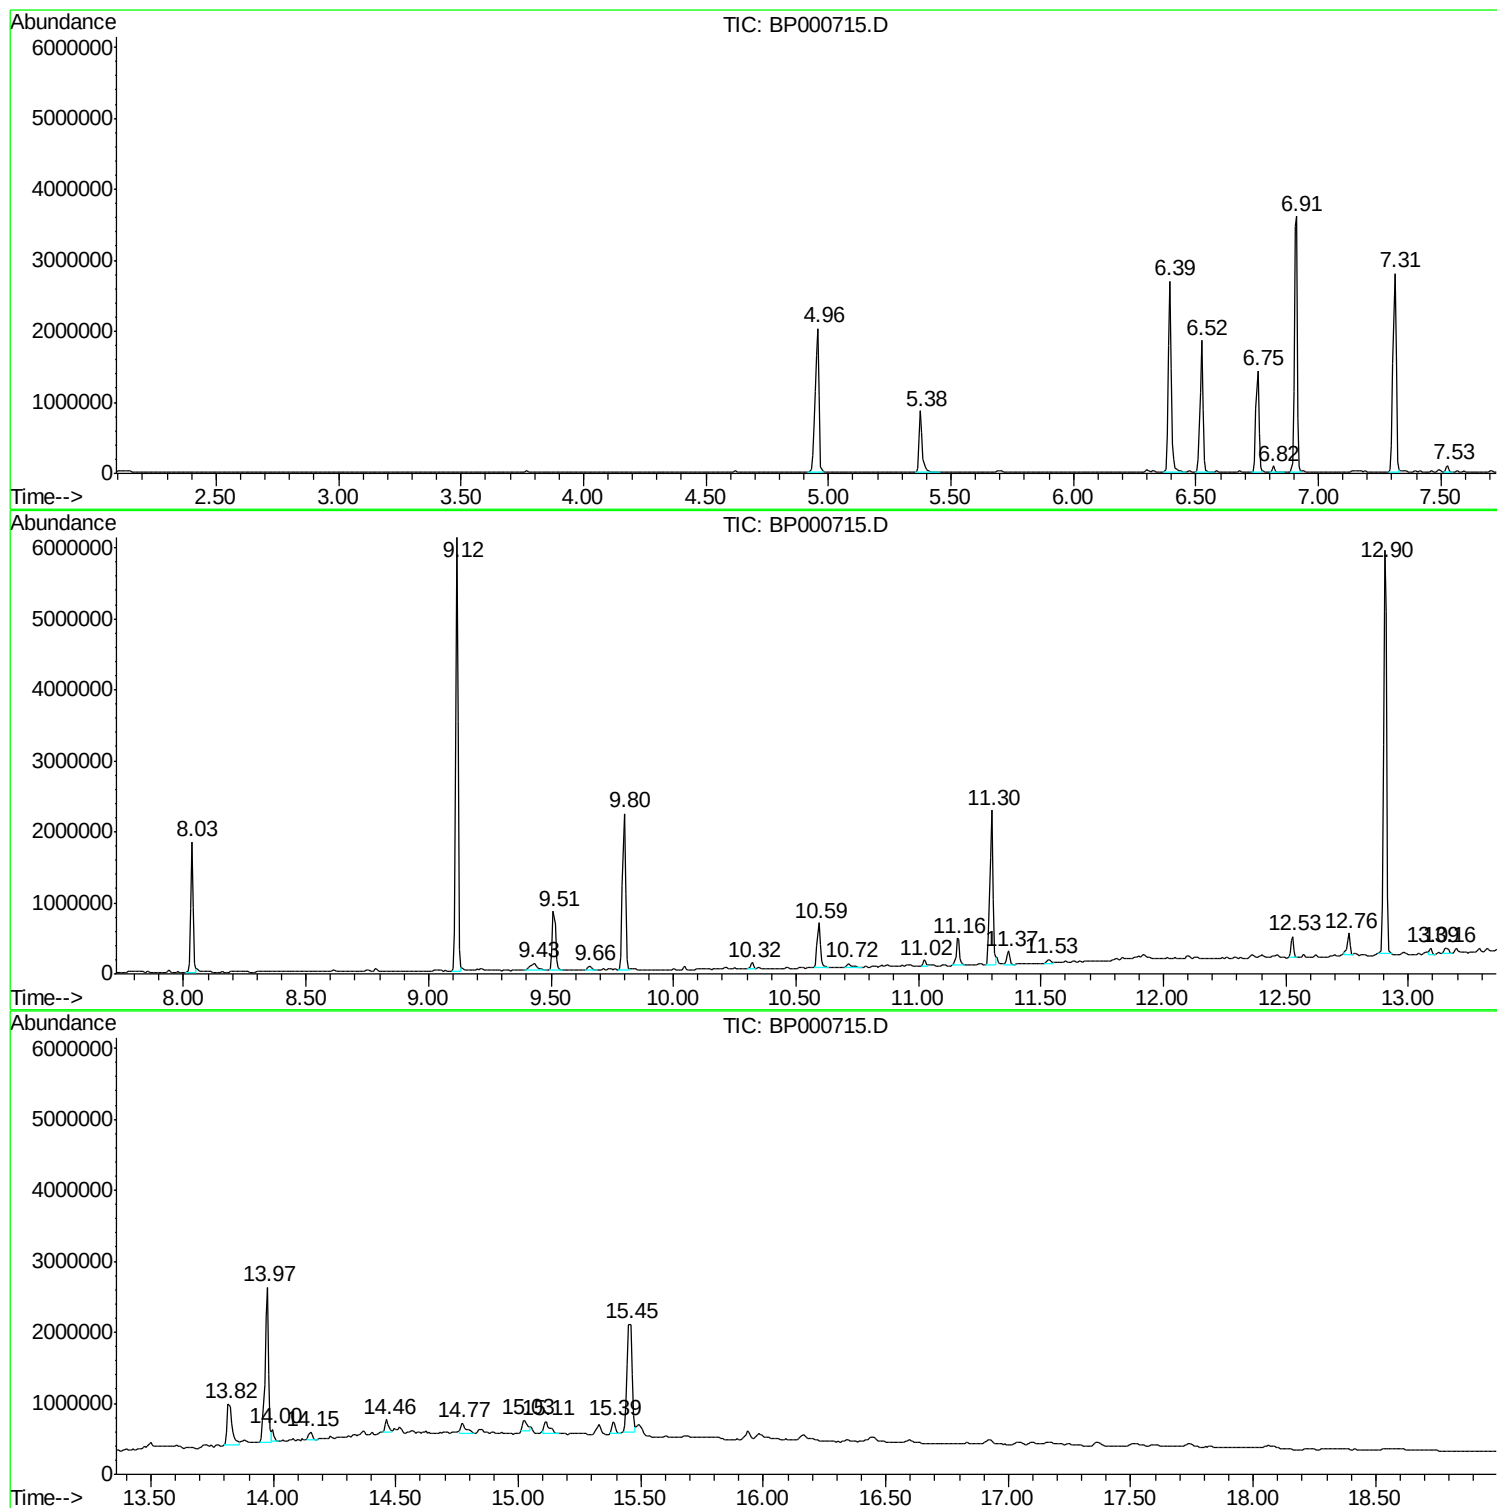

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000715.D
Acq_On : 14 Oct 2019 17:066
Operator : JUJ
Sample : K5348-12REE
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190880-COMPOSITE-LRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
