

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000716.D
 Acq On : 14 Oct 2019 17:31
 Operator : JU
 Sample : K5348-13RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190881-COMPOSITE-MRE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.969	482	490	493	rBV	2887061	4590947	100.00%	12.730%
2	5.381	557	560	573	rVB	208633	208942	4.55%	0.579%
3	6.393	728	732	741	rBV	1774900	1712607	37.30%	4.749%
4	6.522	750	754	762	rVB	817899	650830	14.18%	1.805%
5	6.751	789	793	796	rBV	1426887	1122414	24.45%	3.112%
6	6.816	801	804	809	rVV	97739	72777	1.59%	0.202%
7	6.910	816	820	823	rBV	3286411	2984745	65.01%	8.276%
8	7.310	884	888	891	rBV	2624050	2157044	46.98%	5.981%
9	7.528	922	925	928	rVB	102579	82243	1.79%	0.228%
10	8.034	1007	1011	1014	rBV	1826567	1397729	30.45%	3.876%
11	9.116	1191	1195	1198	rBV	5305054	4141414	90.21%	11.484%
12	9.216	1206	1212	1219	rBV6	28248	63413	1.38%	0.176%
13	9.422	1241	1247	1252	rBV	115431	205920	4.49%	0.571%
14	9.510	1259	1262	1268	rBV	703902	579462	12.62%	1.607%
15	9.657	1284	1287	1292	rBV	73506	74227	1.62%	0.206%
16	9.798	1307	1311	1315	rBV	2163398	1693599	36.89%	4.696%
17	10.322	1397	1400	1402	rVB2	80513	65629	1.43%	0.182%
18	10.592	1443	1446	1452	rBV2	122539	128694	2.80%	0.357%
19	10.716	1464	1467	1475	rVB4	58006	99981	2.18%	0.277%
20	11.022	1517	1519	1522	rBV	91319	86856	1.89%	0.241%
21	11.163	1539	1543	1555	rVB	453306	474726	10.34%	1.316%
22	11.298	1562	1566	1569	rBV	2239103	1884149	41.04%	5.225%
23	11.369	1575	1578	1582	rVB	111740	124695	2.72%	0.346%
24	12.363	1744	1747	1749	rBV	51794	53181	1.16%	0.147%
25	12.528	1771	1775	1778	rBV	368088	330829	7.21%	0.917%
26	12.757	1808	1814	1817	rBV	391101	410280	8.94%	1.138%
27	12.904	1835	1839	1843	rBV	5015809	4547064	99.04%	12.608%
28	13.092	1869	1871	1874	rVB	115357	87626	1.91%	0.243%
29	13.157	1880	1882	1885	rVB	83253	72095	1.57%	0.200%
30	13.822	1992	1995	2002	rBV2	247129	301908	6.58%	0.837%
31	13.975	2016	2021	2024	rBV	2229660	2332064	50.80%	6.467%
32	13.998	2024	2025	2028	rVB	222775	126259	2.75%	0.350%
33	14.463	2102	2104	2107	rVB	129329	106273	2.31%	0.295%
34	14.845	2166	2169	2175	rBV2	182016	191193	4.16%	0.530%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000716.D
Acq On : 14 Oct 2019 17:31
Operator : JU
Sample : K5348-13RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190881-COMPOSITE-MRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.022	2196	2199	2203	rBV	227282	345195	7.52%	0.957%
36	15.110	2212	2214	2217	rBV	105980	108387	2.36%	0.301%
37	15.327	2248	2251	2257	rVB	173138	235272	5.12%	0.652%
38	15.386	2258	2261	2267	rBV	208275	276073	6.01%	0.766%
39	15.457	2268	2273	2276	rBV	1533259	1936924	42.19%	5.371%


Sum of corrected areas: 36063666

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000716.D
Acq On : 14 Oct 2019 17:31
Operator : JU
Sample : K5348-13RE
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190881-COMPOSITE-MRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

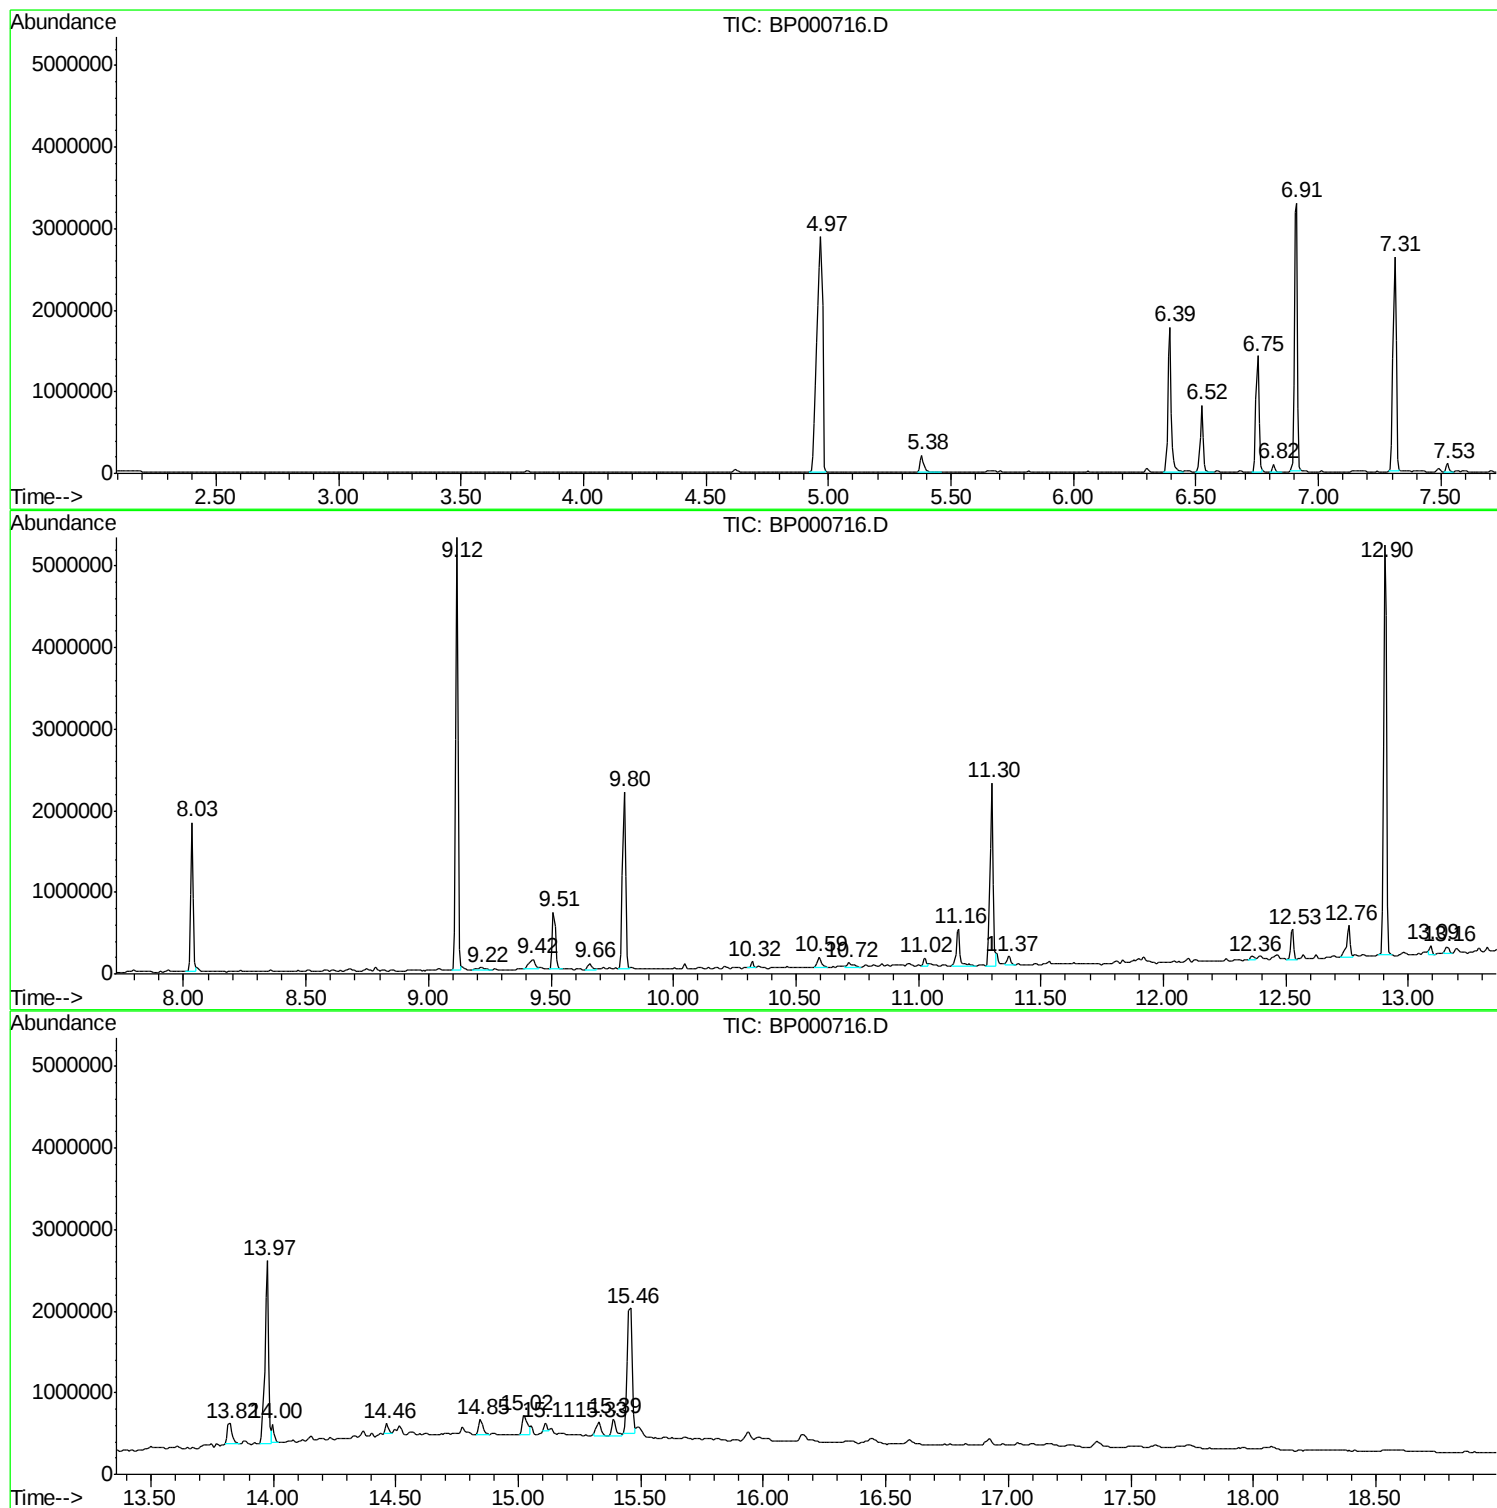

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000716.D
Acq_On : 14 Oct 2019 17:311
Operator : JUJ
Sample : K5348-13REE
Misc :
ALS_Vial : 15 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190881-COMPOSITE-MRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
