

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
 Data File : BP000717.D
 Acq On : 14 Oct 2019 17:55
 Operator : JU
 Sample : K5348-14RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 20190882-COMPOSITE-NRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.963	482	489	492	rBV	2239902	2945391	60.19%	8.465%
2	5.381	556	560	575	rVB	150555	159009	3.25%	0.457%
3	6.393	728	732	741	rBV	1381153	1478581	30.22%	4.249%
4	6.522	748	754	761	rBV	535499	436214	8.91%	1.254%
5	6.752	789	793	796	rBV	1437815	1133483	23.16%	3.258%
6	6.816	801	804	808	rBV	95163	69553	1.42%	0.200%
7	6.904	816	819	823	rBV	3363743	3030655	61.93%	8.710%
8	7.310	884	888	891	rBV	2657651	2108942	43.10%	6.061%
9	7.528	922	925	928	rVB	90194	73569	1.50%	0.211%
10	8.034	1007	1011	1014	rBV	1914361	1420182	29.02%	4.082%
11	9.116	1191	1195	1198	rBV	5760317	4507142	92.11%	12.954%
12	9.434	1242	1249	1256	rBV	83680	159144	3.25%	0.457%
13	9.510	1259	1262	1268	rBV	723054	602389	12.31%	1.731%
14	9.657	1284	1287	1292	rBV	63614	64682	1.32%	0.186%
15	9.798	1307	1311	1315	rBV	2197286	1722596	35.20%	4.951%
16	10.322	1397	1400	1402	rVB2	69509	59681	1.22%	0.172%
17	10.593	1443	1446	1454	rBV2	166765	172710	3.53%	0.496%
18	10.716	1464	1467	1475	rVB5	56422	94589	1.93%	0.272%
19	11.022	1517	1519	1522	rBV	81915	72108	1.47%	0.207%
20	11.157	1539	1542	1547	rBV	422231	386377	7.90%	1.110%
21	11.298	1562	1566	1569	rBV	2076326	1897106	38.77%	5.452%
22	11.369	1574	1578	1582	rVB2	138887	151108	3.09%	0.434%
23	11.916	1669	1671	1680	rVB	77301	112398	2.30%	0.323%
24	12.522	1771	1774	1778	rBV	347729	300660	6.14%	0.864%
25	12.622	1788	1791	1794	rBV2	71187	64090	1.31%	0.184%
26	12.757	1809	1814	1816	rVB	317471	299195	6.11%	0.860%
27	12.904	1835	1839	1842	rBV	5595987	4893468	100.00%	14.064%
28	13.092	1868	1871	1874	rVB	102334	95191	1.95%	0.274%
29	13.128	1874	1877	1879	rBV3	59268	63843	1.30%	0.183%
30	13.157	1879	1882	1885	rVB	75224	69664	1.42%	0.200%
31	13.316	1907	1909	1912	rBV	50767	56407	1.15%	0.162%
32	13.816	1991	1994	2002	rBV	556244	626219	12.80%	1.800%
33	13.975	2016	2021	2024	rBV	2158390	2357734	48.18%	6.776%
34	13.998	2024	2025	2030	rVB	204869	120663	2.47%	0.347%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data File : BP000717.D
Acq On : 14 Oct 2019 17:55
Operator : JU
Sample : K5348-14RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190882-COMPOSITE-NRE

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	14.463	2101	2104	2107	rBV2	142207	135586	2.77%	0.390%
36	15.022	2196	2199	2203	rBV	208759	313984	6.42%	0.902%
37	15.110	2211	2214	2216	rBV	126260	134198	2.74%	0.386%
38	15.328	2248	2251	2257	rVB	155824	205544	4.20%	0.591%
39	15.386	2258	2261	2267	rBV	187368	231578	4.73%	0.666%
40	15.451	2268	2272	2276	rBV	1617439	1968997	40.24%	5.659%


Sum of corrected areas: 34794630

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP101419\
Data File : BP000717.D
Acq On : 14 Oct 2019 17:55
Operator : JU
Sample : K5348-14RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
20190882-COMPOSITE-NRE

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP100119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

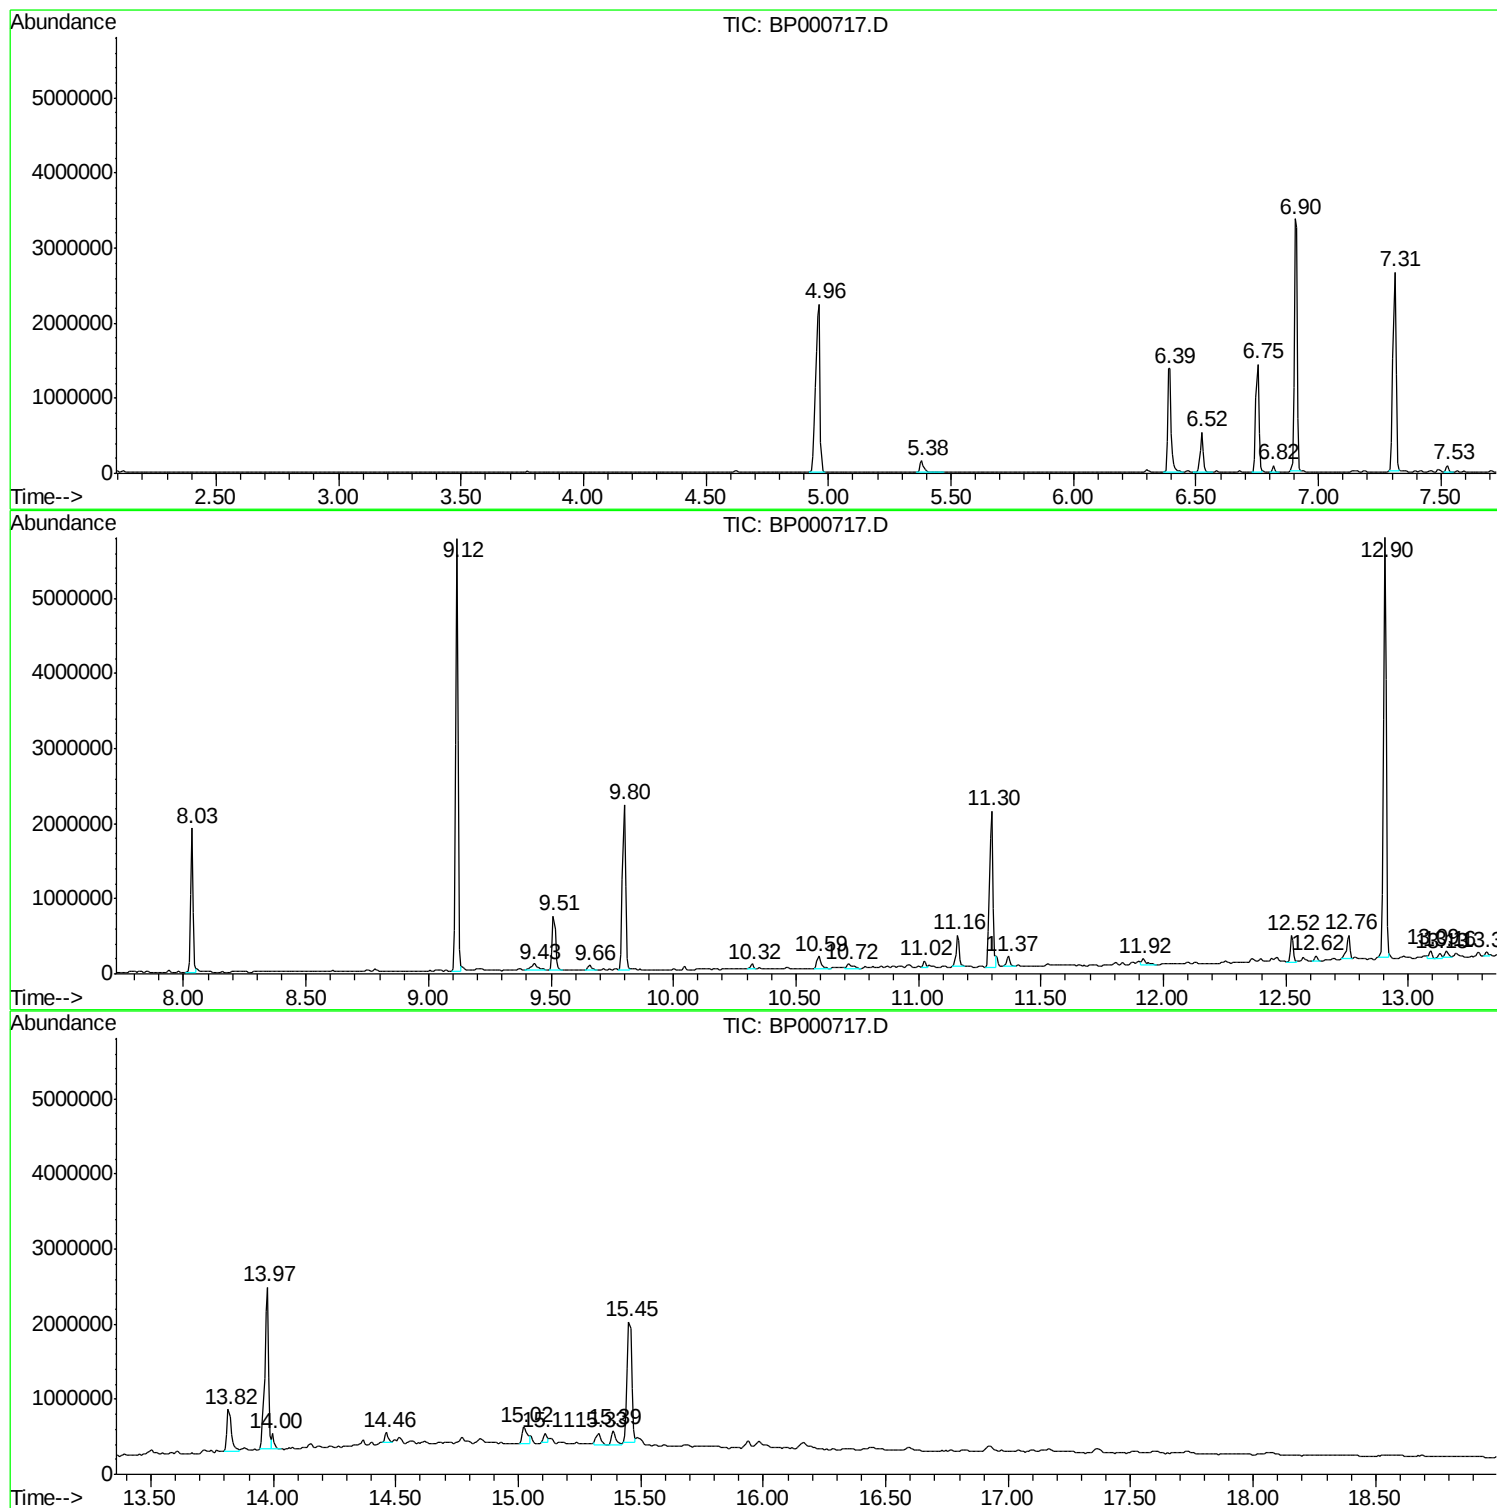

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
Data_File : BP000717.D
Acq_On : 14 Oct 2019 17:555
Operator : JUJ
Sample : K5348-14REE
Misc :
ALS_Vial : 16 Sample_Multiplier: 11

Instrument :
BNA_P
ClientSampleId :
20190882-COMPOSITE-NRE

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
