


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP101419\
 Data File : BP000702.D
 Acq On : 14 Oct 2019 11:28
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP100119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 01 18:03:42 2019

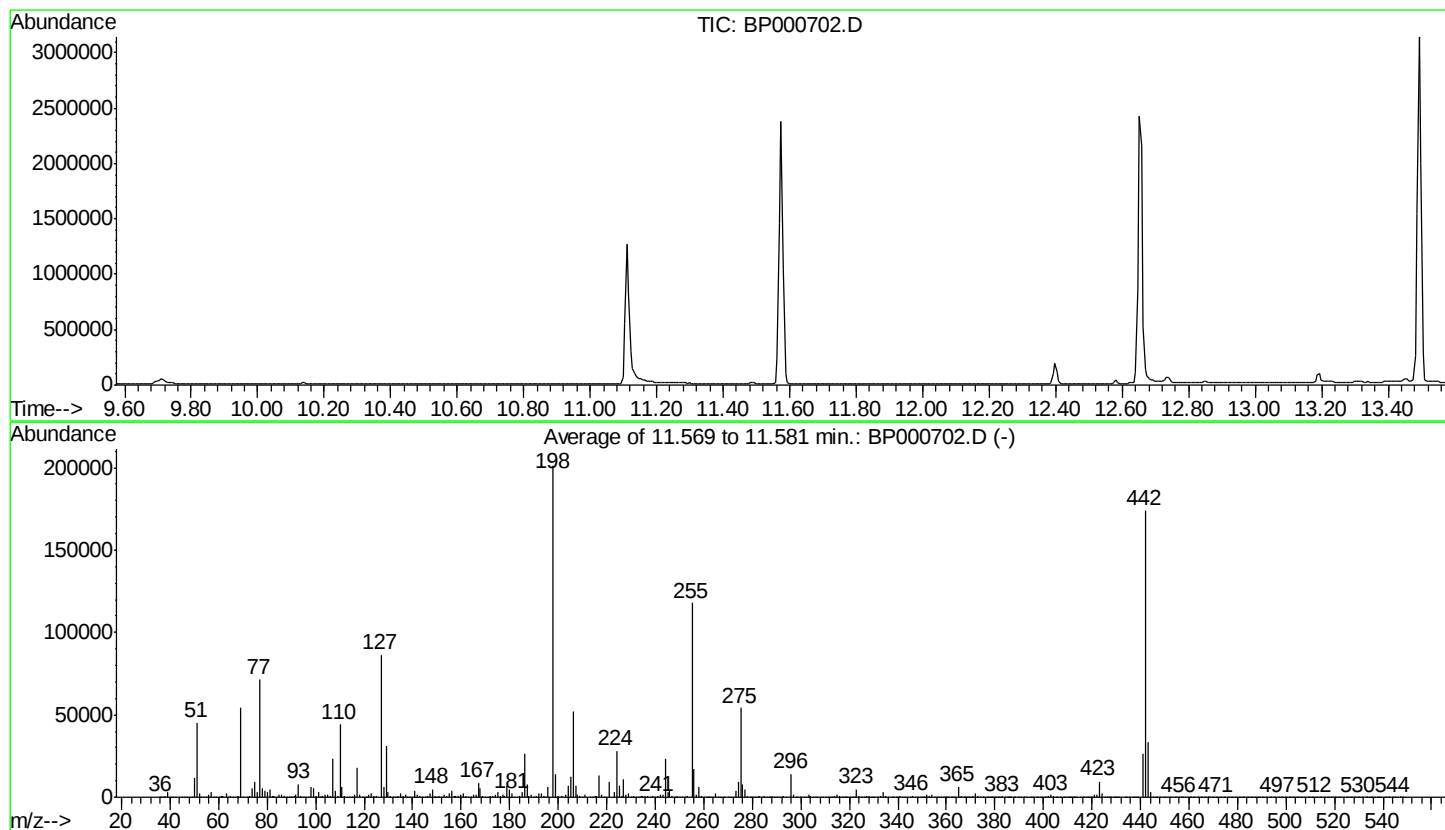

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.5	45291	PASS
68	69	0.00	2	1.8	972	PASS
69	198	0.00	100	27.1	54609	PASS
70	69	0.00	2	0.4	241	PASS
127	198	10	80	42.9	86242	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	201227	PASS
199	198	5	9	6.9	13828	PASS
275	198	10	60	26.9	54130	PASS
365	198	1	100	3.1	6244	PASS
441	198	0.01	100	13.3	26764	PASS
442	198	50	100	86.4	173904	PASS
443	442	15	24	19.2	33350	PASS