
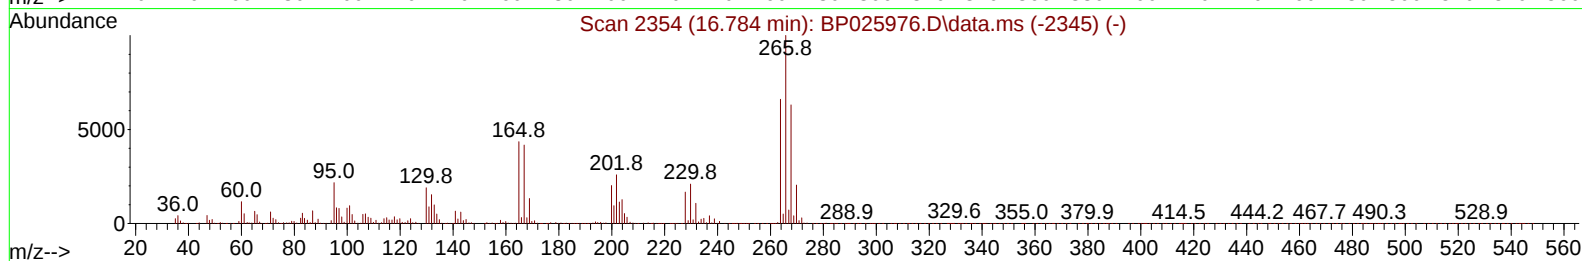
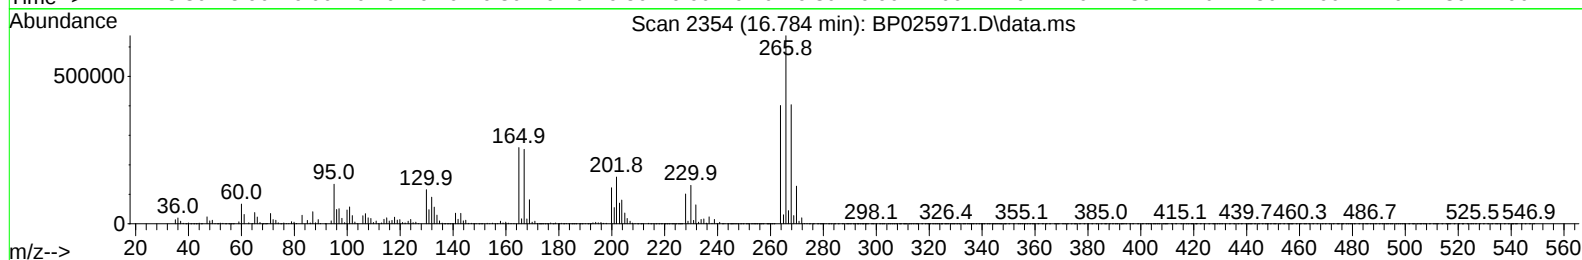


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101525\
Data File : BP025971.D
Acq On : 15 Oct 2025 11:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 00:50:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

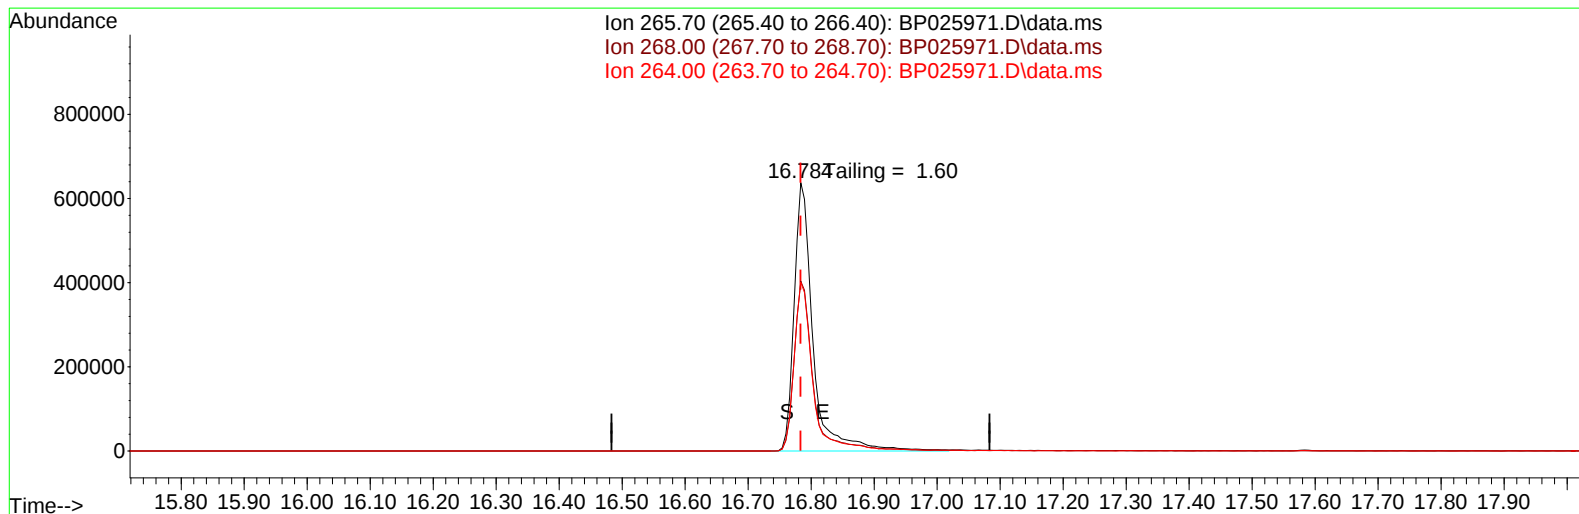

TIC: BP025971.D\data.ms

(70) Pentachlorophenol (C)




16.784min (-0.000) 483538.38 ng

response 1341024

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.29
264.00	66.10	62.92
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP101525\
Data File : BP025971.D
Acq On : 15 Oct 2025 11:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 17 00:50:59 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP101525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 15 23:48:51 2025
Response via : Initial Calibration

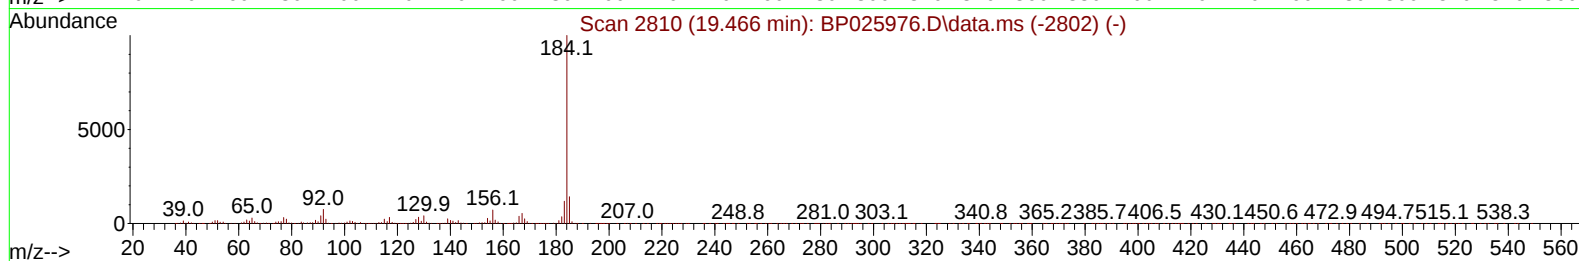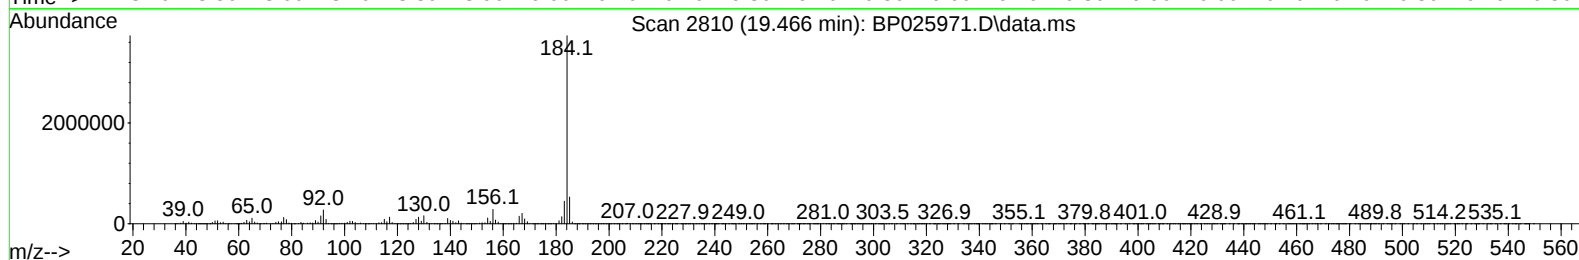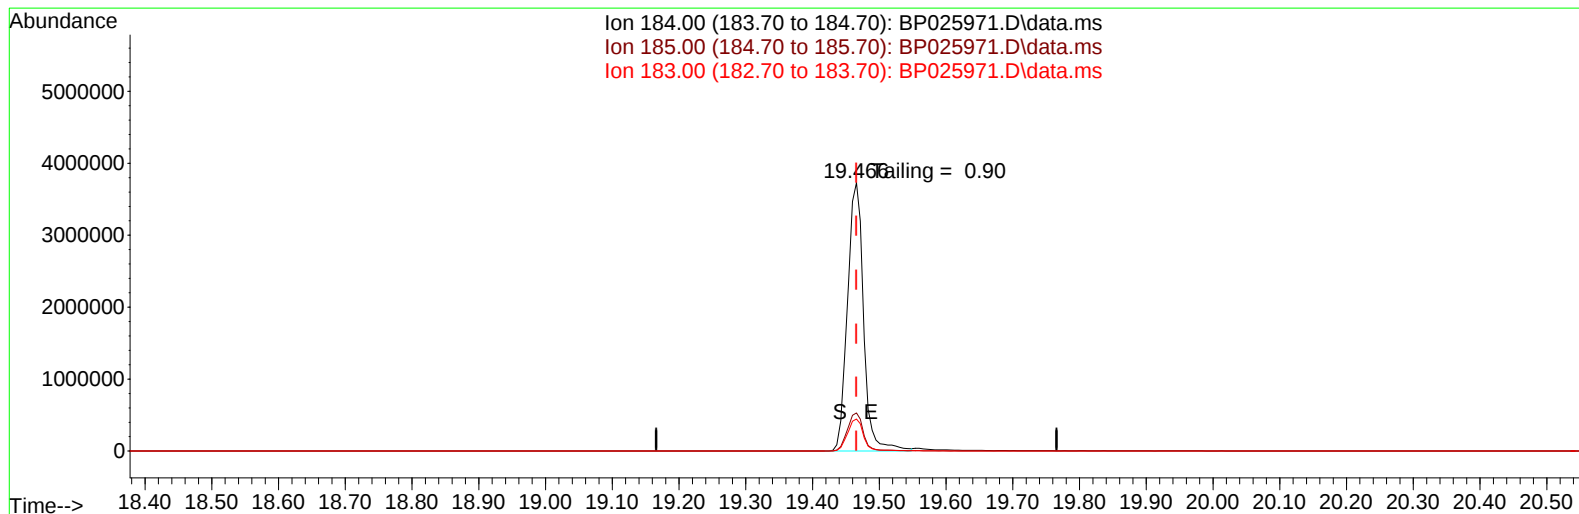

TIC: BP025971.D\data.ms

(77) Benzidine**19.466min (0.000) 636250.68 ng****response 6258686**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.21
183.00	11.80	11.97
0.00	0.00	0.00