

Data File : BP000753.D

Acq On : 15 Oct 2019 10:05

Operator : JU

Sample : SSTDCCC020

Misc :

ALS Vial : 2 Sample Multiplier: 1




Quant Time: Oct 16 02:08:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Tue Oct 15 03:51:25 2019

Response via : Initial Calibration

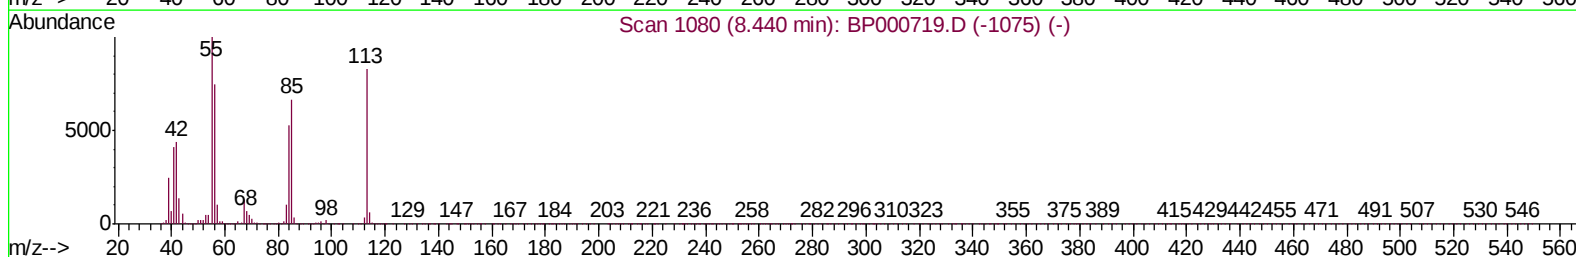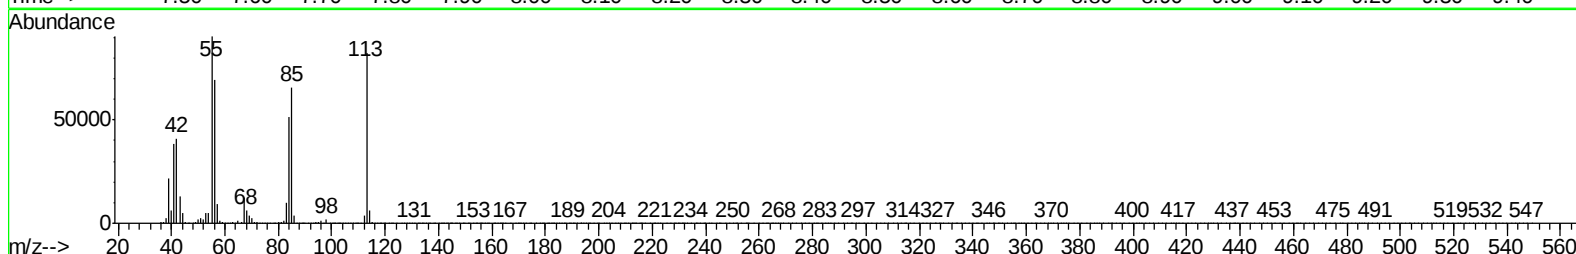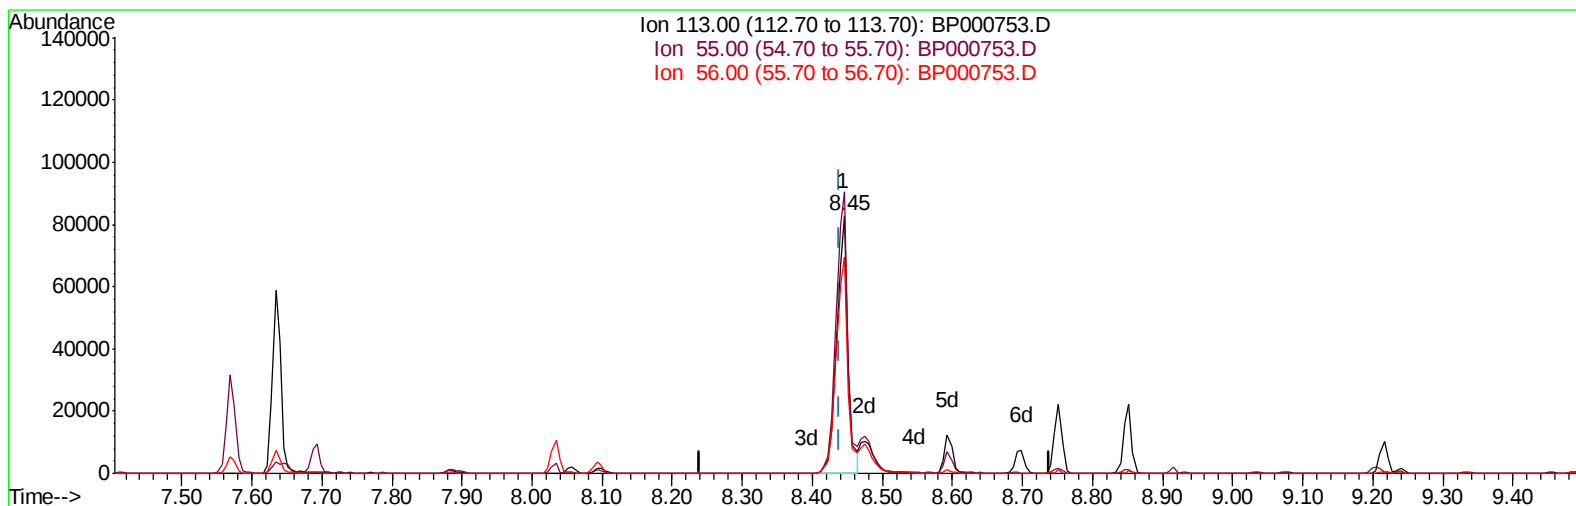

TIC: BP000753.D

(32) Caprolactam

8.446min (+0.006) 17.16ng/ul

response 90688

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	109.37
56.00	86.80	84.21
0.00	0.00	0.00