
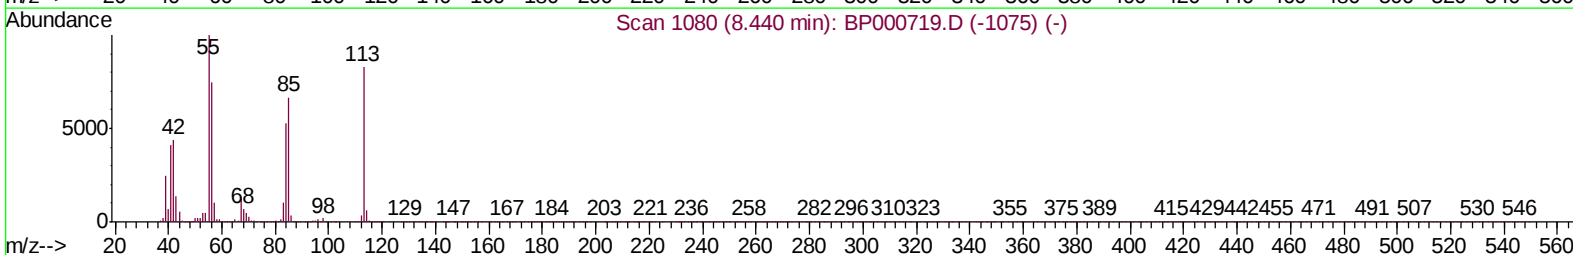
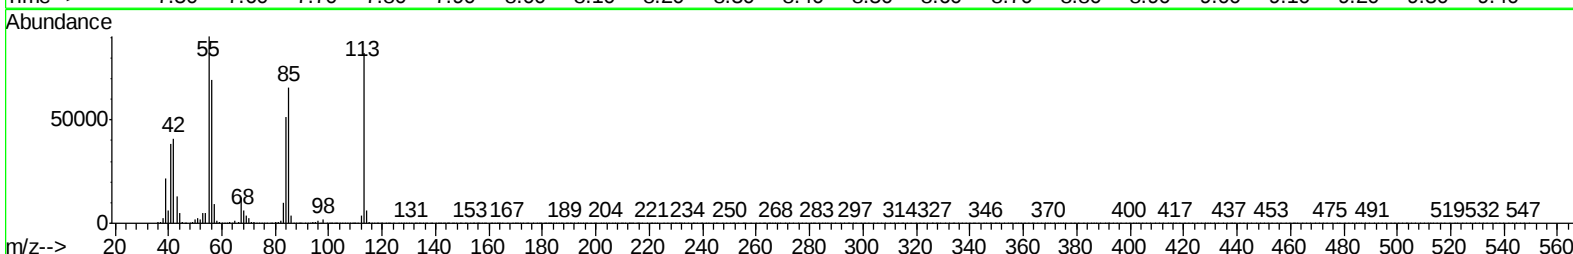


Data File : BP000753.D
Acq On : 15 Oct 2019 10:05
Operator : JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Oct 16 02:08:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 15 03:51:25 2019
Response via : Initial Calibration

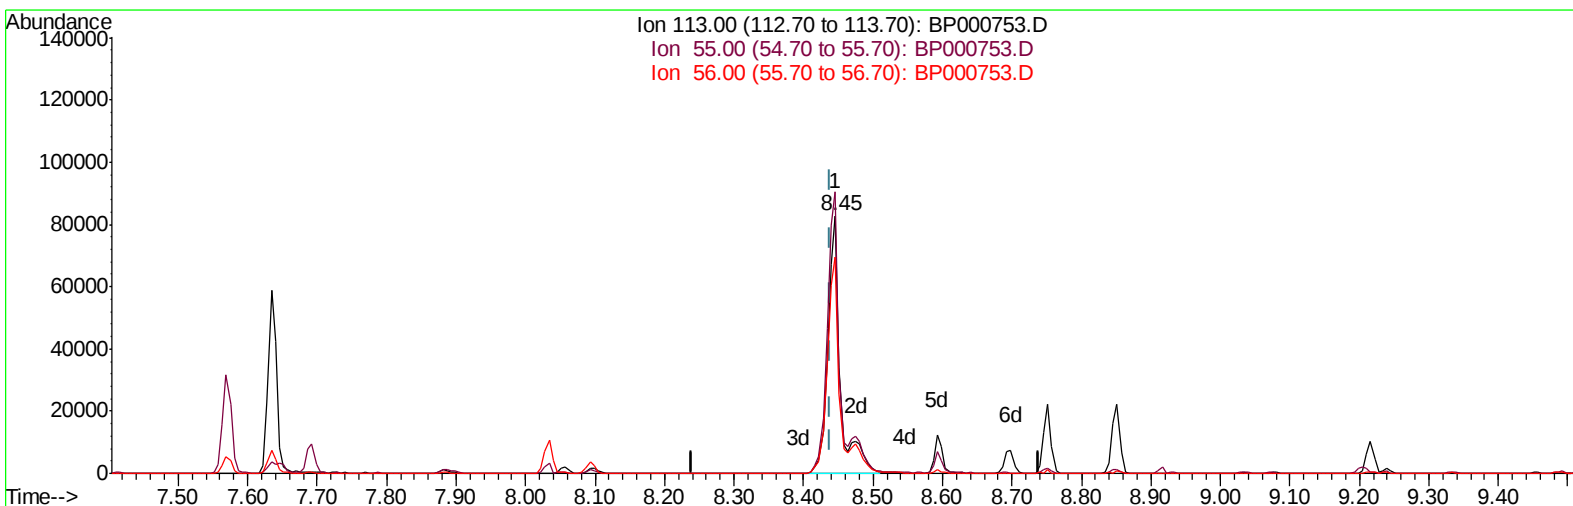

TIC: BP000753.D

(32) Caprolactam

8.446min (+0.006) 19.95ng/ul m

response 105458

Ion	Exp%	Act%
113.00	100	100
55.00	116.30	109.37
56.00	86.80	84.21
0.00	0.00	0.00