

Data File : BP000754.D

Acq On : 15 Oct 2019 10:32

Operator : JU

Sample : K5175-01

Misc :

ALS Vial : 3 Sample Multiplier: 1




Quant Time: Oct 16 02:24:49 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP100919MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Wed Oct 16 02:22:01 2019

Response via : Initial Calibration

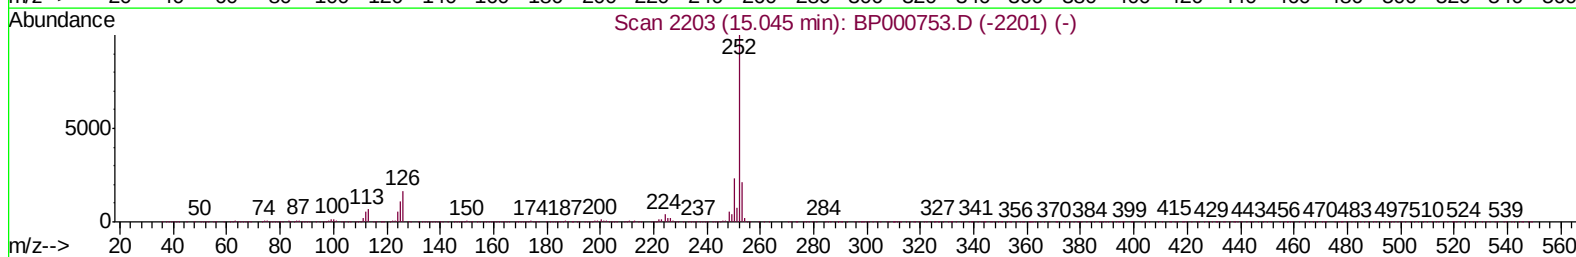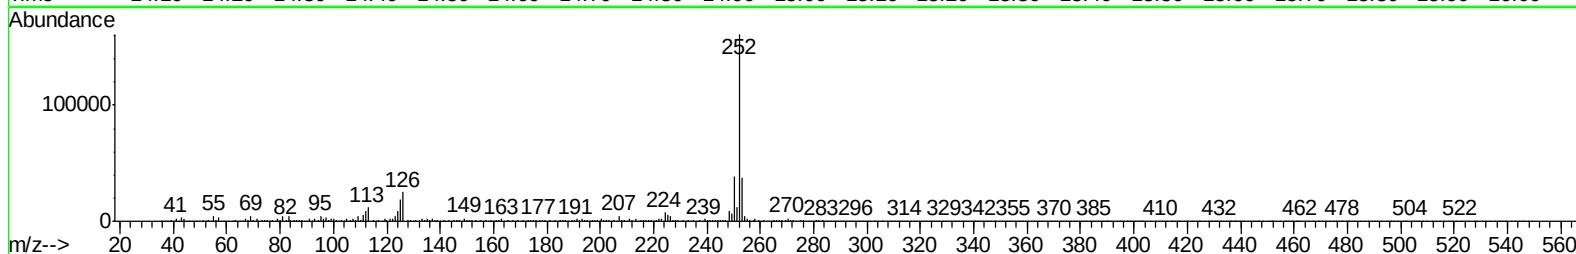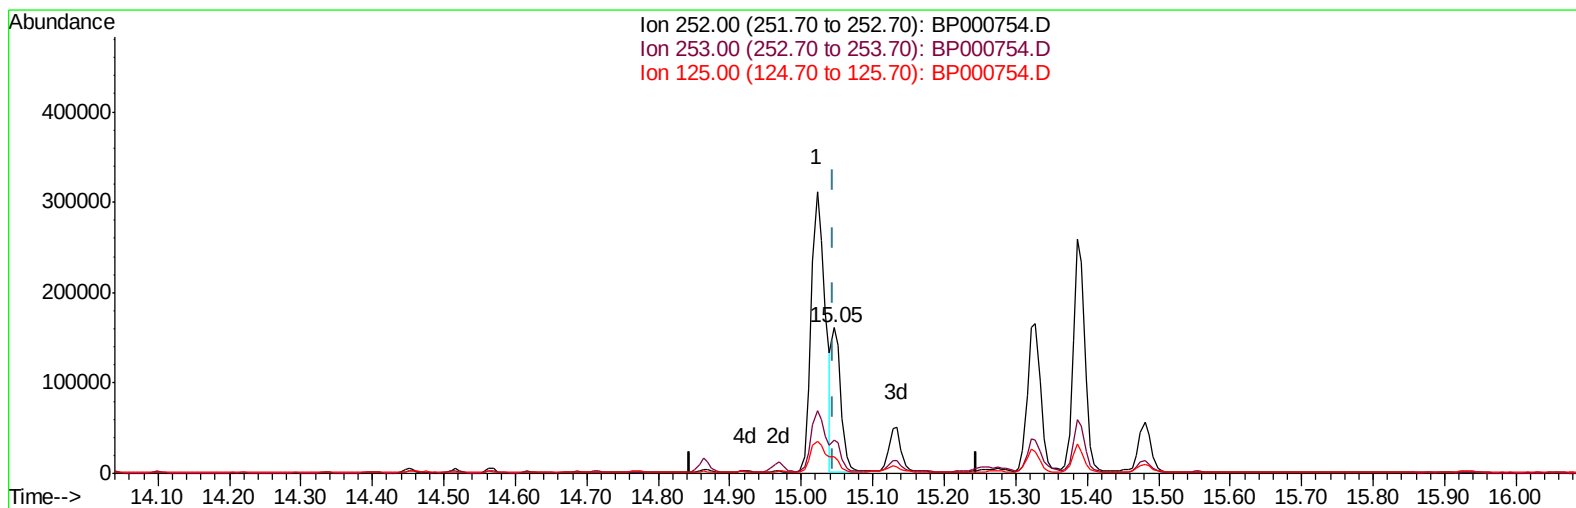

TIC: BP000754.D

(89) Benzo(k)fluoranthene

15.045min (+0.000) 3.44ng/ul m

response 138202

Ion	Exp%	Act%
252.00	100	100
253.00	22.20	23.04
125.00	10.30	11.58
0.00	0.00	0.00